


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071023\
 Data File : BF134182.D
 Acq On : 10 Jul 2023 12:16
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jul 10 18:49:59 2023

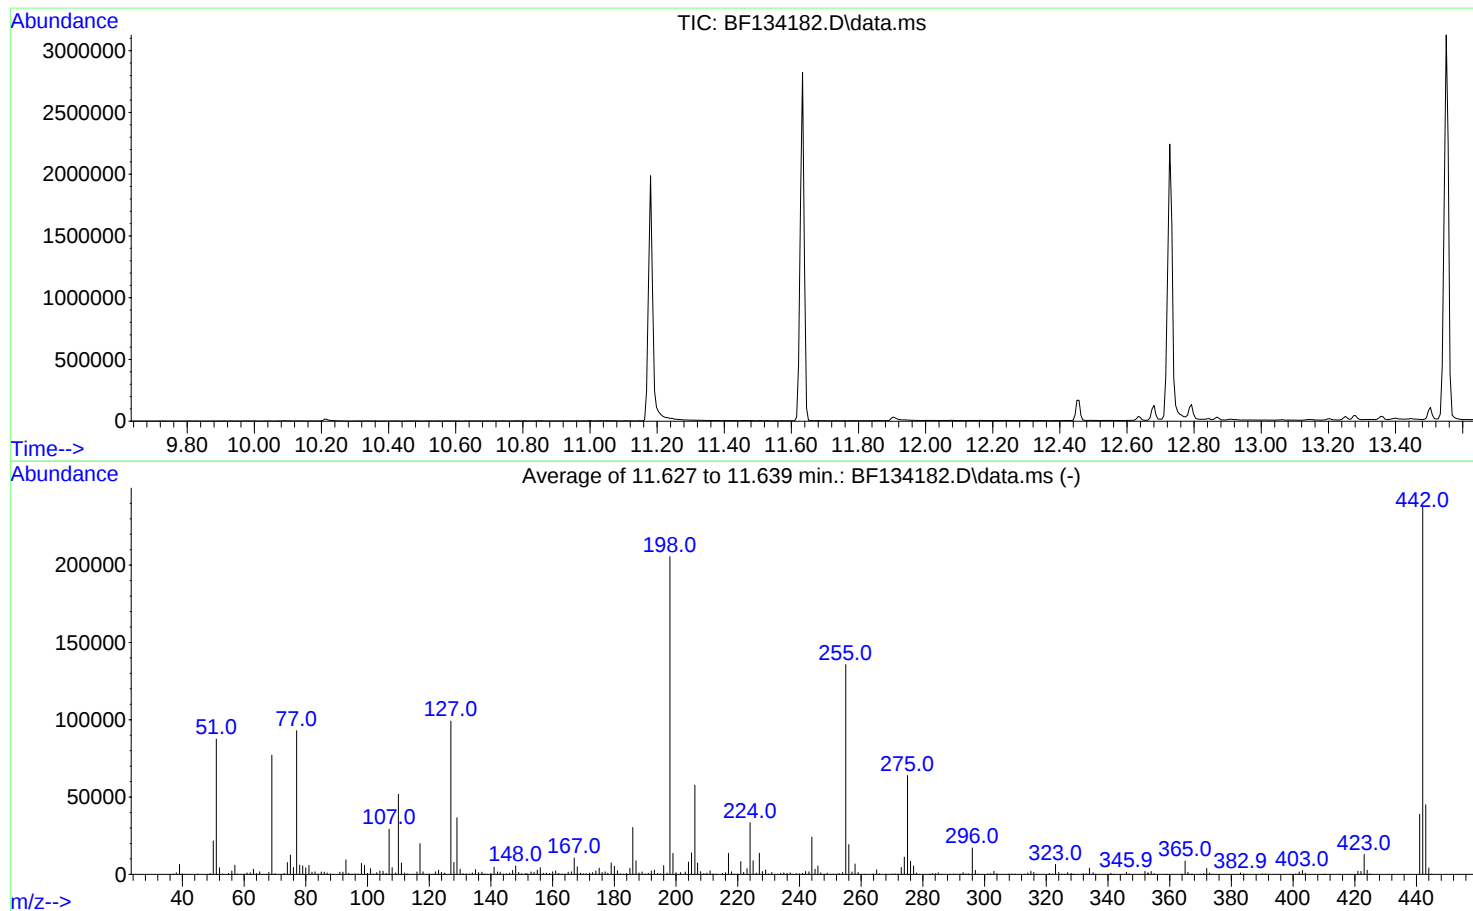




AutoFind: Scans 1622, 1623, 1624; Background Corrected with Scan 1617

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.6	87581	PASS
68	69	0.00	2	1.8	1350	PASS
69	198	0.00	100	37.5	77099	PASS
70	69	0.00	2	0.5	370	PASS
127	198	10	80	48.2	99109	PASS
197	198	0.00	2	0.4	874	PASS
198	198	100	100	100.0	205560	PASS
199	198	5	9	6.6	13524	PASS
275	198	10	60	31.1	63989	PASS
365	198	1	100	4.2	8605	PASS
441	198	0.01	100	18.9	38797	PASS
442	442	50	100	100.0	237931	PASS
443	442	15	24	18.9	44989	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071023\
 Data File : BF134182.D
 Acq On : 10 Jul 2023 12:16
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Jul 10 16:37:53 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 30 18:35:29 2023
 Response via : Initial Calibration

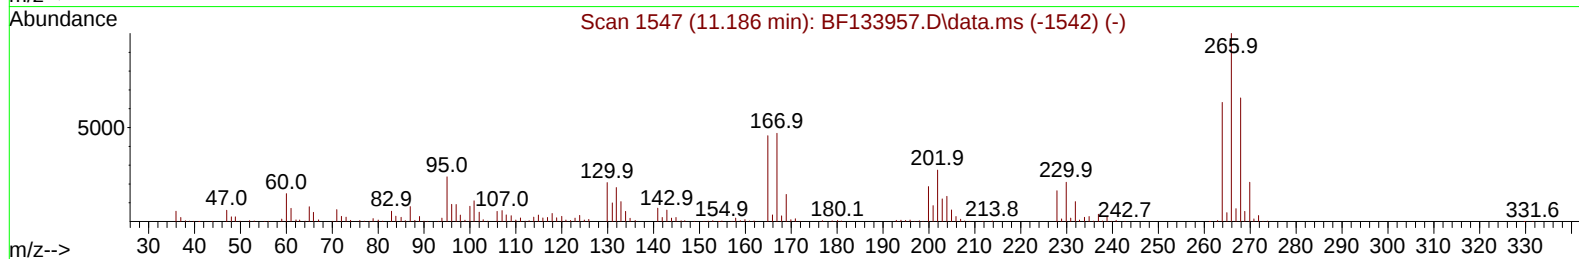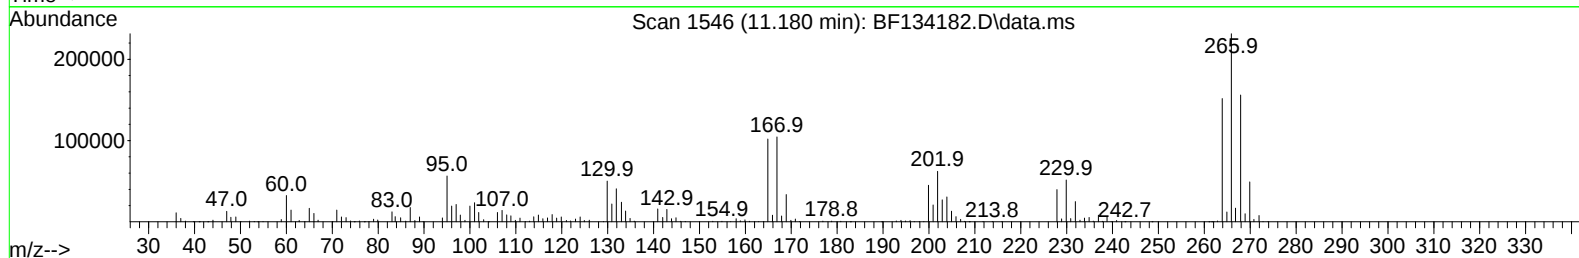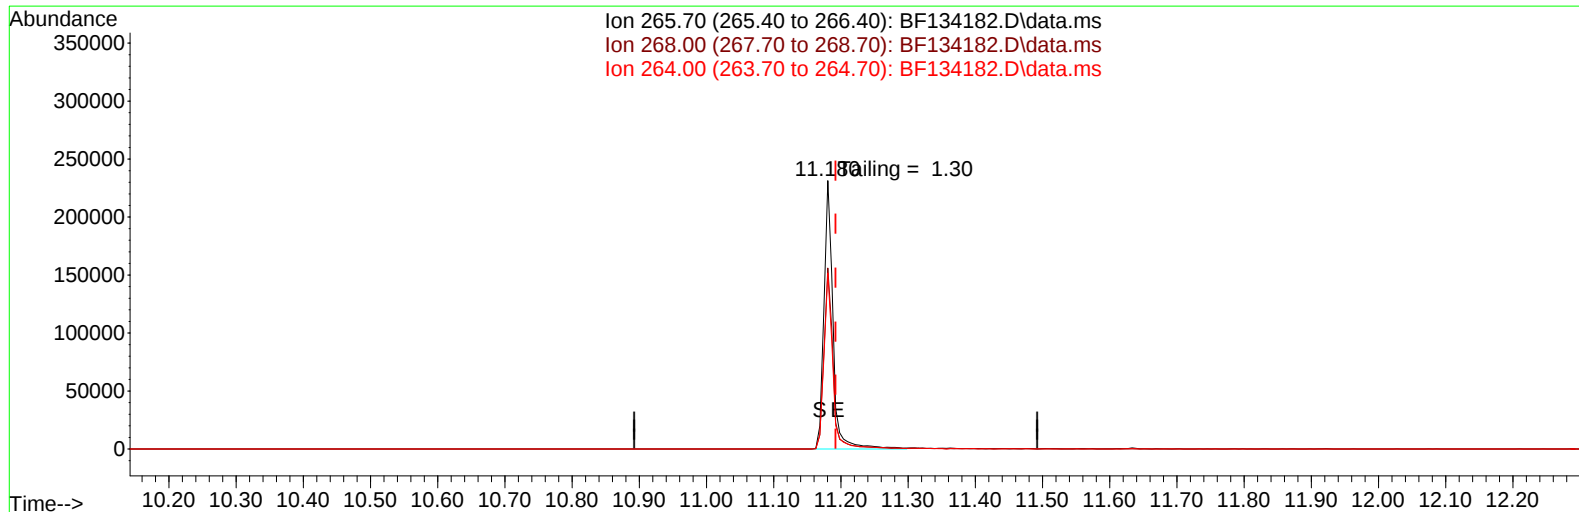

TIC: BF134182.D\data.ms

(70) Pentachlorophenol (C)

11.180min (-0.012) 28675.39 ng




response 218646

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.80	67.42
264.00	63.30	65.57
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071023\
Data File : BF134182.D
Acq On : 10 Jul 2023 12:16
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 10 16:37:53 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 30 18:35:29 2023
Response via : Initial Calibration

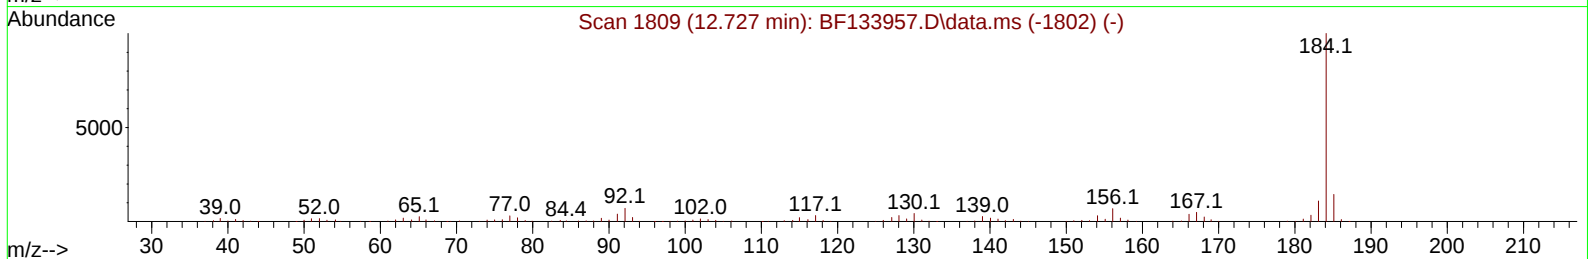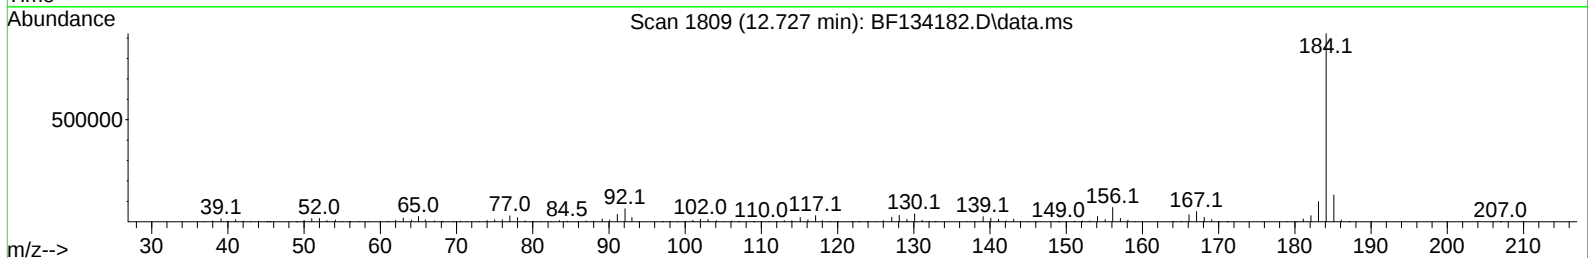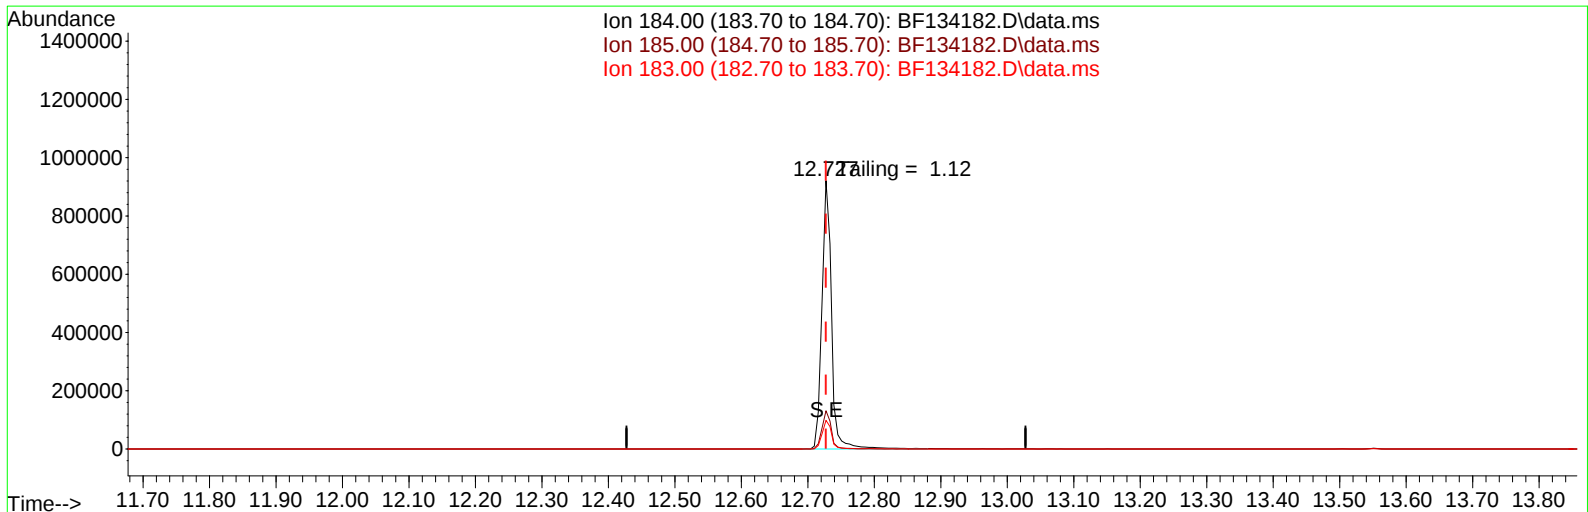

TIC: BF134182.D\data.ms

(77) Benzidine

12.727min (-0.000) 0.00 ng

response 924359

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.26
183.00	11.00	10.72
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/10/2023	BNA_F	<u>BF134182.D</u>
Compound Name	Response	Retention Time
DDT	560727	13.551
DDD	11843	13.28
DDE	1096	12.91
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
12939	573666	2.26

Instrument :
BNA_F
ClientSampleId :
DFTPP