

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF071119\
 Data File : BF115514.D
 Acq On : 12 Jul 2019 00:14
 Operator : HP/JU
 Sample : K3621-03 5X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OK-03-071019-B

Quant Time: Jul 12 03:17:44 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF070519.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 10 16:47:05 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.89	152	128700	20.00	ng	0.00
21) Naphthalene-d8	8.17	136	514491	20.00	ng	0.00
39) Acenaphthene-d10	9.93	164	235735	20.00	ng	0.00
64) Phenanthrene-d10	11.42	188	411088	20.00	ng	0.00
76) Chrysene-d12	14.06	240	343313	20.00	ng	-0.01
87) Perylene-d12	15.54	264	295522	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.50	112	79979	9.60	ng	-0.01
7) Phenol-d6	6.51	99	110629	10.44	ng	-0.01
23) Nitrobenzene-d5	7.45	82	61246	7.03	ng	-0.01
42) 2,4,6-Tribromophenol	10.72	330	23110	8.87	ng	-0.01
45) 2-Fluorobiphenyl	9.25	172	140911	10.49	ng	0.00
79) Terphenyl-d14	13.00	244	138496	8.26	ng	-0.01
Target Compounds						
9) Benzaldehyde	6.66	77	2120	Below Cal	#	81
25) Isophorone	7.45	82	61245	3.245 ng	#	64
51) 2,6-Dinitrotoluene	9.93	165	29189	7.607 ng	#	28
57) 2,4-Dinitrotoluene	9.93	165	29189	5.985 ng	#	24
86) Indeno(1,2,3-cd)pyrene	17.06	276	261	Below Cal	#	50


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF071119\
Data File : BF115514.D
Acq On : 12 Jul 2019 00:14
Operator : HP/JU
Sample : K3621-03 5X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OK-03-071019-B

Quant Time: Jul 12 03:17:44 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF070519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 10 16:47:05 2019
Response via : Initial Calibration




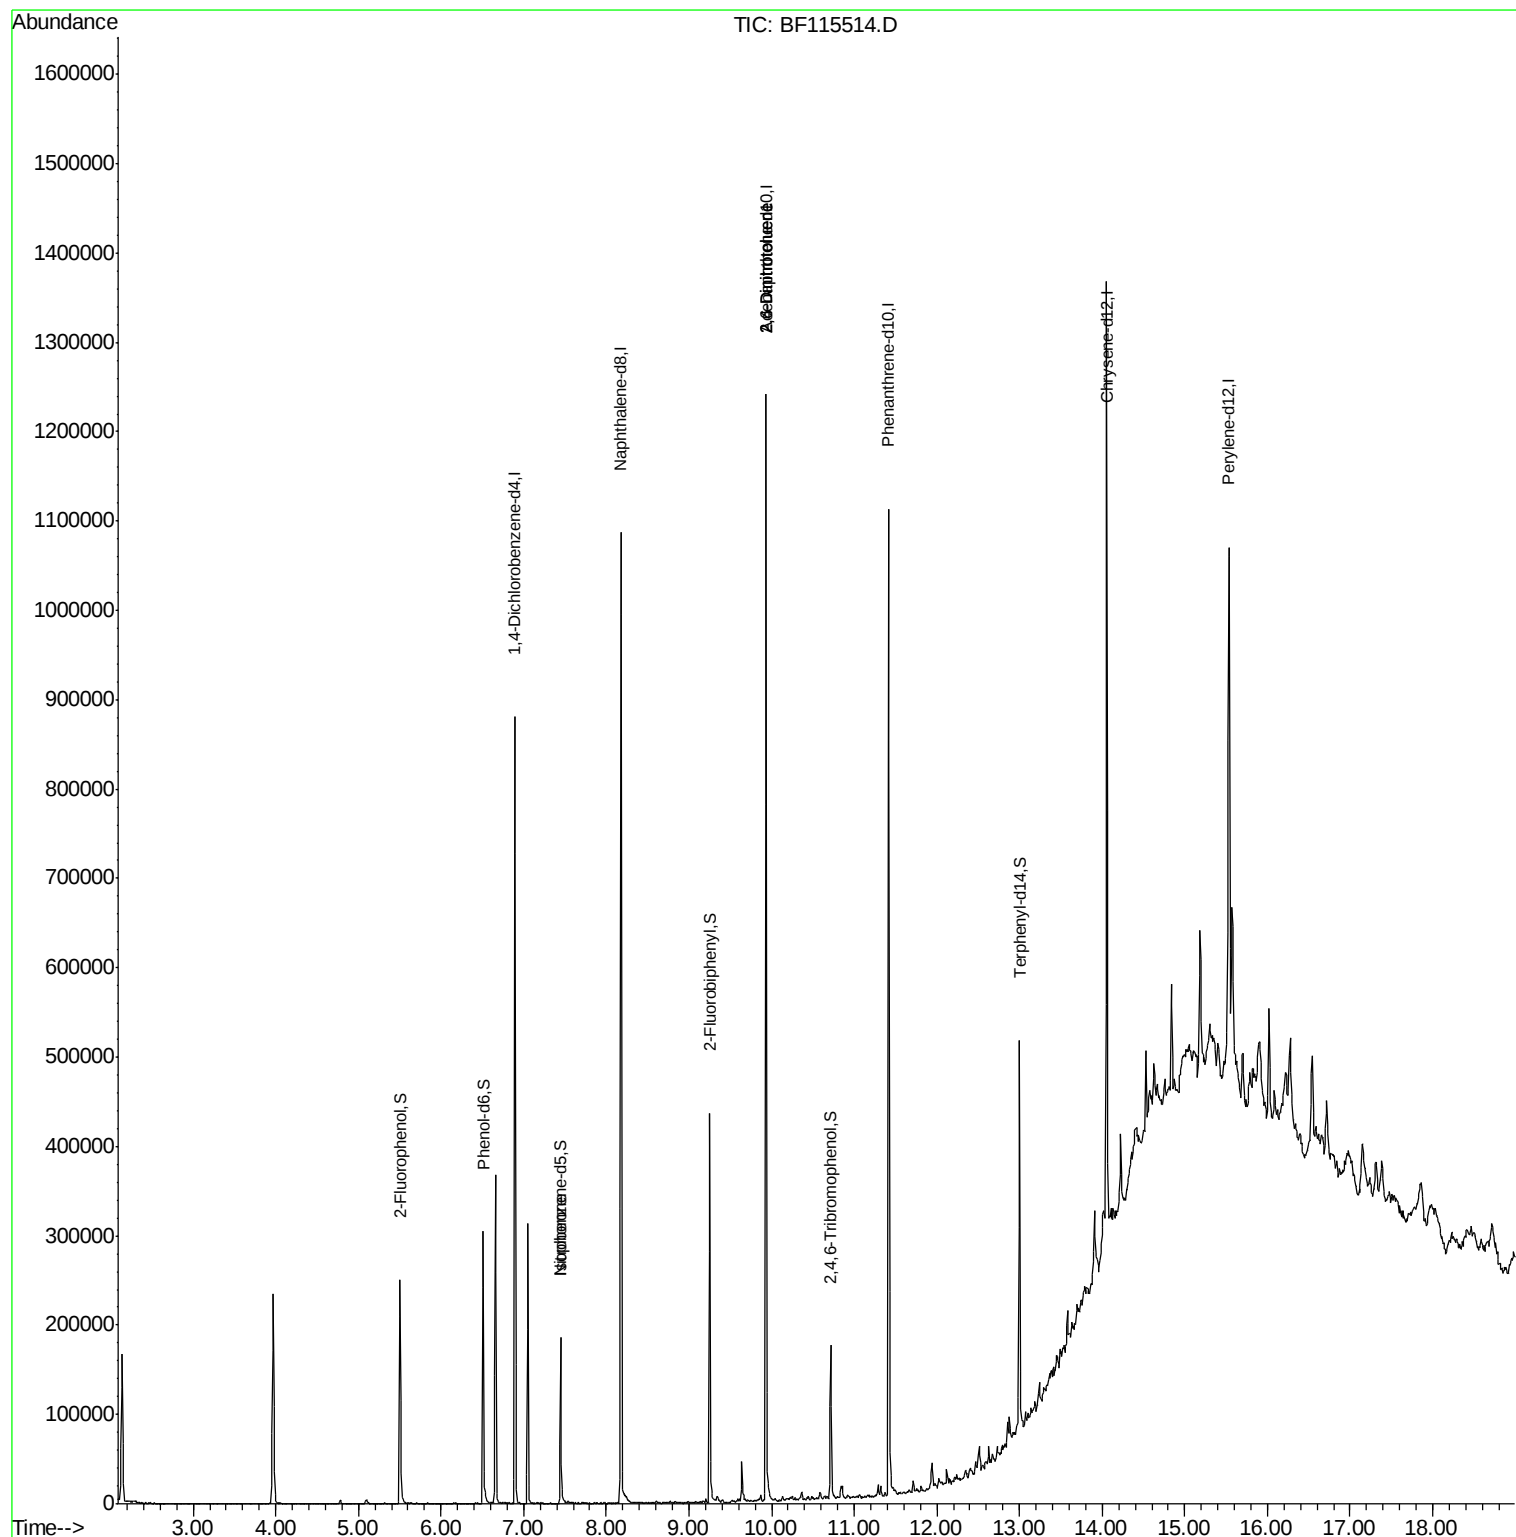


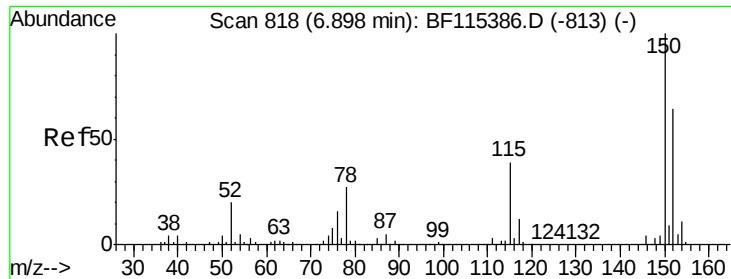

#1
 1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 6.89 min Scan# 817
 Delta R.T. -0.01 min
 Lab File: BF115514.D
 Acq: 12 Jul 2019 00:14




Instrument :
 BNA_F
 ClientSampleId :
 OK-03-071019-B


Tot Ion:152 Resp: 128700
 Ion Ratio Lower Upper
 152 100
 150 159.5 127.4 191.2
 115 62.3 46.2 69.4

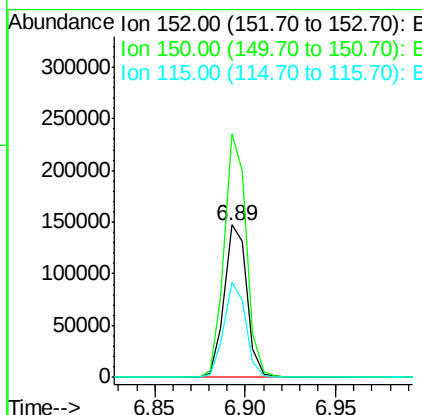

#5
 2-Fluorophenol
 Concen: 9.601 ng
 RT: 5.50 min Scan# 581
 Delta R.T. -0.01 min
 Lab File: BF115514.D
 Acq: 12 Jul 2019 00:14

Tgt Ion:112 Resp: 79979
 Ion Ratio Lower Upper
 112 100
 64 53.8 44.2 66.2
 63 27.4 22.1 33.1

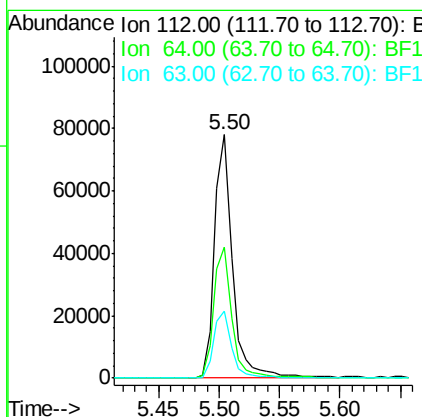

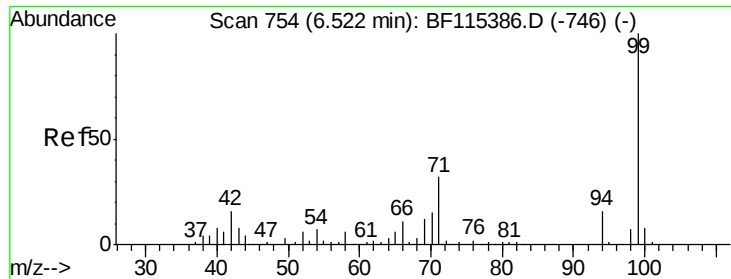

#7

Phenol-d6

Concen: 10.443 ng

RT: 6.51 min Scan# 752

Delta R.T. -0.01 min

Lab File: BF115514.D

Acq: 12 Jul 2019 00:14

Instrument :

BNA_F

ClientSampleId :

OK-03-071019-B


Tot Ion: 99 Resp: 110629

Ion Ratio Lower Upper

99 100

42 14.4 12.8 19.2




71 29.9 26.5 39.7



Abundance Ion 99.00 (98.70 to 99.70): BF1

Ion 42.00 (41.70 to 42.70): BF1

Ion 71.00 (70.70 to 71.70): BF1

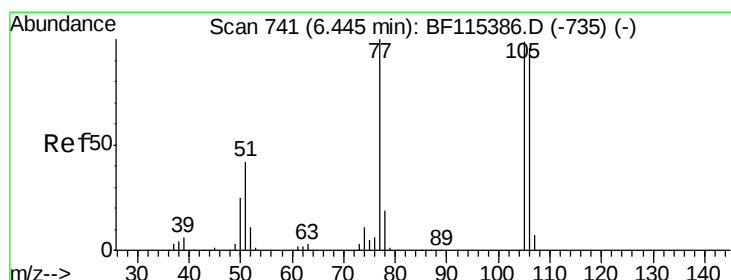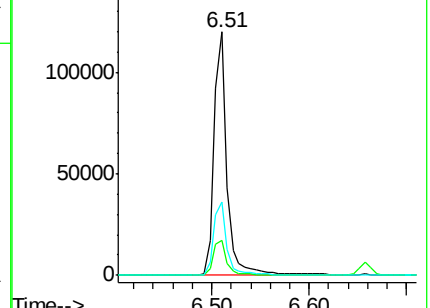

#9

Benzaldehyde

Concen: Below Cal

RT: 6.66 min Scan# 777

Delta R.T. 0.21 min

Lab File: BF115514.D

Acq: 12 Jul 2019 00:14


Tgt Ion: 77 Resp: 2120

Ion Ratio Lower Upper

77 100

105 86.2 82.9 122.9



106 75.6 77.8 117.8#

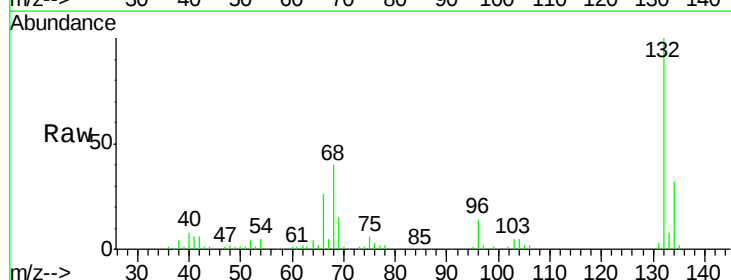


Abundance Ion 77.00 (76.70 to 77.70): BF1

Ion 105.00 (104.70 to 105.70): BF1

Ion 106.00 (105.70 to 106.70): BF1

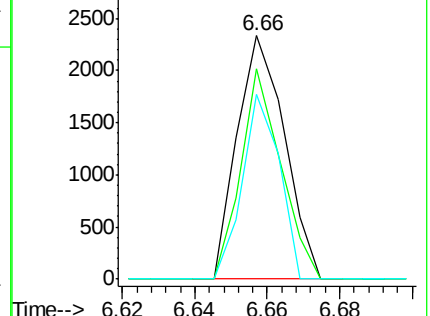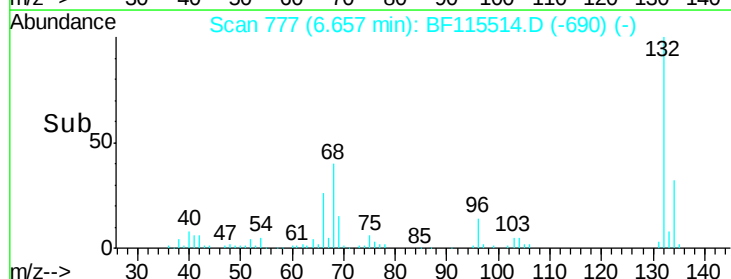

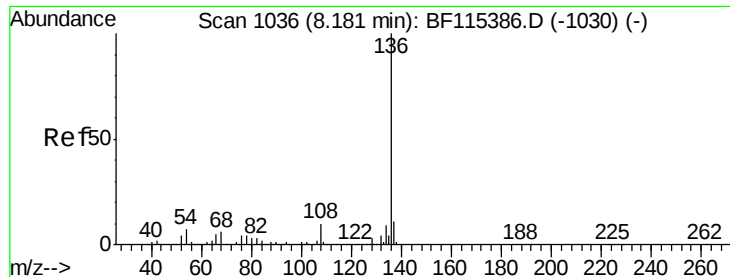

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.17 min Scan# 1035

Delta R.T. -0.01 min

Lab File: BF115514.D

Acq: 12 Jul 2019 00:14

Instrument :

BNA_F

ClientSampleId :

OK-03-071019-B

Tot Ion:136 Resp: 514491


Ion Ratio Lower Upper

136 100

137 11.1 8.8 13.2

54 6.9 5.4 8.0

68 6.5 4.8 7.2



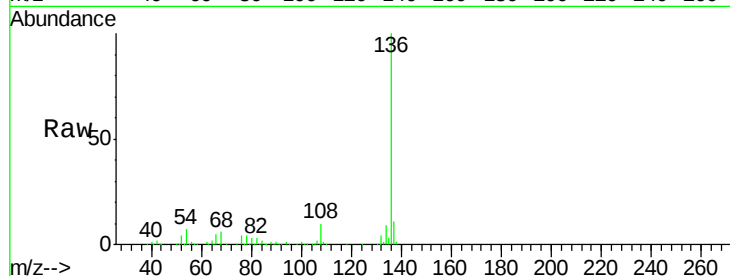


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF1

Ion 68.00 (67.70 to 68.70): BF1

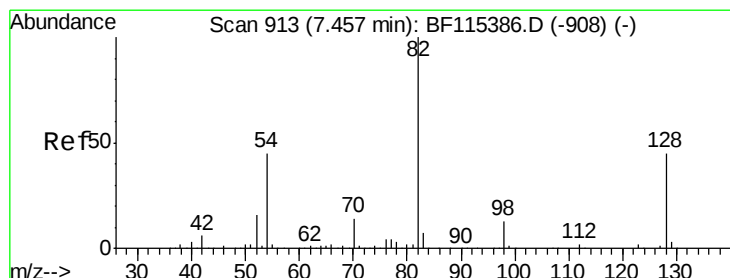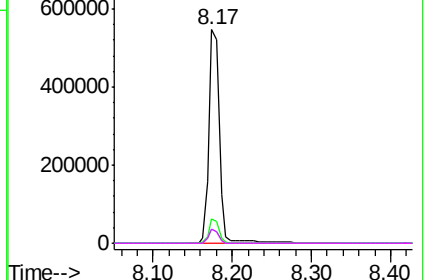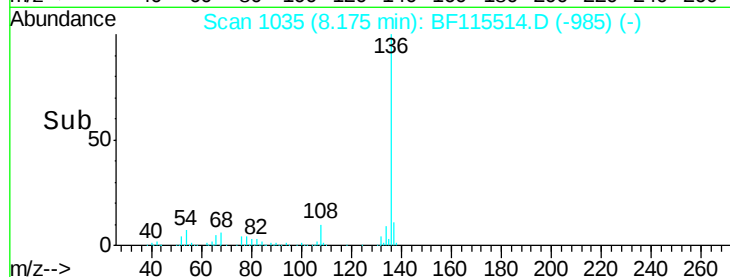

#23

Nitrobenzene-d5

Concen: 7.033 ng

RT: 7.45 min Scan# 911

Delta R.T. -0.01 min

Lab File: BF115514.D

Acq: 12 Jul 2019 00:14


Tgt Ion: 82 Resp: 61246

Ion Ratio Lower Upper

82 100

128 43.1 36.7 55.1



54 42.9 35.6 53.4

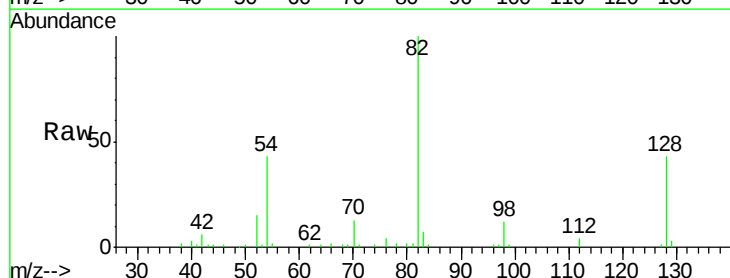


Abundance Ion 82.00 (81.70 to 82.70): BF1

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BF1

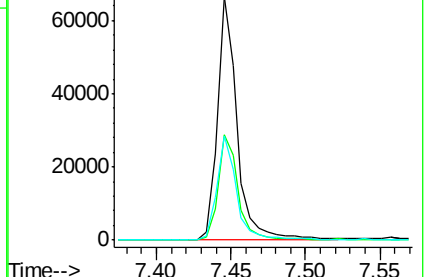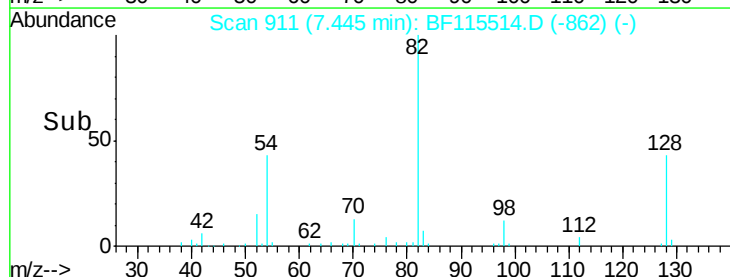

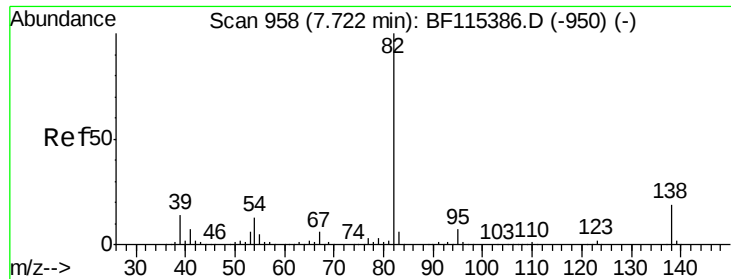

#25

Isophorone

Concen: 3.245 ng

RT: 7.45 min Scan# 911

Delta R.T. -0.28 min

Lab File: BF115514.D

Acq: 12 Jul 2019 00:14

Instrument :

BNA_F

ClientSampleId :

OK-03-071019-B


Tot Ion: 82 Resp: 61245

Ion Ratio Lower Upper

82 100

95 0.0 5.4 8.2#




138 0.0 15.1 22.7#

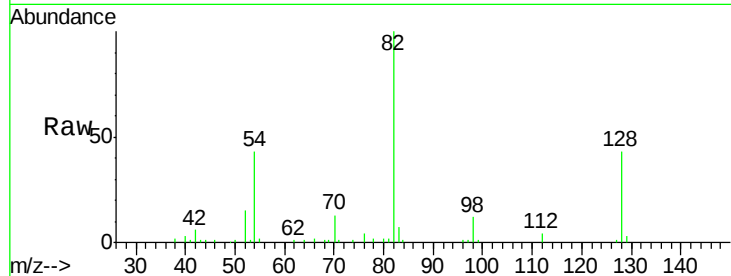

Abundance Ion 82.00 (81.70 to 82.70): BF1

Ion 95.00 (94.70 to 95.70): BF1

Ion 138.00 (137.70 to 138.70): BF1

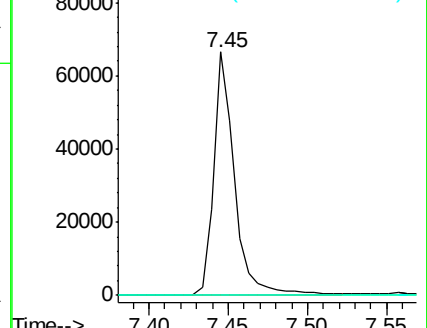

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.93 min Scan# 1334

Delta R.T. -0.01 min

Lab File: BF115514.D

Acq: 12 Jul 2019 00:14


Tgt Ion: 164 Resp: 235735

Ion Ratio Lower Upper

164 100

162 102.1 82.3 123.5



160 45.7 37.2 55.8




Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E




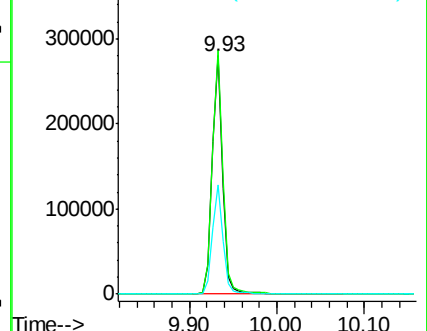




#42
 2,4,6-Tribromophenol
 Concen: 8.866 ng
 RT: 10.72 min Scan# 1467
 Delta R.T. -0.01 min
 Lab File: BF115514.D
 Acq: 12 Jul 2019 00:14




Instrument :
 BNA_F
 ClientSampleId :
 OK-03-071019-B


Tot Ion:330 Resp: 23110
 Ion Ratio Lower Upper
 330 100
 332 99.4 77.4 116.0
 141 31.9 24.7 37.1

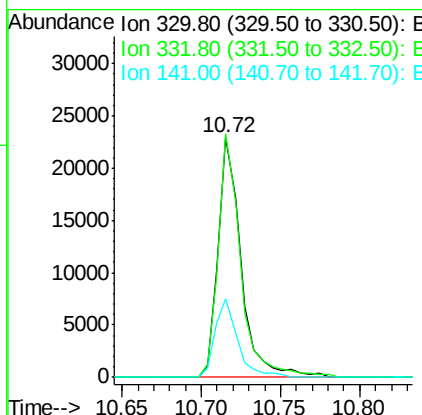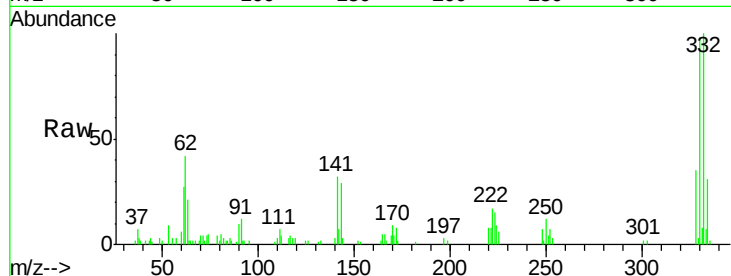

#45
 2-Fluorobiphenyl
 Concen: 10.489 ng
 RT: 9.25 min Scan# 1218
 Delta R.T. -0.01 min
 Lab File: BF115514.D
 Acq: 12 Jul 2019 00:14

Tgt Ion:172 Resp: 140911
 Ion Ratio Lower Upper
 172 100
 171 34.8 29.8 44.8
 170 23.2 20.0 30.0


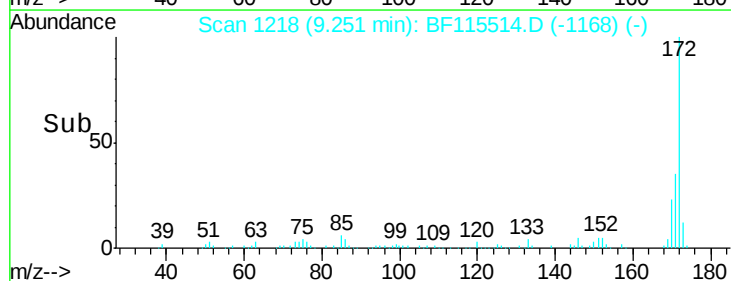
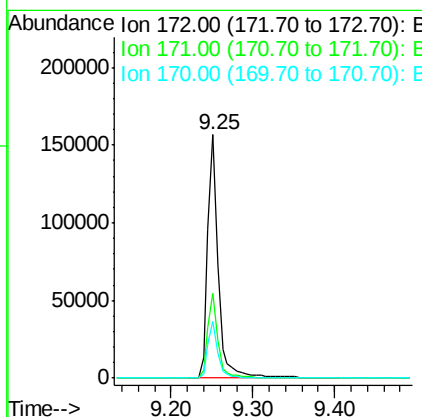



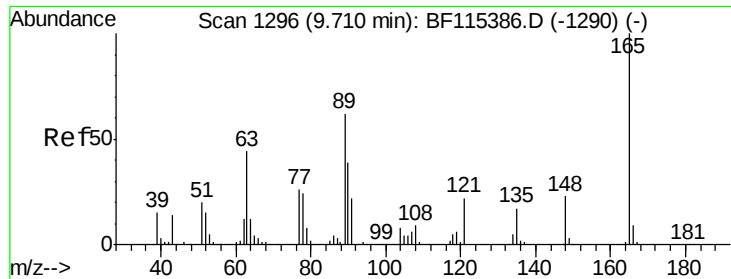

#51
 2,6-Dinitrotoluene
 Concen: 7.607 ng
 RT: 9.93 min Scan# 1334
 Delta R.T. 0.22 min
 Lab File: BF115514.D
 Acq: 12 Jul 2019 00:14




Instrument :
 BNA_F
 ClientSampleId :
 OK-03-071019-B


Tot Ion	Ratio	Lower	Upper
165	100		
63	1.4	39.7	59.5#
89	1.3	42.8	64.2#

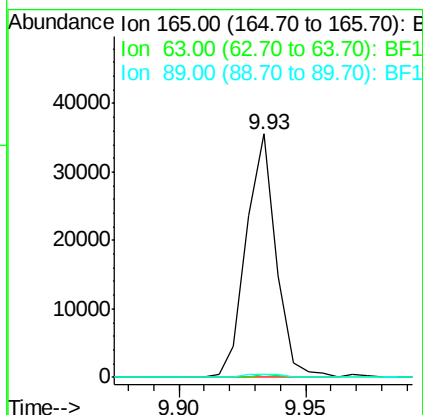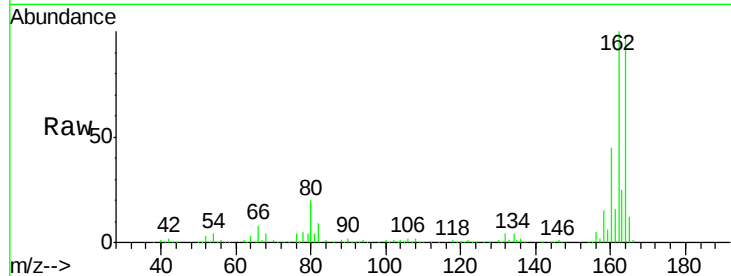

#57
 2,4-Dinitrotoluene
 Concen: 5.985 ng
 RT: 9.93 min Scan# 1334
 Delta R.T. -0.18 min
 Lab File: BF115514.D
 Acq: 12 Jul 2019 00:14

Tgt Ion	Ratio	Lower	Upper
165	100		
63	1.4	33.0	49.4#
89	1.3	58.5	87.7#
182	0.0	2.1	3.1#


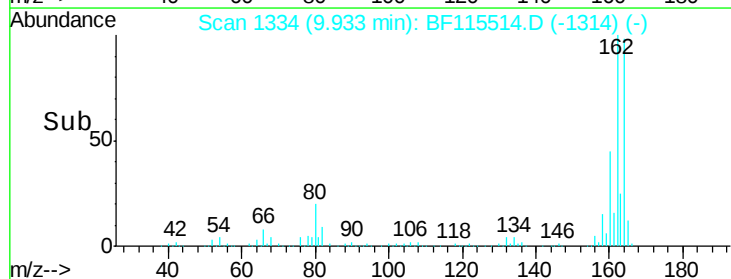
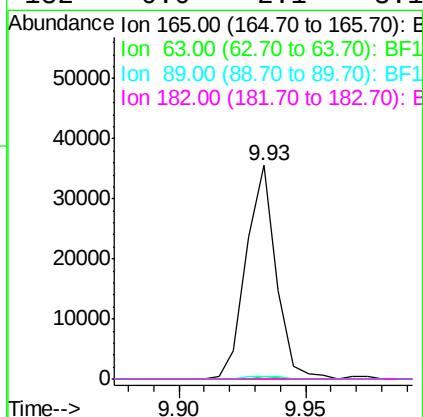



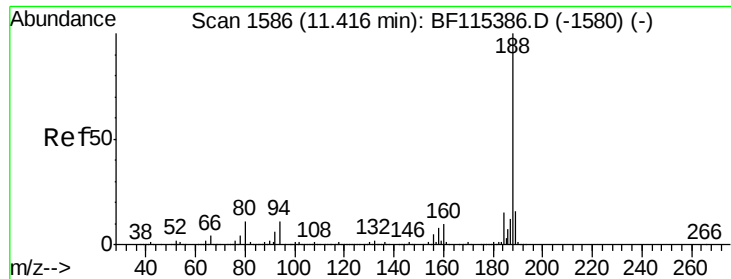

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.42 min Scan# 1586
Delta R.T. -0.01 min
Lab File: BF115514.D
Acq: 12 Jul 2019 00:14




Instrument :
BNA_F
ClientSampleId :
OK-03-071019-B


Tot Ion:188 Resp: 411088
Ion Ratio Lower Upper
188 100
94 9.9 7.8 11.8
80 10.3 8.4 12.6

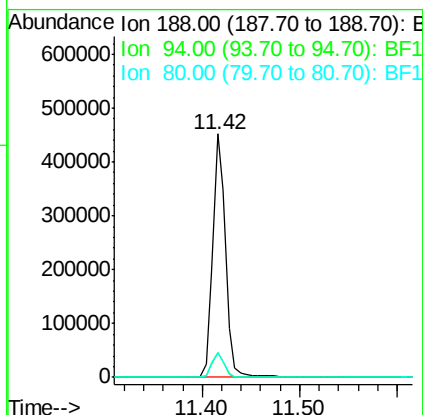

#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.06 min Scan# 2035
Delta R.T. -0.01 min
Lab File: BF115514.D
Acq: 12 Jul 2019 00:14

Tgt Ion:240 Resp: 343313
Ion Ratio Lower Upper
240 100
120 10.7 10.2 15.4
236 26.5 21.1 31.7

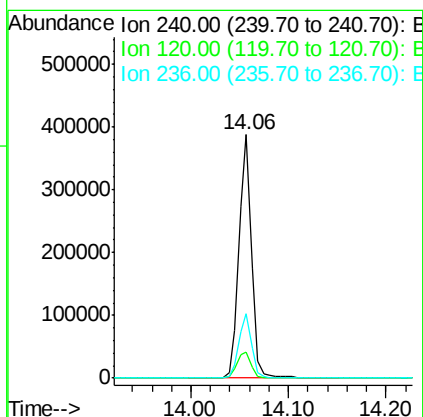

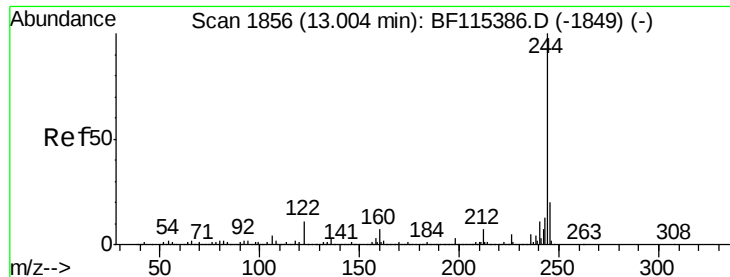

#79

Terphenyl-d14

Concen: 8.260 ng

RT: 13.00 min Scan# 1855

Delta R.T. -0.01 min

Lab File: BF115514.D

Acq: 12 Jul 2019 00:14

Instrument :

BNA_F

ClientSampleId :

OK-03-071019-B


Tot Ion:244 Resp: 138496

Ion Ratio Lower Upper

244 100

212 6.5 5.7 8.5




122 11.0 9.1 13.7

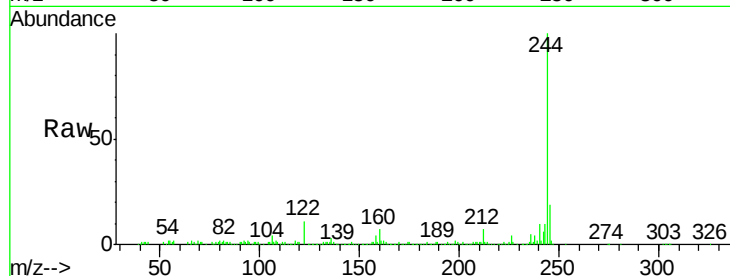

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

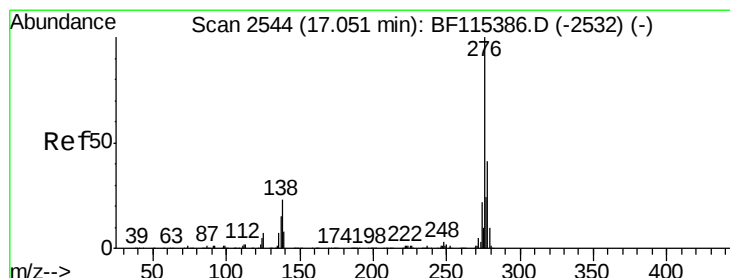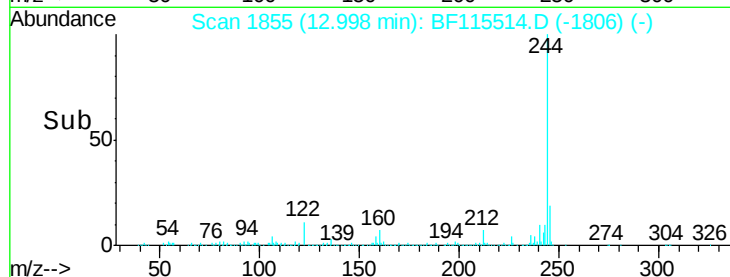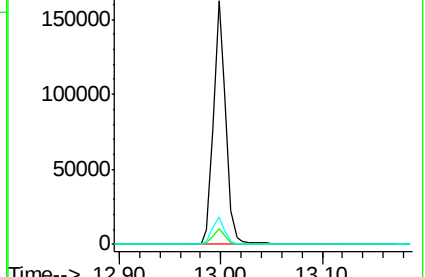

#86

Indeno(1,2,3-cd)pyrene

Concen: Below Cal

RT: 17.06 min Scan# 2546

Delta R.T. 0.01 min

Lab File: BF115514.D

Acq: 12 Jul 2019 00:14


Tgt Ion:276 Resp: 261

Ion Ratio Lower Upper

276 100

138 0.0 20.6 31.0#



277 0.0 20.2 30.2#



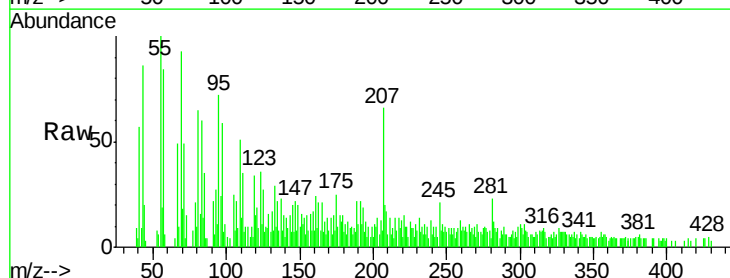


Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

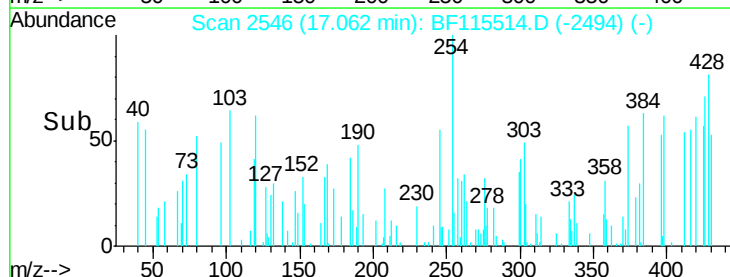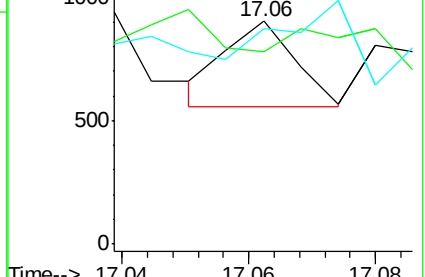

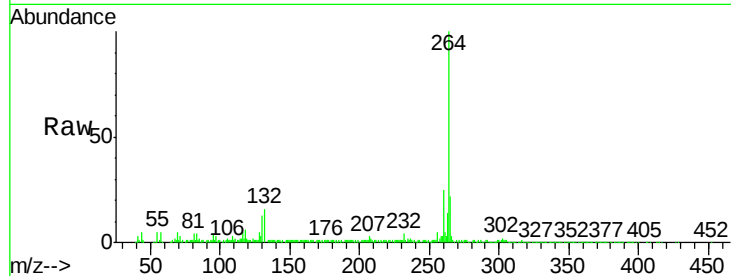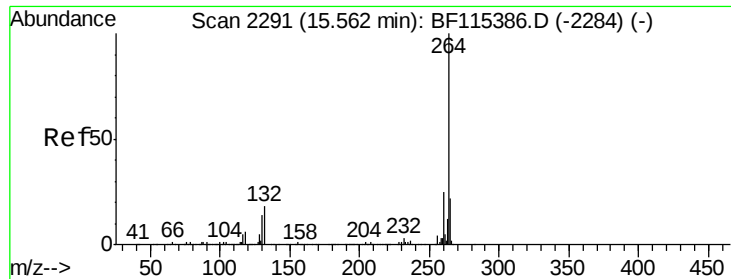

#87
Pervlene-d12
Concen: 20.000 ng
RT: 15.54 min Scan# 2287
Delta R.T. -0.02 min
Lab File: BF115514.D
Acq: 12 Jul 2019 00:14

Instrument :
BNA_F
ClientSampleId :
OK-03-071019-B

Tot Ion:	264	Resp:	295522
Ion	Ratio	Lower	Upper
264	100		
260	24.8	20.1	30.1
265	21.7	17.8	26.6

