
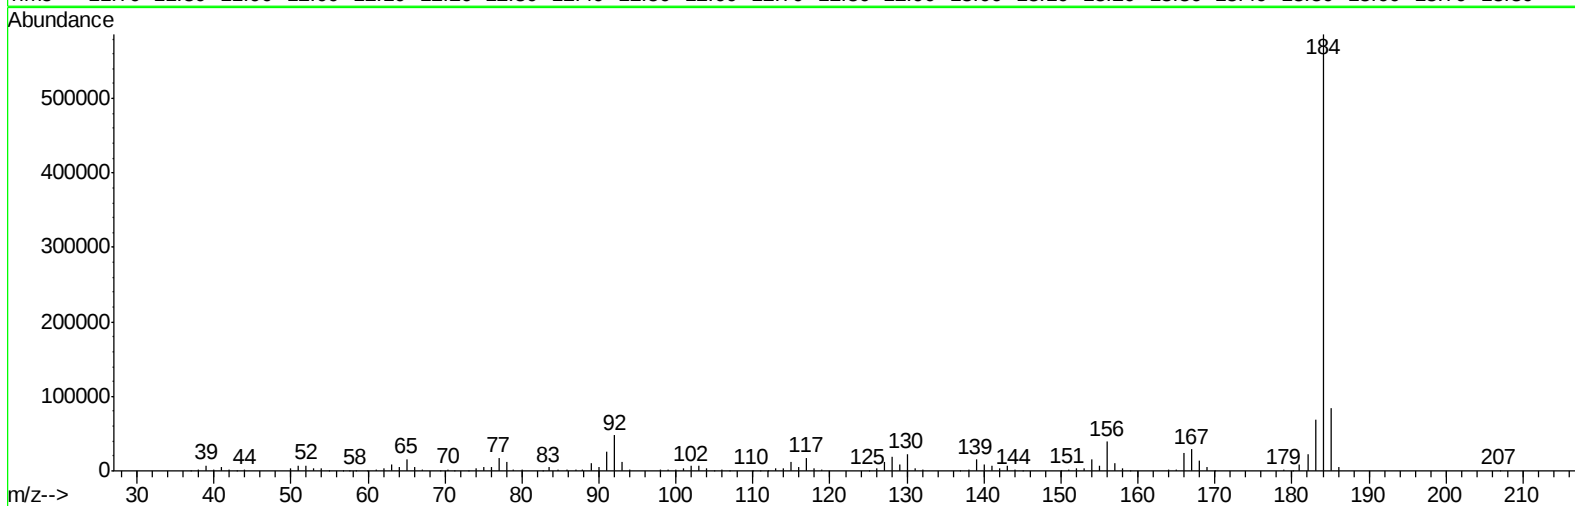


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF071119\
Data File : BF115492.D
Acq On : 11 Jul 2019 9:49
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 12 03:09:35 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF070519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 10 16:47:05 2019
Response via : Initial Calibration

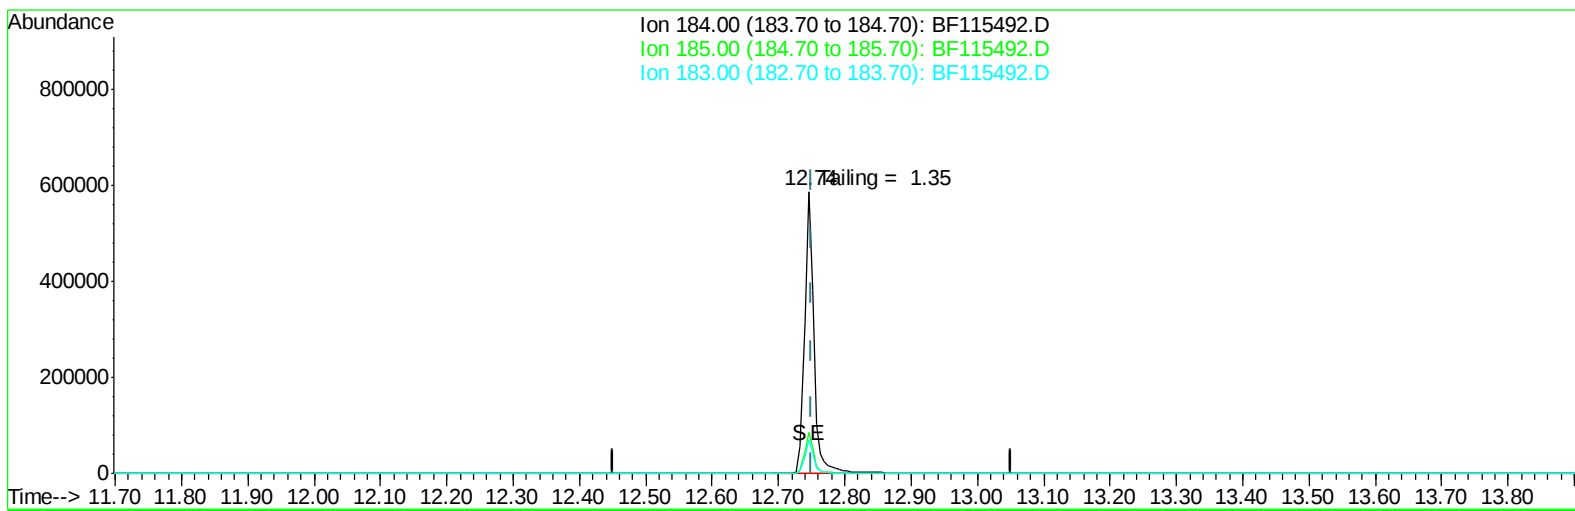

TIC: BF115492.D

(77) Benzidine



12.745min (-0.006) 0.00ng

response 561039

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	14.52
183.00	12.10	11.68
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF071119\
Data File : BF115492.D
Acq On : 11 Jul 2019 9:49
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 12 03:09:35 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF070519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 10 16:47:05 2019
Response via : Initial Calibration

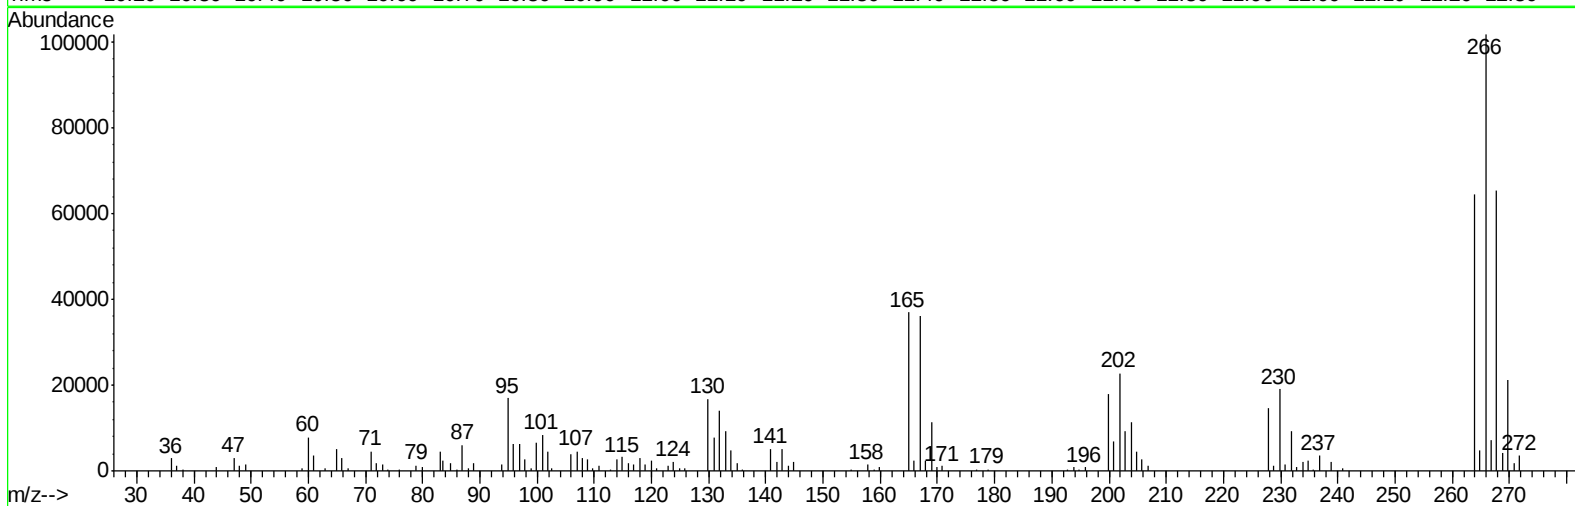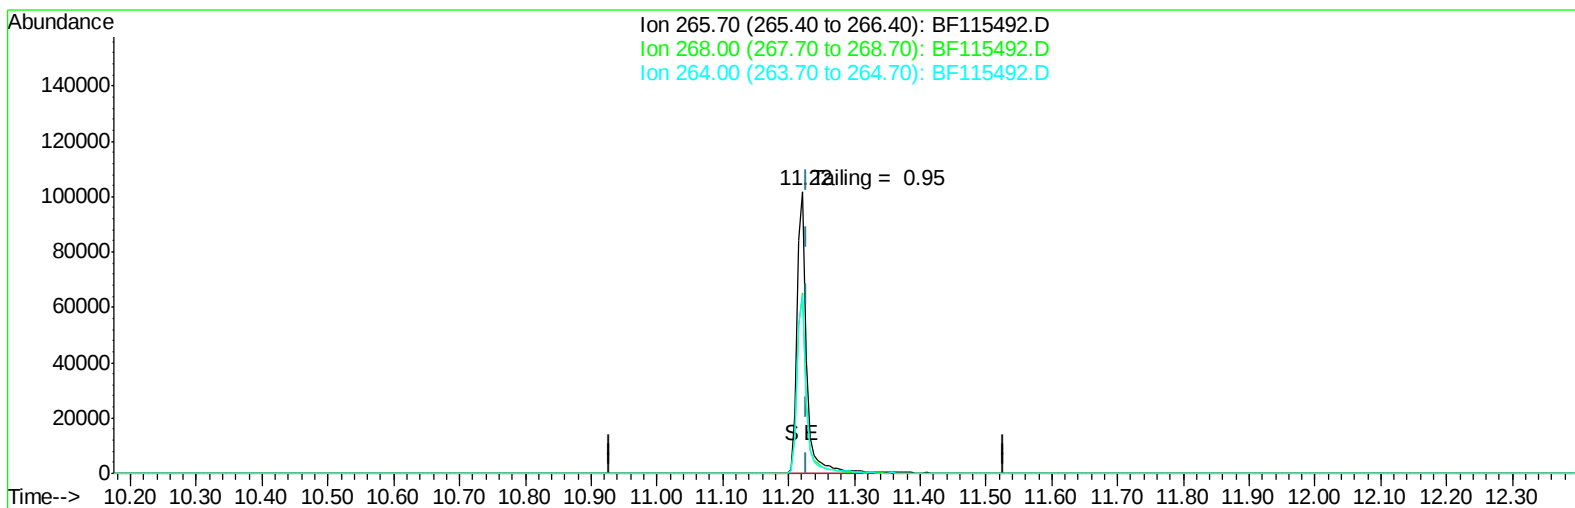

TIC: BF115492.D

(70) Pentachlorophenol (C)

11.222min (-0.006) 32715.44ng

response 105185

Ion	Exp%	Act%
265.70	100	100
268.00	64.00	64.14
264.00	63.20	63.36
0.00	0.00	0.00