


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF071119\
 Data File : BF115492.D
 Acq On : 11 Jul 2019 9:49
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF070519.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jul 10 16:47:05 2019

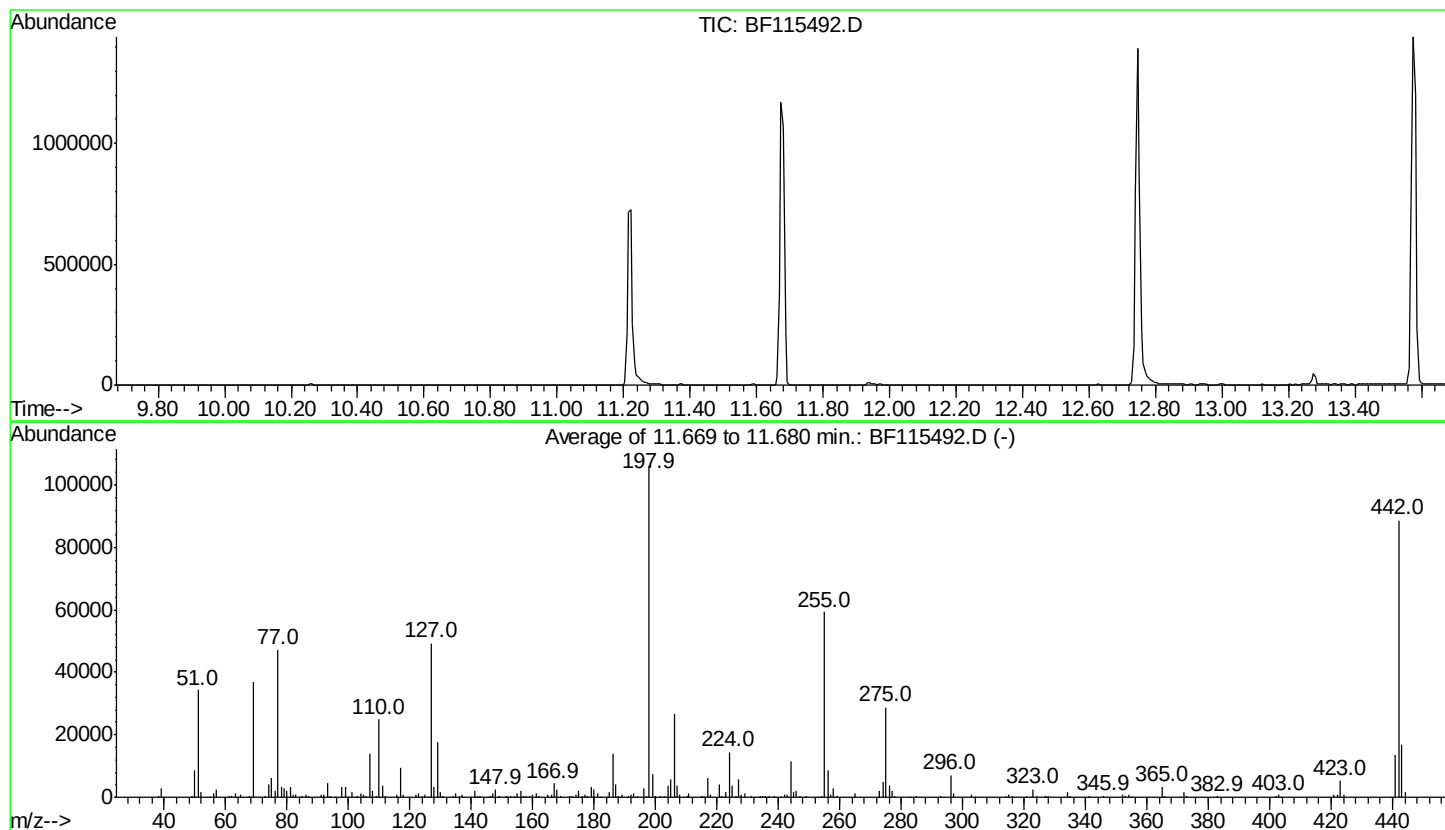

AutoFind: Scans 1629, 1630, 1631; Background Corrected with Scan 1624

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.4	34370	PASS
68	69	0.00	2	1.6	574	PASS
69	198	0.00	100	34.7	36808	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	46.4	49216	PASS
197	198	0.00	2	0.5	568	PASS
198	198	100	100	100.0	106157	PASS
199	198	5	9	6.8	7214	PASS
275	198	10	60	27.0	28704	PASS
365	198	1	100	3.2	3344	PASS
441	198	0.01	100	12.6	13397	PASS
442	198	50	100	83.5	88634	PASS
443	442	15	24	18.8	16681	PASS