


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF071119\
Data File : BF115501.D
Acq On : 11 Jul 2019 18:24
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF070519.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Jul 10 16:47:05 2019

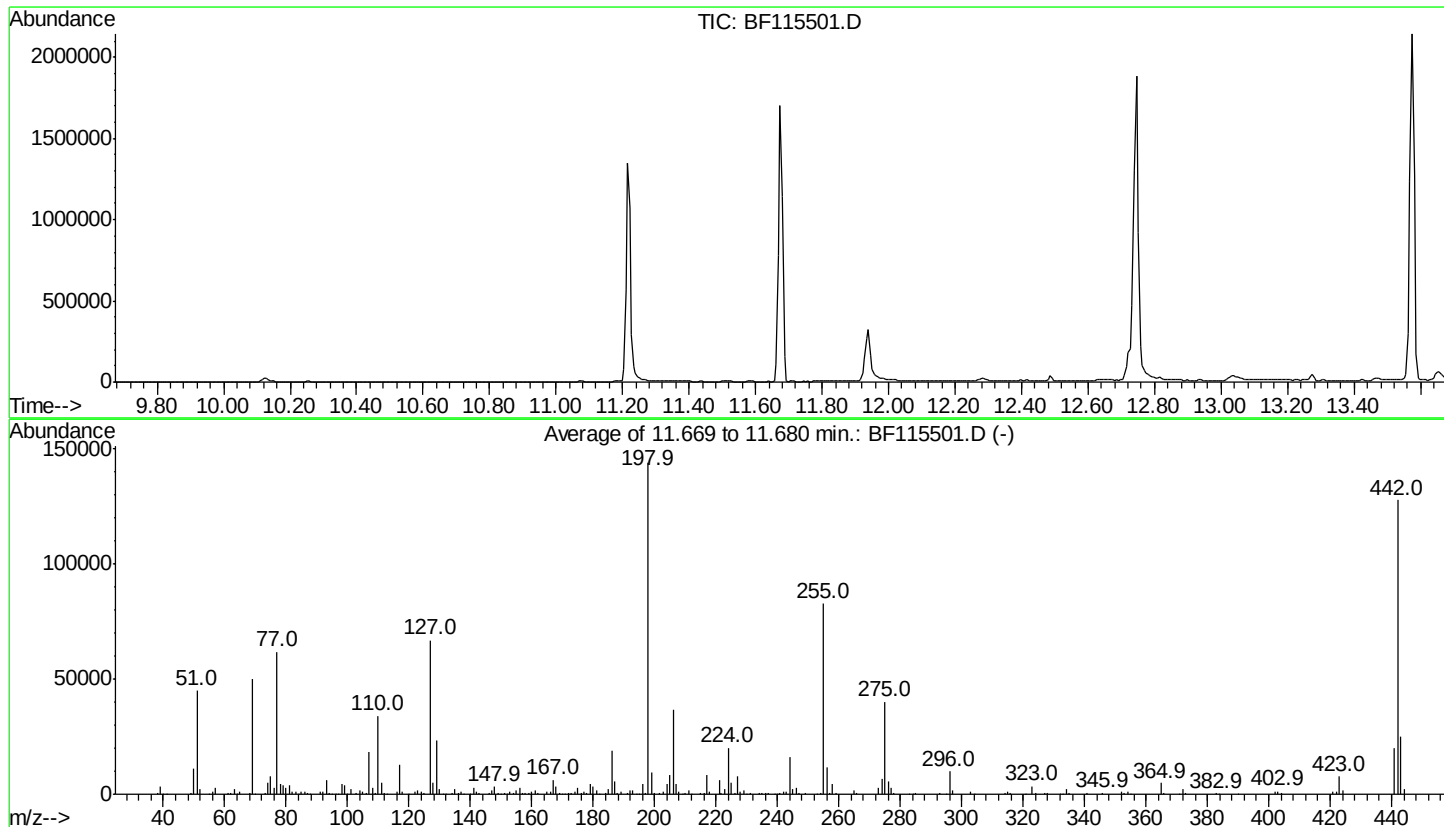

AutoFind: Scans 1629, 1630, 1631; Background Corrected with Scan 1624

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.2	44906	PASS
68	69	0.00	2	1.7	824	PASS
69	198	0.00	100	34.7	49888	PASS
70	69	0.00	2	0.6	291	PASS
127	198	10	80	46.3	66696	PASS
197	198	0.00	2	0.6	841	PASS
198	198	100	100	100.0	143914	PASS
199	198	5	9	6.7	9694	PASS
275	198	10	60	27.9	40101	PASS
365	198	1	100	3.3	4747	PASS
441	198	0.01	100	13.8	19877	PASS
442	198	50	100	88.6	127573	PASS
443	442	15	24	19.5	24879	PASS