
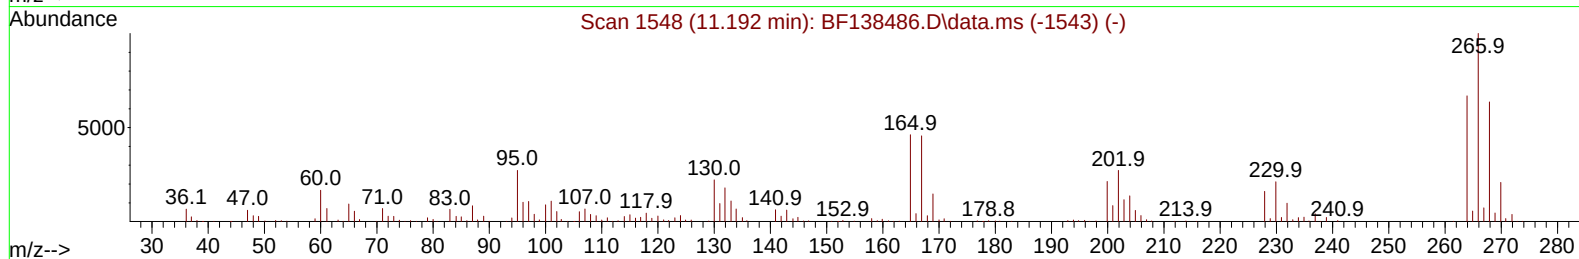
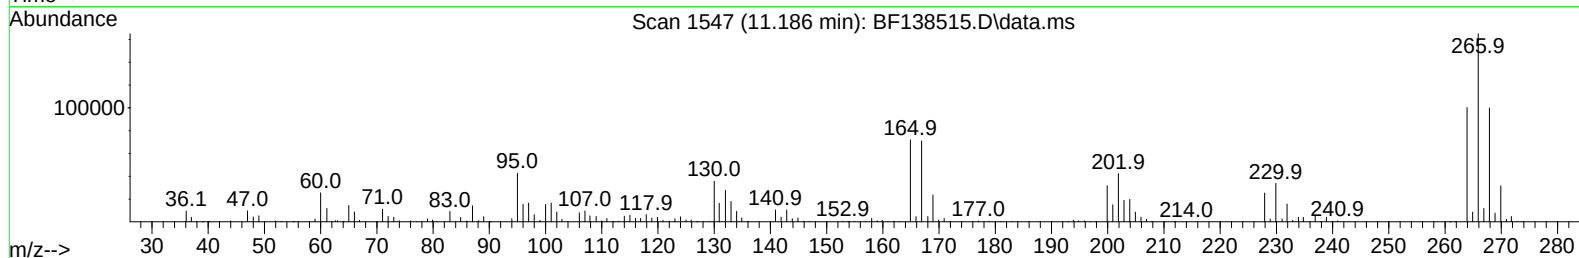


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071124\
Data File : BF138515.D
Acq On : 11 Jul 2024 10:54
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 11 12:23:54 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF070924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 09 16:58:40 2024
Response via : Initial Calibration

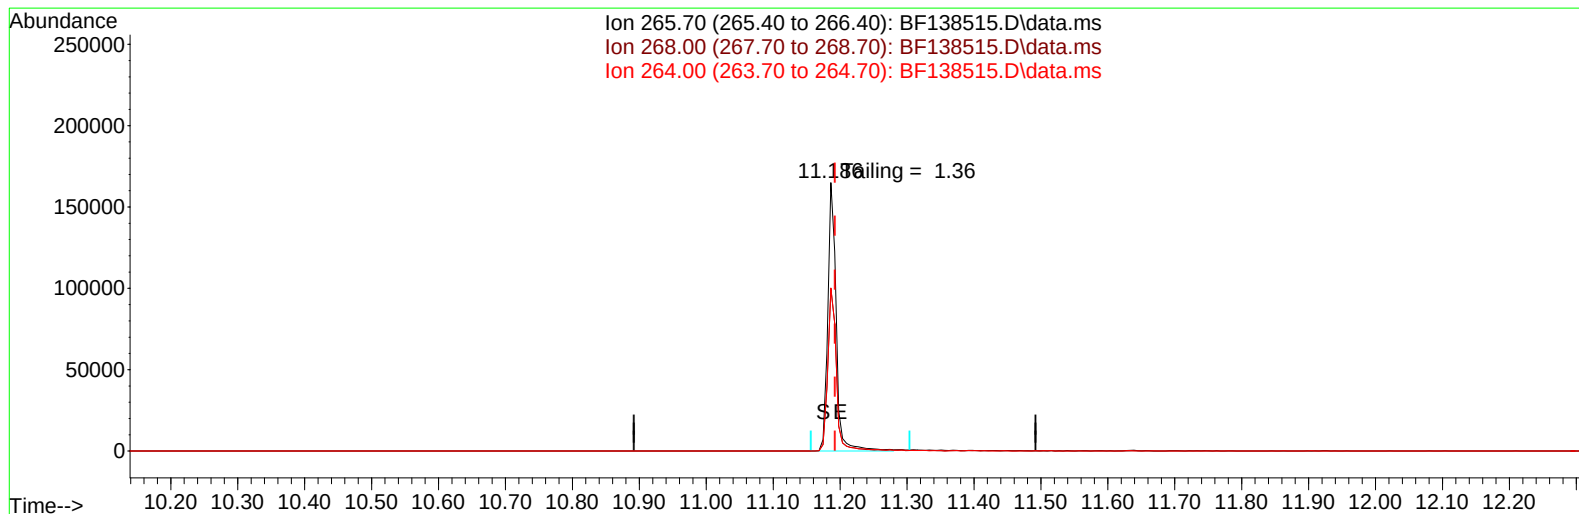

TIC: BF138515.D\data.ms

(70) Pentachlorophenol (C)




11.186min (-0.006) 25923.40 ng

response 146251

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	60.54
264.00	66.90	60.78
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071124\
Data File : BF138515.D
Acq On : 11 Jul 2024 10:54
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 11 12:23:54 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF070924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 09 16:58:40 2024
Response via : Initial Calibration

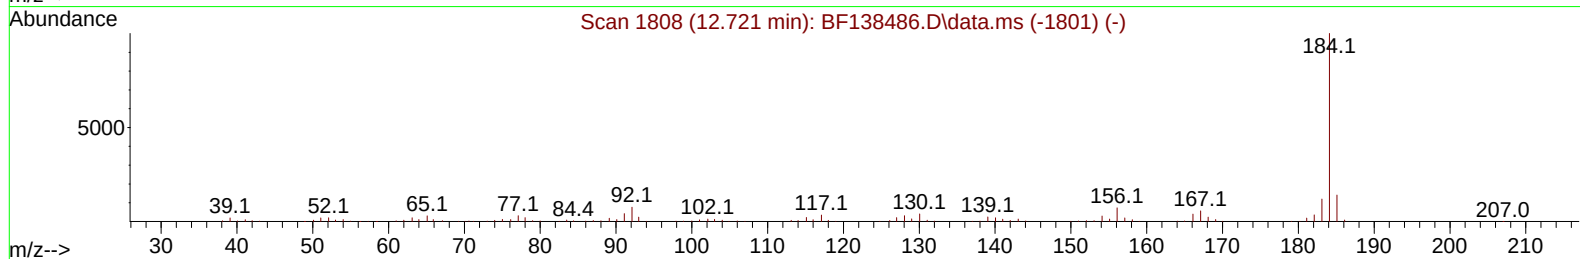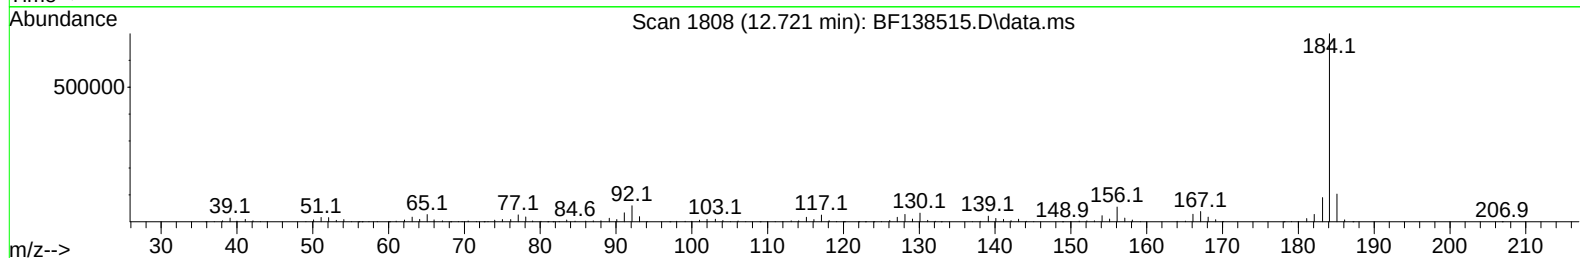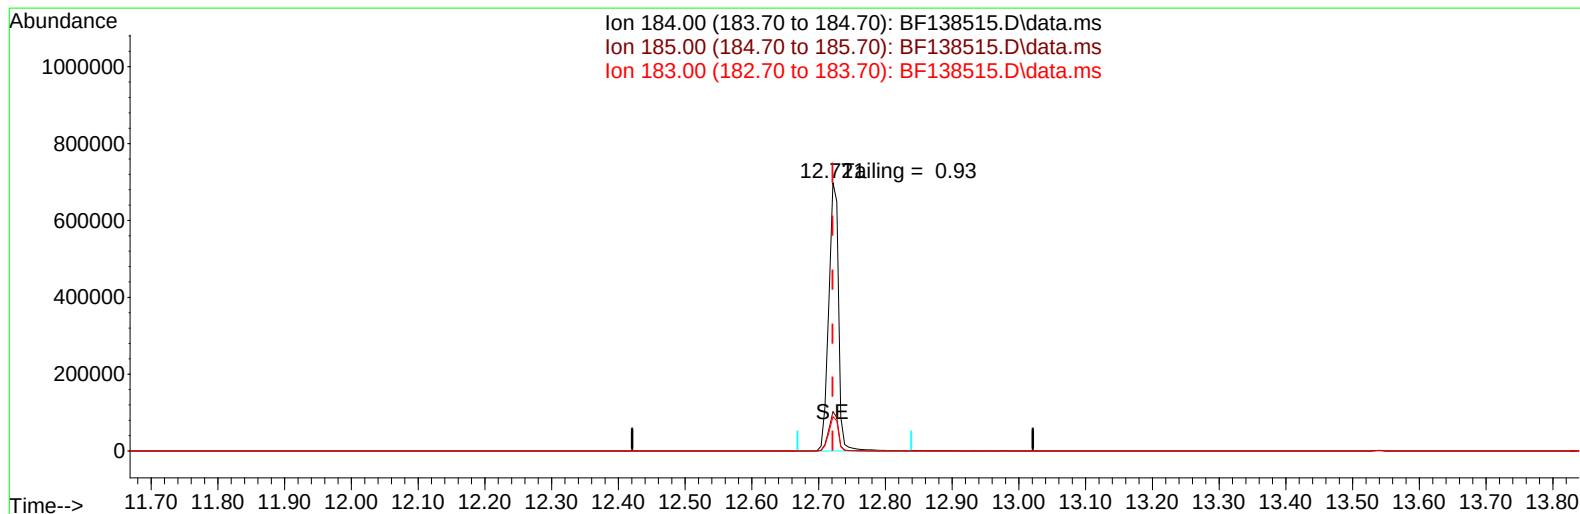

TIC: BF138515.D\data.ms

(77) Benzidine

12.721min (+ 0.000) 0.00 ng

response 714499

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.73
183.00	11.90	12.85
0.00	0.00	0.00