
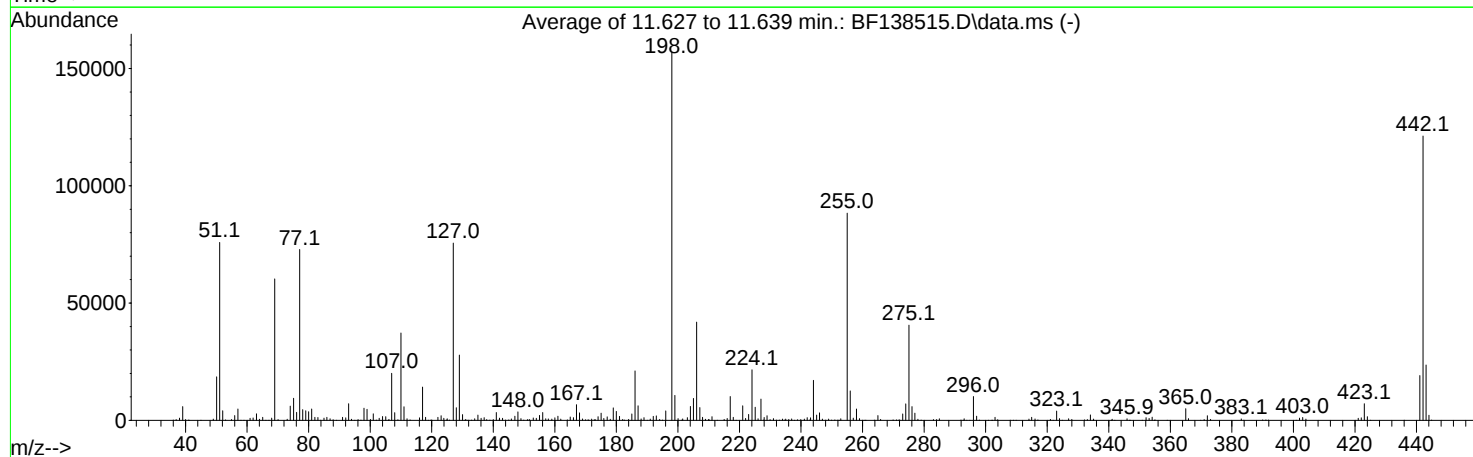


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071124\
Data File : BF138515.D
Acq On : 11 Jul 2024 10:54
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF070924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jul 09 16:58:40 2024

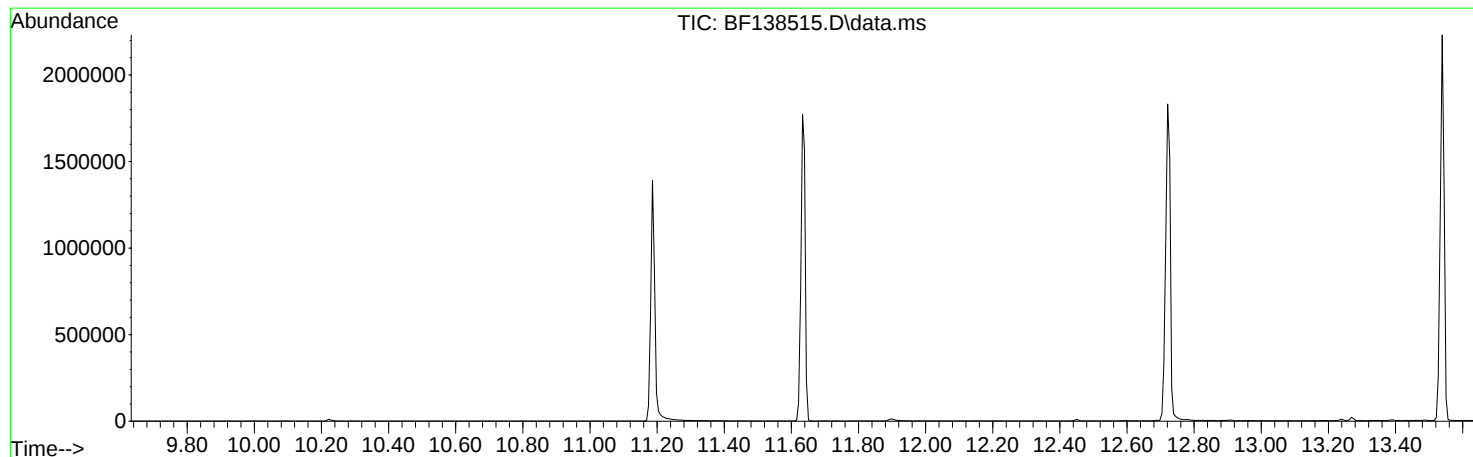




AutoFind: Scans 1622, 1623, 1624; Background Corrected with Scan 1617

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	48.4	75856	PASS
68	69	0.00	2	1.6	985	PASS
69	198	0.00	100	38.5	60323	PASS
70	69	0.00	2	0.6	348	PASS
127	198	10	80	48.2	75587	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	156829	PASS
199	198	5	9	6.8	10677	PASS
275	198	10	60	25.9	40568	PASS
365	198	1	100	3.2	4990	PASS
441	198	0.01	100	12.2	19097	PASS
442	442	50	100	100.0	121235	PASS
443	442	15	24	19.5	23607	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071124\
Data File : BF138515.D
Acq On : 11 Jul 2024 10:54
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 11 12:23:54 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF070924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 09 16:58:40 2024
Response via : Initial Calibration

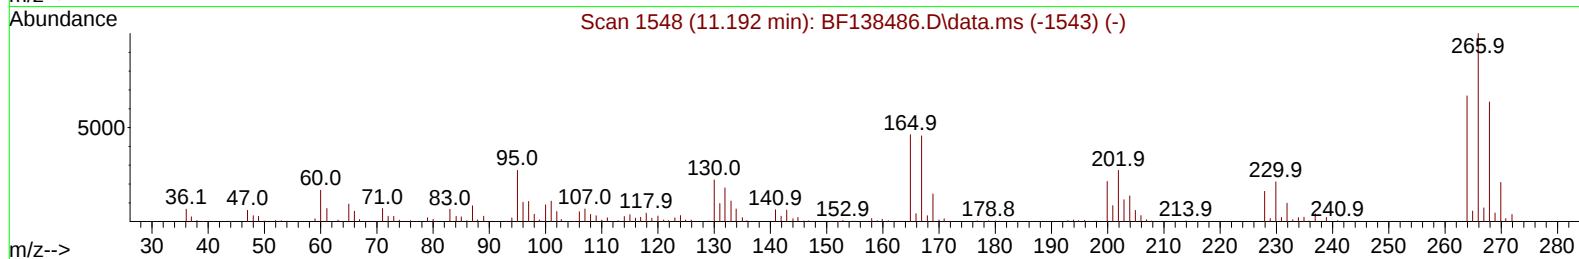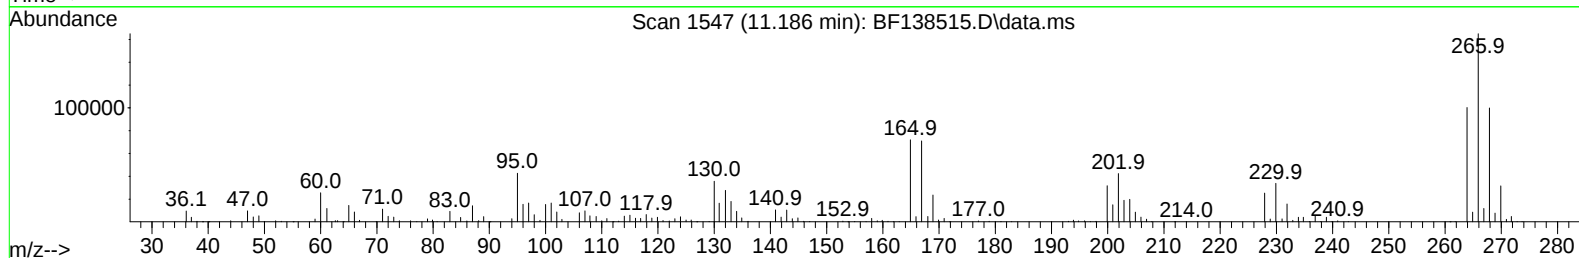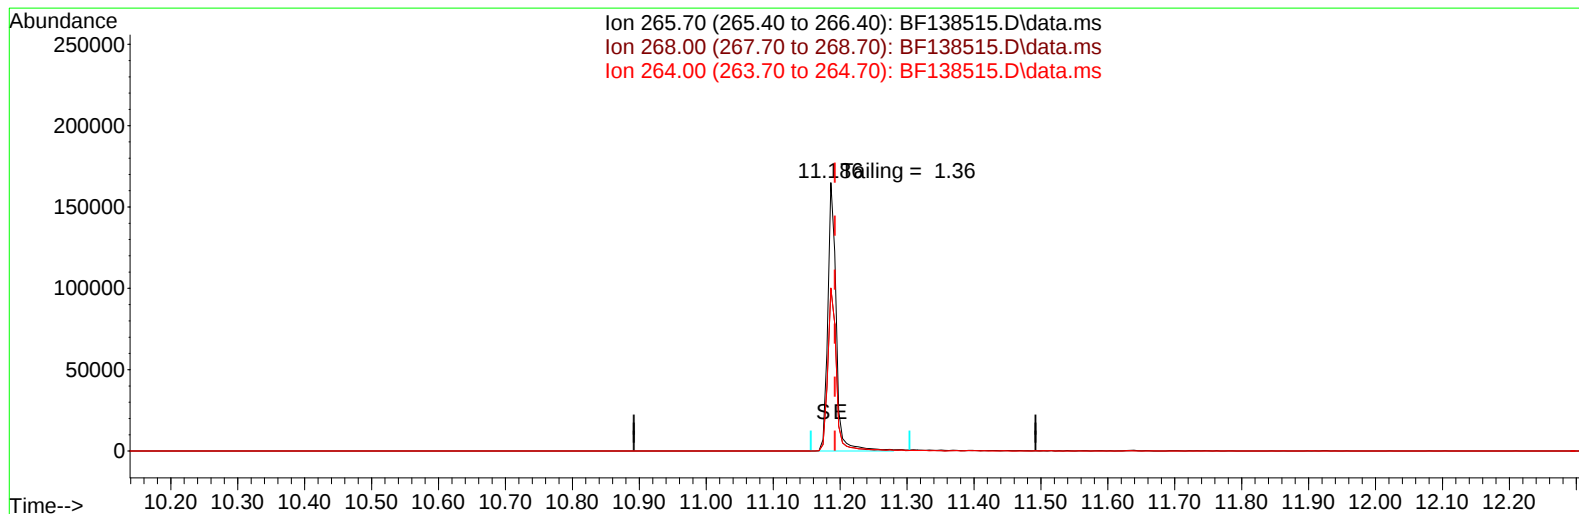

TIC: BF138515.D\data.ms

(70) Pentachlorophenol (C)

11.186min (-0.006) 25923.40 ng




response 146251

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	60.54
264.00	66.90	60.78
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071124\
Data File : BF138515.D
Acq On : 11 Jul 2024 10:54
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 11 12:23:54 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF070924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 09 16:58:40 2024
Response via : Initial Calibration

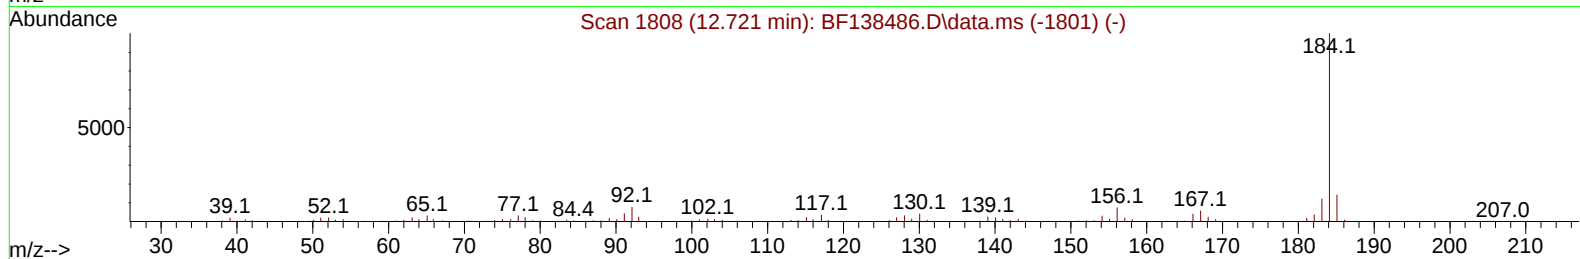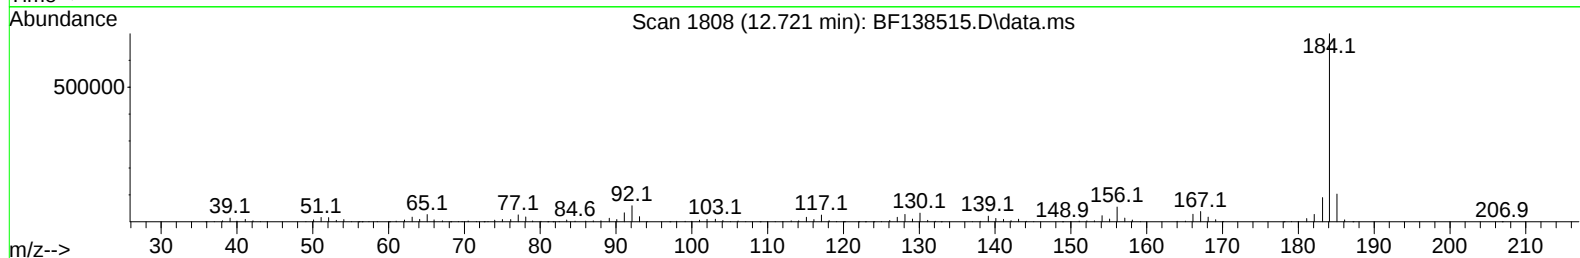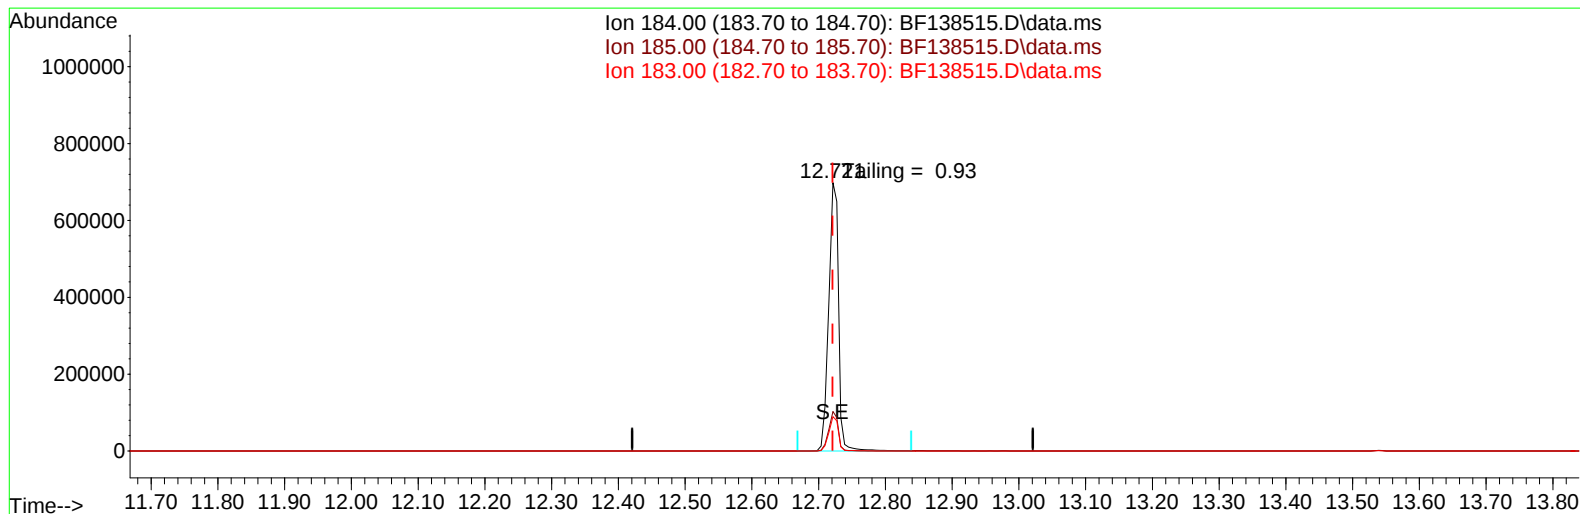

TIC: BF138515.D\data.ms

(77) Benzidine

12.721min (+ 0.000) 0.00 ng

response 714499

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.73
183.00	11.90	12.85
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/11/2024	BNA_F	<u>BF138515.D</u>
Compound Name	Response	Retention Time
DDT	348875	13.539
DDD	5465	13.268
DDE	493	12.904
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5958	354833	1.68

Instrument :
BNA_F
ClientSampleId :
DFTPP