

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF071218\
 Data File : BF107343.D
 Acq On : 12 Jul 2018 17:08
 Operator : JU/SJ
 Sample : J3824-01 5X
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 HD-02-071018

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.148	475	478	484	rBV	29458	32841	6.78%	0.674%
2	5.566	546	549	565	rBV	223155	265678	54.82%	5.457%
3	6.572	717	720	739	rBV	210239	276293	57.01%	5.675%
4	6.707	739	743	752	rVB	300658	286853	59.19%	5.891%
5	6.925	777	780	789	rBV	369670	338403	69.82%	6.950%
6	7.084	803	807	818	rBB	251652	227581	46.96%	4.674%
7	7.495	874	877	891	rBV	156982	168652	34.80%	3.464%
8	8.213	995	999	1016	rBV	465943	447247	92.28%	9.186%
9	9.289	1178	1182	1191	rBV	322627	336288	69.39%	6.907%
10	9.683	1244	1249	1255	rBV	34073	37524	7.74%	0.771%
11	9.930	1286	1291	1295	rBV2	2907	5859	1.21%	0.120%
12	9.977	1295	1299	1311	rVB	501034	479154	98.87%	9.841%
13	10.383	1363	1368	1371	rVB2	5052	5280	1.09%	0.108%
14	10.777	1431	1435	1442	rBV	144243	150090	30.97%	3.083%
15	10.866	1446	1450	1453	rVV2	6341	8983	1.85%	0.184%
16	10.895	1453	1455	1461	rVB3	5417	6003	1.24%	0.123%
17	11.471	1550	1553	1560	rBV	459949	441850	91.17%	9.075%
18	12.477	1721	1724	1726	rBV2	4591	4944	1.02%	0.102%
19	12.524	1726	1732	1737	rVB5	5946	10846	2.24%	0.223%
20	12.930	1799	1801	1804	rBV	7318	5602	1.16%	0.115%
21	13.054	1819	1822	1826	rBV	366645	302530	62.42%	6.213%
22	13.260	1854	1857	1859	rVB	8115	5655	1.17%	0.116%
23	13.489	1893	1896	1899	rBV4	3971	5944	1.23%	0.122%
24	13.601	1911	1915	1918	rBV2	10031	11644	2.40%	0.239%
25	13.771	1941	1944	1947	rBV5	4333	6838	1.41%	0.140%
26	13.942	1969	1973	1978	rBV3	25708	45884	9.47%	0.942%
27	14.042	1988	1990	1993	rBV4	5248	6827	1.41%	0.140%
28	14.130	2001	2005	2010	rBV	475401	484648	100.00%	9.954%
29	14.248	2023	2025	2031	rBV4	9612	12616	2.60%	0.259%
30	14.560	2075	2078	2080	rBV2	25348	27402	5.65%	0.563%
31	15.671	2263	2267	2277	rVB	304606	423018	87.28%	8.688%


Sum of corrected areas: 4868977

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF071218\
Data File : BF107343.D
Acq On : 12 Jul 2018 17:08
Operator : JU/SJ
Sample : J3824-01 5X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
HD-02-071018

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

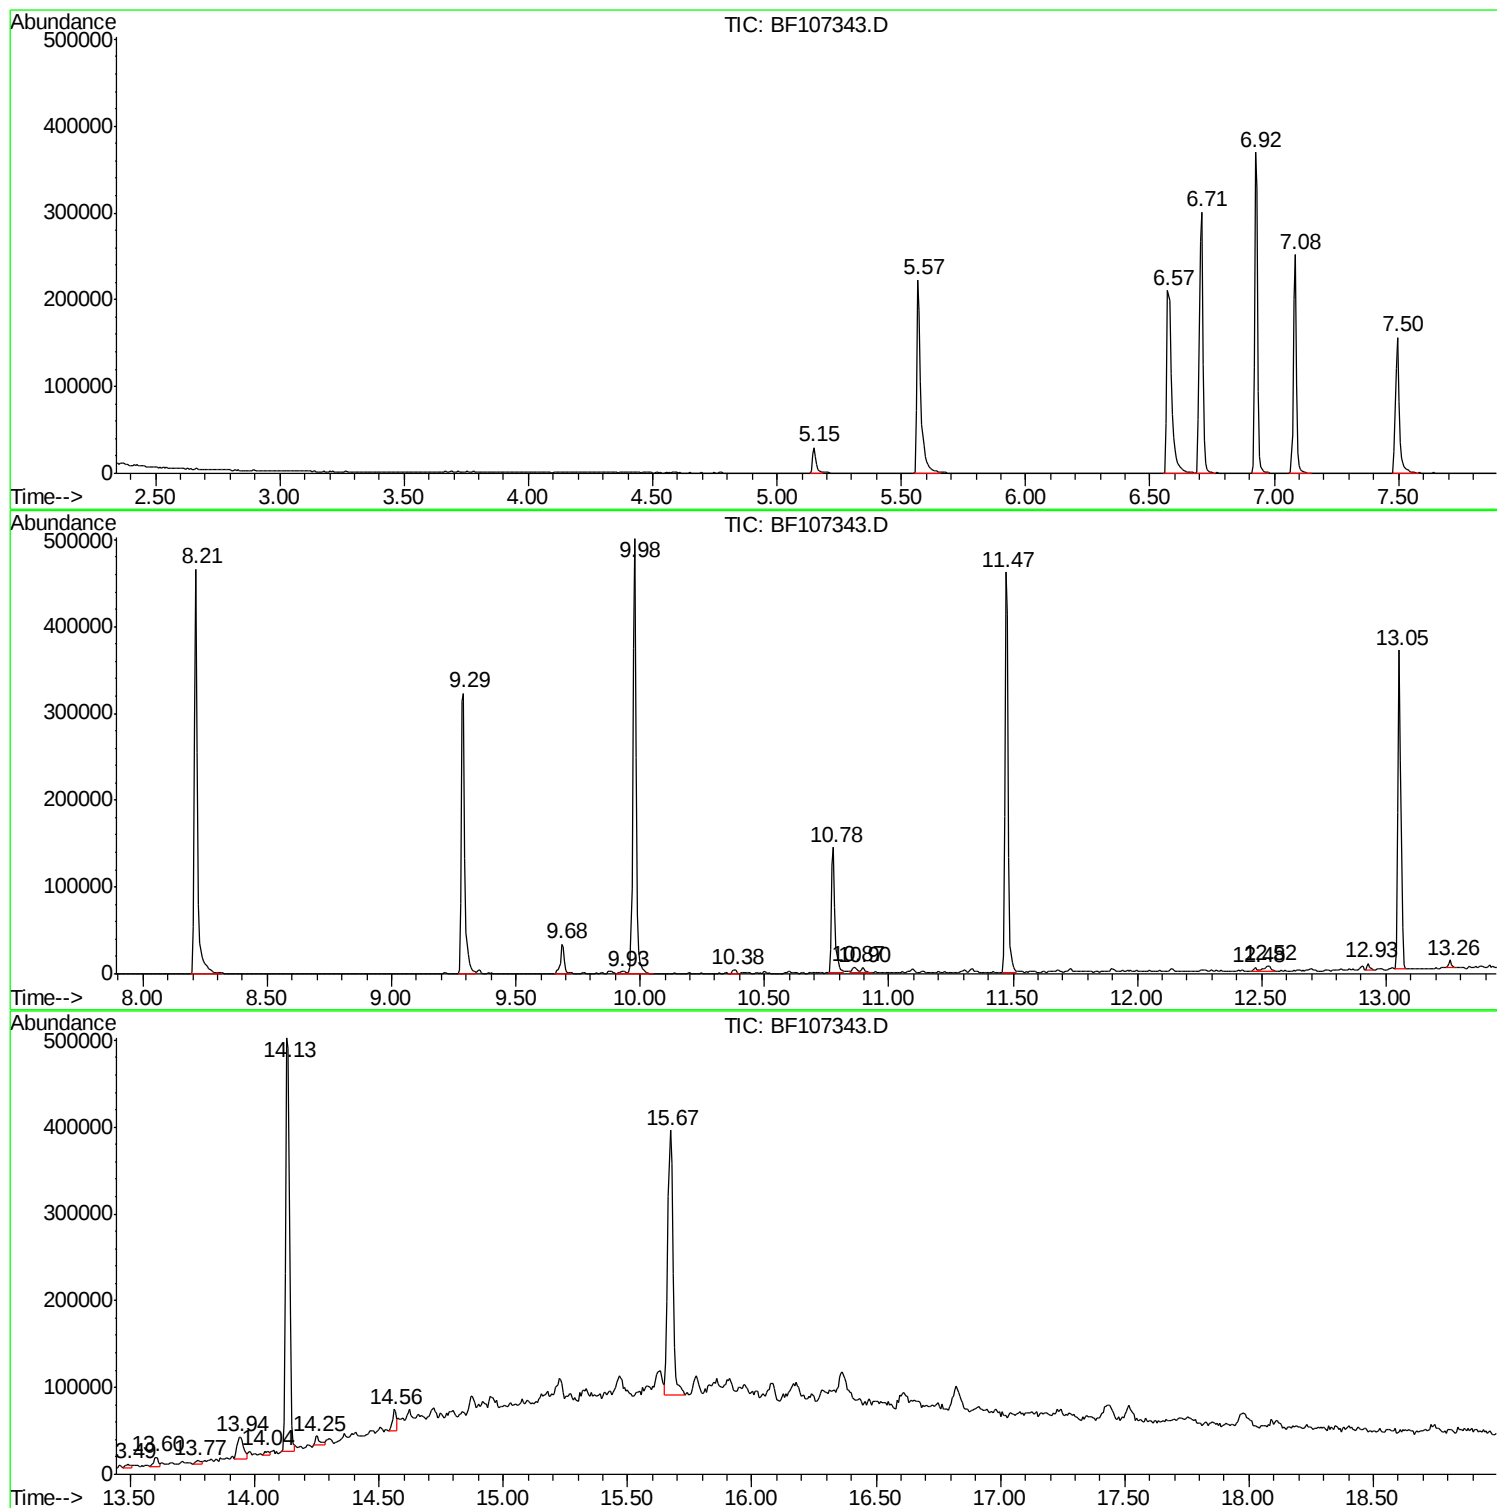

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF071218\
Data File : BF107343.D
Acq On : 12 Jul 2018 17:08
Operator : JU/SJ
Sample : J3824-01 5X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
HD-02-071018










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.71	16.95 ng	286853	1,4-Dichlorobenzene-d4	6.92

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	25
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	17
3		Tranvlcypropine-propionyl	189	C12H15NO	1000123-86-3	12
4		5-Aminoindole	132	C8H8N2	005192-03-0	12
5		1-Methylpyrrolo[1,2-a]pyrazine	132	C8H8N2	064608-59-9	9

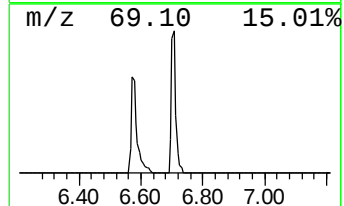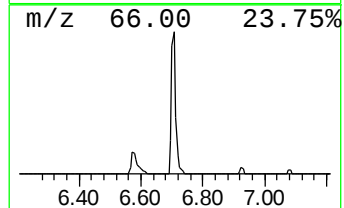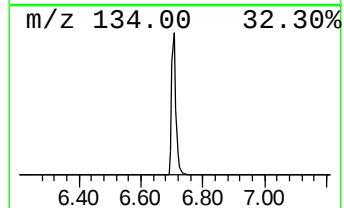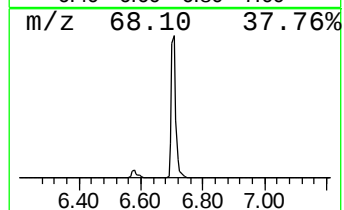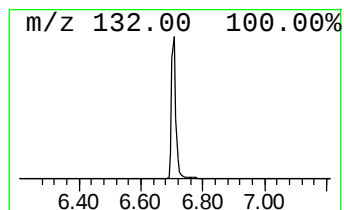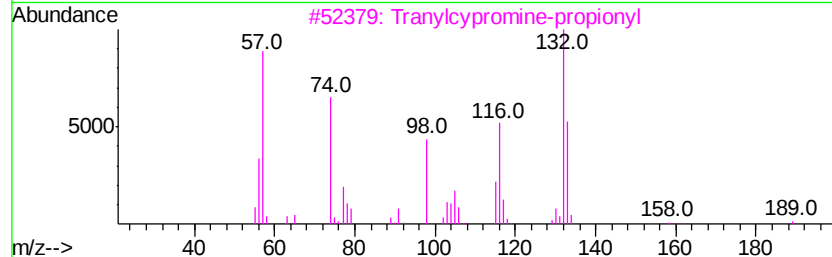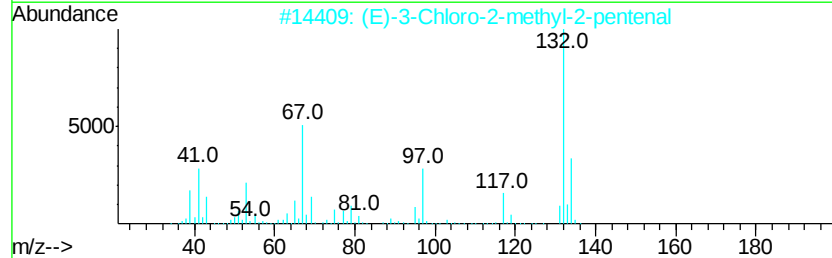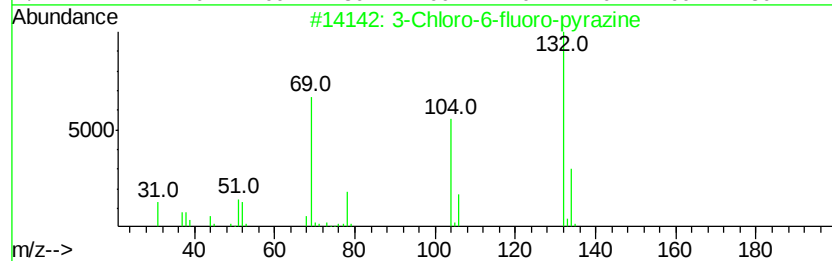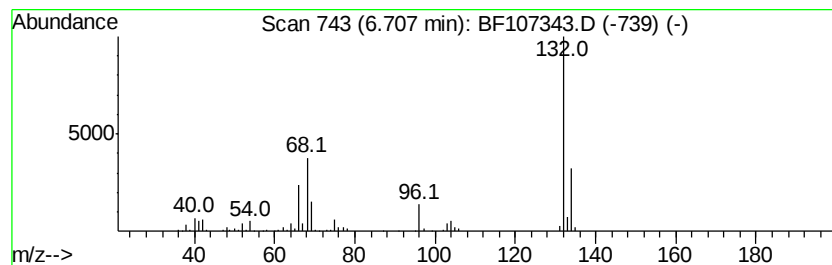

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF071218\
Data File : BF107343.D
Acq On : 12 Jul 2018 17:08
Operator : JU/SJ
Sample : J3824-01 5X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
HD-02-071018

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown	6.71	16.9	ng	286853	1	6.92	338403	20.0