

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF071218\
 Data File : BF107344.D
 Acq On : 12 Jul 2018 17:35
 Operator : JU/SJ
 Sample : J3914-01DL 100X
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 B1DL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.719	743	745	751	rBB	5735	6489	1.32%	0.208%
2	6.925	777	780	795	rBV	334226	344111	69.89%	11.045%
3	7.084	804	807	812	rBV	8932	8899	1.81%	0.286%
4	8.213	995	999	1027	rBV	492821	469269	95.31%	15.063%
5	9.295	1180	1183	1189	rBB2	6099	8019	1.63%	0.257%
6	9.978	1295	1299	1312	rBV	475863	492358	100.00%	15.804%
7	11.083	1483	1487	1494	rBB	398752	372672	75.69%	11.962%
8	11.478	1550	1554	1562	rBV	422941	435616	88.48%	13.982%
9	12.701	1758	1762	1767	rBV	10570	11963	2.43%	0.384%
10	12.930	1799	1801	1806	rVB	8157	7508	1.52%	0.241%
11	13.060	1820	1823	1826	rVB	7624	7445	1.51%	0.239%
12	13.866	1956	1960	1965	rBV5	9731	15307	3.11%	0.491%
13	14.013	1983	1985	1990	rVB4	7391	8128	1.65%	0.261%
14	14.130	2001	2005	2014	rBV	455504	484100	98.32%	15.539%
15	14.272	2026	2029	2032	rBV4	9120	9320	1.89%	0.299%
16	15.213	2187	2189	2197	rBV3	9258	15411	3.13%	0.495%
17	15.671	2262	2267	2275	rVB	311297	418827	85.07%	13.444%


Sum of corrected areas: 3115442

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF071218\
Data File : BF107344.D
Acq On : 12 Jul 2018 17:35
Operator : JU/SJ
Sample : J3914-01DL 100X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
B1DL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

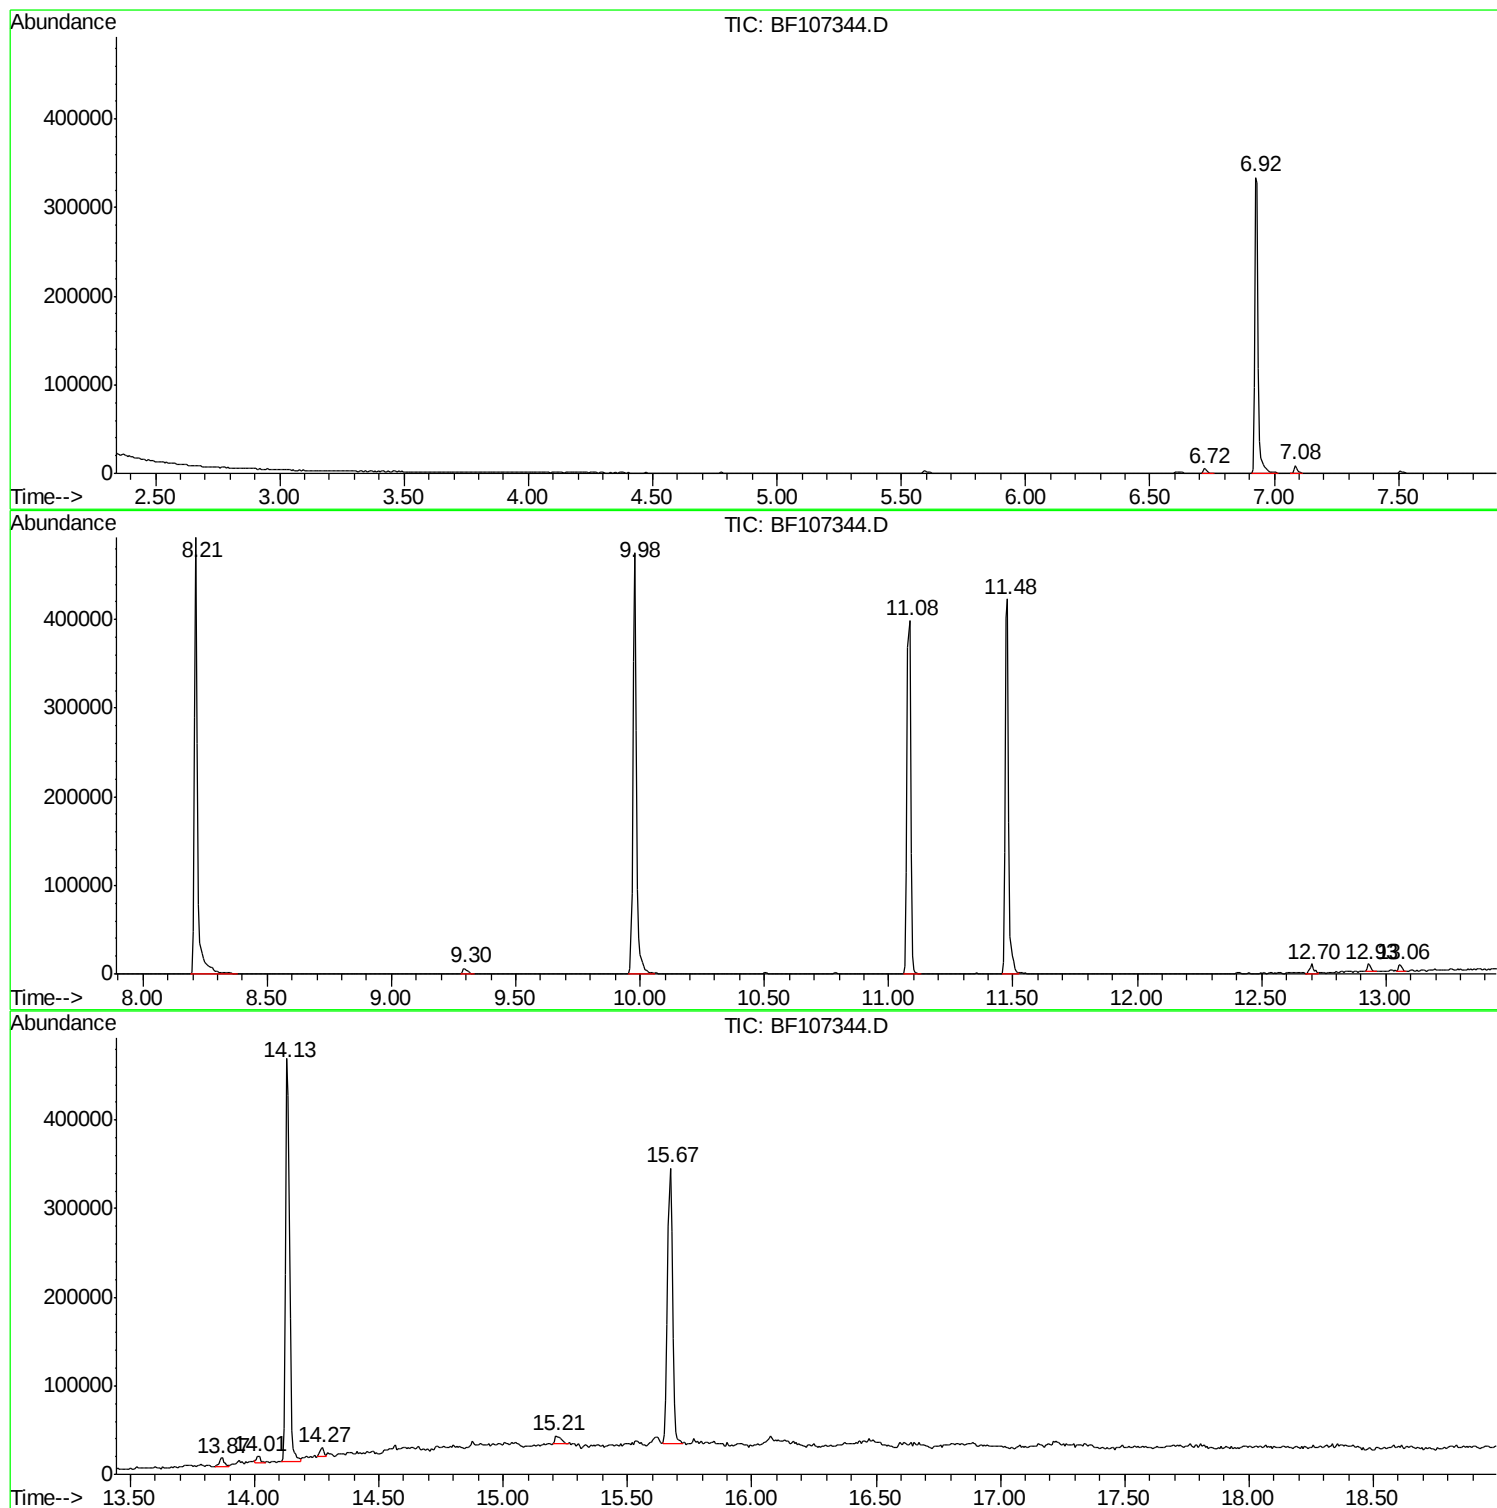

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF071218\
Data_File : BF107344.D
Acq_On : 12-Jul-2018 17:355
Operator : JU/SJJ
Sample : J3914-01DL_100XX
Misc :
ALS_Vial : 16 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
B1DL

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061918.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
