


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071218\
 Data File : BF107329.D
 Acq On : 12 Jul 2018 10:02
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jul 13 11:54:53 2018

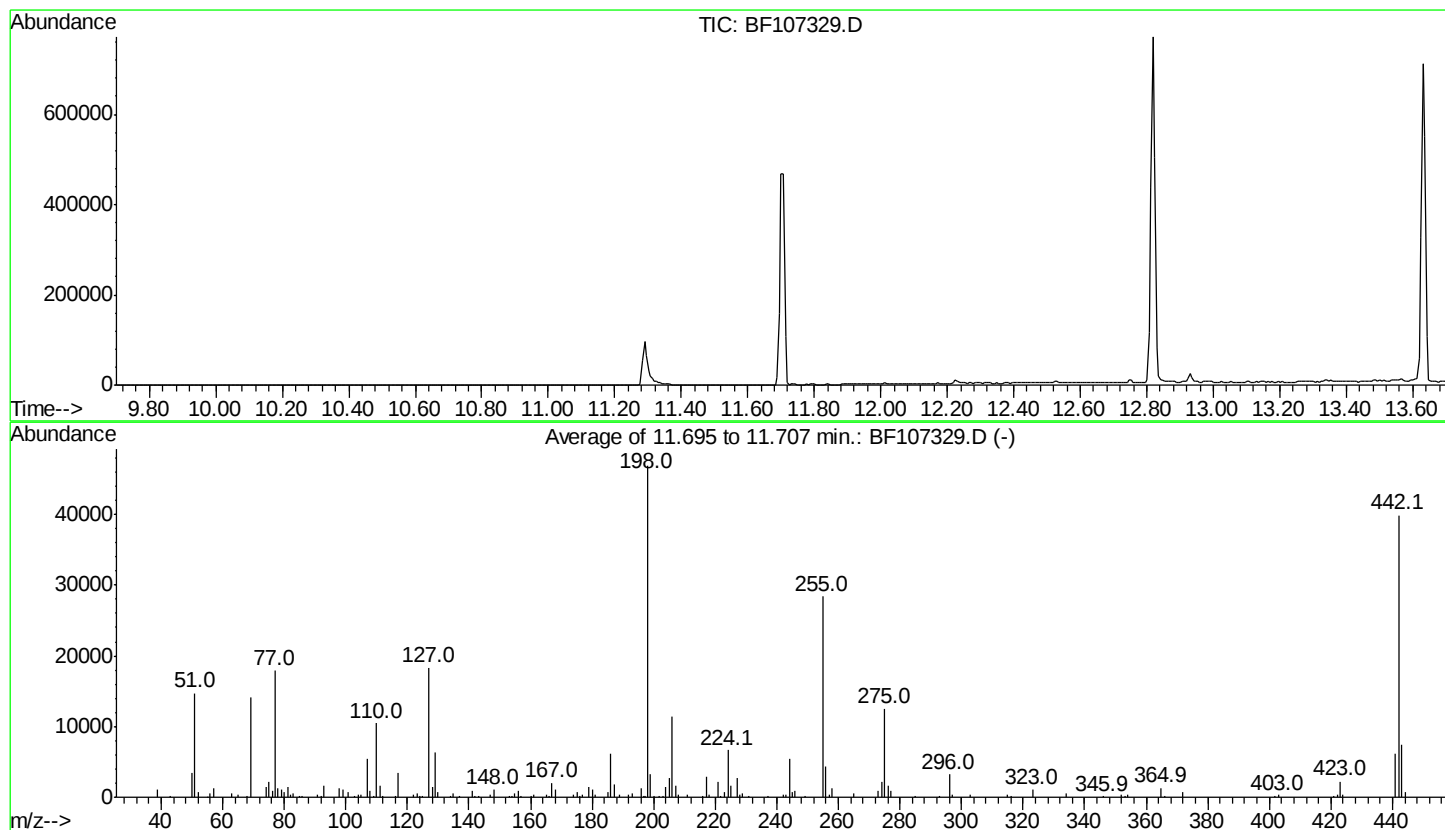

AutoFind: Scans 1591, 1592, 1593; Background Corrected with Scan 1587

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.4	14730	PASS
68	69	0.00	2	1.1	156	PASS
69	198	0.00	100	30.1	14104	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	39.1	18342	PASS
197	198	0.00	2	0.3	136	PASS
198	198	100	100	100.0	46906	PASS
199	198	5	9	7.1	3327	PASS
275	198	10	60	26.8	12552	PASS
365	198	1	100	2.8	1327	PASS
441	198	0.01	100	13.1	6149	PASS
442	198	50	100	85.0	39869	PASS
443	442	15	24	18.8	7506	PASS