
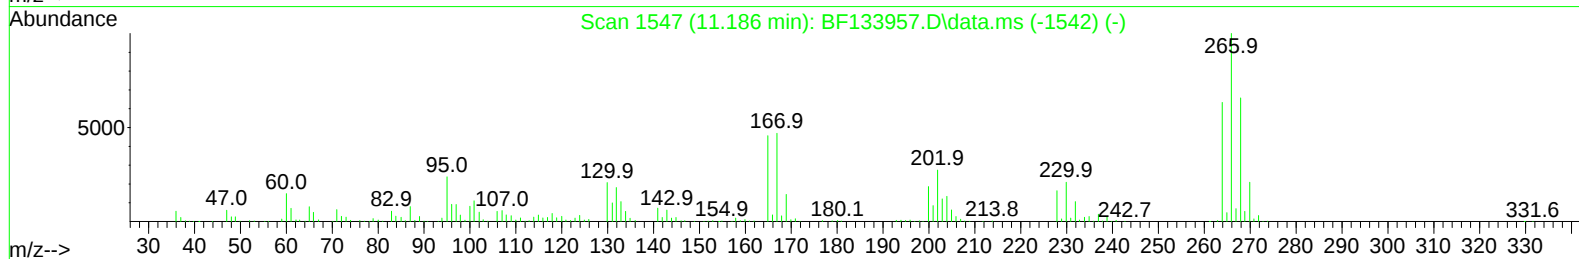
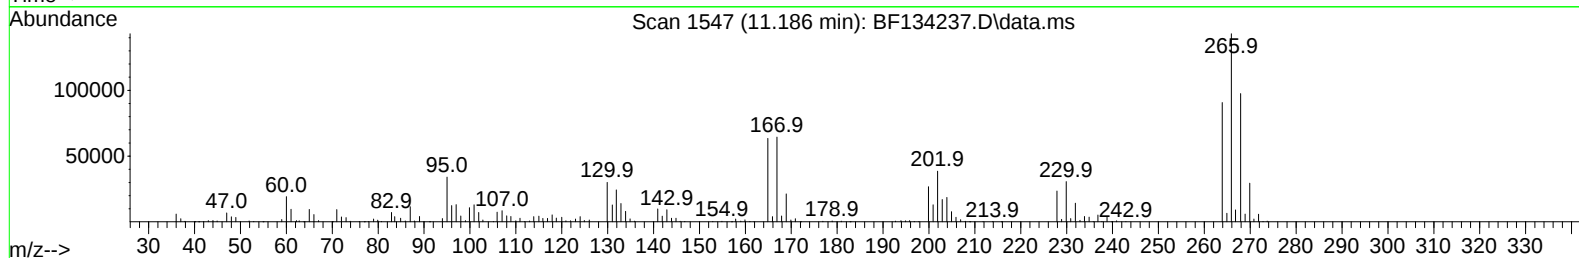


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071223\
Data File : BF134237.D
Acq On : 12 Jul 2023 09:31
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 12 13:17:13 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 11 13:06:48 2023
Response via : Initial Calibration

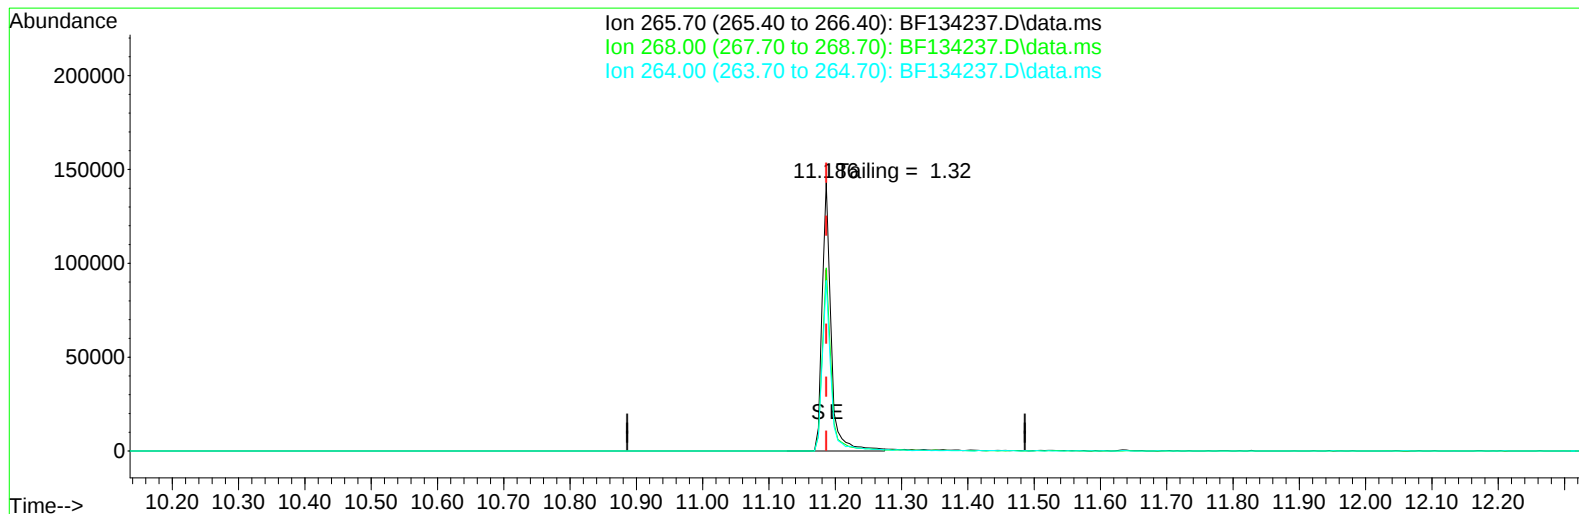

TIC: BF134237.D\data.ms

(70) Pentachlorophenol (C)




11.186min (+ 0.000) 27676.38 ng

response 135021

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.80	68.18
264.00	63.30	63.47
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071223\
Data File : BF134237.D
Acq On : 12 Jul 2023 09:31
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 12 13:17:13 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 11 13:06:48 2023
Response via : Initial Calibration

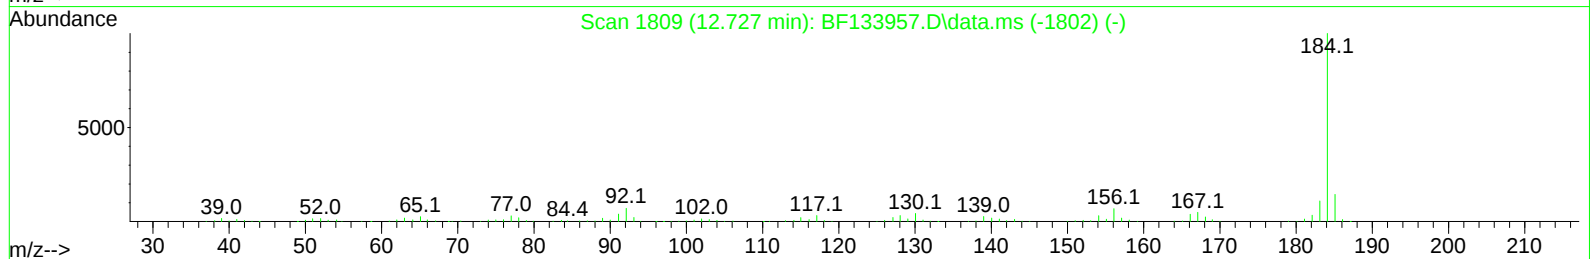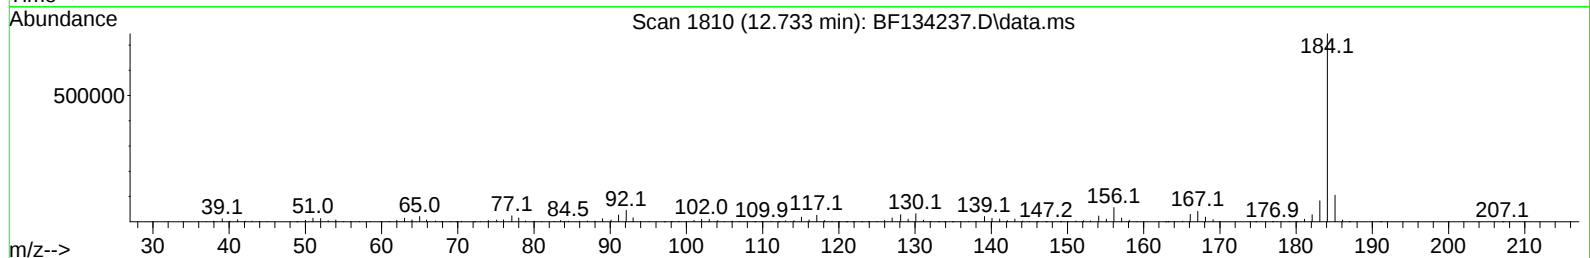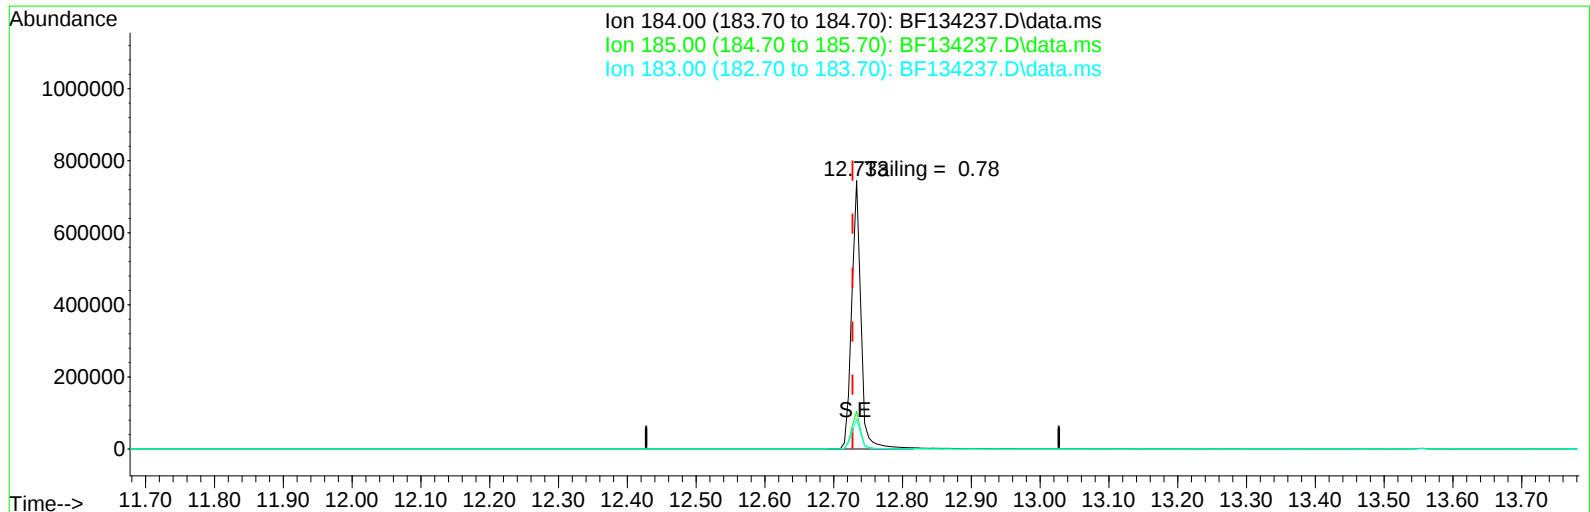

TIC: BF134237.D\data.ms

(77) Benzidine

12.733min (+ 0.006) 120162.34 ng m

response 686204

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.12
183.00	11.00	11.20
0.00	0.00	0.00