
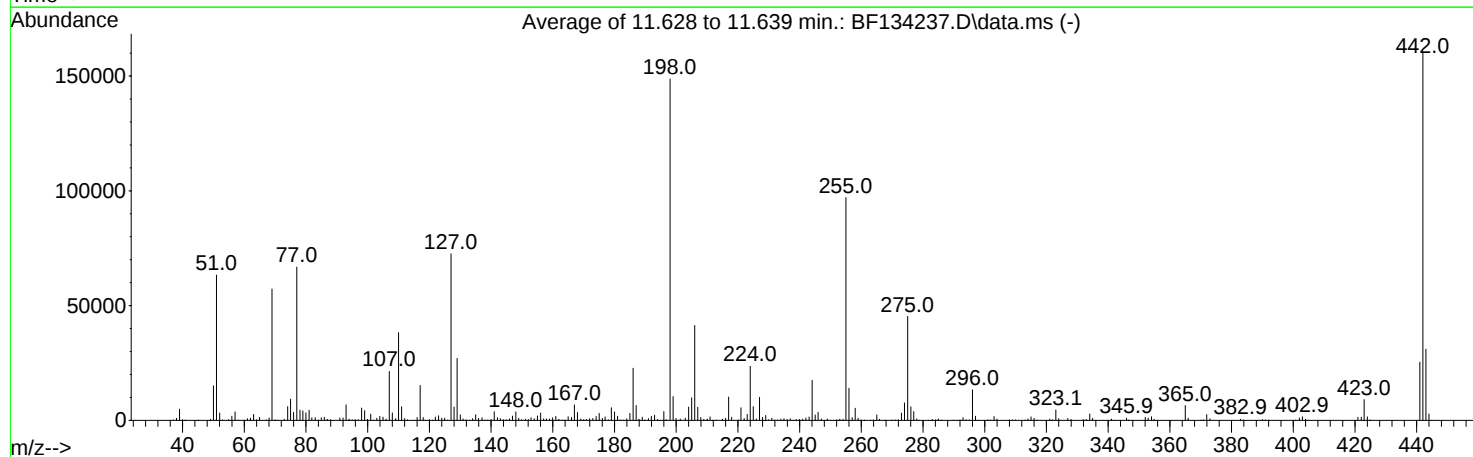


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071223\
Data File : BF134237.D
Acq On : 12 Jul 2023 09:31
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jul 11 13:06:48 2023

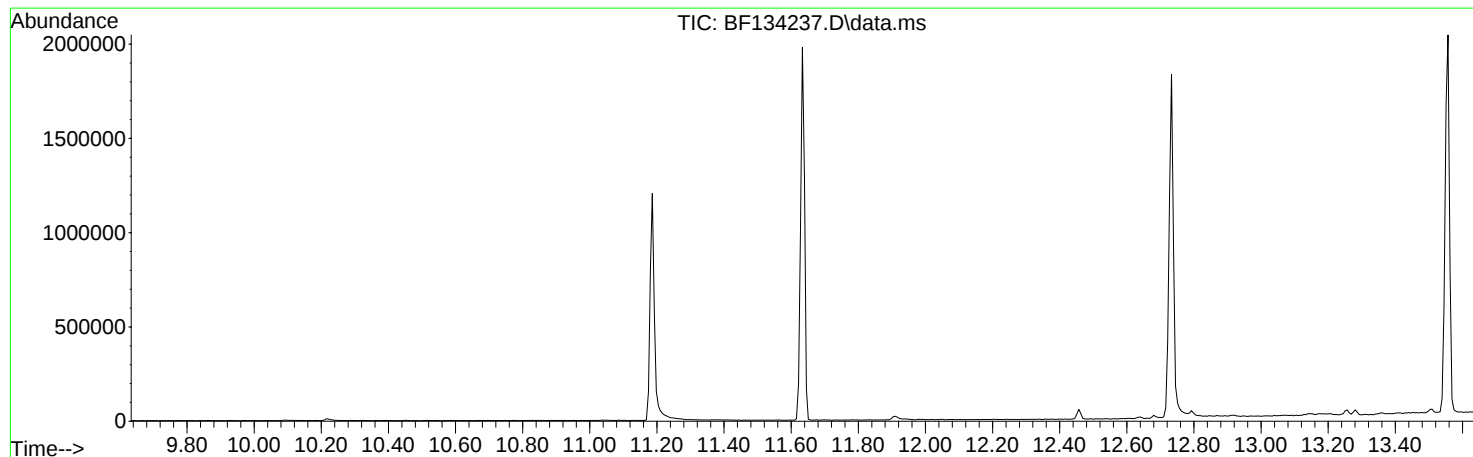




AutoFind: Scans 1622, 1623, 1624; Background Corrected with Scan 1617

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.6	63312	PASS
68	69	0.00	2	1.9	1069	PASS
69	198	0.00	100	38.5	57215	PASS
70	69	0.00	2	0.4	235	PASS
127	198	10	80	48.8	72600	PASS
197	198	0.00	2	0.2	355	PASS
198	198	100	100	100.0	148792	PASS
199	198	5	9	7.0	10397	PASS
275	198	10	60	30.4	45291	PASS
365	198	1	100	4.4	6522	PASS
441	198	0.01	100	17.1	25403	PASS
442	442	50	100	100.0	160277	PASS
443	442	15	24	19.3	31006	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071223\
 Data File : BF134237.D
 Acq On : 12 Jul 2023 09:31
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Jul 12 13:17:13 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 11 13:06:48 2023
 Response via : Initial Calibration

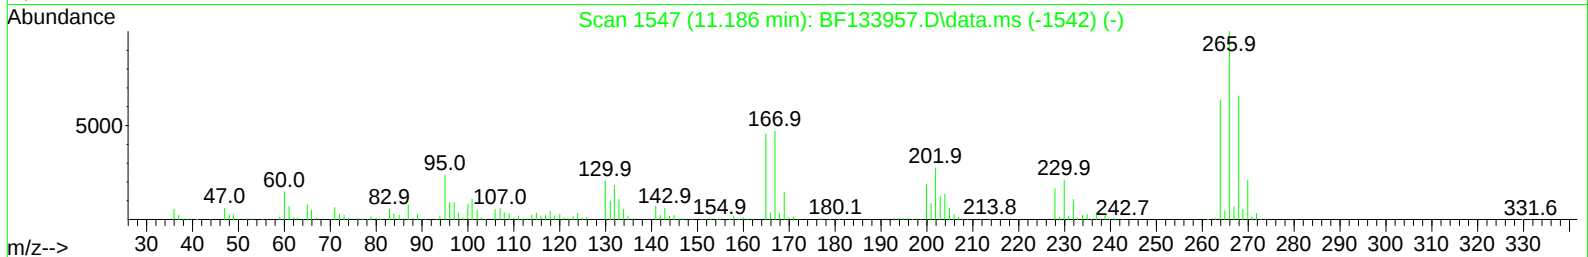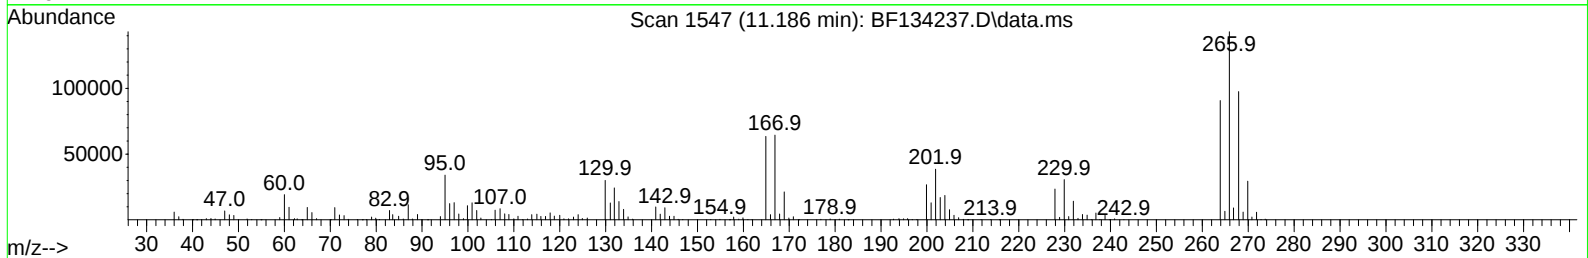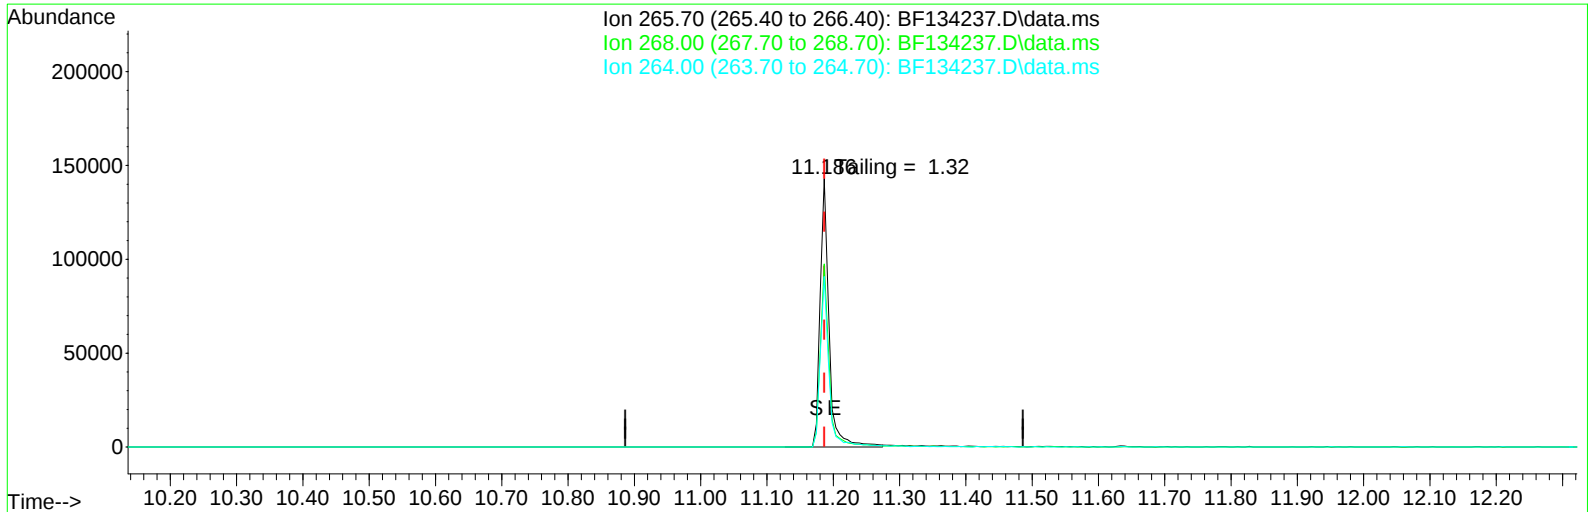

TIC: BF134237.D\data.ms

(70) Pentachlorophenol (C)

11.186min (+ 0.000) 27676.38 ng




response 135021

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.80	68.18
264.00	63.30	63.47
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071223\
Data File : BF134237.D
Acq On : 12 Jul 2023 09:31
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 12 13:17:13 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 11 13:06:48 2023
Response via : Initial Calibration

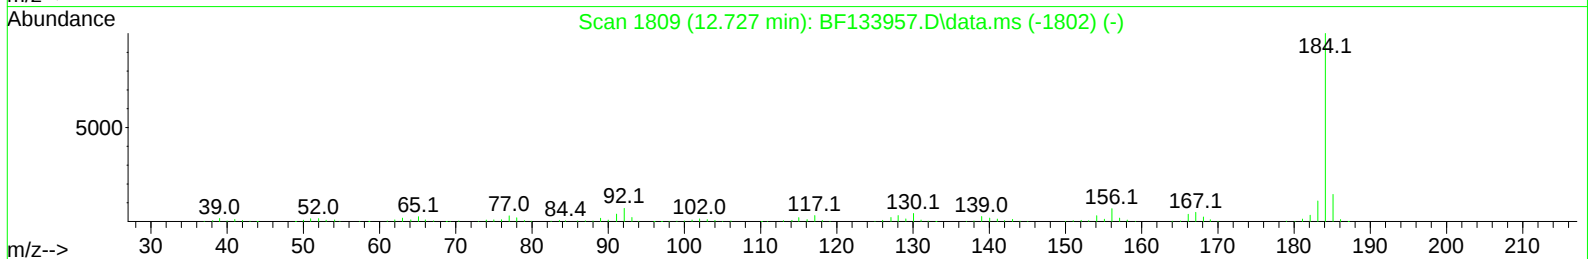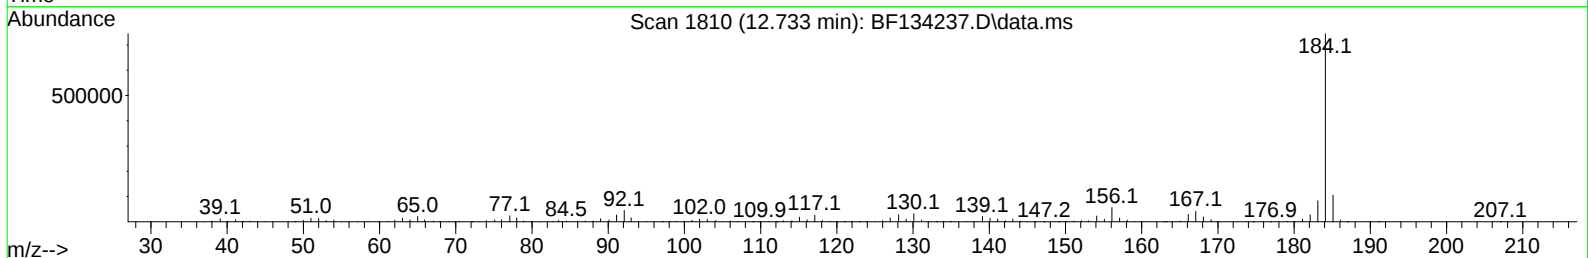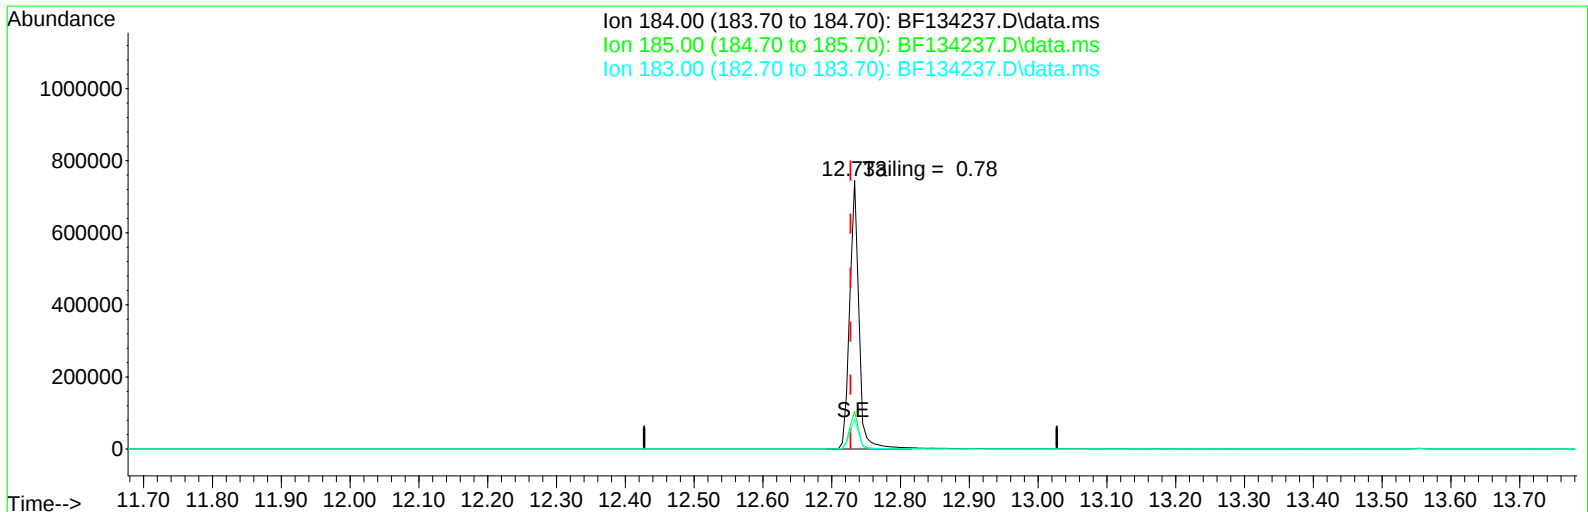

TIC: BF134237.D\data.ms

(77) Benzidine

12.733min (+ 0.006) 120162.34 ng m

response 686204

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.12
183.00	11.00	11.20
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/12/2023	BNA_F	<u>BF134237.D</u>
Compound Name	Response	Retention Time
DDT	353793	13.557
DDD	8765	13.257
DDE	878	12.916
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9643	363436	2.65

Instrument :
BNA_F
ClientSampleId :
DFTPP