


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071224\
Data File : BF138539.D
Acq On : 12 Jul 2024 11:23
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF070924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jul 09 16:58:40 2024

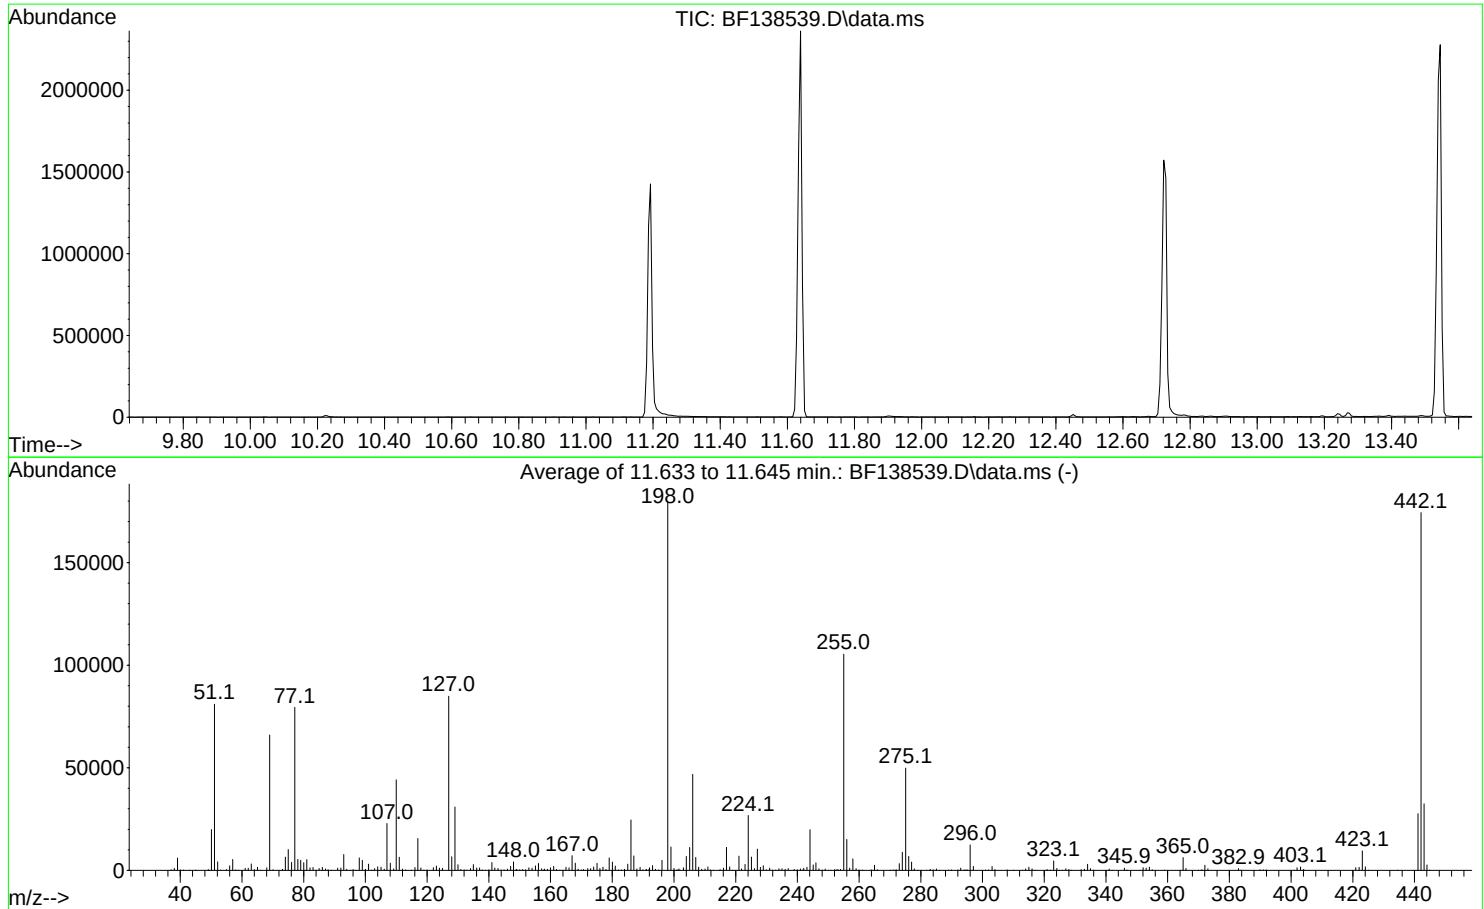

AutoFind: Scans 1623, 1624, 1625; Background Corrected with Scan 1617

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.1	80941	PASS
68	69	0.00	2	1.9	1266	PASS
69	198	0.00	100	36.8	65960	PASS
70	69	0.00	2	0.5	304	PASS
127	198	10	80	47.3	84848	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	179309	PASS
199	198	5	9	6.4	11431	PASS
275	198	10	60	27.8	49824	PASS
365	198	1	100	3.5	6248	PASS
441	198	0.01	100	15.4	27600	PASS
442	442	50	100	100.0	174408	PASS
443	442	15	24	18.6	32445	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
7/12/2024	BNA_F	<u>BF138539.D</u>
Compound Name	Response	Retention Time
DDT	402732	13.545
DDD	7349	13.269
DDE	928	12.904
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8277	411009	2.01

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071224\
Data File : BF138539.D
Acq On : 12 Jul 2024 11:23
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 12 12:35:54 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF070924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 09 16:58:40 2024
Response via : Initial Calibration

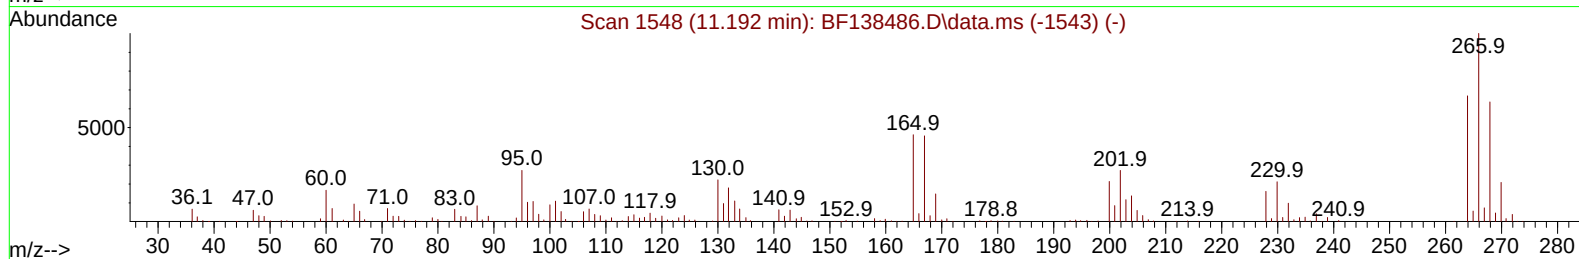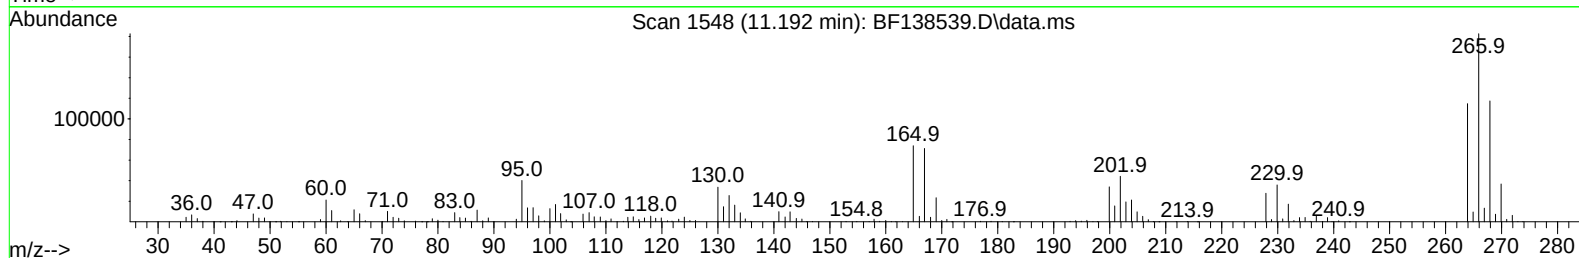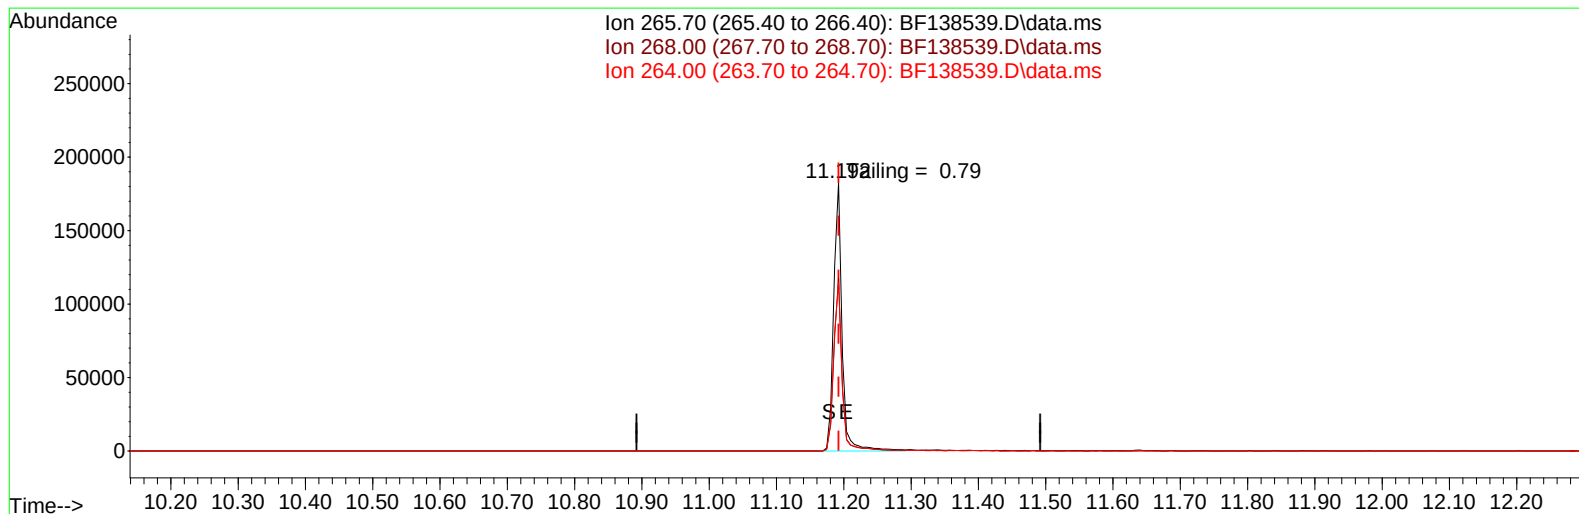

TIC: BF138539.D\data.ms

(70) Pentachlorophenol (C)

11.192min (+ 0.000) 28501.97 ng




response 159643

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	64.26
264.00	66.90	62.86
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071224\
Data File : BF138539.D
Acq On : 12 Jul 2024 11:23
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 12 12:35:54 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF070924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 09 16:58:40 2024
Response via : Initial Calibration

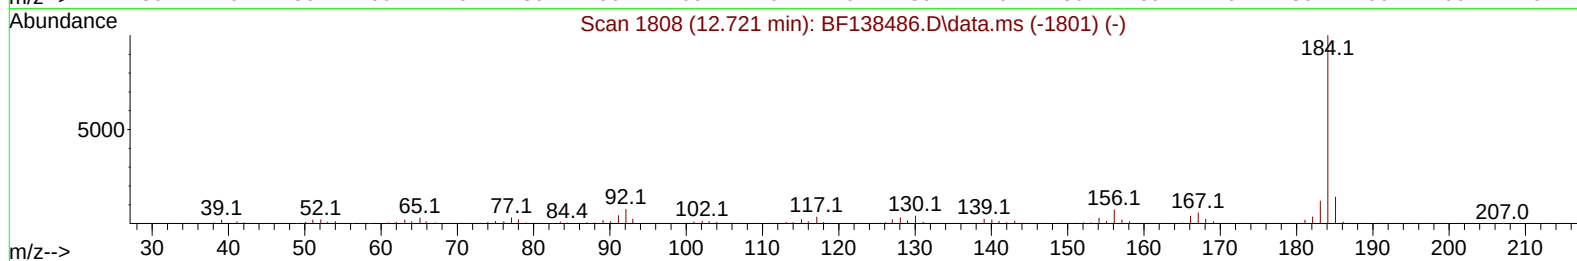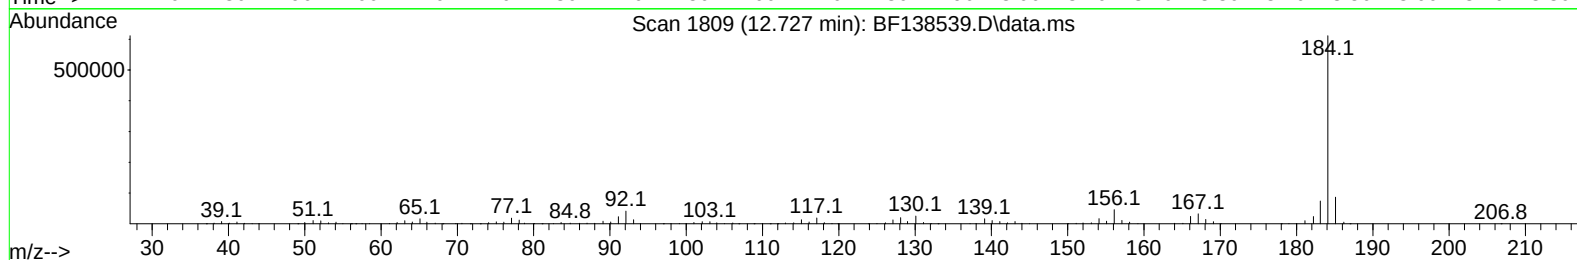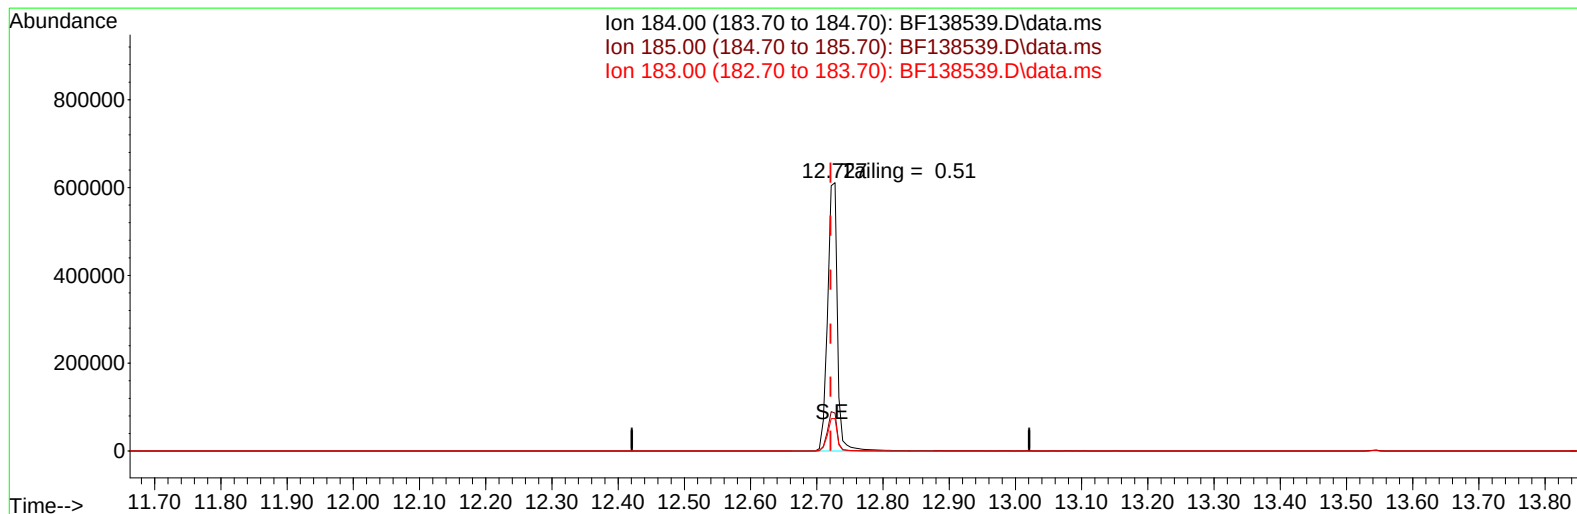

TIC: BF138539.D\data.ms

(77) Benzidine

12.727min (+ 0.006) 0.00 ng

response 631886

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.15
183.00	11.90	12.14
0.00	0.00	0.00