

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071323\
 Data File : BF134278.D
 Acq On : 14 Jul 2023 00:27
 Operator : CG\JU
 Sample : 03428-01RE
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PNNL-APM-0621-1RE

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF134278.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.193	13	18	27	rVB	23483	34559	2.01%	0.287%
2	5.075	504	508	515	rBV	59617	73265	4.25%	0.608%
3	5.475	572	576	594	rBV	1594564	1455257	84.51%	12.070%
4	6.481	743	747	765	rBV	1609528	1460712	84.83%	12.115%
5	6.839	805	808	815	rBV	513722	419873	24.38%	3.482%
6	7.404	900	904	907	rBV	1125419	912907	53.02%	7.572%
7	8.122	1022	1026	1030	rBV	671794	528889	30.71%	4.387%
8	9.198	1205	1209	1212	rBV	2237656	1721931	100.00%	14.282%
9	9.880	1321	1325	1328	rBV	702713	567845	32.98%	4.710%
10	10.598	1443	1447	1456	rVB	348690	292628	16.99%	2.427%
11	10.675	1456	1460	1469	rBV	1205197	1097925	63.76%	9.106%
12	10.904	1496	1499	1503	rBV	74225	63080	3.66%	0.523%
13	10.986	1509	1513	1516	rBV	26891	30530	1.77%	0.253%
14	11.286	1562	1564	1566	rVB	31330	23719	1.38%	0.197%
15	11.374	1575	1579	1586	rBV	671460	568109	32.99%	4.712%
16	11.904	1665	1669	1678	rBV	253393	269934	15.68%	2.239%
17	12.692	1800	1803	1810	rBV2	73082	100436	5.83%	0.833%
18	12.968	1846	1850	1854	rBV	1635734	1579593	91.73%	13.101%
19	13.198	1887	1889	1894	rBV4	21280	28904	1.68%	0.240%
20	13.892	2003	2007	2015	rBV6	69355	152786	8.87%	1.267%
21	14.039	2028	2032	2038	rVB	368593	357313	20.75%	2.964%
22	15.545	2284	2288	2296	rVB	217716	316634	18.39%	2.626%




Sum of corrected areas: 12056829

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071323\
Data File : BF134278.D
Acq On : 14 Jul 2023 00:27
Operator : CG\JU
Sample : 03428-01RE
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PNNL-APM-0621-1RE

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

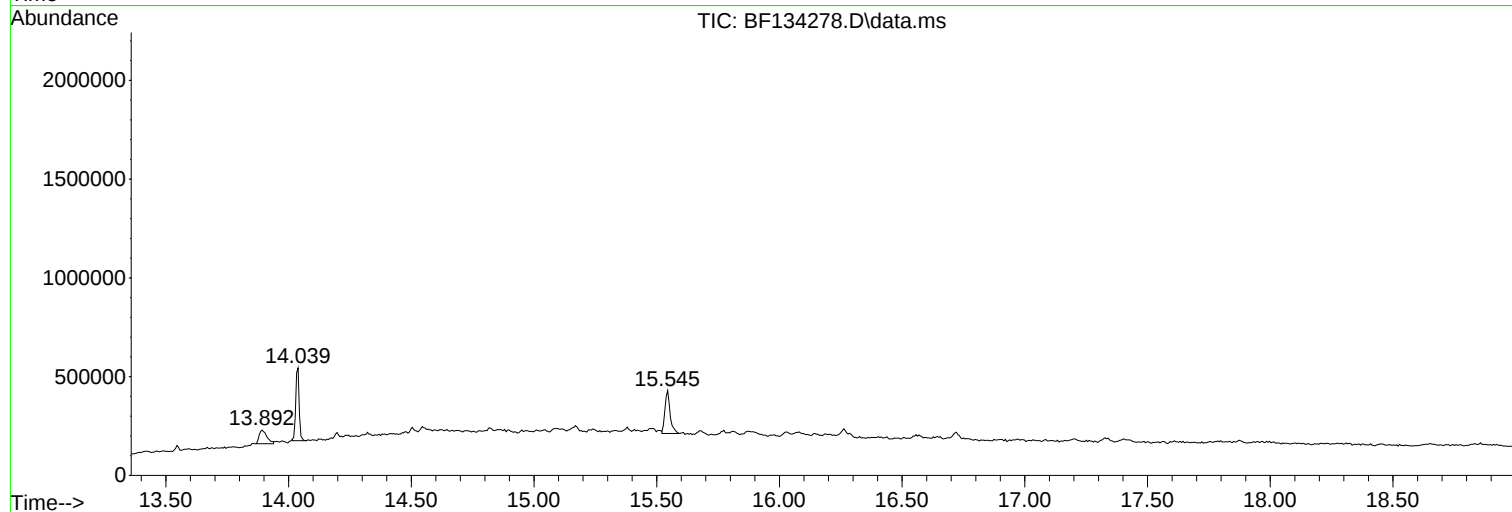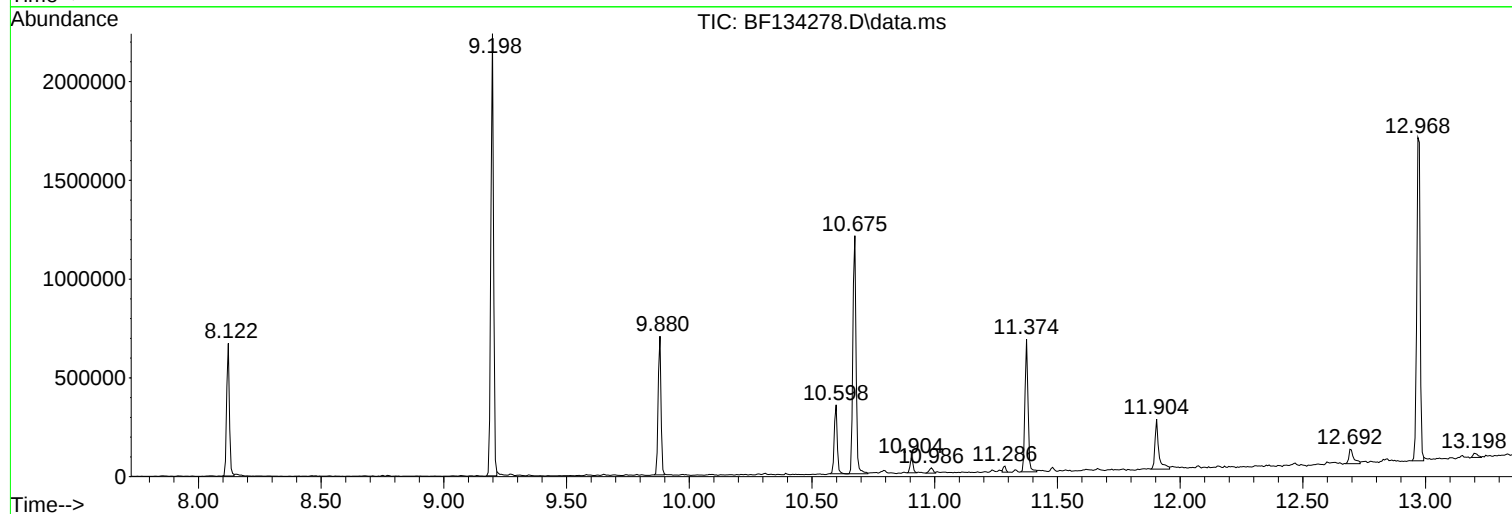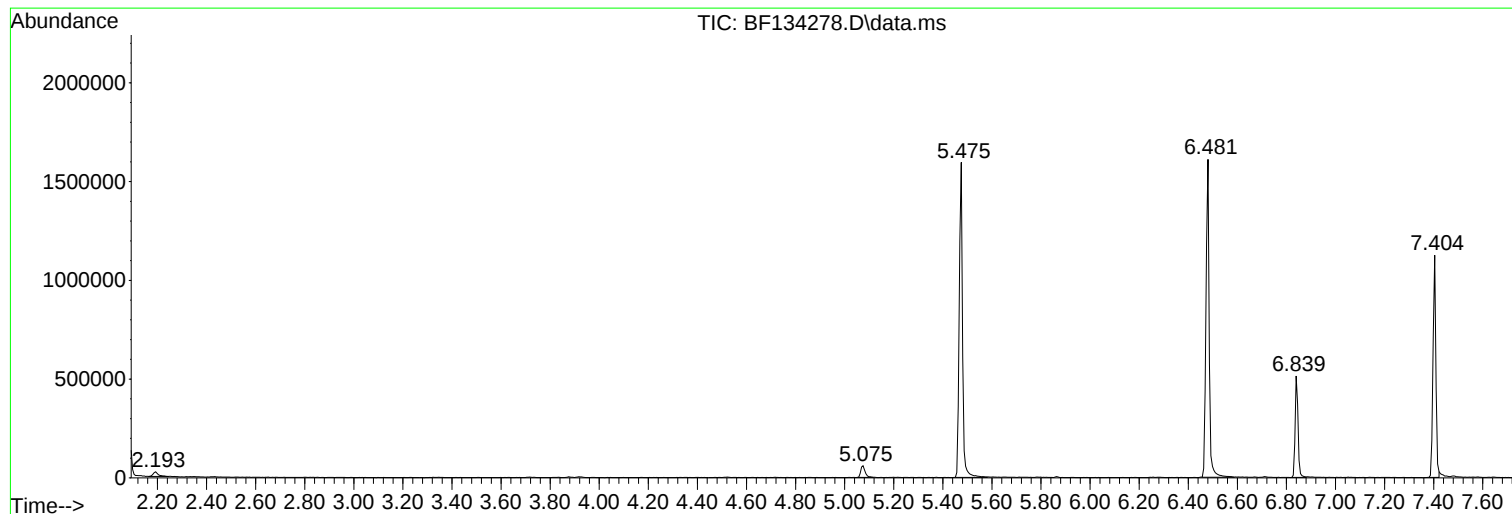

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071323\
Data File : BF134278.D
Acq On : 14 Jul 2023 00:27
Operator : CG\JU
Sample : 03428-01RE
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PNNL-APM-0621-1RE

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071323\
Data File : BF134278.D
Acq On : 14 Jul 2023 00:27
Operator : CG\JU
Sample : 03428-01RE
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PNNL-APM-0621-1RE

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------