
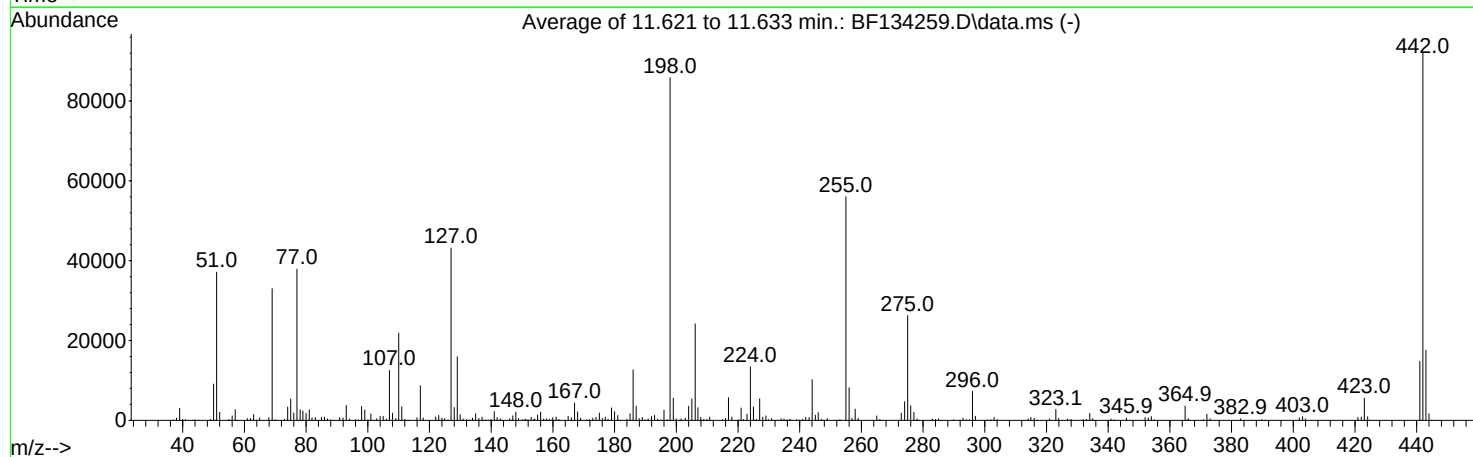


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071323\
Data File : BF134259.D
Acq On : 13 Jul 2023 13:27
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jul 11 13:06:48 2023

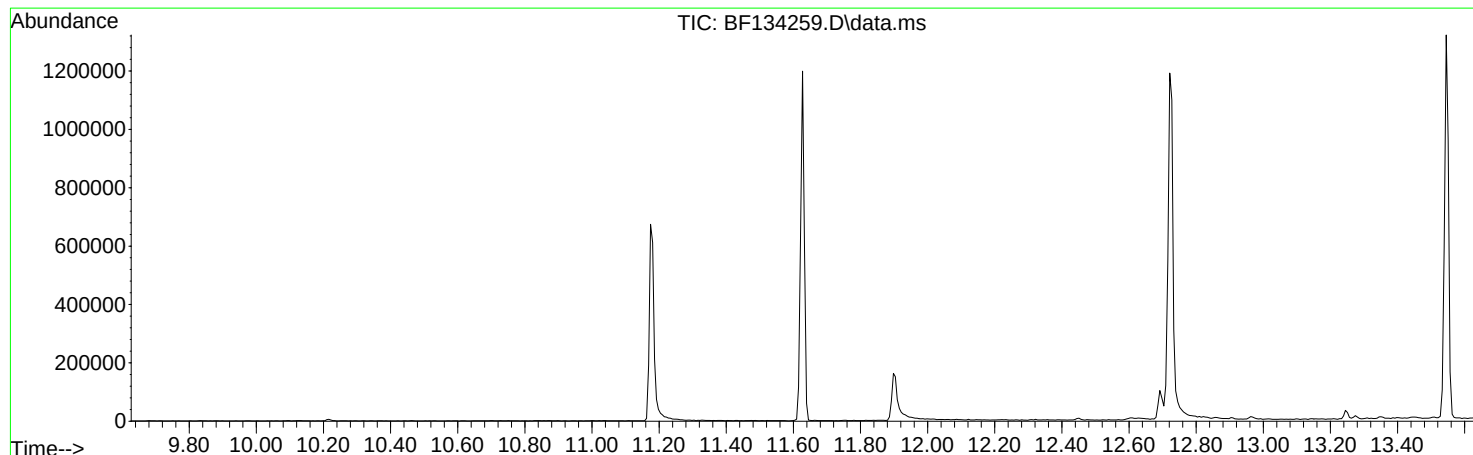




AutoFind: Scans 1621, 1622, 1623; Background Corrected with Scan 1616

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.2	37118	PASS
68	69	0.00	2	2.0	673	PASS
69	198	0.00	100	38.4	32988	PASS
70	69	0.00	2	0.5	177	PASS
127	198	10	80	50.3	43189	PASS
197	198	0.00	2	0.2	197	PASS
198	198	100	100	100.0	85851	PASS
199	198	5	9	6.5	5594	PASS
275	198	10	60	30.6	26245	PASS
365	198	1	100	4.2	3615	PASS
441	198	0.01	100	17.2	14806	PASS
442	442	50	100	100.0	92152	PASS
443	442	15	24	19.0	17550	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071323\
 Data File : BF134259.D
 Acq On : 13 Jul 2023 13:27
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Jul 14 04:03:58 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 11 13:06:48 2023
 Response via : Initial Calibration

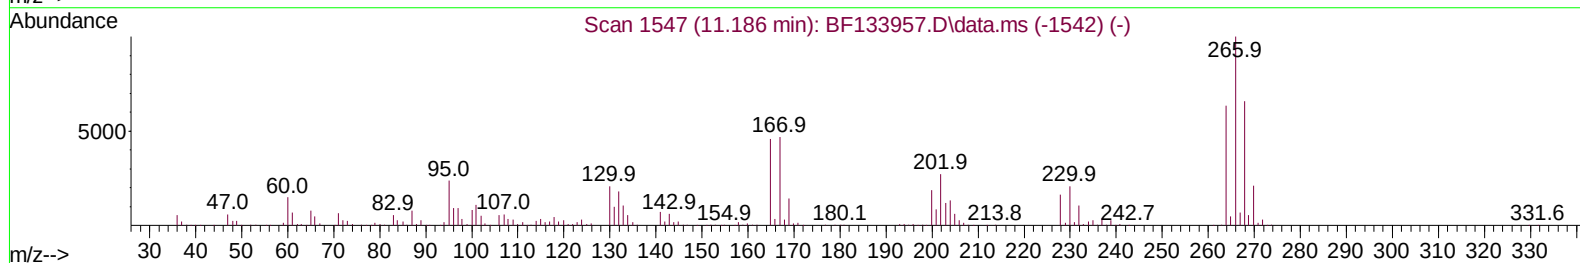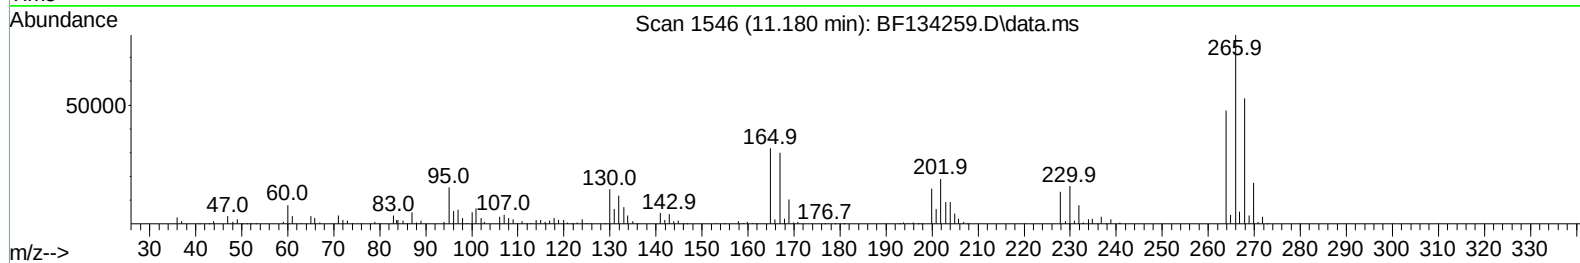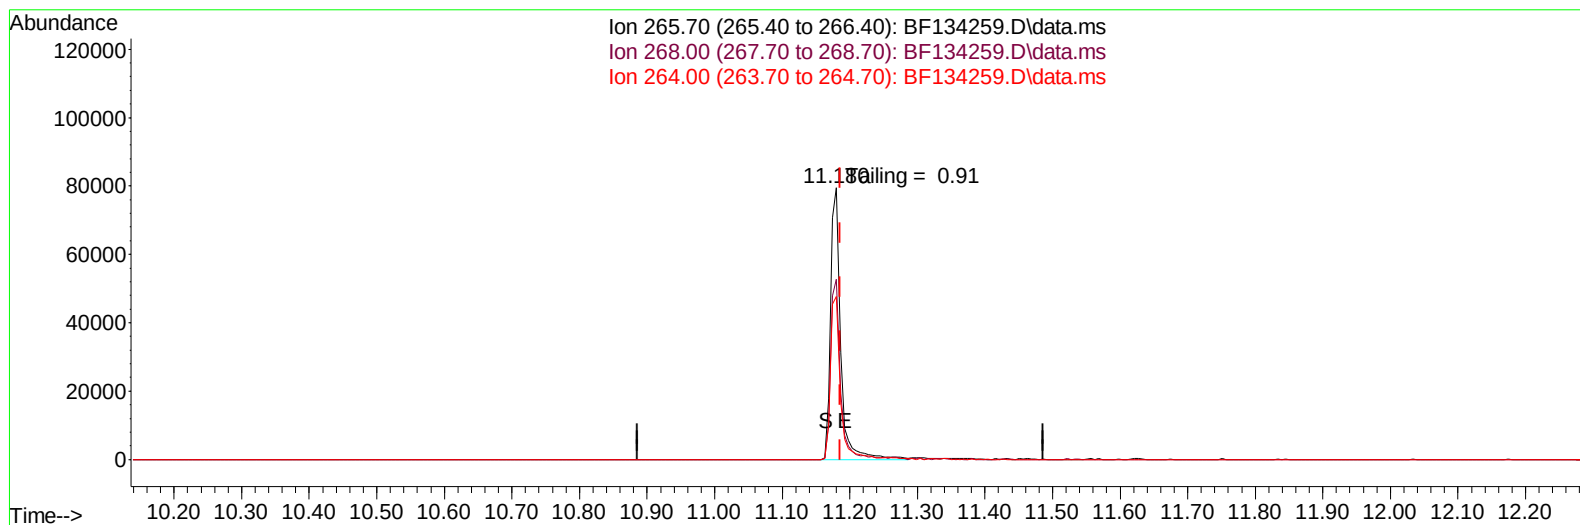

TIC: BF134259.D\data.ms

(70) Pentachlorophenol (C)

11.180min (-0.006) 26924.74 ng




response 82119

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.80	66.39
264.00	63.30	59.99
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071323\
Data File : BF134259.D
Acq On : 13 Jul 2023 13:27
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 14 04:03:58 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 11 13:06:48 2023
Response via : Initial Calibration

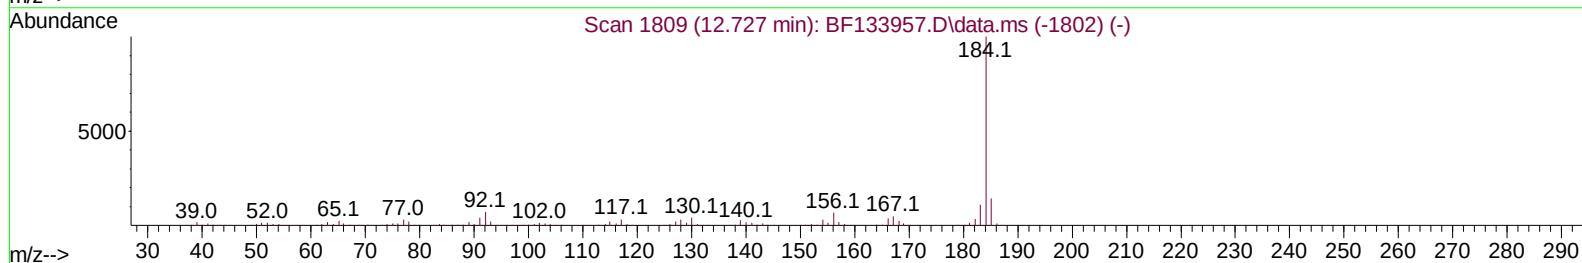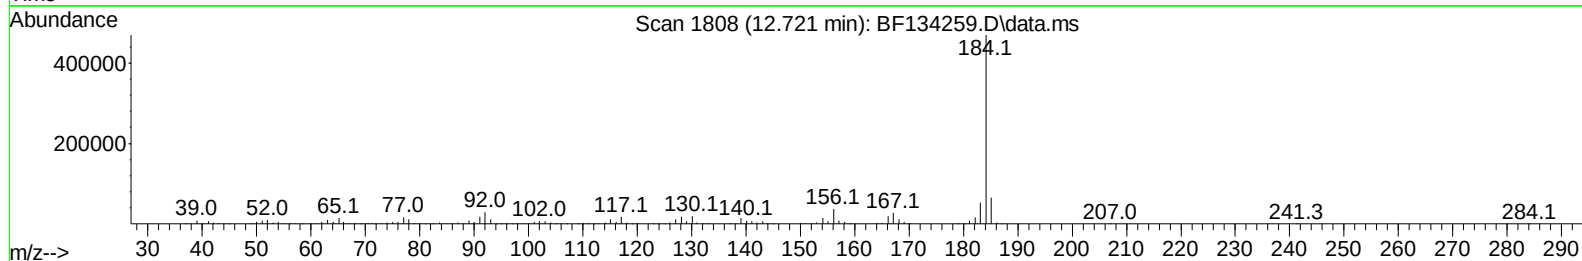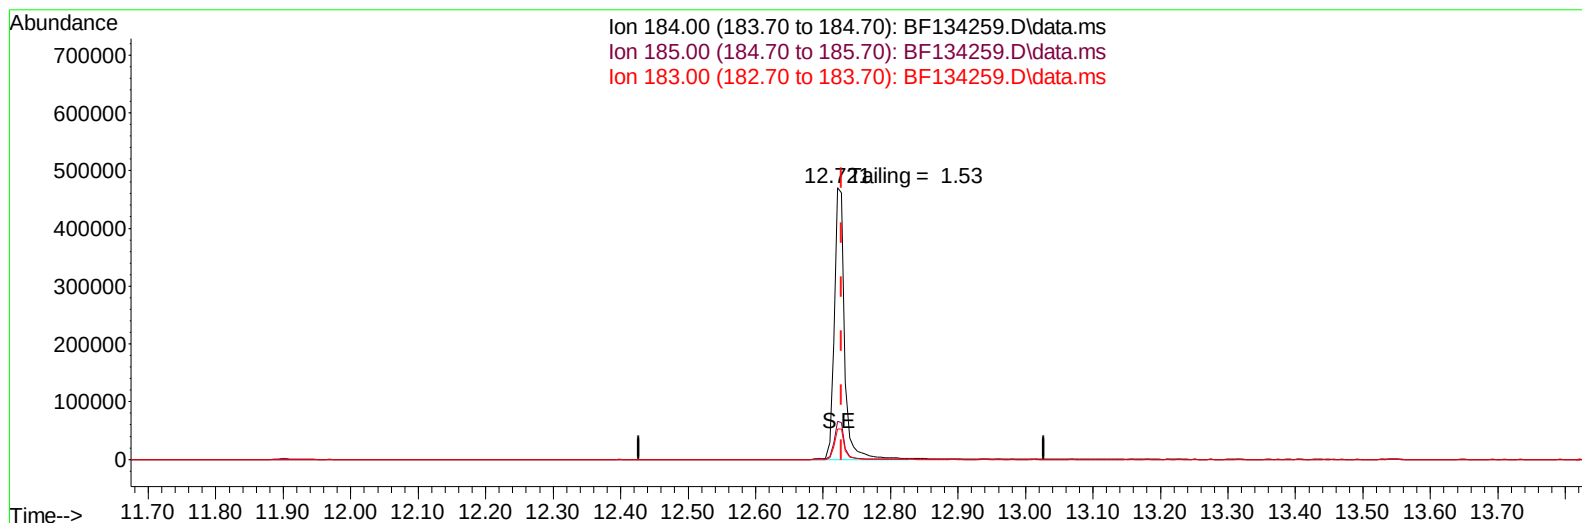

TIC: BF134259.D\data.ms

(77) Benzidine

12.721min (-0.006) 398510.06 ng

response 502561

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.10
183.00	11.00	11.24
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/13/2023	BNA_F	<u>BF134259.D</u>
Compound Name	Response	Retention Time
DDT	216612	13.545
DDD	7264	13.245
DDE	564	12.904
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7828	224440	3.49

Instrument :
BNA_F
ClientSampleId :
DFTPP