
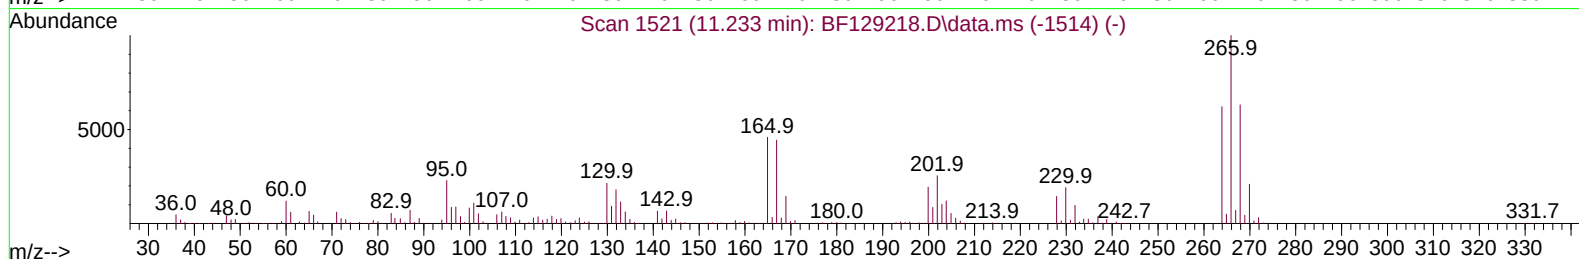
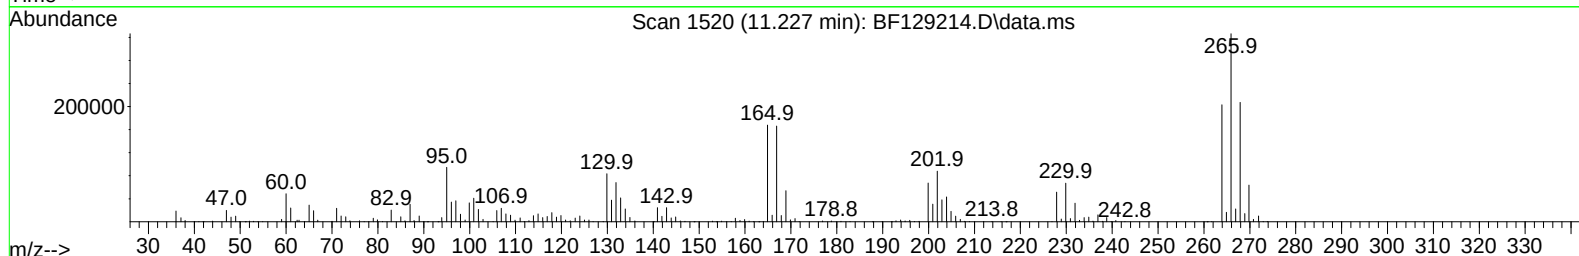


```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071422\  
Data File : BF129214.D  
Acq On    : 14 Jul 2022  11:47  
Operator  : CG\JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Quant Time: Jul 14 18:57:55 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 14 16:23:13 2022
Response via : Initial Calibration

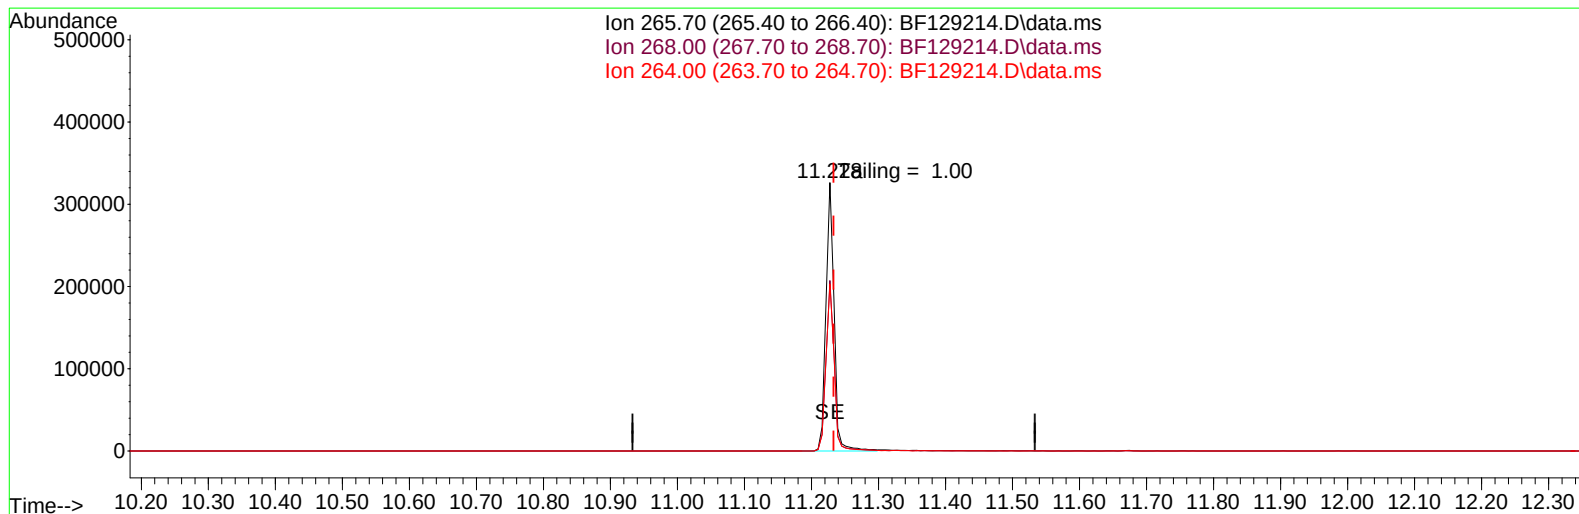

TIC: BF129214.D\data.ms

(70) Pentachlorophenol (C)




11.227min (-0.006) 678770.33 ng

response **279151**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	63.52
264.00	61.80	62.27
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071422\
Data File : BF129214.D
Acq On : 14 Jul 2022 11:47
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 14 18:57:55 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 14 16:23:13 2022
Response via : Initial Calibration

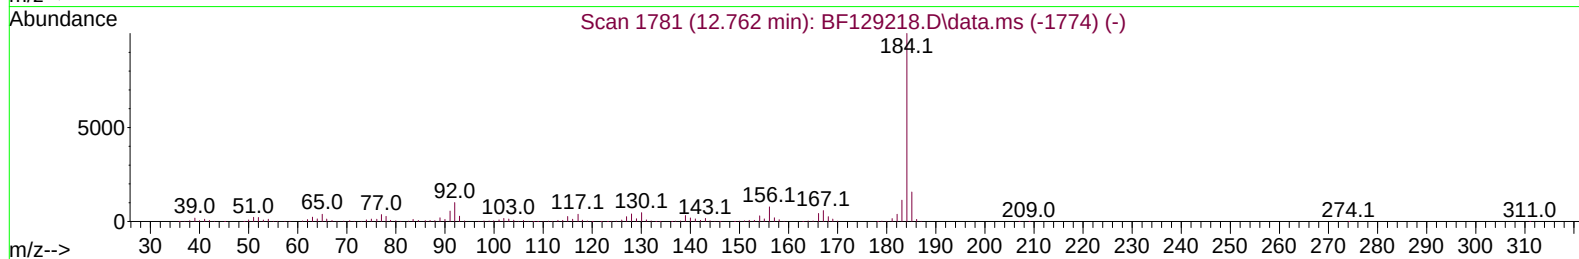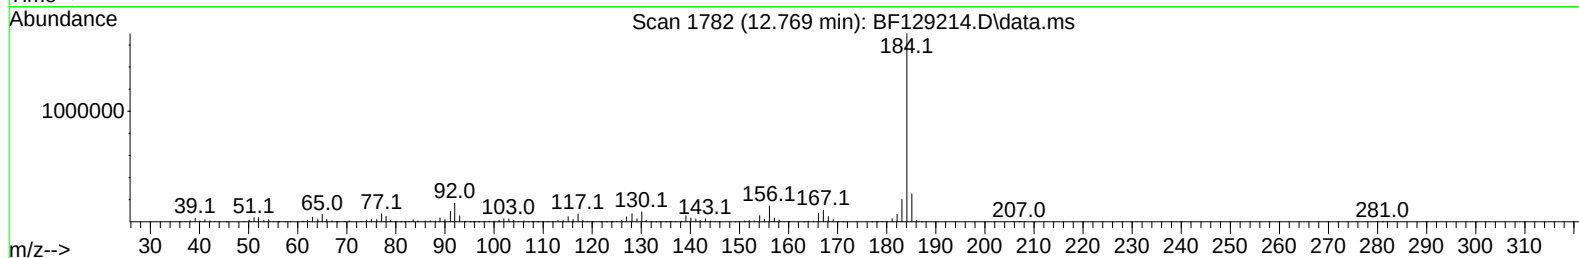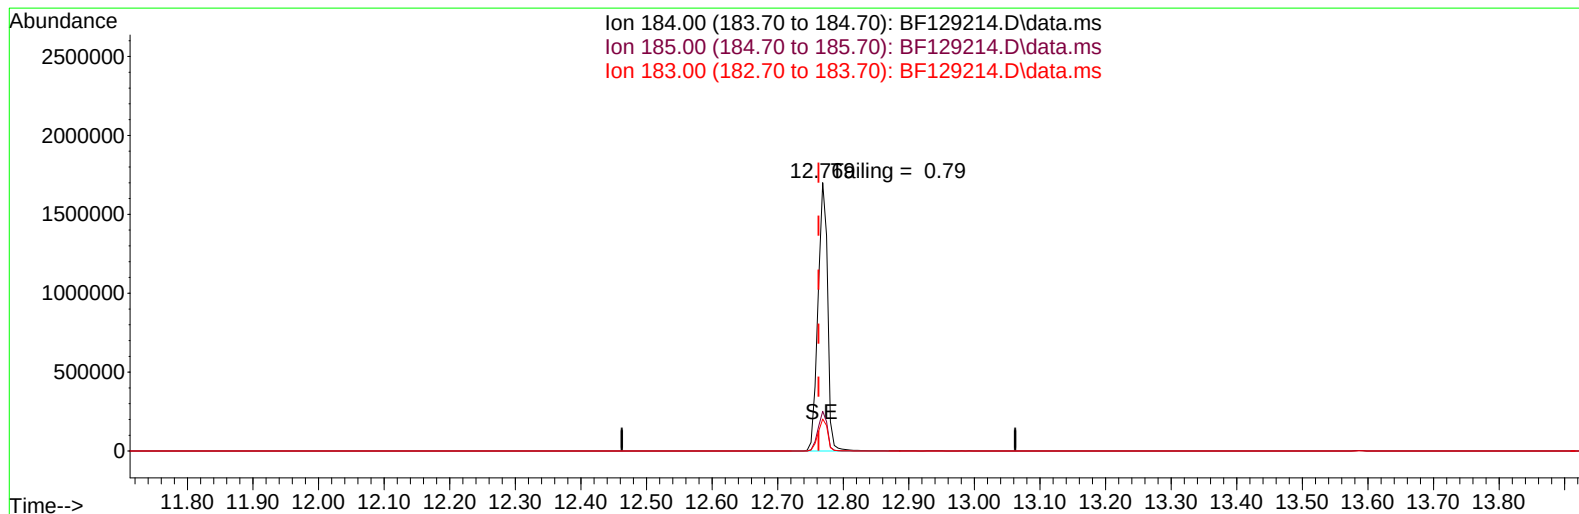

TIC: BF129214.D\data.ms

(77) Benzidine**12.769min (+ 0.006) 969767.31 ng****response 1747468**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.79
183.00	11.60	11.97
0.00	0.00	0.00