

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071422\
 Data File : BF129224.D
 Acq On : 14 Jul 2022 17:13
 Operator : CG\JU
 Sample : PB146162BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB146162BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071422.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF129224.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.046	289	299	305	rBV	136170	182780	1.80%	0.274%
2	5.534	546	552	555	rBV	6822074	7719582	76.07%	11.564%
3	6.522	714	720	723	rBV	6552278	8178447	80.59%	12.252%
4	6.898	780	784	787	rVB	2232732	2072333	20.42%	3.104%
5	7.457	873	879	882	rBV	4681233	5513521	54.33%	8.259%
6	8.181	996	1002	1005	rBV	2775795	2969899	29.27%	4.449%
7	9.257	1178	1185	1188	rBV	8861259	9884133	97.40%	14.807%
8	9.939	1294	1301	1304	rBV	3236666	3310563	32.62%	4.959%
9	10.728	1428	1435	1438	rBV	5988818	6263854	61.72%	9.383%
10	11.428	1547	1554	1557	rBV	3588672	3256330	32.09%	4.878%
11	13.016	1817	1824	1827	rBV	8957012	10148129	100.00%	15.202%
12	14.069	1999	2003	2007	rBV	3244320	2819198	27.78%	4.223%
13	14.157	2012	2018	2026	rBV	694193	805842	7.94%	1.207%
14	15.174	2188	2191	2196	rBV	103498	116567	1.15%	0.175%
15	15.563	2250	2257	2269	rBV	2225024	2799892	27.59%	4.194%
16	16.015	2329	2334	2341	rVB	139658	208272	2.05%	0.312%
17	16.533	2416	2422	2428	rBV	126423	224281	2.21%	0.336%
18	17.145	2520	2526	2534	rVB3	74870	167384	1.65%	0.251%
19	17.868	2643	2649	2658	rVB2	48470	112934	1.11%	0.169%




Sum of corrected areas: 66753941

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071422\
Data File : BF129224.D
Acq On : 14 Jul 2022 17:13
Operator : CG\JU
Sample : PB146162BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB146162BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

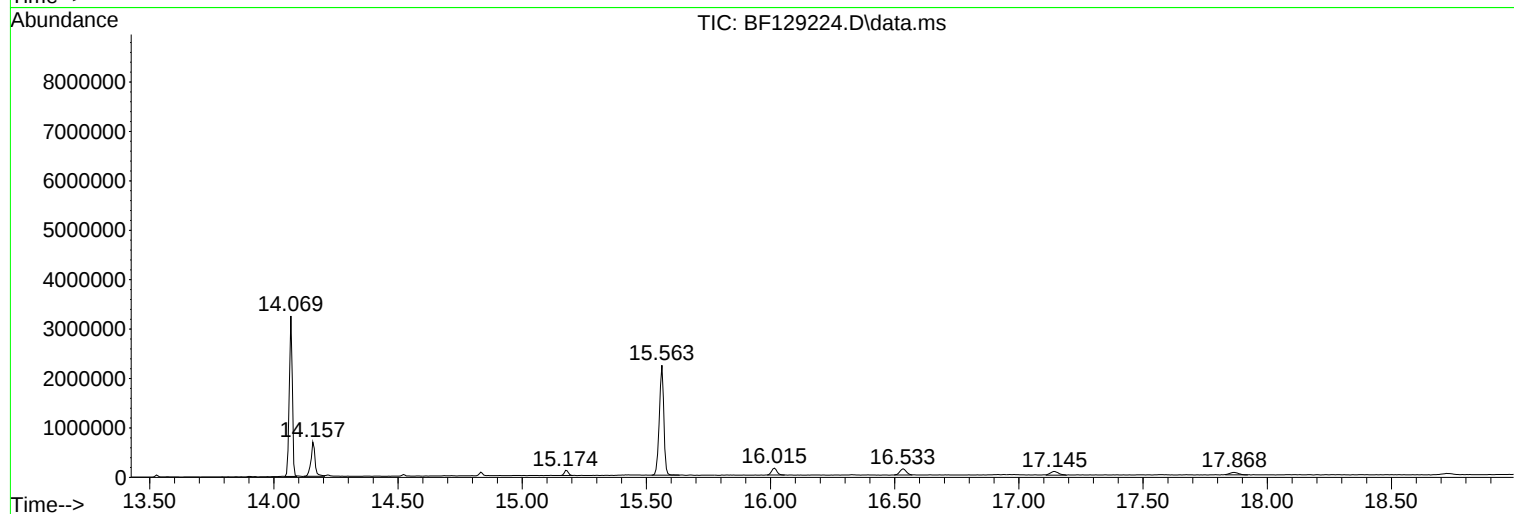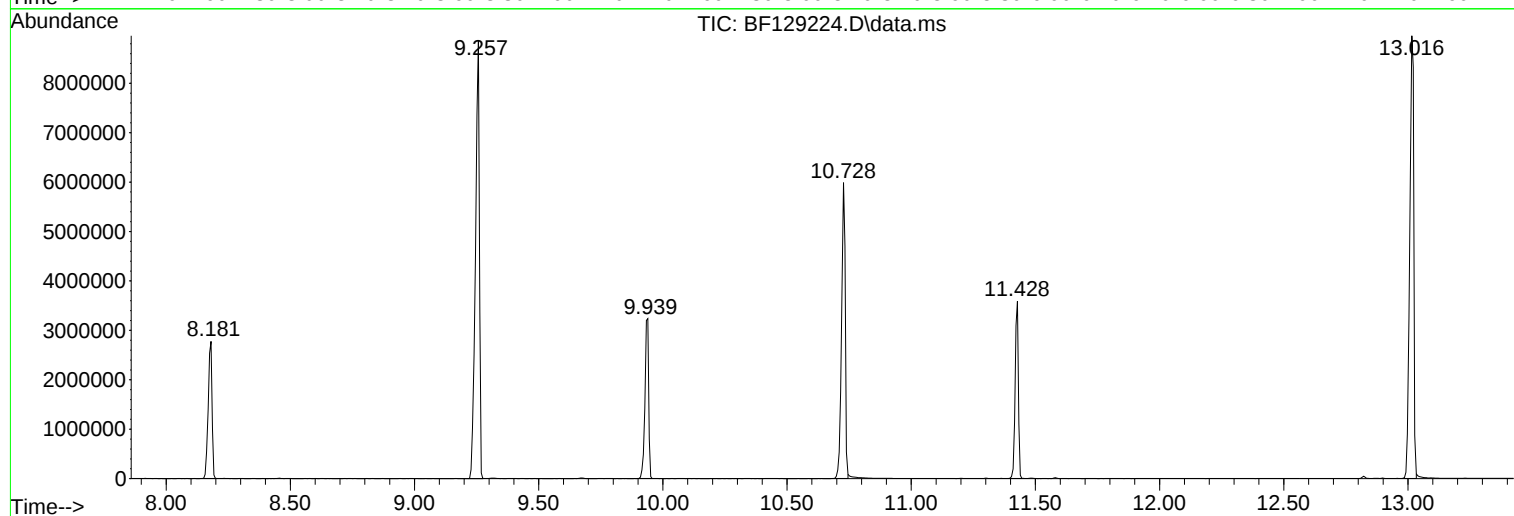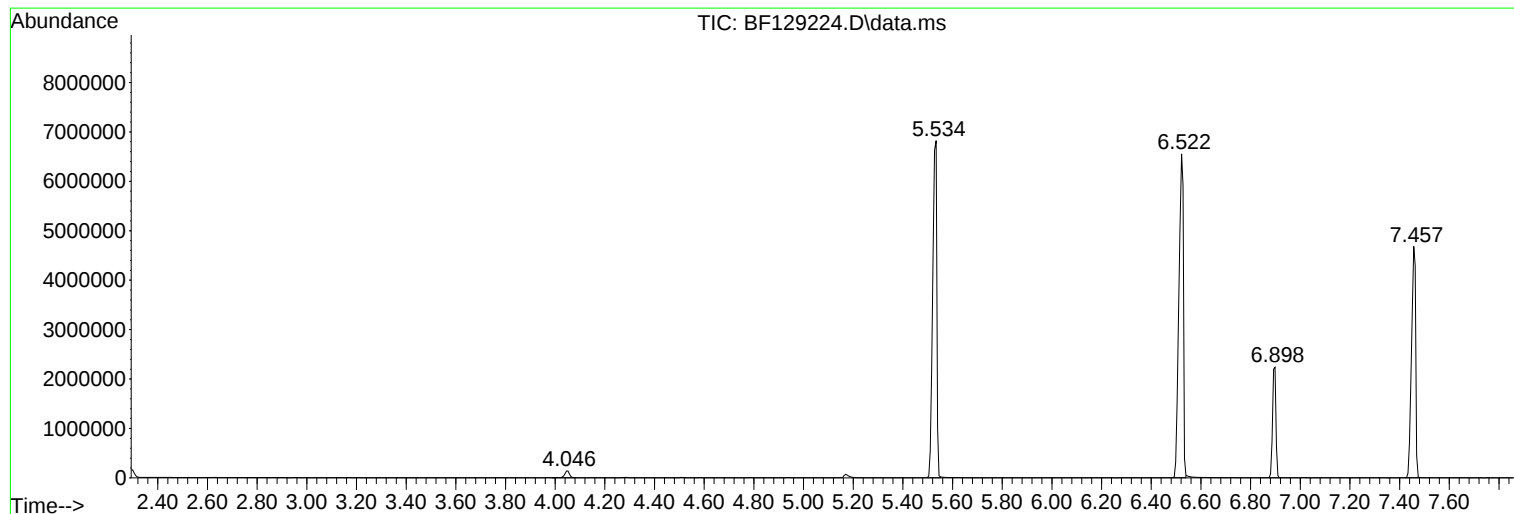

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071422\
Data File : BF129224.D
Acq On : 14 Jul 2022 17:13
Operator : CG\JU
Sample : PB146162BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB146162BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Triphenylphosphine oxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
14.157	5.72 ng	805842	Chrysene-d12	14.069

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Triphenylphosphine oxide	278	C18H15OP	000791-28-6	93
2			(E)-7-Benzylidene-1-azabicyclo[3...	293	C15H19NO3S	1000483-83-4	91
3			Formaldehyde, (triphenylphosphor...	304	C19H17N2P	015990-54-2	64
4			4-Nitro-4'-methyldiphenylsulfone	277	C13H11NO4S	004094-37-5	43
5			Carbazol-1-one, 1,2,3,4-tetrahyd...	277	C18H15NO2	299962-12-2	38

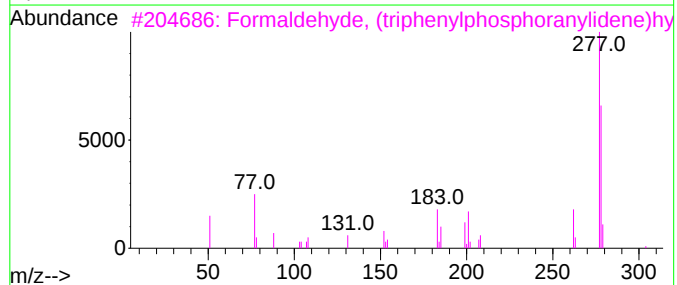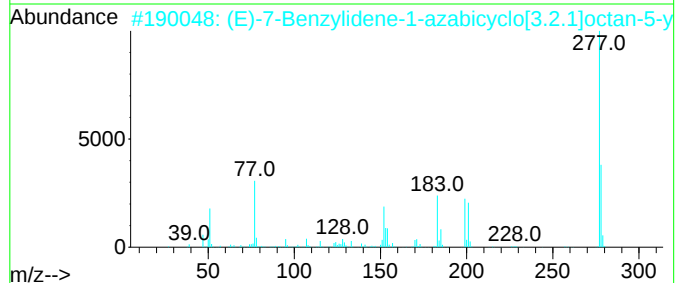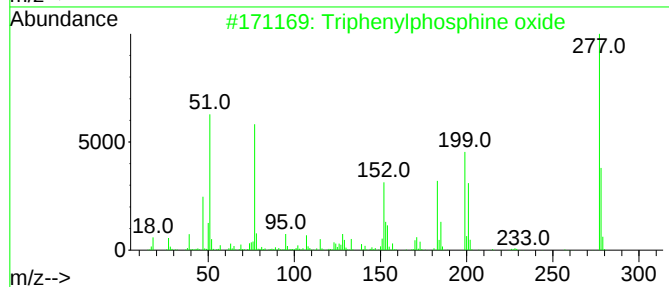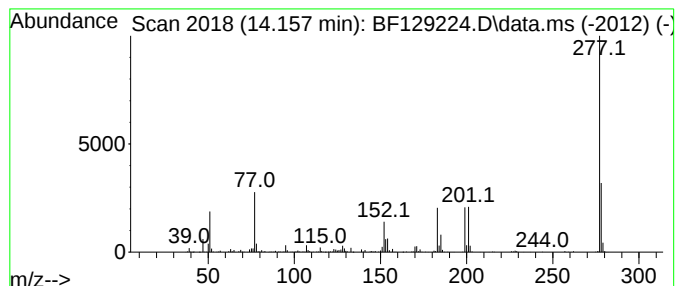

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071422\
Data File : BF129224.D
Acq On : 14 Jul 2022 17:13
Operator : CG\JU
Sample : PB146162BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB146162BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Triphenylphosph...	14.157	5.7	ng	805842	5	14.069	2819200	20.0