
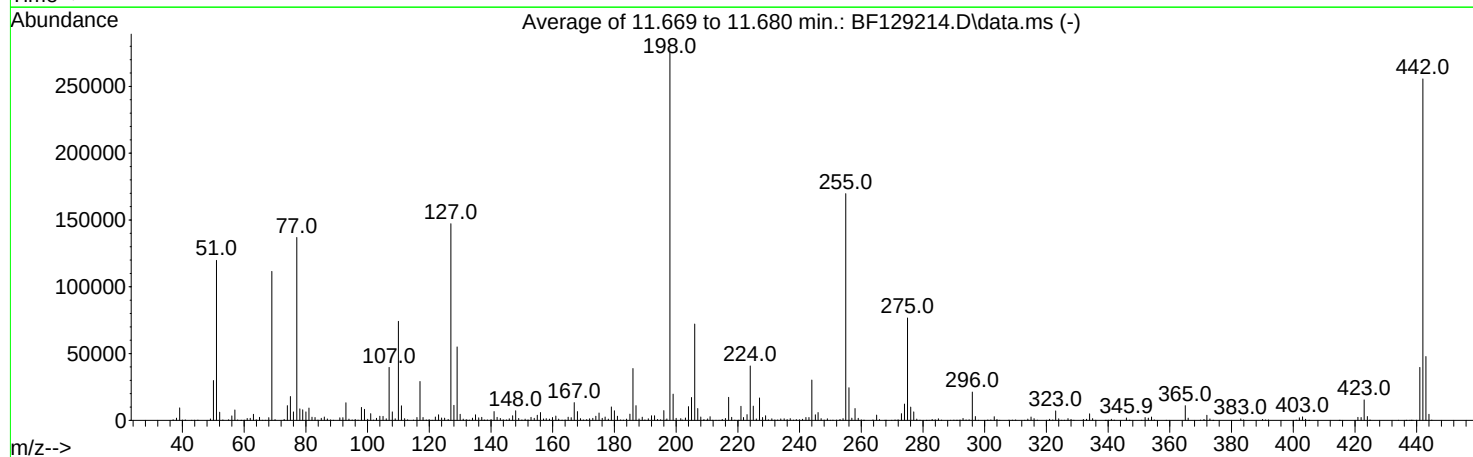


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071422\
Data File : BF129214.D
Acq On : 14 Jul 2022 11:47
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071422.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Jul 14 16:23:13 2022

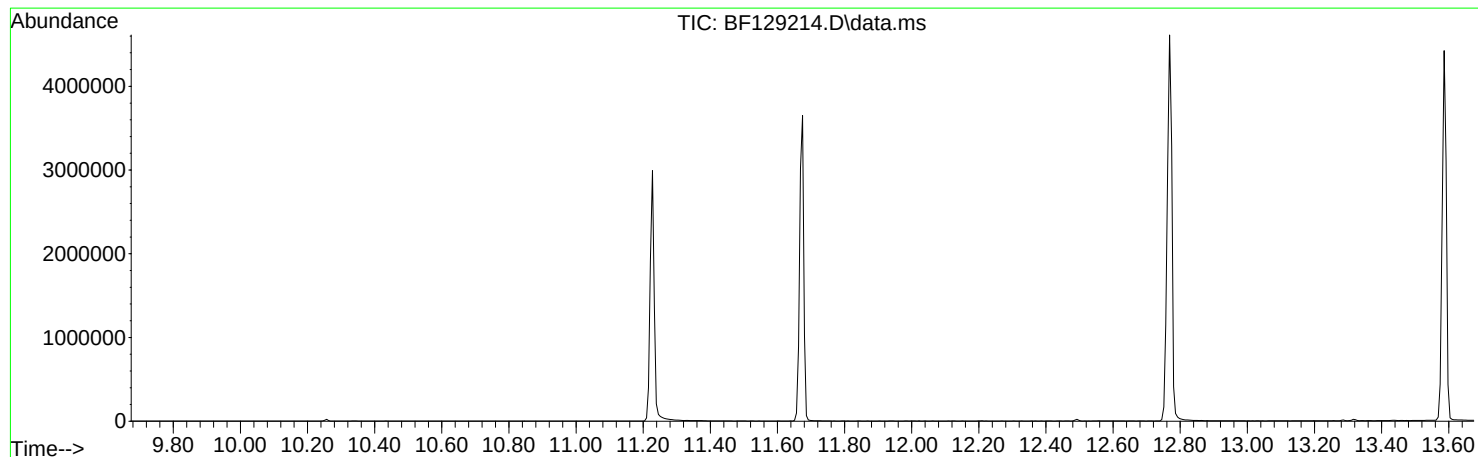




AutoFind: Scans 1595, 1596, 1597; Background Corrected with Scan 1589

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.5	119776	PASS
68	69	0.00	2	1.8	2036	PASS
69	198	0.00	100	40.5	111469	PASS
70	69	0.00	2	0.6	656	PASS
127	198	10	80	53.4	147160	PASS
197	198	0.00	2	0.4	1059	PASS
198	198	100	100	100.0	275360	PASS
199	198	5	9	7.1	19608	PASS
275	198	10	60	27.8	76637	PASS
365	198	1	100	4.0	11059	PASS
441	198	0.01	100	14.4	39635	PASS
442	442	50	100	100.0	255637	PASS
443	442	15	24	18.7	47755	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071422\
Data File : BF129214.D
Acq On : 14 Jul 2022 11:47
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 14 18:57:55 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 14 16:23:13 2022
Response via : Initial Calibration

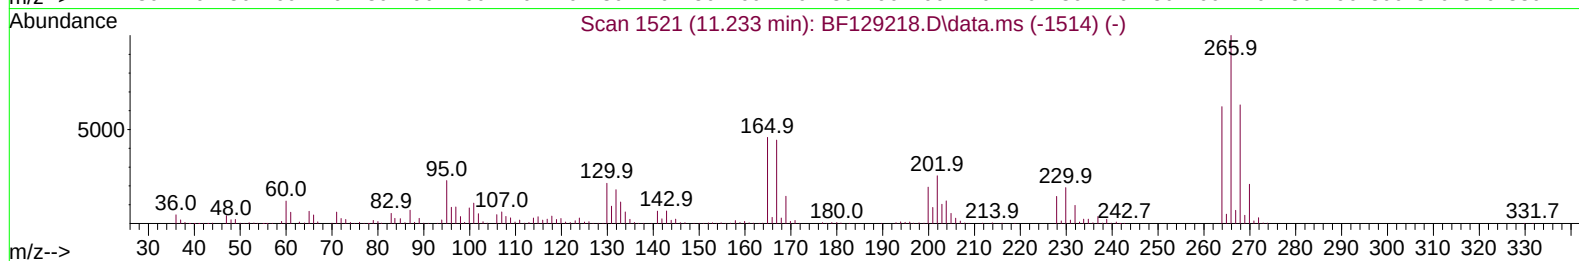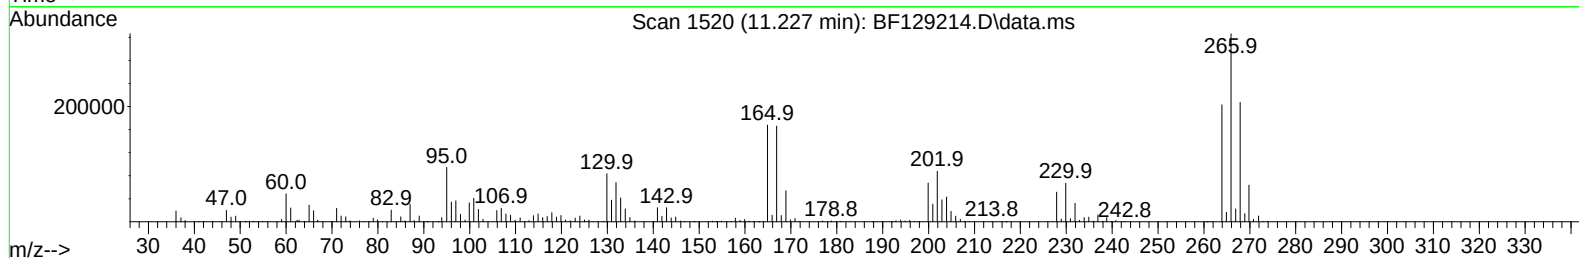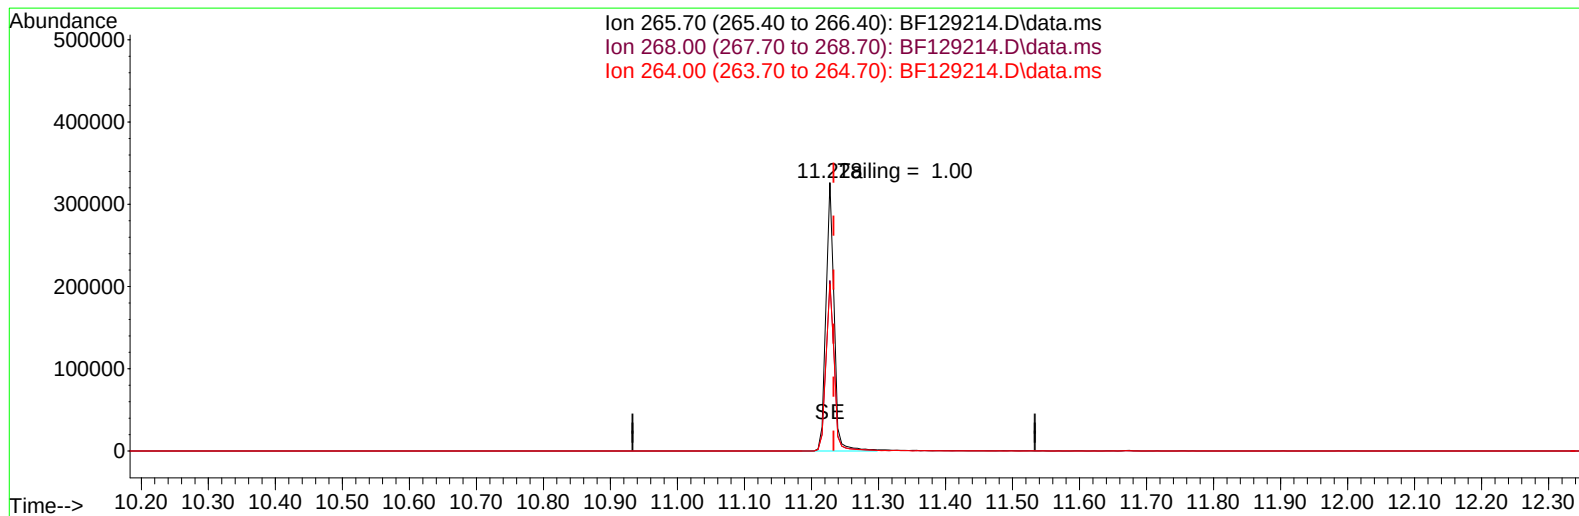

TIC: BF129214.D\data.ms

(70) Pentachlorophenol (C)

11.227min (-0.006) 678770.33 ng




response 279151

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	63.52
264.00	61.80	62.27
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071422\
Data File : BF129214.D
Acq On : 14 Jul 2022 11:47
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 14 18:57:55 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 14 16:23:13 2022
Response via : Initial Calibration

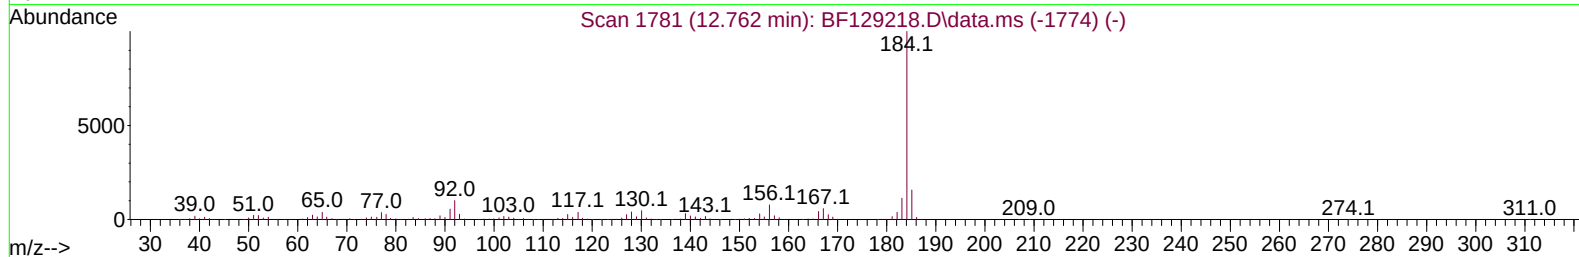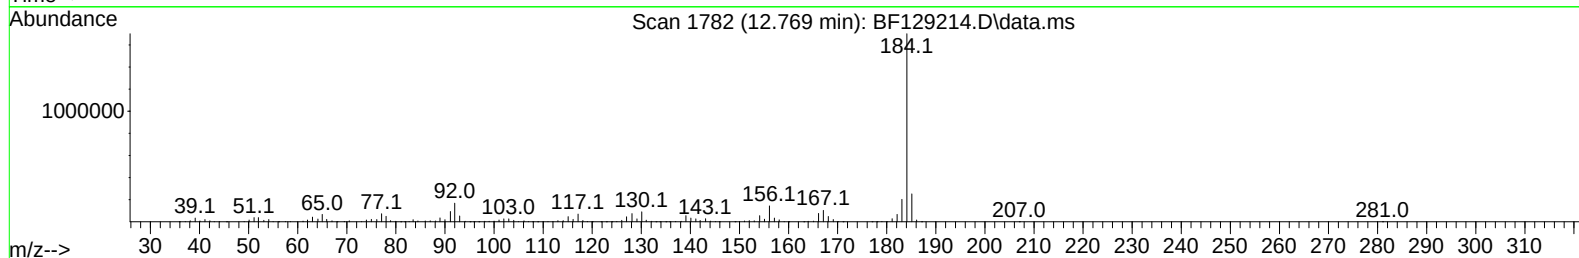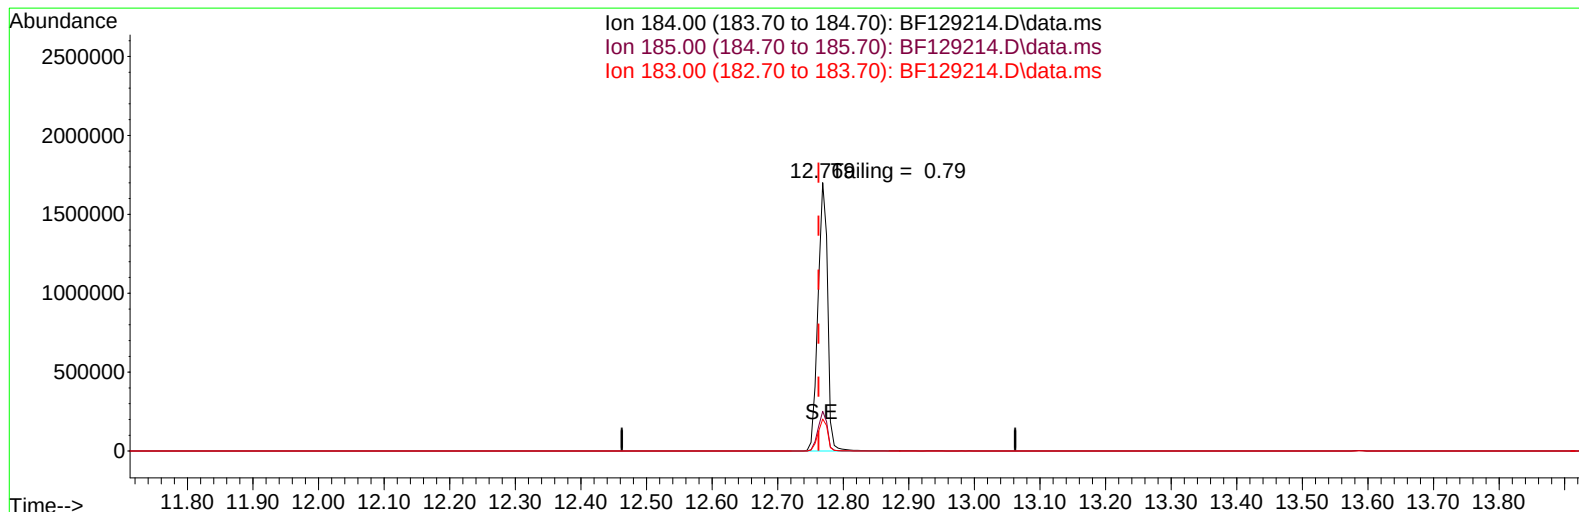

TIC: BF129214.D\data.ms

(77) Benzidine

12.769min (+ 0.006) 969767.31 ng

response 1747468

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.79
183.00	11.60	11.97
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/14/2022	BNA_F	<u>BF129214.D</u>
Compound Name	Response	Retention Time
DDT	679420	13.58
DDD	1482	13.28
DDE	95	12.95
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
1577	680997	0.23

Instrument :
BNA_F
ClientSampleId :
DFTPP