
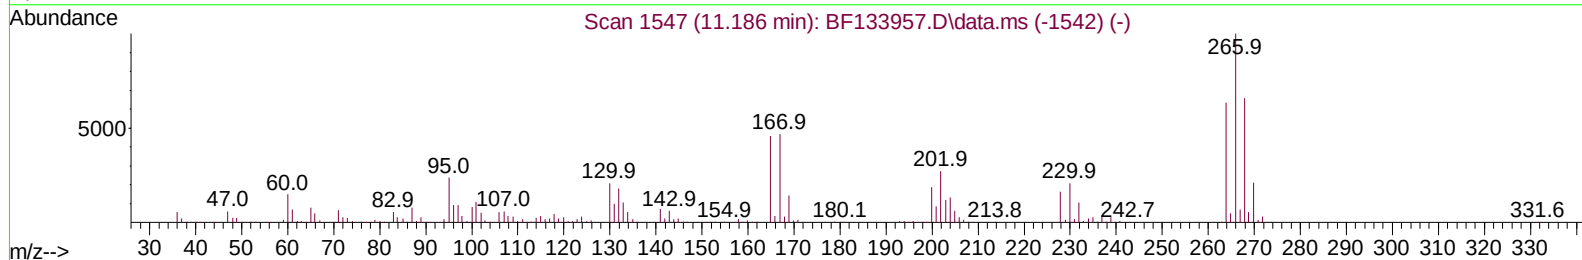
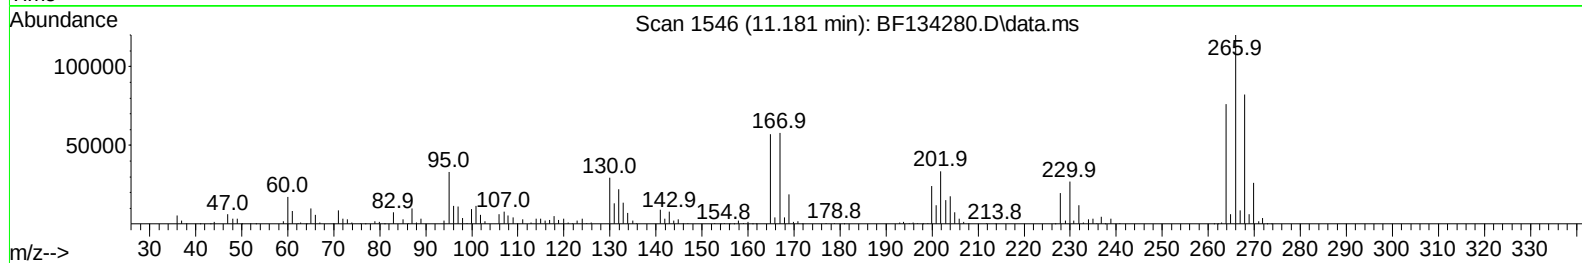


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071423\
Data File : BF134280.D
Acq On : 14 Jul 2023 08:47
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 15 01:29:54 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 14 22:51:27 2023
Response via : Initial Calibration

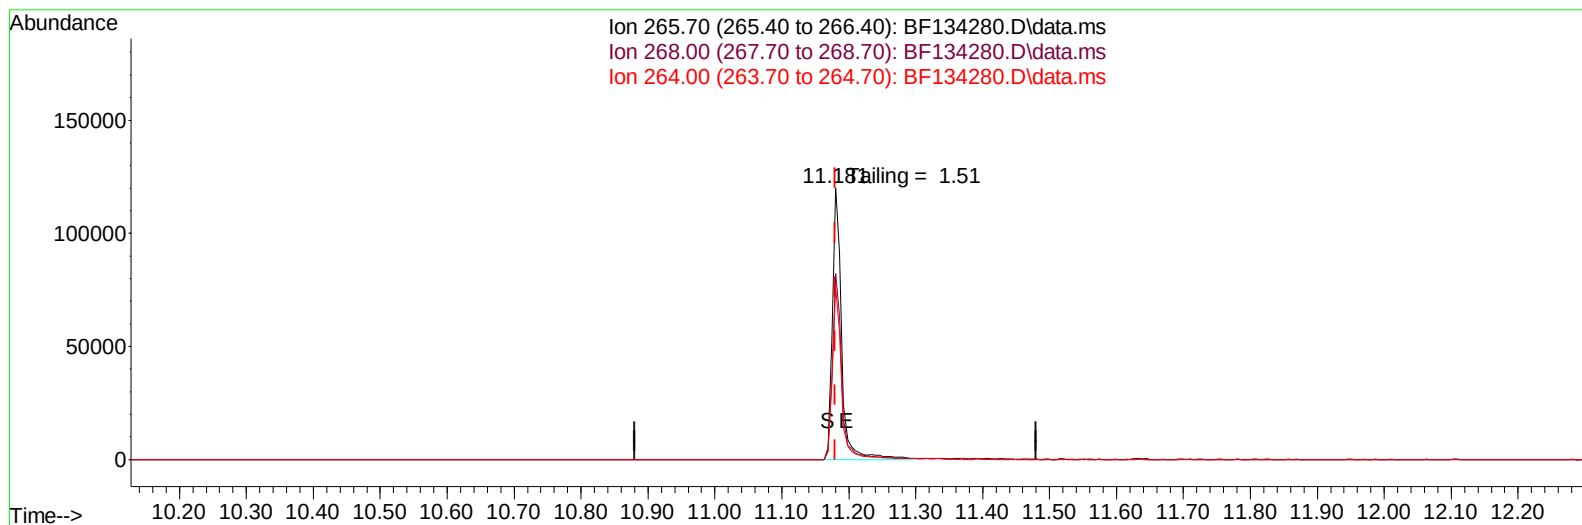

TIC: BF134280.D\data.ms

(70) Pentachlorophenol (C)




11.181min (+ 0.000) 31604.45 ng

response 117291

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.80	68.46
264.00	63.30	63.48
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071423\  
Data File : BF134280.D  
Acq On    : 14 Jul 2023  08:47  
Operator  : CG\JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Quant Time: Jul 15 01:29:54 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 14 22:51:27 2023
Response via : Initial Calibration

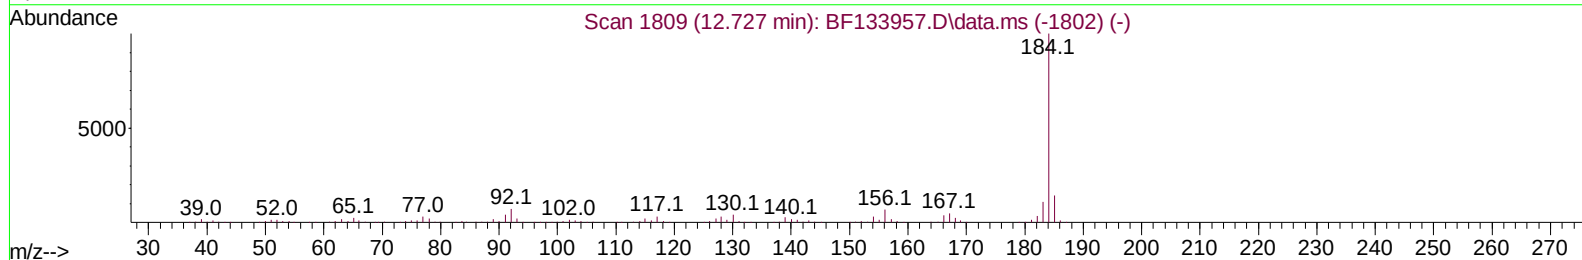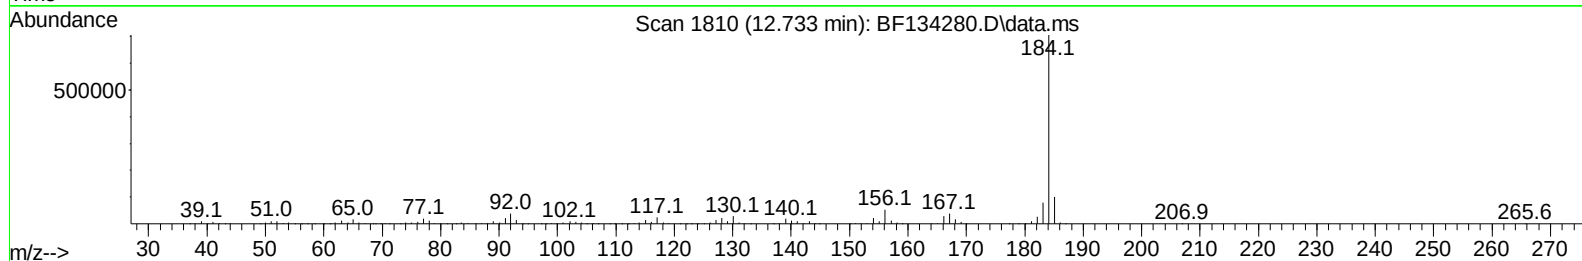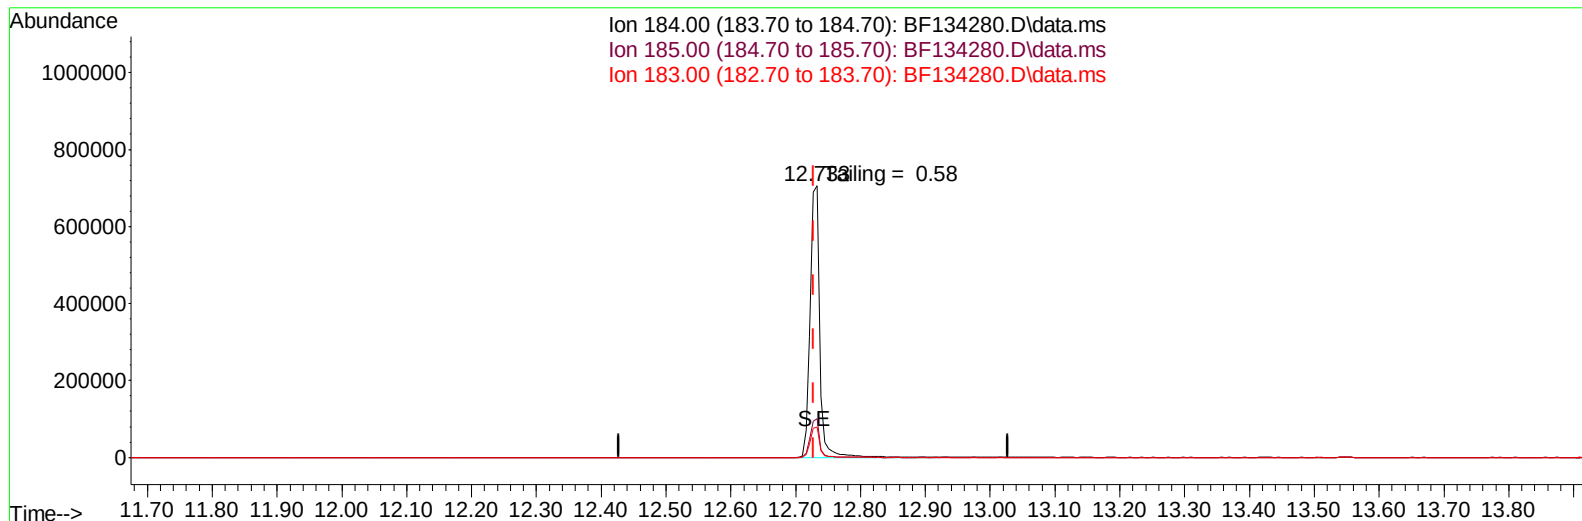

TIC: BF134280.D\data.ms

(77) Benzidine

12.733min (+ 0.006) 270392.79 ng

response **739889**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.25
183.00	11.00	11.27
0.00	0.00	0.00