
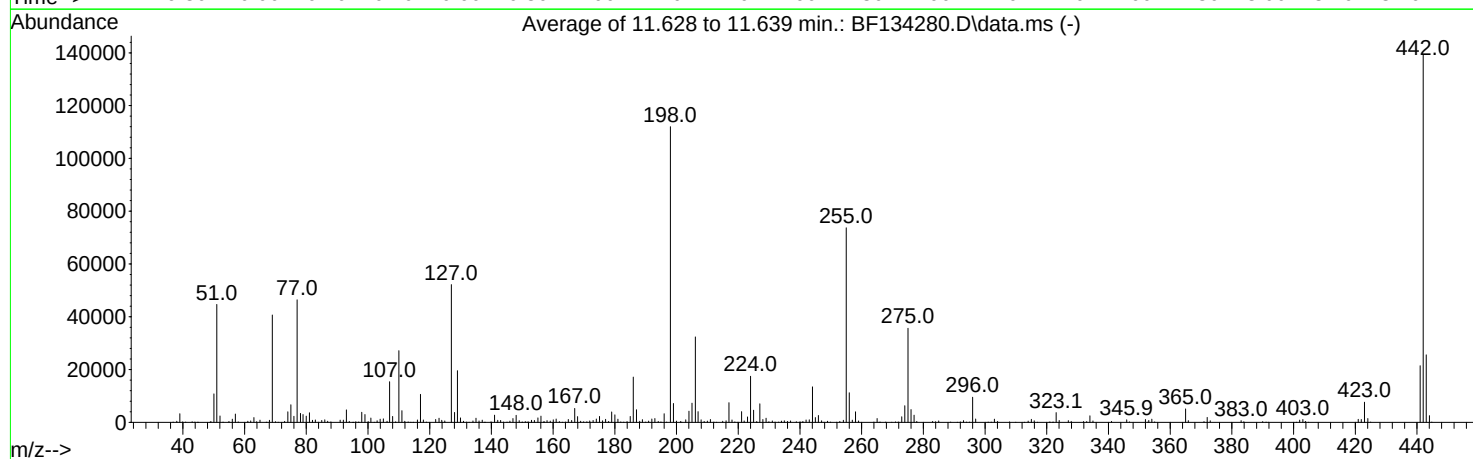


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071423\
Data File : BF134280.D
Acq On : 14 Jul 2023 08:47
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Jul 14 22:51:27 2023

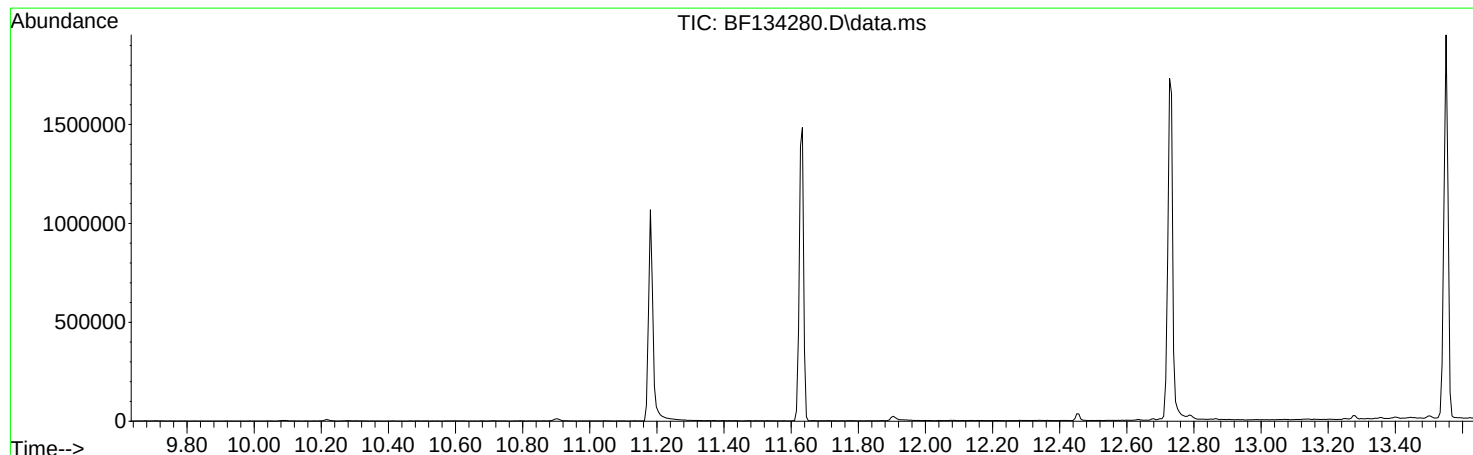

AutoFind: Scans 1622, 1623, 1624; Background Corrected with Scan 1617

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.9	44665	PASS
68	69	0.00	2	2.0	813	PASS
69	198	0.00	100	36.3	40690	PASS
70	69	0.00	2	0.6	246	PASS
127	198	10	80	46.6	52210	PASS
197	198	0.00	2	0.1	127	PASS
198	198	100	100	100.0	112035	PASS
199	198	5	9	6.4	7131	PASS
275	198	10	60	31.8	35623	PASS
365	198	1	100	4.5	5069	PASS
441	198	0.01	100	19.2	21492	PASS
442	442	50	100	100.0	139368	PASS
443	442	15	24	18.4	25608	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
7/14/2023	BNA_F	<u>BF134280.D</u>
Compound Name	Response	Retention Time
DDT	319480	13.551
DDD	4777	13.274
DDE	174	12.91
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4951	324431	1.53

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071423\
Data File : BF134280.D
Acq On : 14 Jul 2023 08:47
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 15 01:29:54 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 14 22:51:27 2023
Response via : Initial Calibration

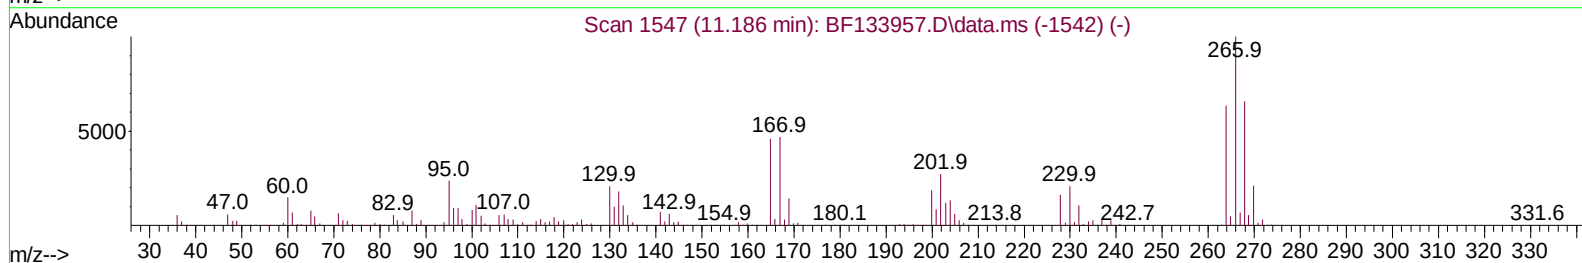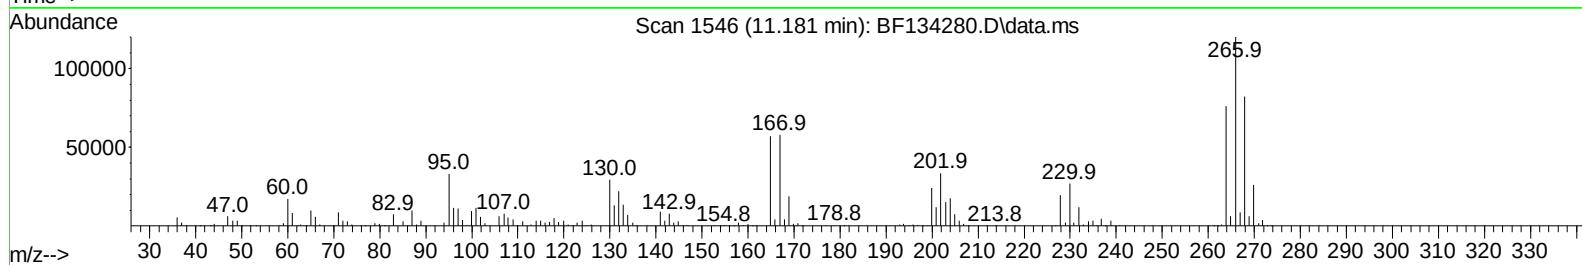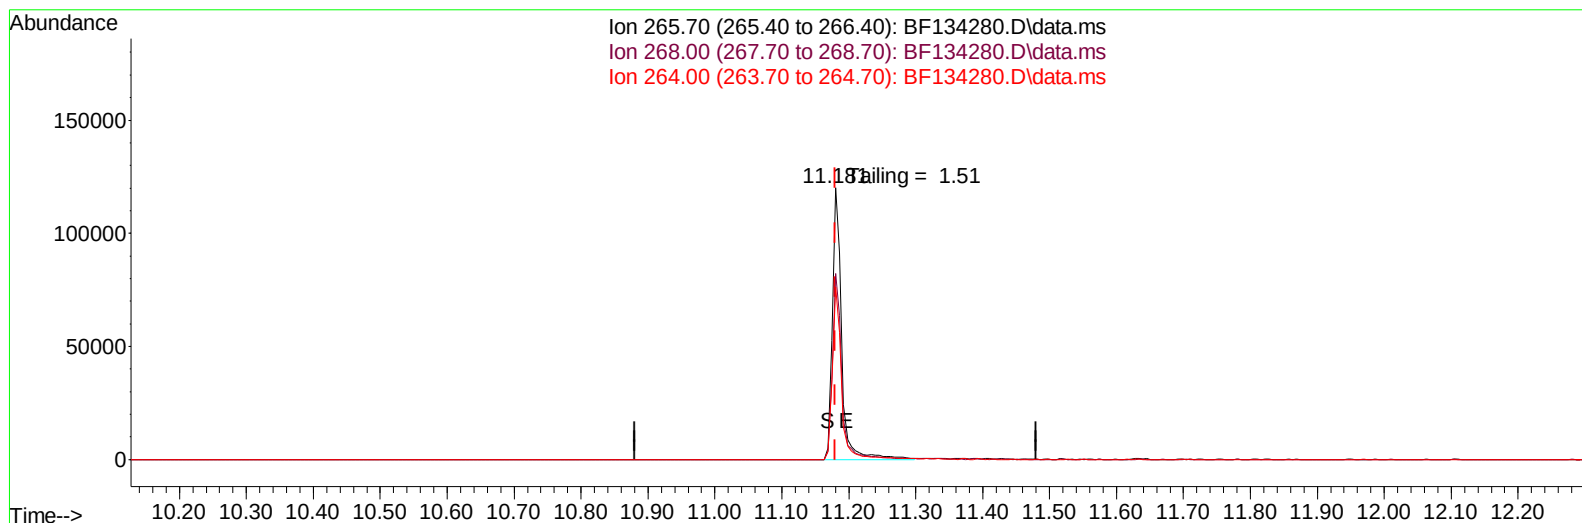

TIC: BF134280.D\data.ms

(70) Pentachlorophenol (C)

11.181min (+ 0.000) 31604.45 ng

response 117291

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.80	68.46
264.00	63.30	63.48
0.00	0.00	0.00

