


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071423\
Data File : BF134291.D
Acq On : 14 Jul 2023 15:21
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Jul 14 22:51:27 2023

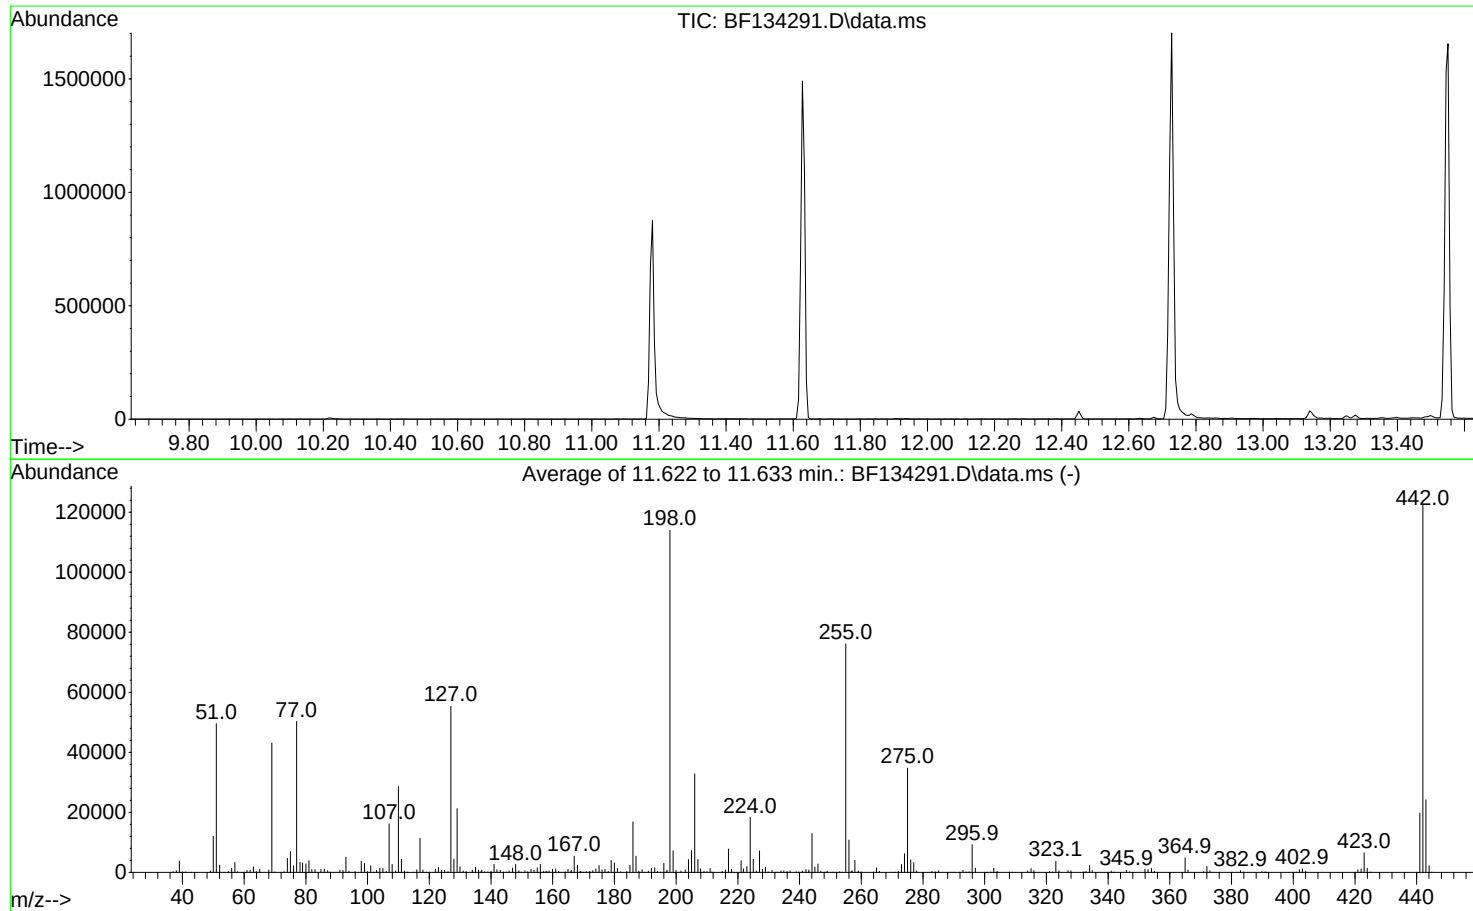

AutoFind: Scans 1621, 1622, 1623; Background Corrected with Scan 1616

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.5	49509	PASS
68	69	0.00	2	1.9	823	PASS
69	198	0.00	100	37.8	43069	PASS
70	69	0.00	2	0.4	170	PASS
127	198	10	80	48.6	55341	PASS
197	198	0.00	2	0.7	743	PASS
198	198	100	100	100.0	113941	PASS
199	198	5	9	6.3	7176	PASS
275	198	10	60	30.4	34691	PASS
365	198	1	100	4.2	4814	PASS
441	198	0.01	100	17.3	19764	PASS
442	442	50	100	100.0	122563	PASS
443	442	15	24	19.7	24132	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
7/14/2023	BNA_F	<u>BF134291.D</u>
Compound Name	Response	Retention Time
DDT	302096	13.551
DDD	5980	13.274
DDE	847	12.91
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6827	308923	2.21

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071423\
Data File : BF134291.D
Acq On : 14 Jul 2023 15:21
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 15 01:31:24 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 14 22:51:27 2023
Response via : Initial Calibration

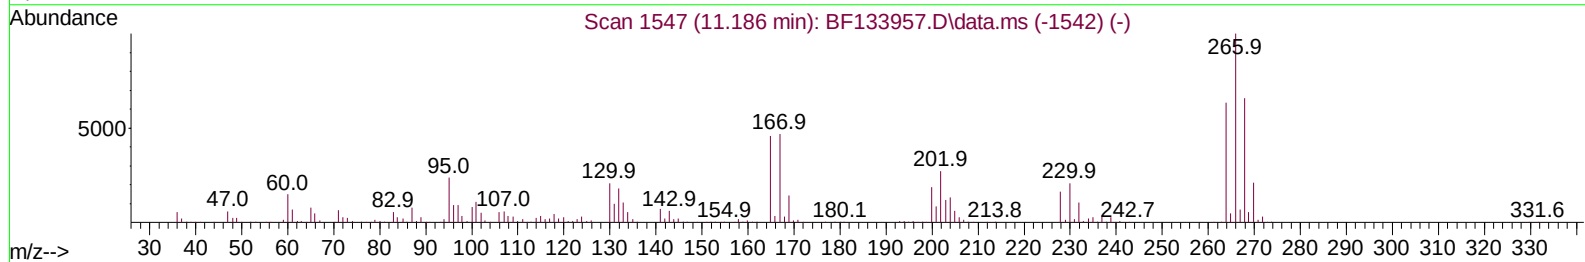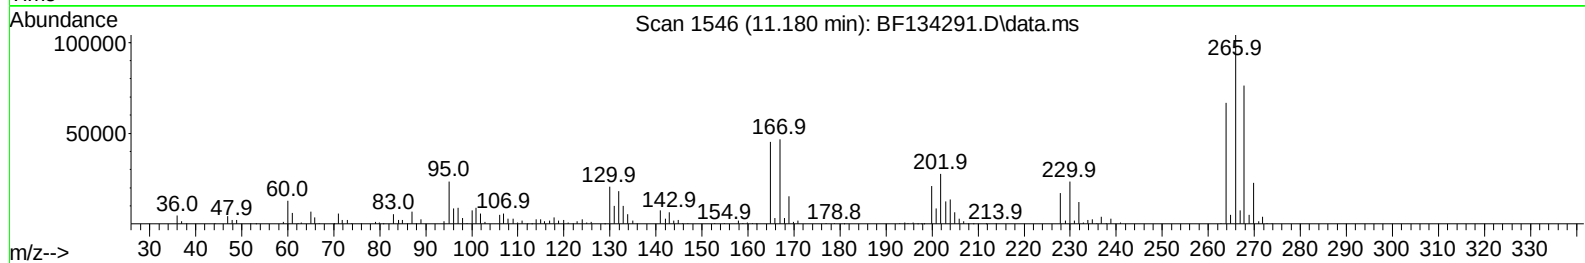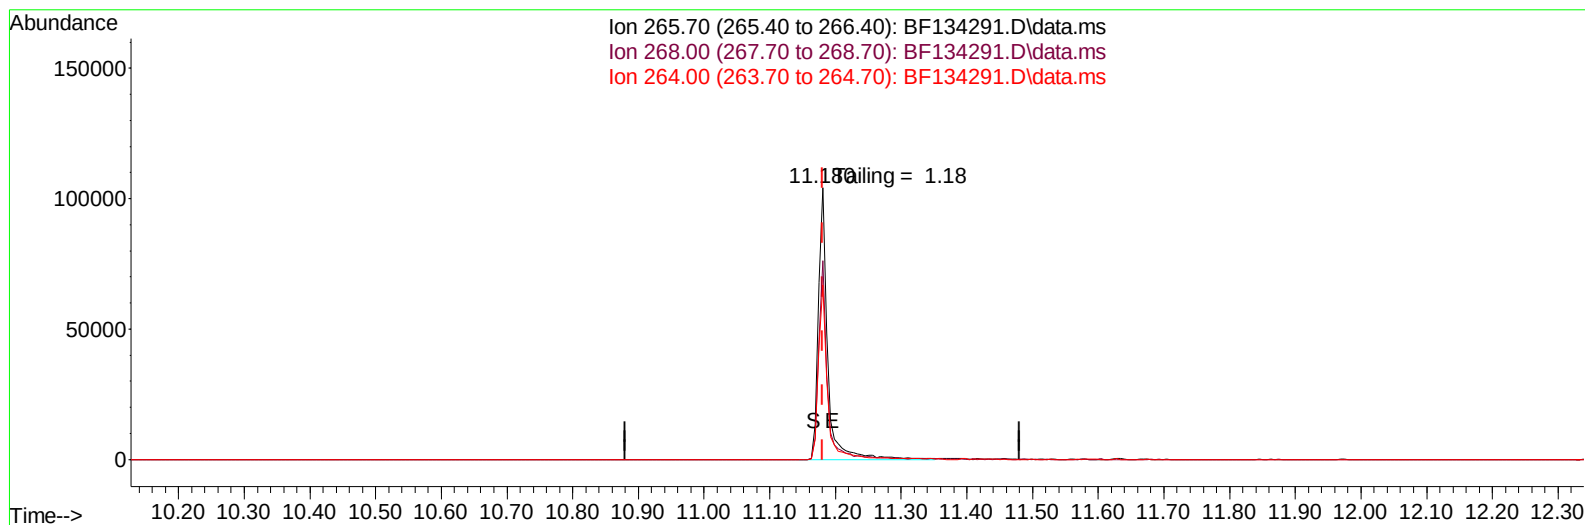

TIC: BF134291.D\data.ms

(70) Pentachlorophenol (C)

11.180min (+ 0.000) 57890.57 ng




response 103516

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.80	73.22
264.00	63.30	64.17
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071423\
 Data File : BF134291.D
 Acq On : 14 Jul 2023 15:21
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Jul 15 01:31:24 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 14 22:51:27 2023
 Response via : Initial Calibration

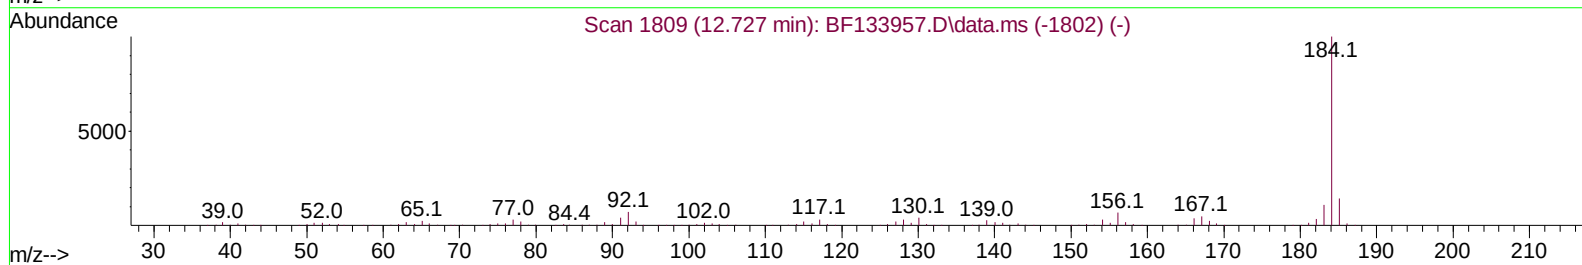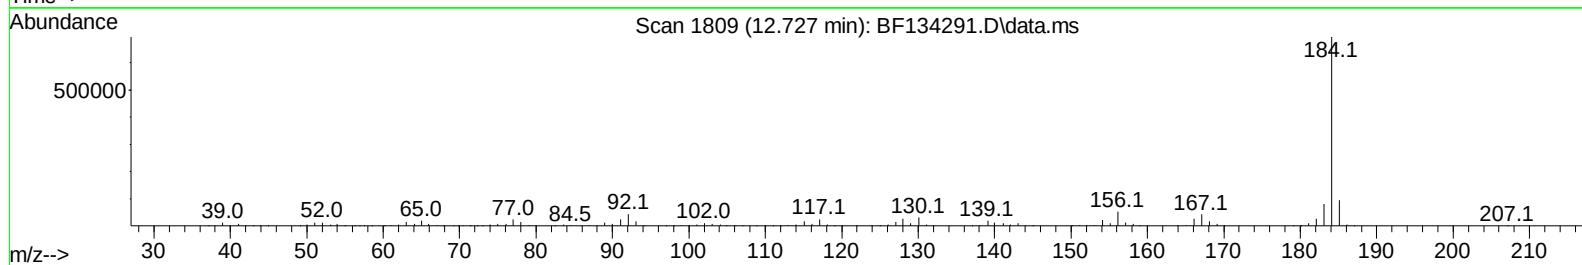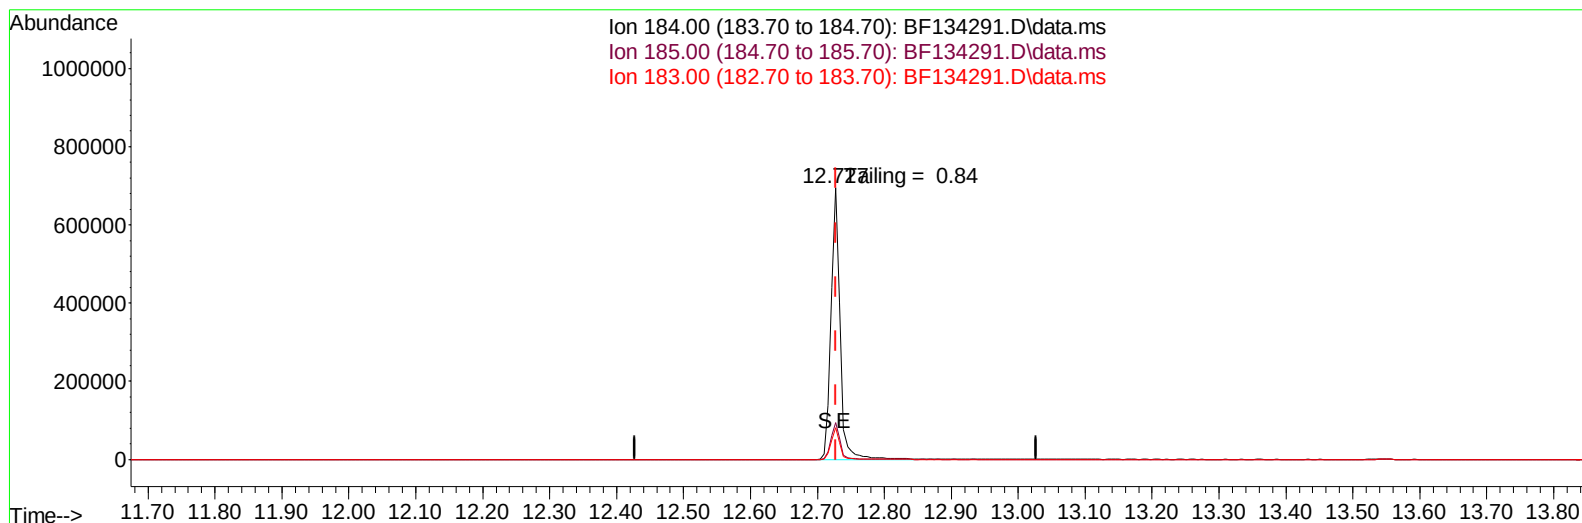

TIC: BF134291.D\data.ms

(77) Benzidine

12.727min (+ 0.000) 156533.88 ng

response 666707

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	13.65
183.00	11.00	11.59
0.00	0.00	0.00