
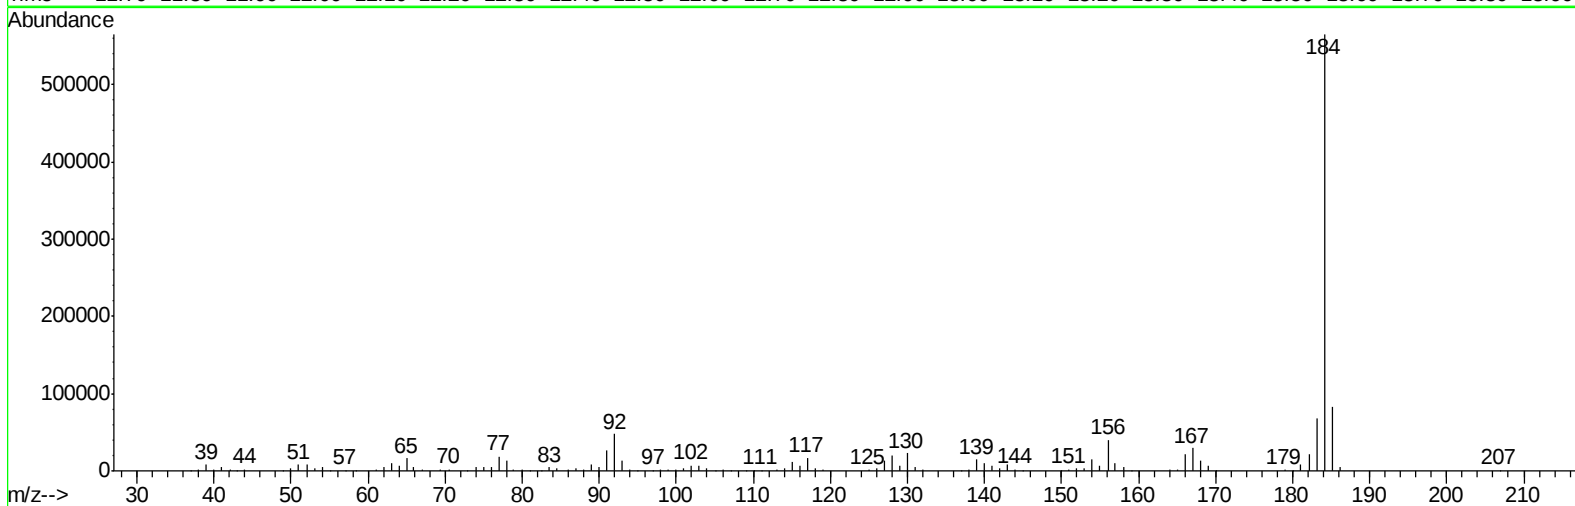


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF071519\
Data File : BF115550.D
Acq On : 15 Jul 2019 7:31
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 16 01:33:15 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF071219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 12 14:03:52 2019
Response via : Initial Calibration

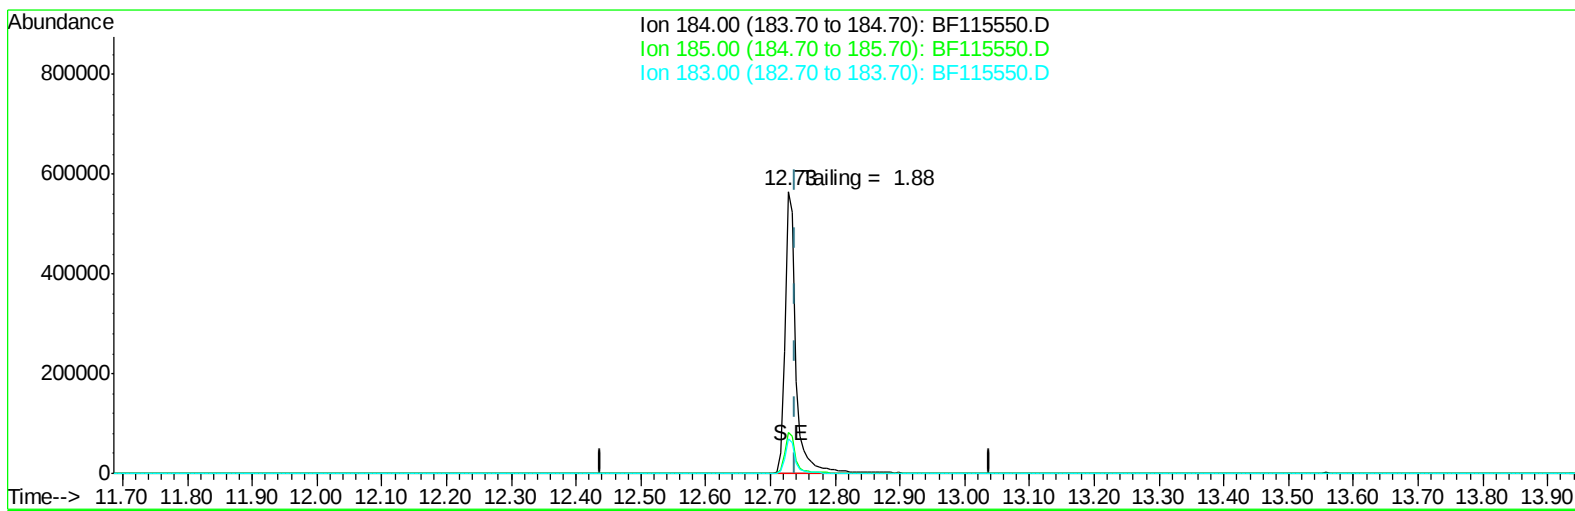

TIC: BF115550.D

(77) Benzidine



12.727min (-0.012) 0.00ng

response 655285

Ion	Exp%	Act%
184.00	100	100
185.00	15.00	14.73
183.00	11.60	12.12
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF071519\
Data File : BF115550.D
Acq On : 15 Jul 2019 7:31
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 16 01:33:15 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF071219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 12 14:03:52 2019
Response via : Initial Calibration

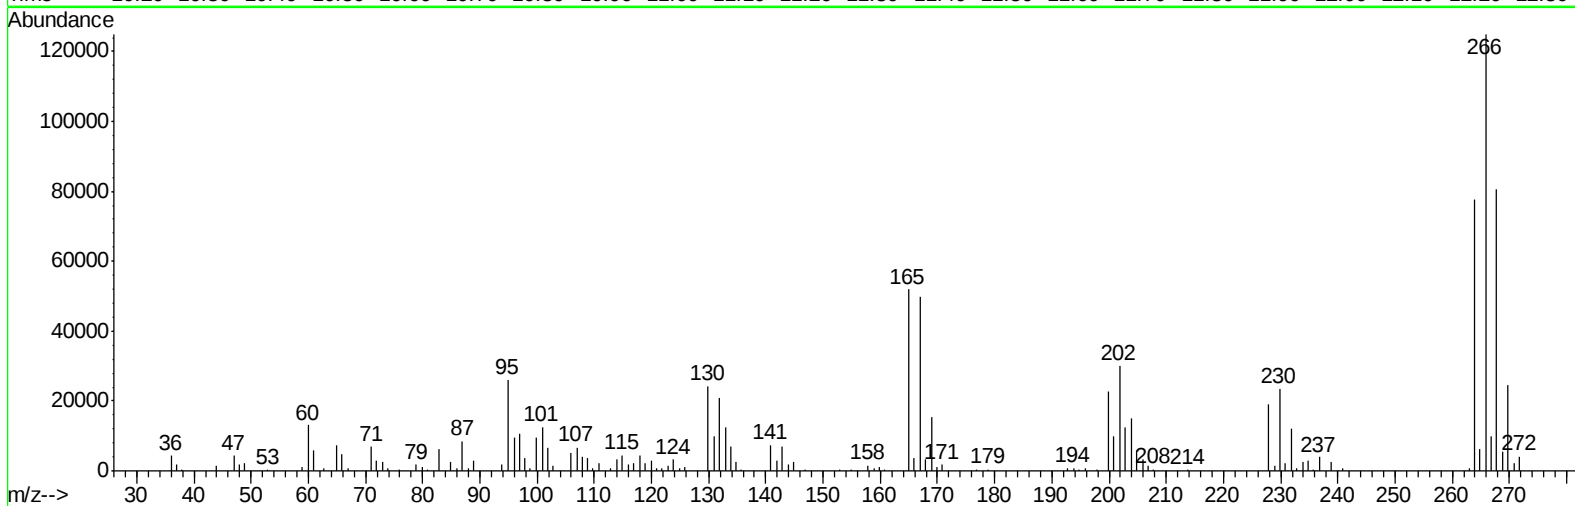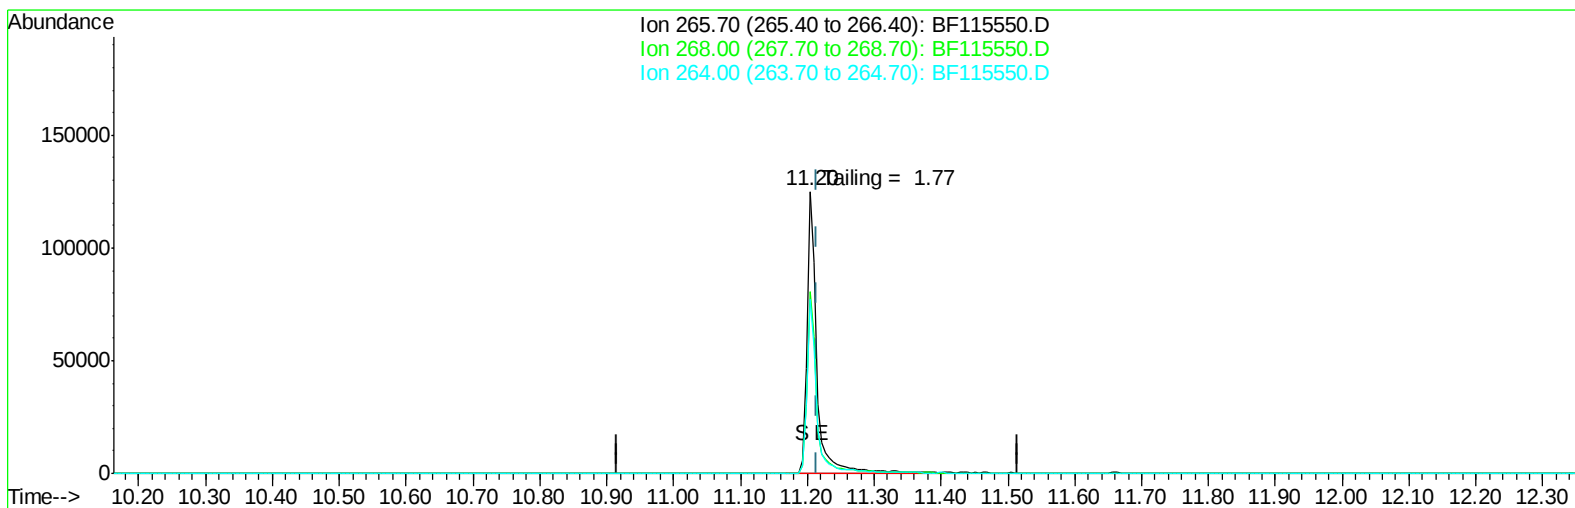

TIC: BF115550.D

(70) Pentachlorophenol (C)

11.204min (-0.012) 32006.12ng

response 129523

Ion	Exp%	Act%
265.70	100	100
268.00	64.50	64.60
264.00	63.30	62.04
0.00	0.00	0.00