

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071519\
 Data File : BF115569.D
 Acq On : 15 Jul 2019 21:00
 Operator : HP/JU
 Sample : PB121261TB
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB121261TB

Quant Time: Jul 16 04:02:54 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF071219.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 12 14:03:52 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.88	152	190722	20.00	ng	0.00
21) Naphthalene-d8	8.16	136	737761	20.00	ng	-0.01
39) Acenaphthene-d10	9.92	164	379126	20.00	ng	-0.01
64) Phenanthrene-d10	11.40	188	757952	20.00	ng	-0.01
76) Chrysene-d12	14.03	240	541443	20.00	ng	-0.02
87) Perylene-d12	15.50	264	471337	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.52	112	1367334	117.27	ng	0.01
7) Phenol-d6	6.51	99	1809499	122.30	ng	0.00
23) Nitrobenzene-d5	7.44	82	1126530	88.79	ng	-0.01
42) 2,4,6-Tribromophenol	10.70	330	542137	122.51	ng	-0.01
45) 2-Fluorobiphenyl	9.24	172	2121112	97.92	ng	-0.01
79) Terphenyl-d14	12.99	244	2358674	80.38	ng	0.00


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071519\
Data File : BF115569.D
Acq On : 15 Jul 2019 21:00
Operator : HP/JU
Sample : PB121261TB
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB121261TB

Quant Time: Jul 16 04:02:54 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF071219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 12 14:03:52 2019
Response via : Initial Calibration

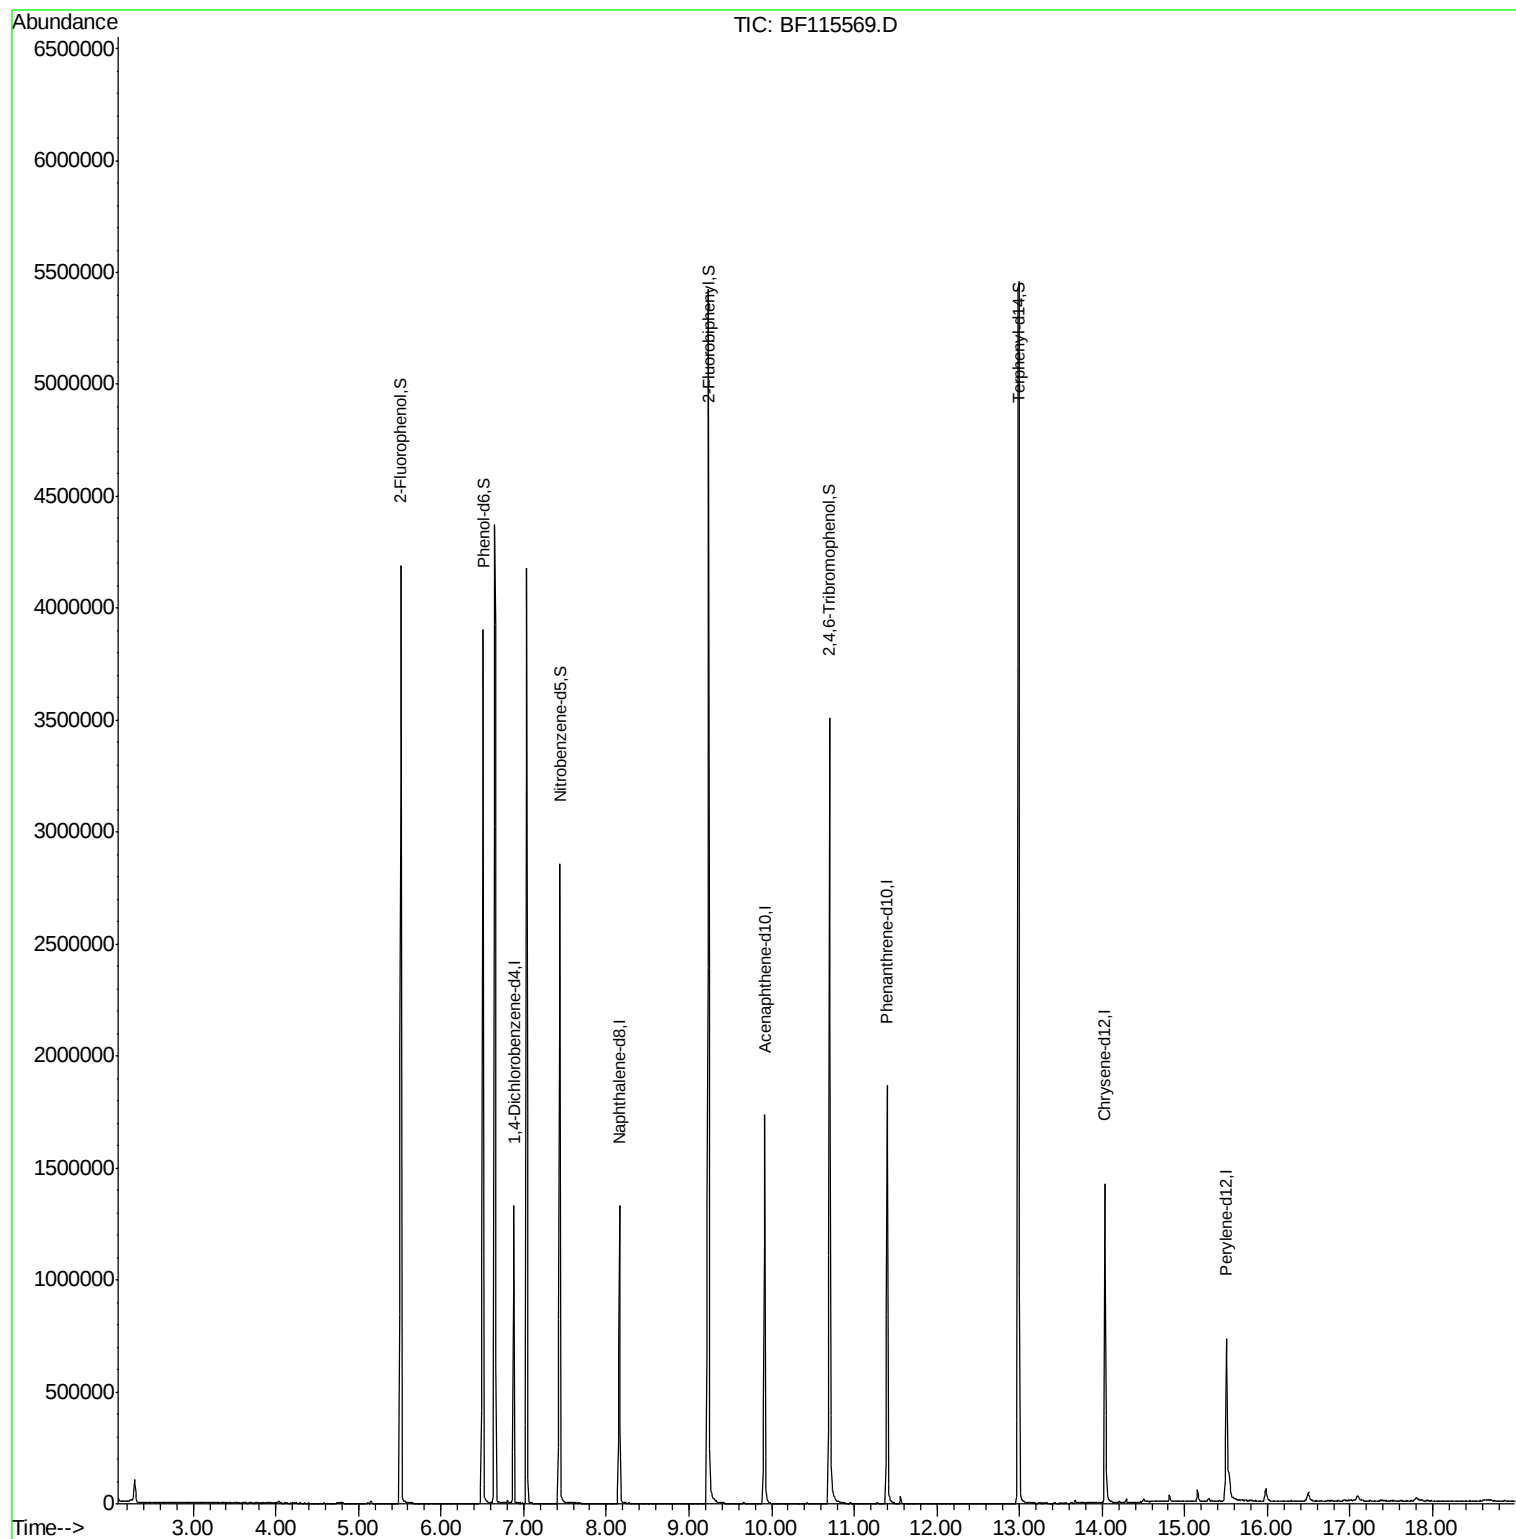

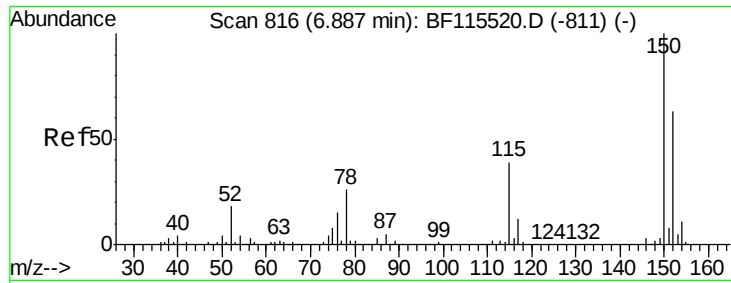

#1

1,4-Dichlorobenzene-d4

Concen: 20.000 ng

RT: 6.88 min Scan# 815

Delta R.T. -0.01 min

Lab File: BF115569.D

Acq: 15 Jul 2019 21:00

Instrument :

BNA_F

ClientSampleId :

PB121261TB


Tgt Ion:152 Resp: 190722

Ion Ratio Lower Upper

152 100

150 154.3 129.7 194.5

115 59.5 48.2 72.4



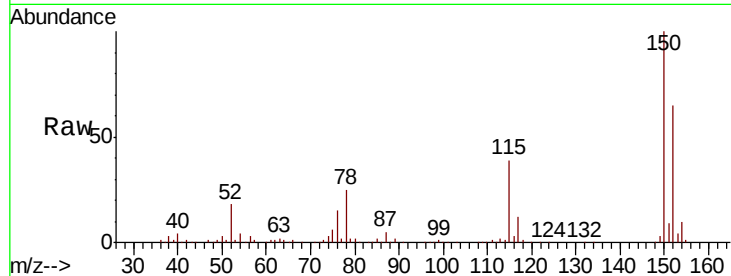


Abundance

Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

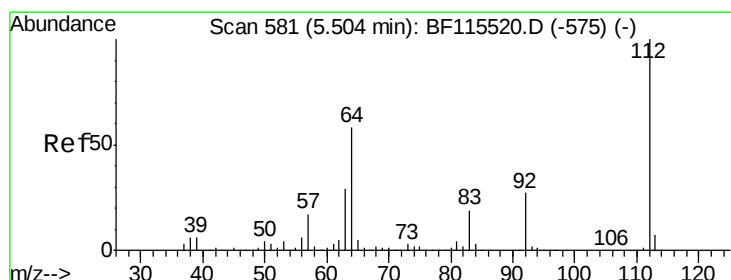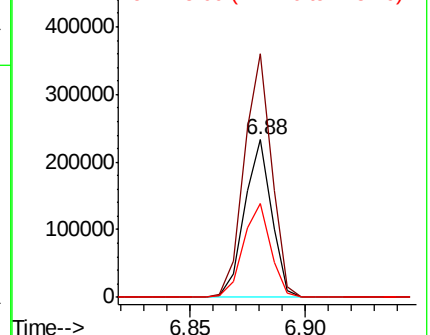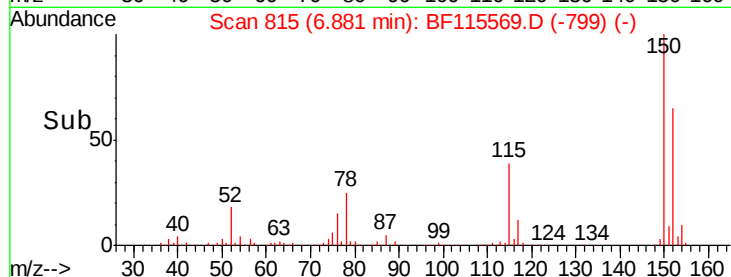

#5

2-Fluorophenol

Concen: 117.268 ng

RT: 5.52 min Scan# 583

Delta R.T. 0.01 min

Lab File: BF115569.D

Acq: 15 Jul 2019 21:00


Tgt Ion:112 Resp: 1367334

Ion Ratio Lower Upper

112 100

64 57.7 46.8 70.2

63 29.5 24.1 36.1


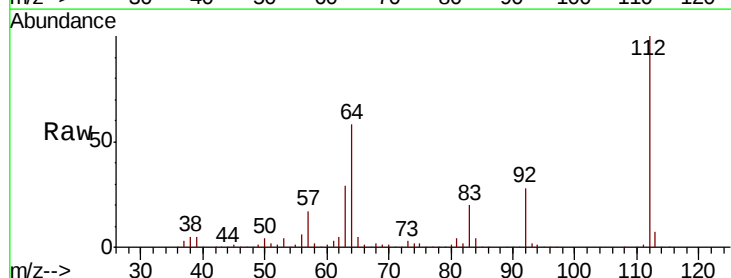



Abundance

Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF1

Ion 63.00 (62.70 to 63.70): BF1

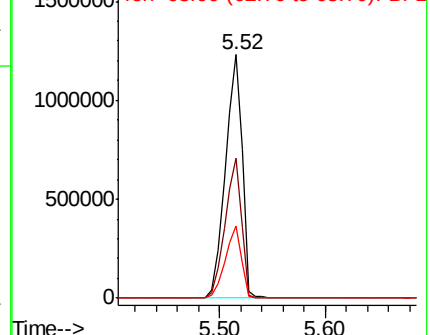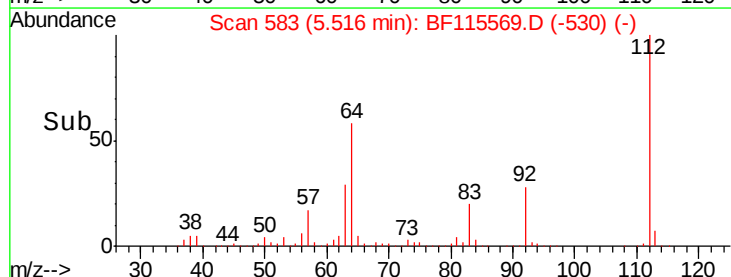

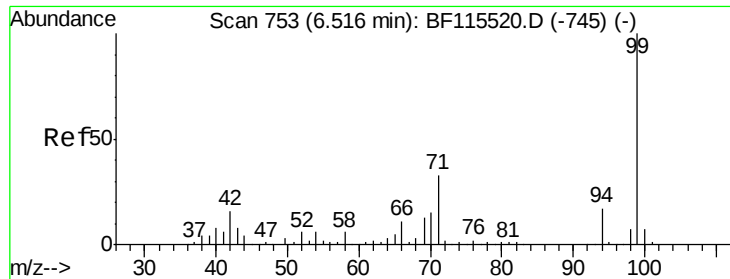

#7

Phenol-d6

Concen: 122.304 ng

RT: 6.51 min Scan# 752

Delta R.T. -0.01 min

Lab File: BF115569.D

Acq: 15 Jul 2019 21:00

Instrument :

BNA_F

ClientSampleId :

PB121261TB


Tgt Ion: 99 Resp: 1809499

Ion Ratio Lower Upper

99 100

42 16.1 13.6 20.4




71 35.1 28.5 42.7

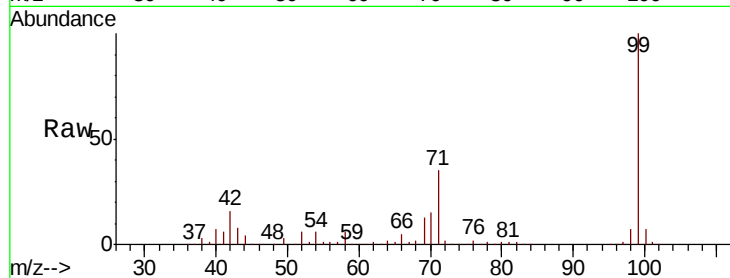

Abundance Ion 99.00 (98.70 to 99.70): BF1

Ion 42.00 (41.70 to 42.70): BF1

Ion 71.00 (70.70 to 71.70): BF1

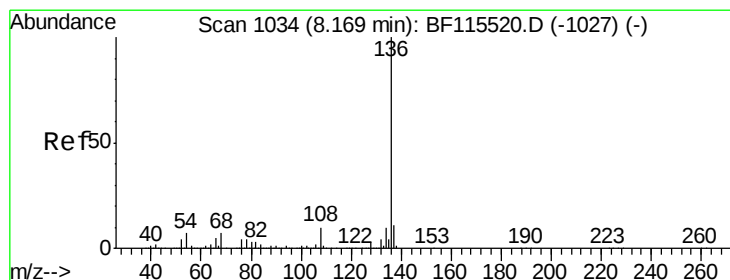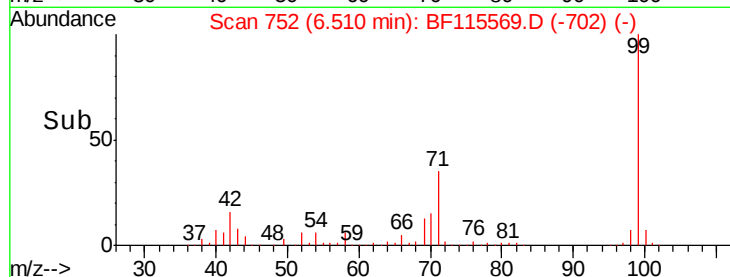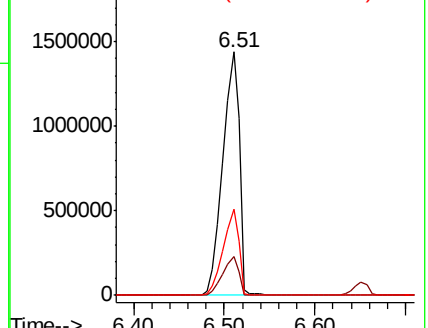

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.16 min Scan# 1032

Delta R.T. -0.01 min

Lab File: BF115569.D

Acq: 15 Jul 2019 21:00

Tgt Ion: 136 Resp: 737761


Ion Ratio Lower Upper

136 100

137 11.3 9.0 13.4

54 6.9 5.6 8.4

68 6.6 5.0 7.6


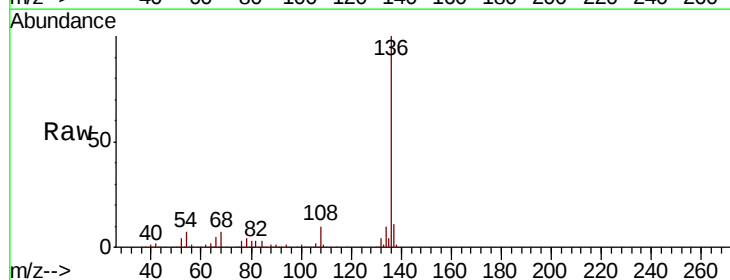



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF1

Ion 68.00 (67.70 to 68.70): BF1

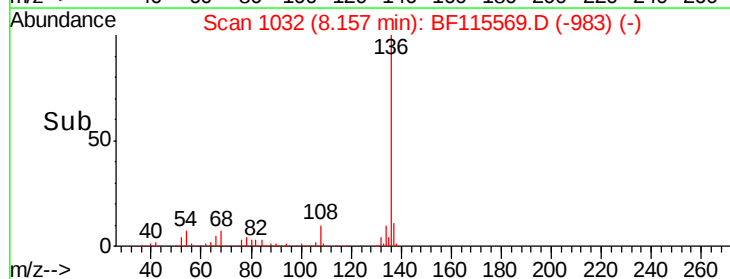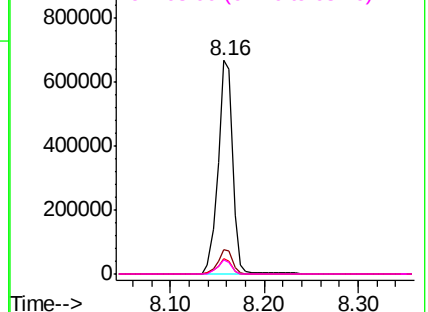


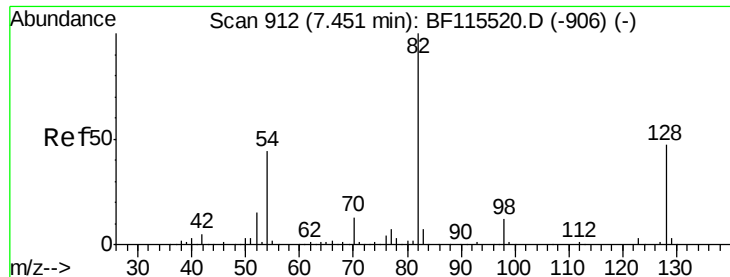




#23
 Nitrobenzene-d5
 Concen: 88.787 ng
 RT: 7.44 min Scan# 910
 Delta R.T. -0.01 min
 Lab File: BF115569.D
 Acq: 15 Jul 2019 21:00

Instrument :
 BNA_F
 ClientSampleId :
 PB121261TB

Tgt Ion: 82 Resp: 1126530
 Ion Ratio Lower Upper
 82 100
 128 47.9 38.6 57.8
 54 44.0 35.6 53.4

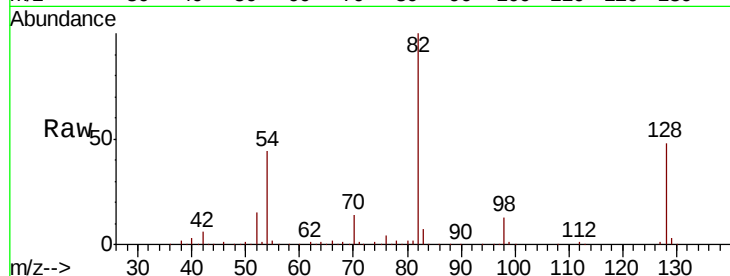


Abundance Ion 82.00 (81.70 to 82.70): BF1
 Ion 128.00 (127.70 to 128.70): E
 Ion 54.00 (53.70 to 54.70): BF1

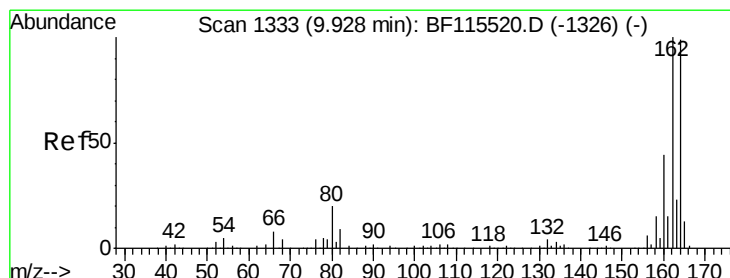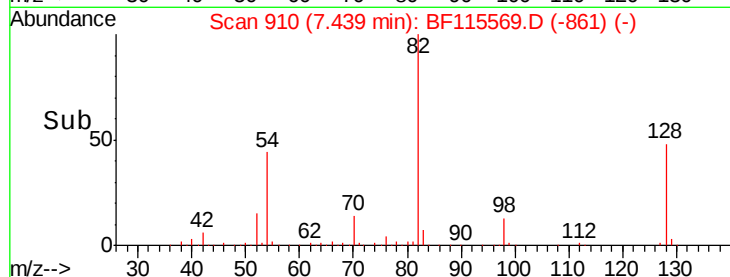
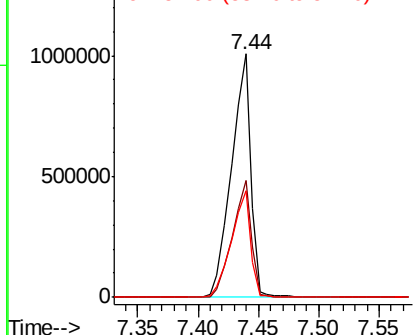



#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 9.92 min Scan# 1331
 Delta R.T. -0.01 min
 Lab File: BF115569.D
 Acq: 15 Jul 2019 21:00

Tgt Ion: 164 Resp: 379126
 Ion Ratio Lower Upper
 164 100
 162 101.3 82.9 124.3
 160 46.0 36.8 55.2

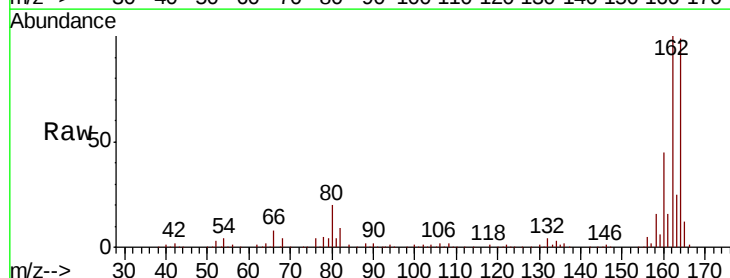

Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

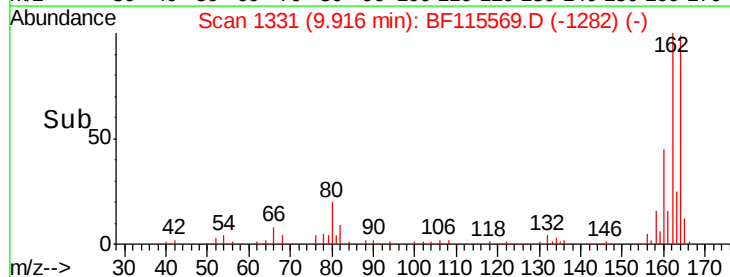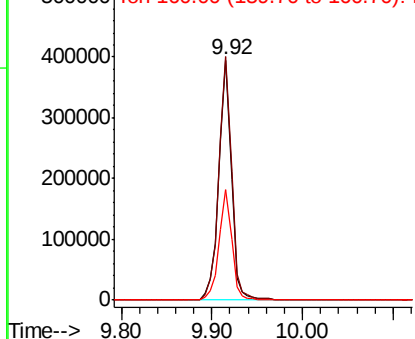


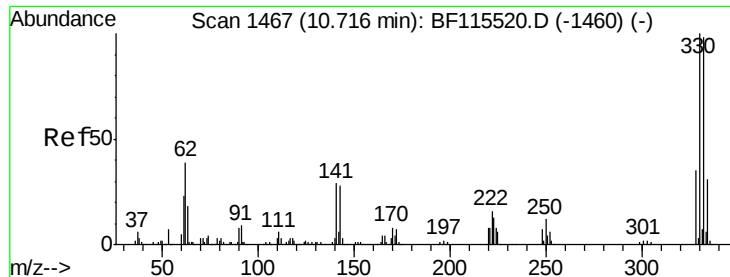




#42
 2,4,6-Tribromophenol
 Concen: 122.508 ng
 RT: 10.70 min Scan# 1465
 Delta R.T. -0.01 min
 Lab File: BF115569.D
 Acq: 15 Jul 2019 21:00

Instrument :
 BNA_F
 ClientSampleId :
 PB121261TB

Tgt Ion:330 Resp: 542137
 Ion Ratio Lower Upper
 330 100
 332 97.1 77.4 116.2
 141 29.5 22.4 33.6

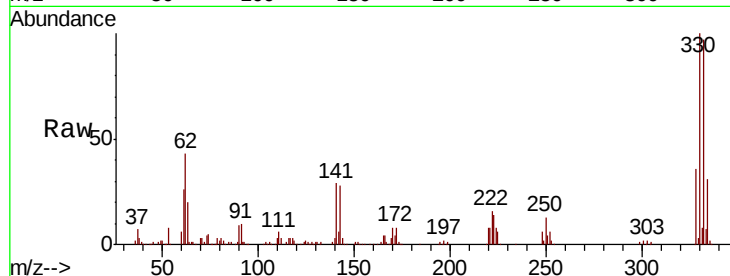


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

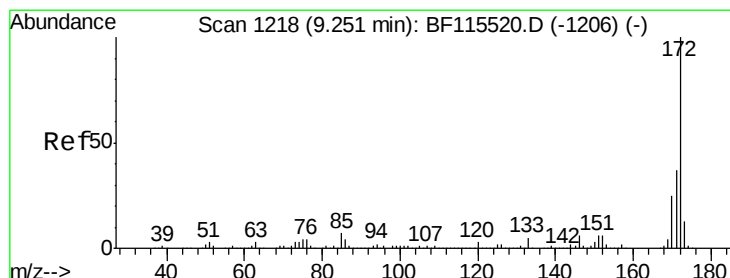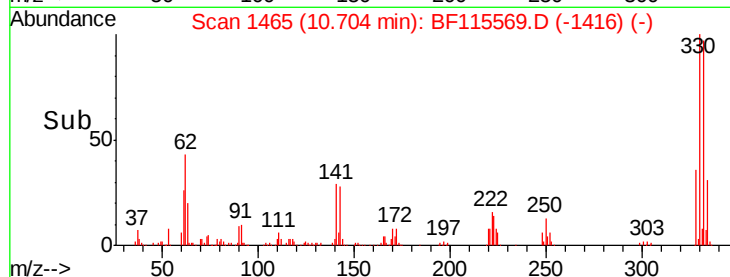
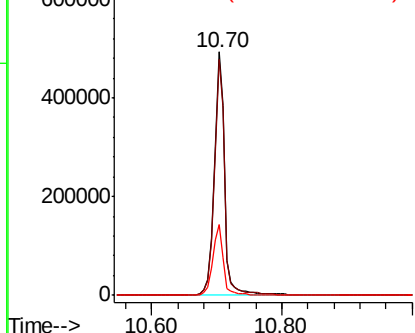



#45
 2-Fluorobiphenyl
 Concen: 97.924 ng
 RT: 9.24 min Scan# 1216
 Delta R.T. -0.01 min
 Lab File: BF115569.D
 Acq: 15 Jul 2019 21:00

Tgt Ion:172 Resp: 2121112
 Ion Ratio Lower Upper
 172 100
 171 36.9 30.6 46.0
 170 25.1 20.5 30.7

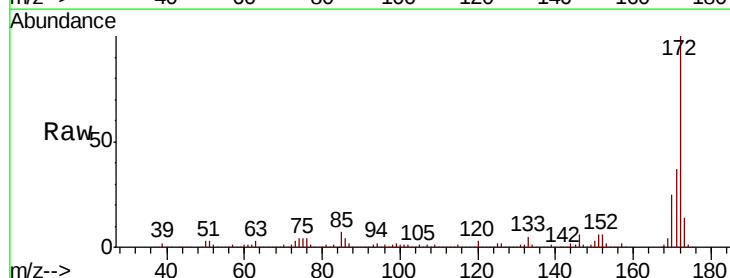

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E



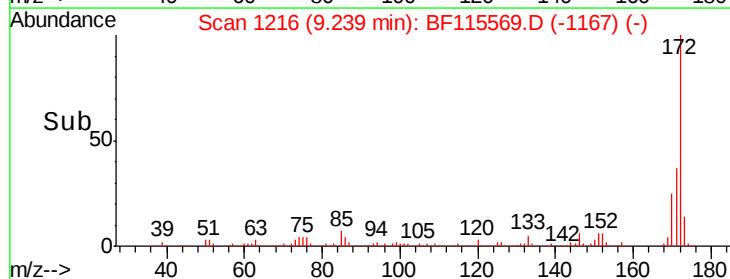
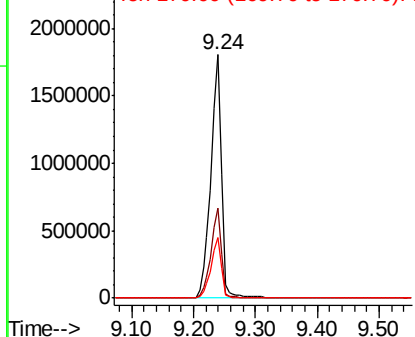


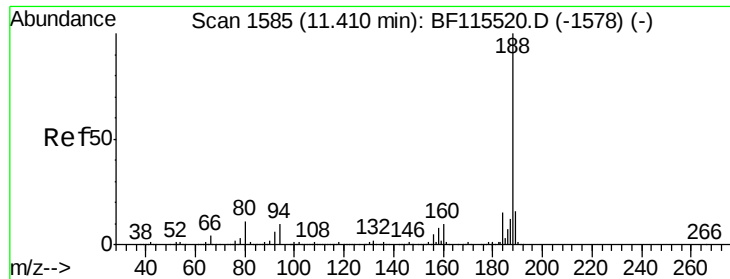

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.40 min Scan# 1583
Delta R.T. -0.01 min
Lab File: BF115569.D
Acq: 15 Jul 2019 21:00




Instrument :
BNA_F
ClientSampleId :
PB121261TB


Tgt Ion:188 Resp: 757952
Ion Ratio Lower Upper
188 100
94 10.6 7.8 11.6
80 11.8 8.6 13.0

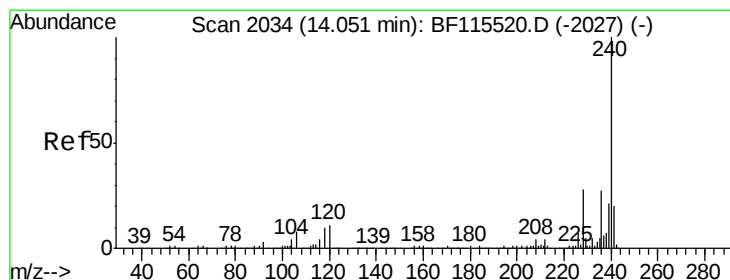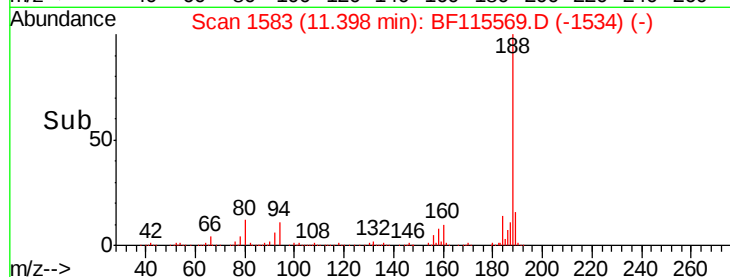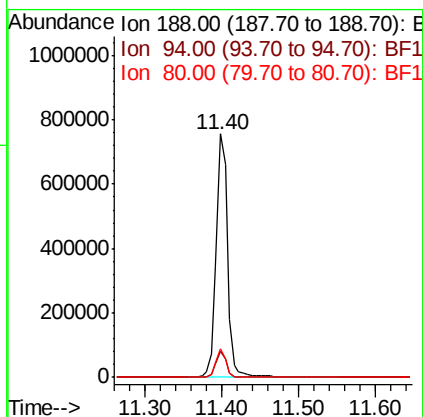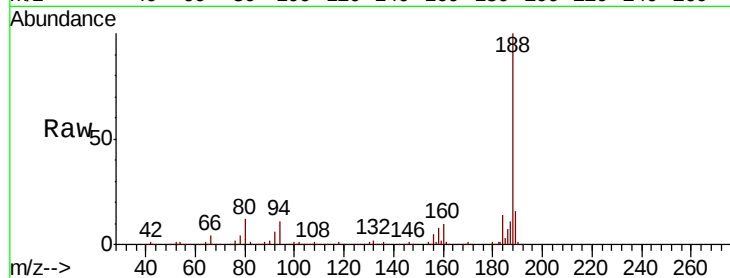

#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.03 min Scan# 2031
Delta R.T. -0.02 min
Lab File: BF115569.D
Acq: 15 Jul 2019 21:00

Tgt Ion:240 Resp: 541443
Ion Ratio Lower Upper
240 100
120 12.1 8.6 13.0
236 26.6 21.3 31.9

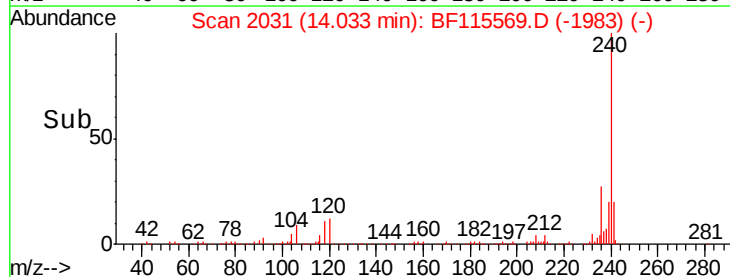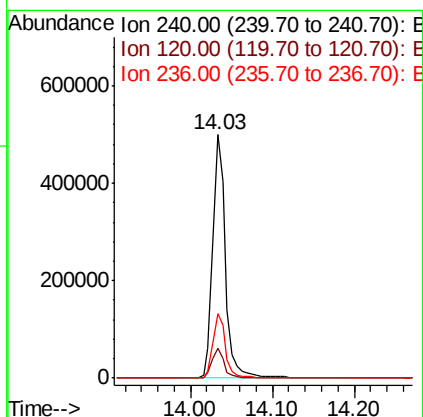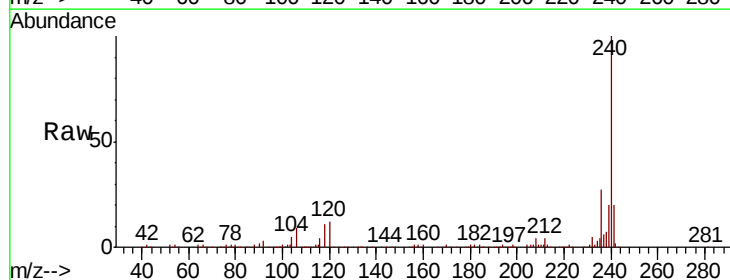

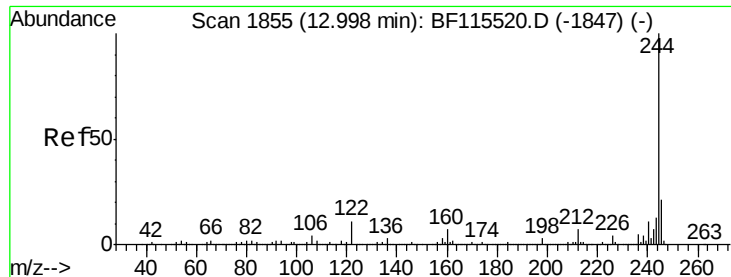

#79

Terphenyl-d14

Concen: 80.381 ng

RT: 12.99 min Scan# 1854

Delta R.T. -0.01 min

Lab File: BF115569.D

Acq: 15 Jul 2019 21:00

Instrument :

BNA_F

ClientSampleId :

PB121261TB


Tgt Ion:244 Resp: 2358674

Ion Ratio Lower Upper

244 100

212 7.1 6.0 9.0




122 10.2 8.6 12.8

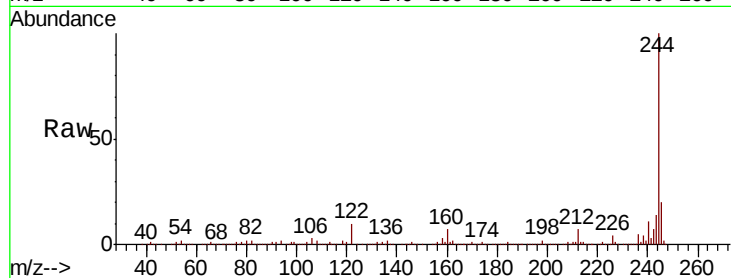

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

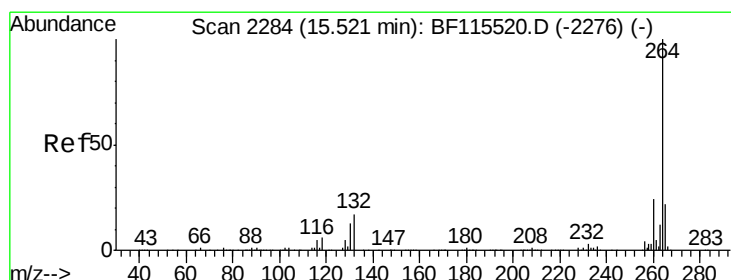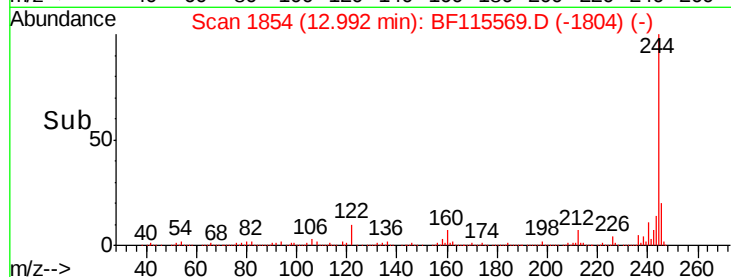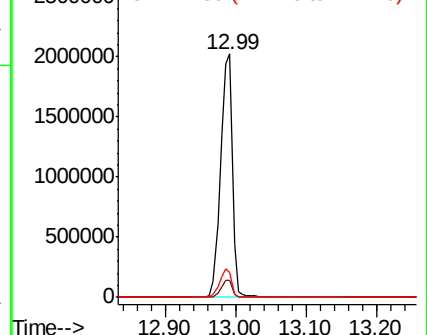

#87

Perylene-d12

Concen: 20.000 ng

RT: 15.50 min Scan# 2281

Delta R.T. -0.02 min

Lab File: BF115569.D

Acq: 15 Jul 2019 21:00


Tgt Ion:264 Resp: 471337

Ion Ratio Lower Upper

264 100

260 24.7 19.8 29.8

265 21.6 17.7 26.5

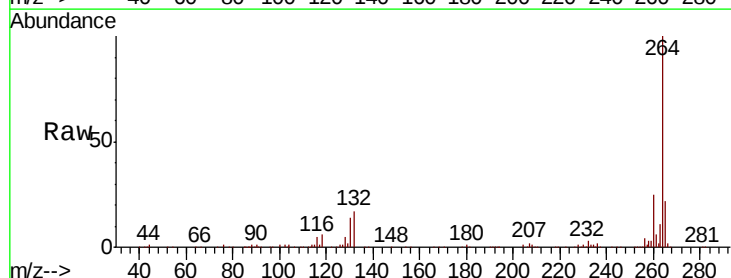

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

