
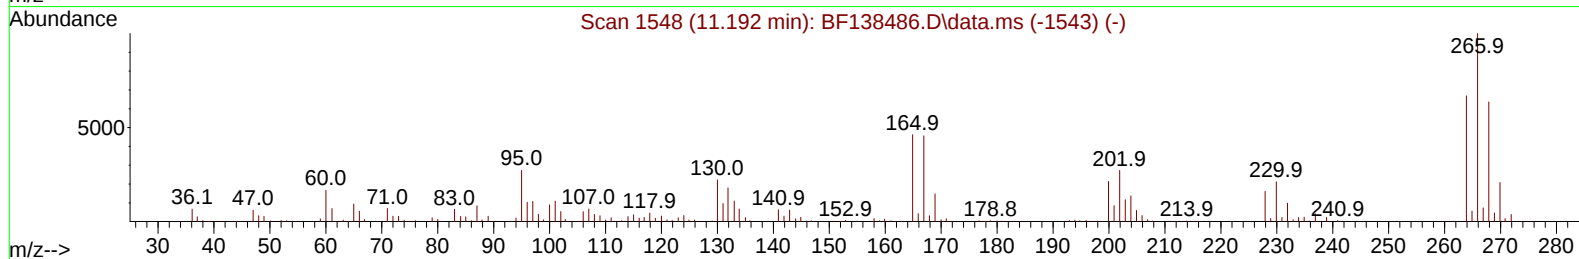
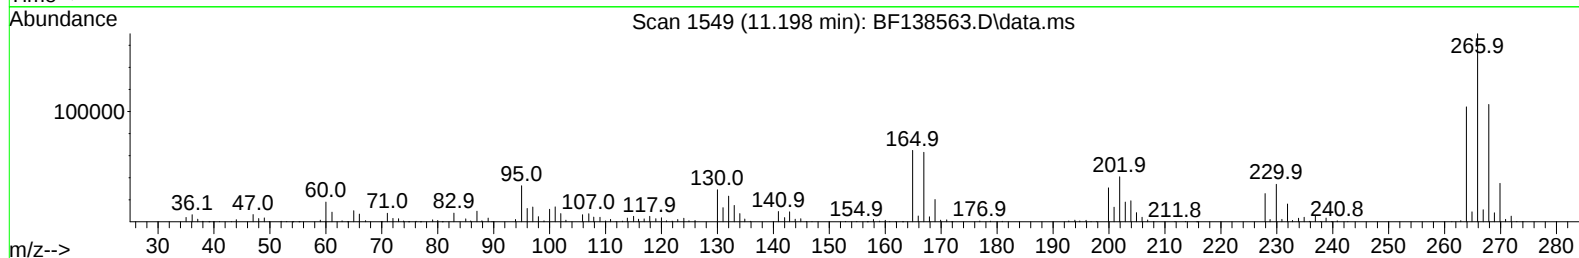


```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071524\  
Data File : BF138563.D  
Acq On    : 15 Jul 2024  11:22  
Operator  : CG\JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Quant Time: Jul 15 12:51:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF070924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 09 16:58:40 2024
Response via : Initial Calibration

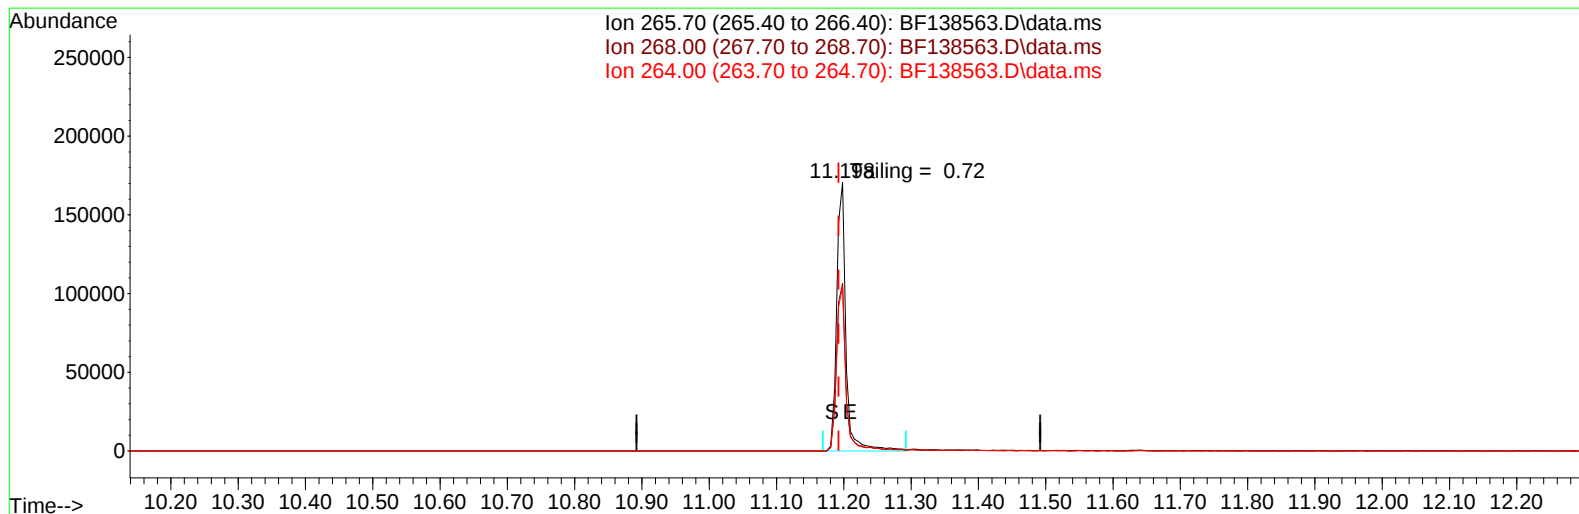

TIC: BF138563.D\data.ms

(70) Pentachlorophenol (C)




11.198min (+ 0.006) 23870.60 ng

response	162894
----------	--------

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	62.46
264.00	66.90	61.16
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071524\
Data File : BF138563.D
Acq On : 15 Jul 2024 11:22
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 15 12:51:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF070924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 09 16:58:40 2024
Response via : Initial Calibration

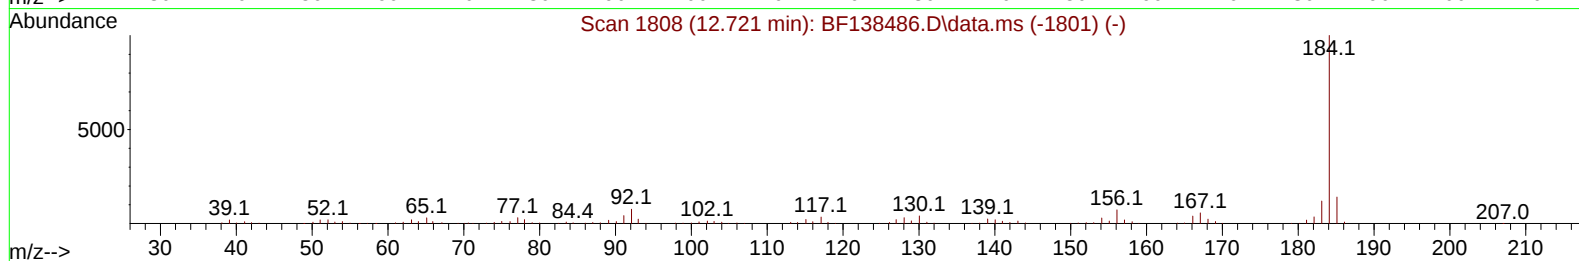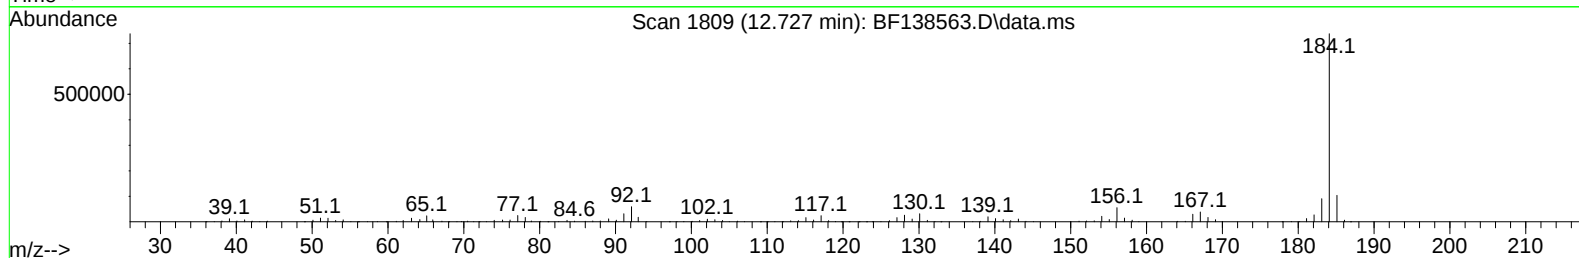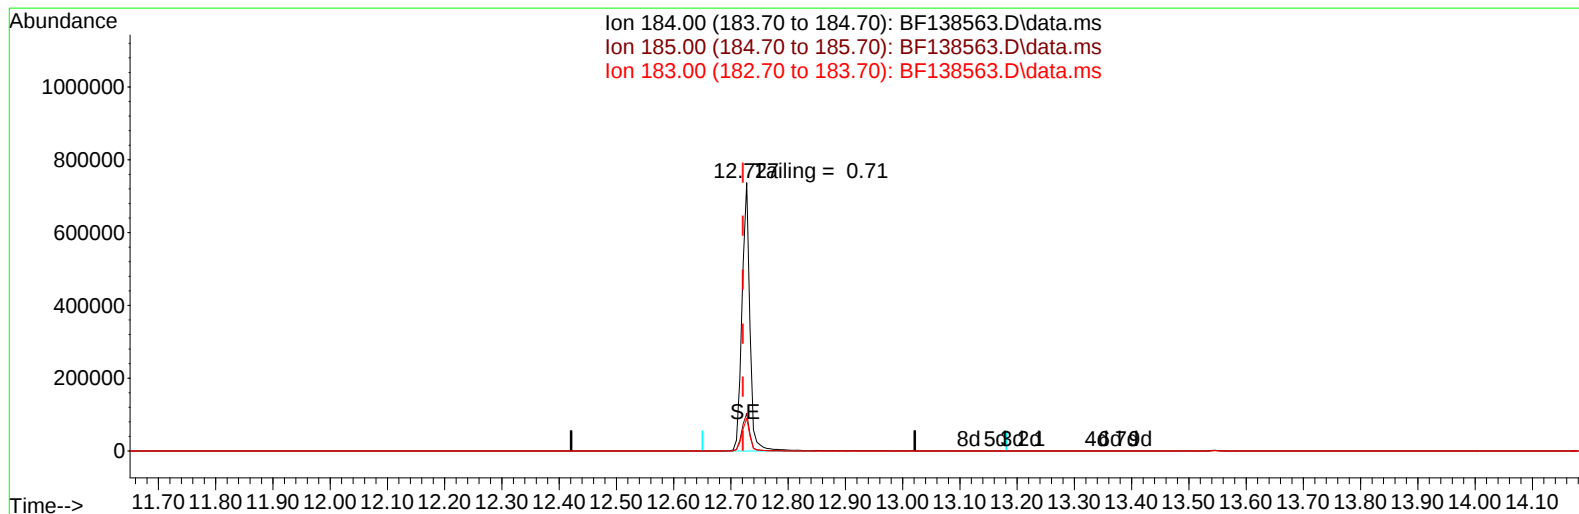

TIC: BF138563.D\data.ms

(77) Benzidine

12.727min (+ 0.006) 528725.98 ng m

response 707003

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.05
183.00	11.90	12.26
0.00	0.00	0.00