


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071524\
Data File : BF138563.D
Acq On : 15 Jul 2024 11:22
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF070924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jul 09 16:58:40 2024

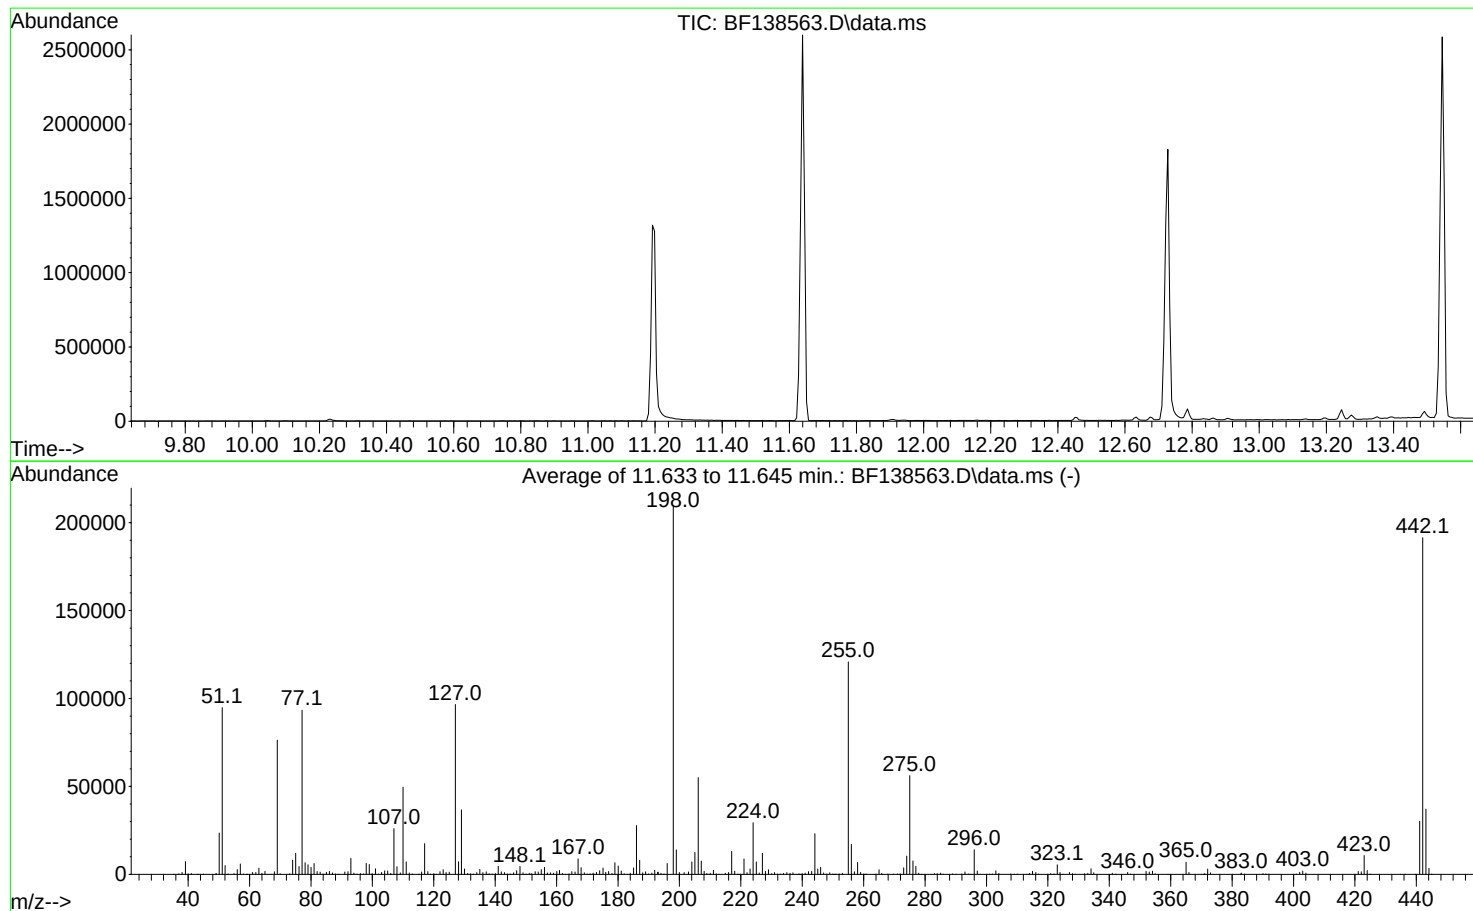




AutoFind: Scans 1623, 1624, 1625; Background Corrected with Scan 1618

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.3	94781	PASS
68	69	0.00	2	2.0	1507	PASS
69	198	0.00	100	36.5	76322	PASS
70	69	0.00	2	0.5	359	PASS
127	198	10	80	46.2	96595	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	209173	PASS
199	198	5	9	6.7	13968	PASS
275	198	10	60	26.9	56168	PASS
365	198	1	100	3.3	6950	PASS
441	198	0.01	100	14.4	30215	PASS
442	442	50	100	100.0	191411	PASS
443	442	15	24	19.4	37112	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071524\
Data File : BF138563.D
Acq On : 15 Jul 2024 11:22
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 15 12:51:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF070924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 09 16:58:40 2024
Response via : Initial Calibration

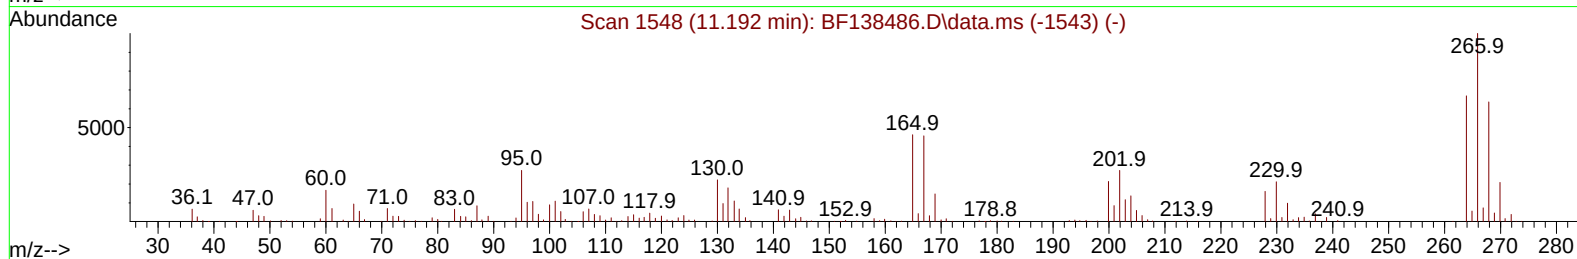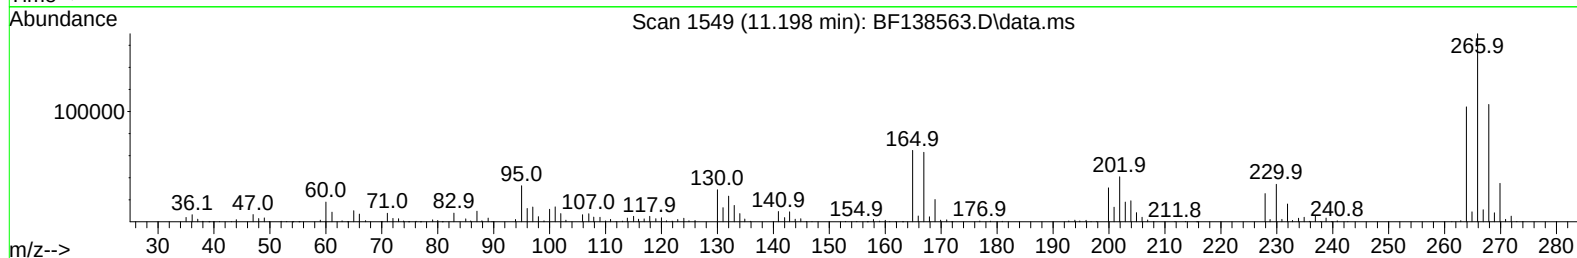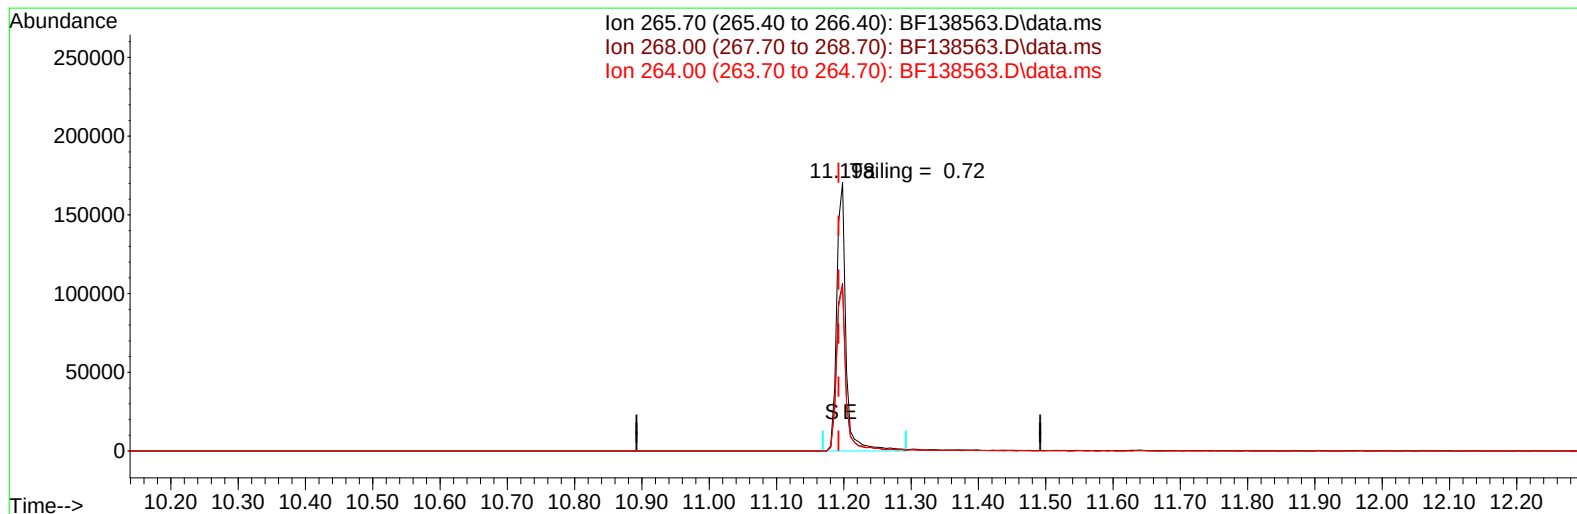

TIC: BF138563.D\data.ms

(70) Pentachlorophenol (C)

11.198min (+ 0.006) 23870.60 ng




response 162894

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	62.46
264.00	66.90	61.16
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071524\
Data File : BF138563.D
Acq On : 15 Jul 2024 11:22
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 15 12:51:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF070924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 09 16:58:40 2024
Response via : Initial Calibration

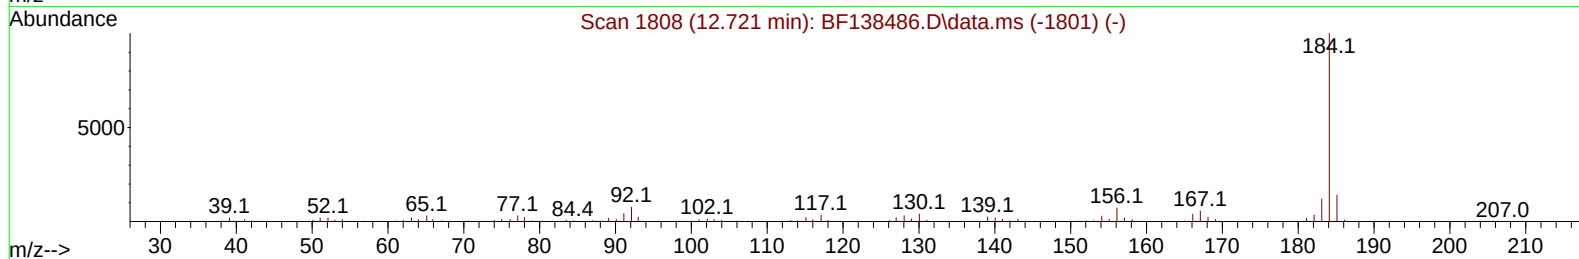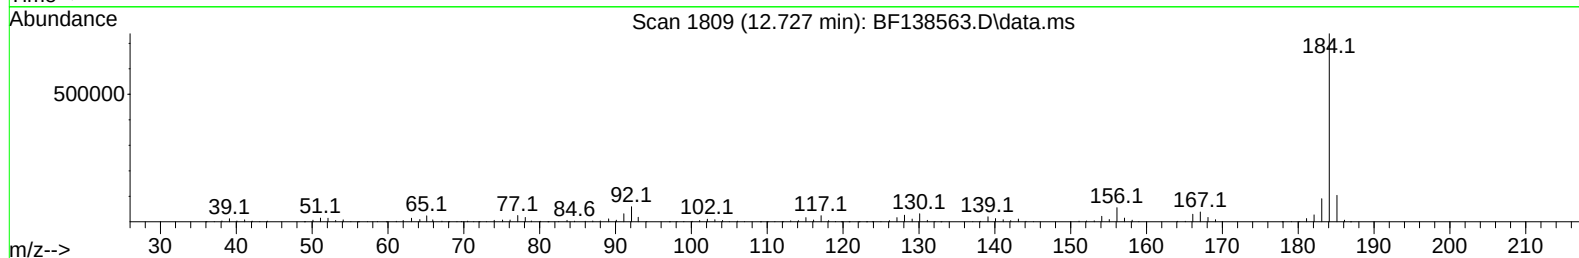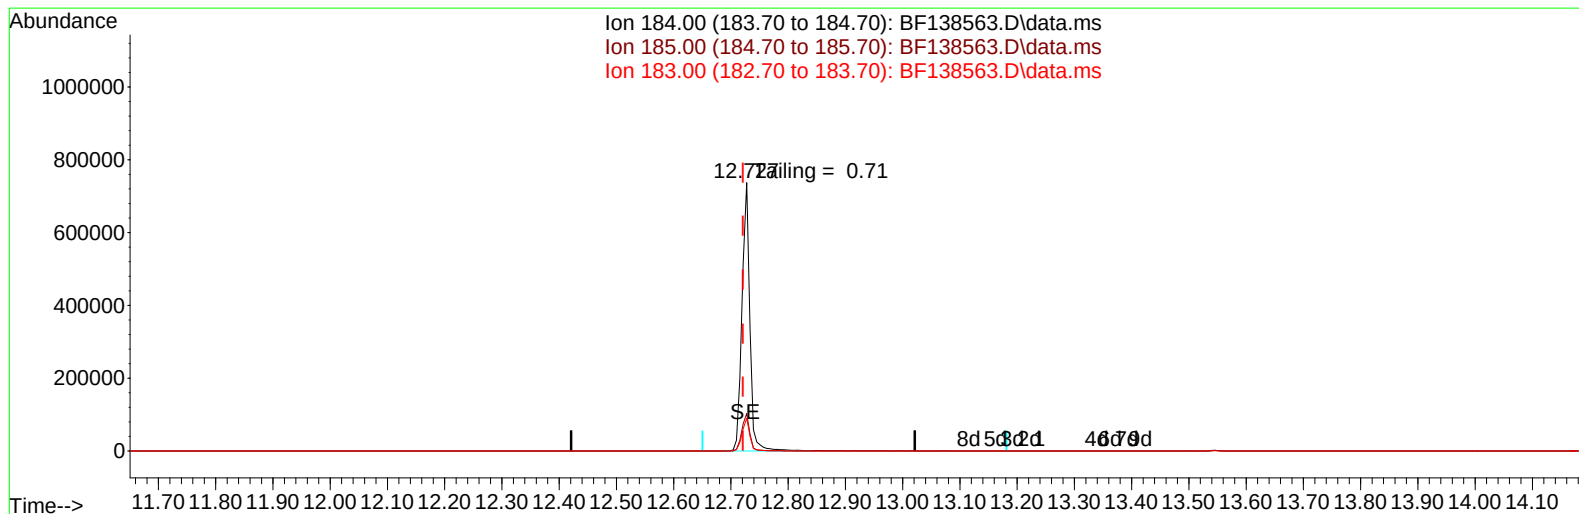

TIC: BF138563.D\data.ms

(77) Benzidine

12.727min (+ 0.006) 528725.98 ng m

response 707003

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.05
183.00	11.90	12.26
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/15/2024	BNA_F	<u>BF138563.D</u>
Compound Name	Response	Retention Time
DDT	424952	13.545
DDD	15767	13.245
DDE	1608	12.91
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
17375	442327	3.93

Instrument :
BNA_F
ClientSampleId :
DFTPP