
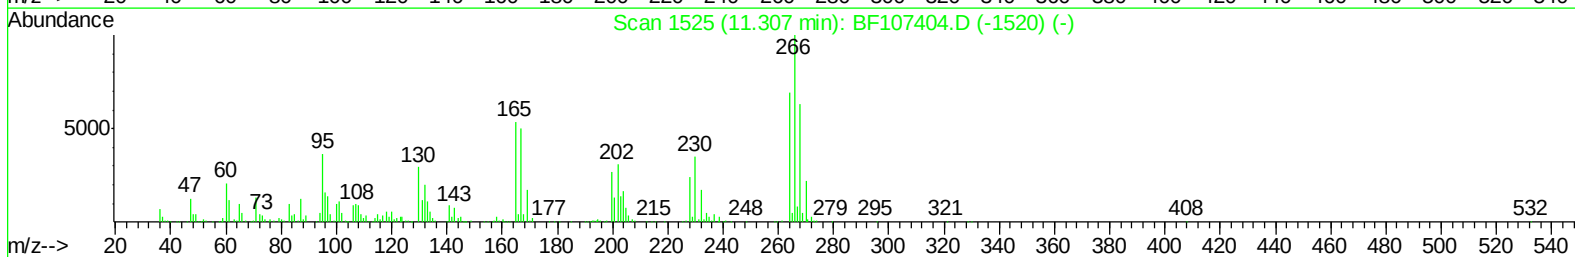
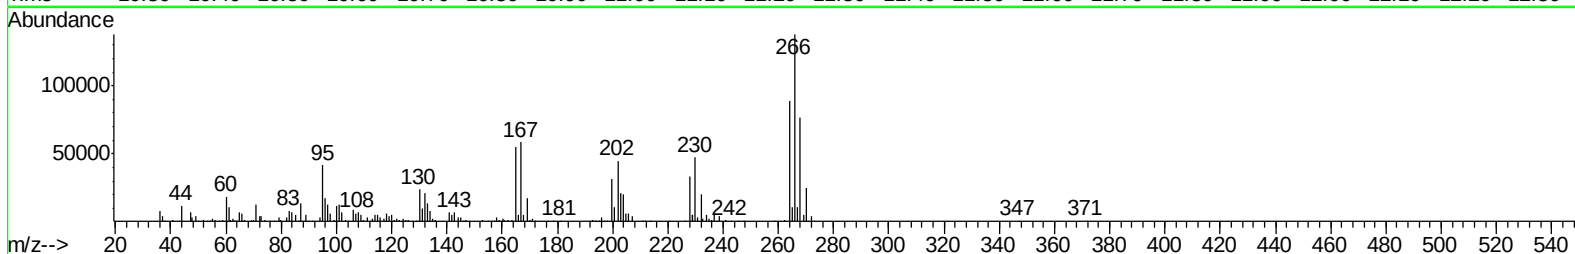


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF071618\
Data File : BF107400.D
Acq On : 16 Jul 2018 13:14
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 17 08:12:32 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF071618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 16 17:24:26 2018
Response via : Initial Calibration

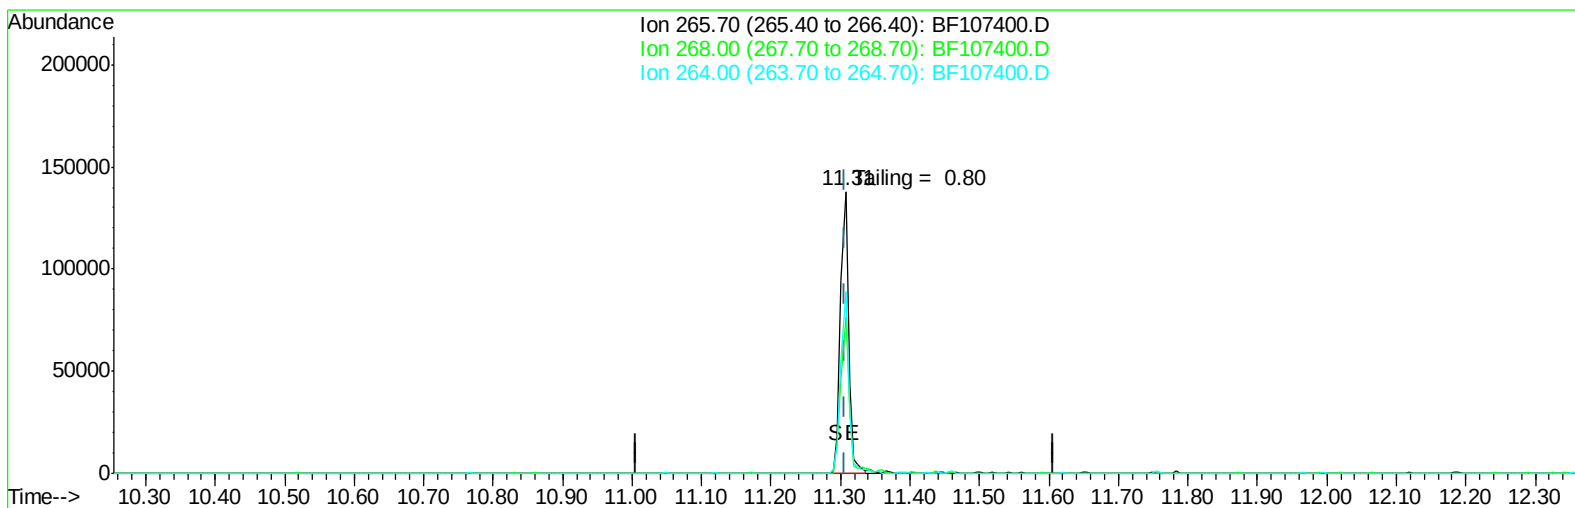

TIC: BF107400.D

(69) Pentachlorophenol (C)




11.307min (-0.000) 119361.93ng

response 110231

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	55.53
264.00	61.90	64.35
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF071618\
 Data File : BF107400.D
 Acq On : 16 Jul 2018 13:14
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 17 08:12:32 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF071618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 16 17:24:26 2018
 Response via : Initial Calibration

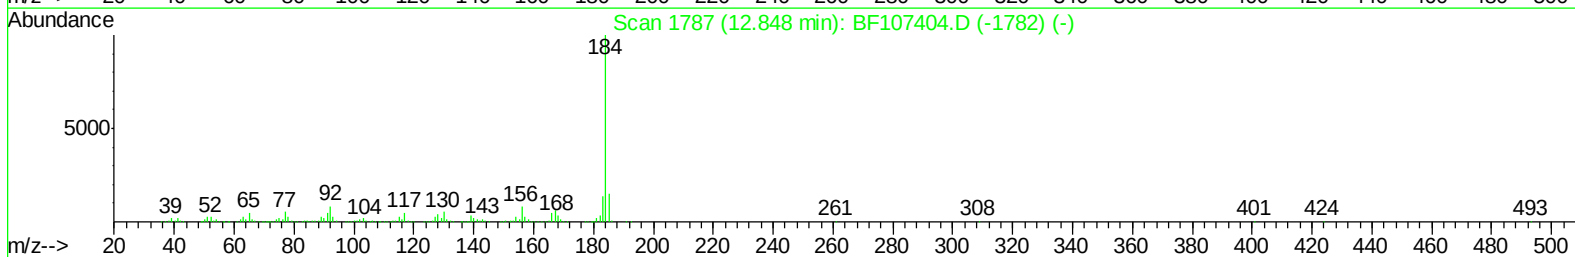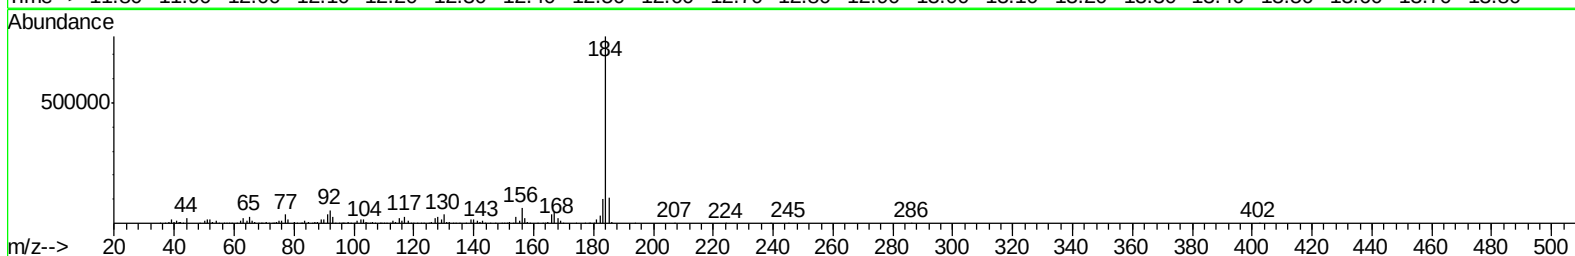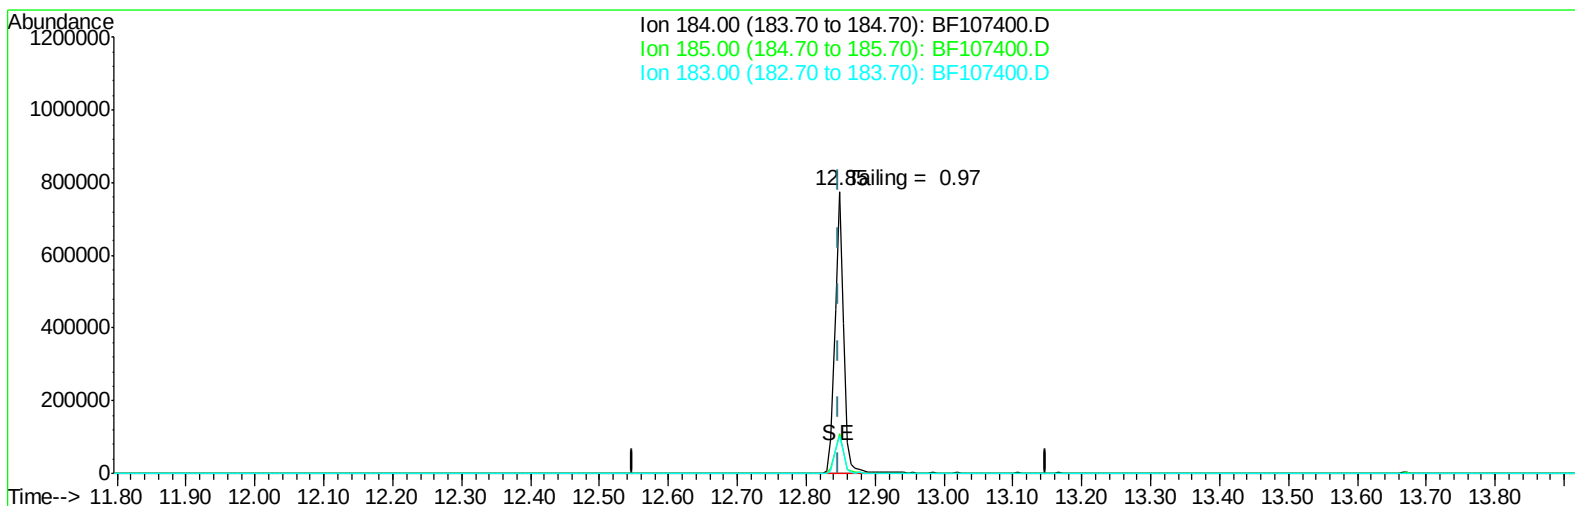

TIC: BF107400.D

(76) Benzidine

12.848min (-0.000) 16726.23ng

response 674458

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	13.96
183.00	11.60	12.99
0.00	0.00	0.00