


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071618\
 Data File : BF107400.D
 Acq On : 16 Jul 2018 13:14
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF071618.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jul 17 11:29:08 2018

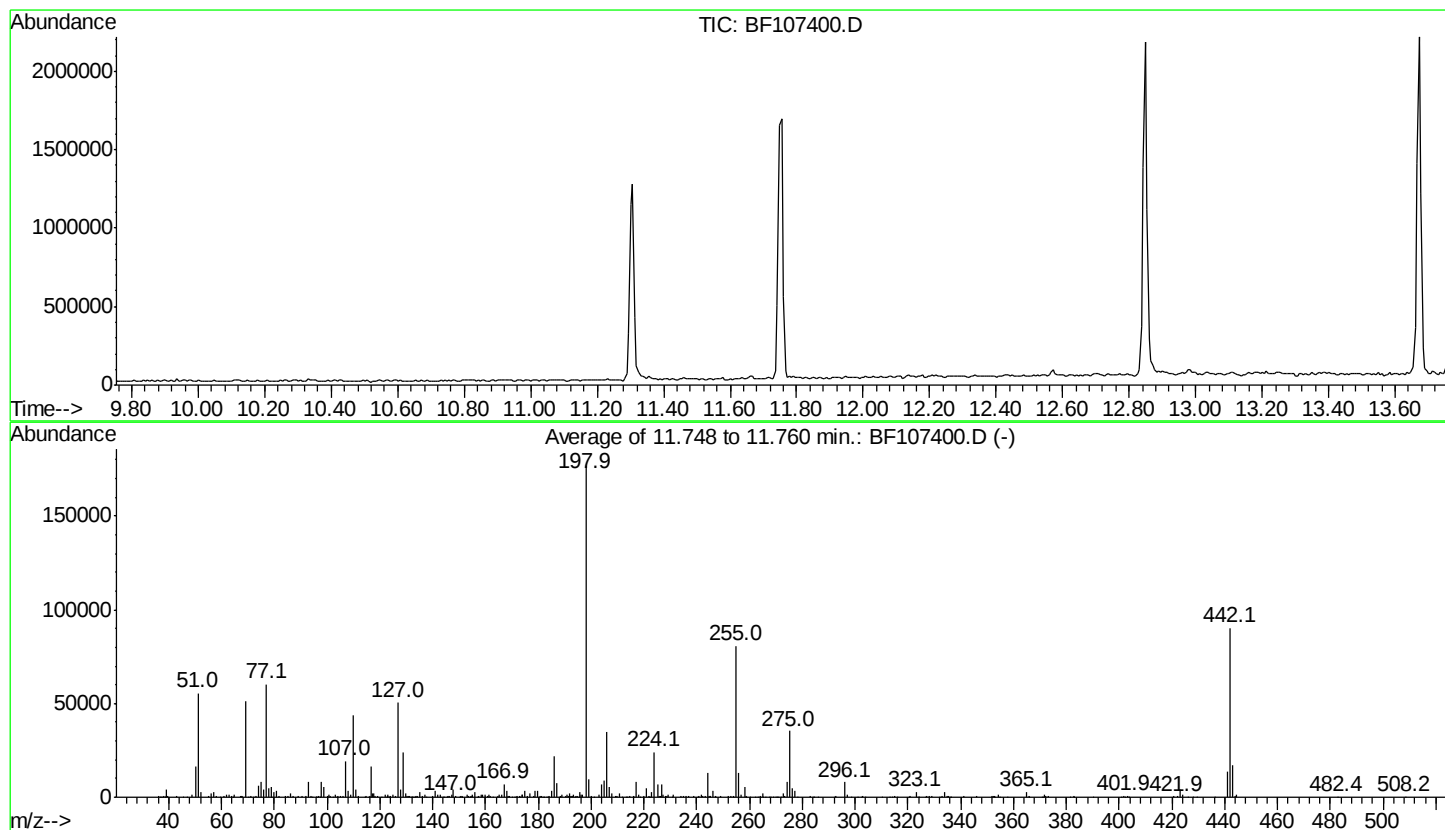

AutoFind: Scans 1600, 1601, 1602; Background Corrected with Scan 1594

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.3	55463	PASS
68	69	0.00	2	2.0	1046	PASS
69	198	0.00	100	28.9	51213	PASS
70	69	0.00	2	0.6	287	PASS
127	198	10	80	28.5	50496	PASS
197	198	0.00	2	0.6	1060	PASS
198	198	100	100	100.0	176928	PASS
199	198	5	9	5.6	9919	PASS
275	198	10	60	20.1	35501	PASS
365	198	1	100	1.7	2926	PASS
441	198	0.01	100	7.8	13798	PASS
442	198	50	100	51.1	90341	PASS
443	442	15	24	18.7	16856	PASS