


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071618\
 Data File : BF107409.D
 Acq On : 16 Jul 2018 18:17
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF071618.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jul 17 11:29:08 2018

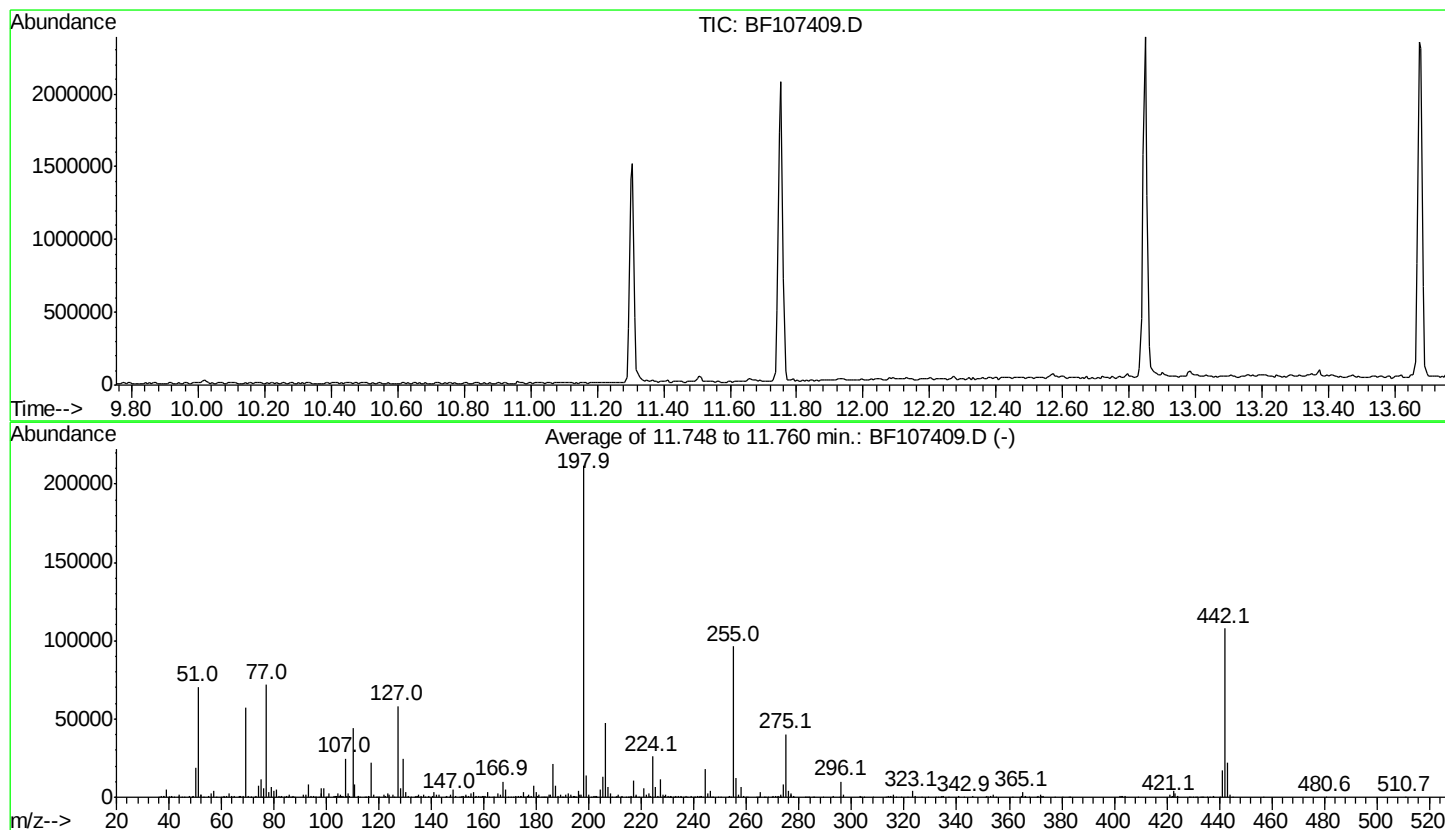

AutoFind: Scans 1600, 1601, 1602; Background Corrected with Scan 1594

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.2	70356	PASS
68	69	0.00	2	1.9	1121	PASS
69	198	0.00	100	27.2	57594	PASS
70	69	0.00	2	1.0	581	PASS
127	198	10	80	27.4	58064	PASS
197	198	0.00	2	0.7	1443	PASS
198	198	100	100	100.0	211736	PASS
199	198	5	9	6.6	13997	PASS
275	198	10	60	18.9	40072	PASS
365	198	1	100	1.7	3650	PASS
441	198	0.01	100	8.2	17328	PASS
442	198	50	100	50.9	107706	PASS
443	442	15	24	20.3	21843	PASS