

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF071619\
 Data File : BF115601.D
 Acq On : 16 Jul 2019 17:03
 Operator : HP/JU
 Sample : K3620-04
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 CL-01-071219-B

Quant Time: Jul 17 04:55:17 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF071219.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 12 14:03:52 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.88	152	168206	20.00	ng	0.00
21) Naphthalene-d8	8.16	136	548623	20.00	ng	0.00
39) Acenaphthene-d10	9.92	164	283993	20.00	ng	-0.01
64) Phenanthrene-d10	11.40	188	544803	20.00	ng	0.00
76) Chrysene-d12	14.04	240	348644	20.00	ng	-0.01
87) Perylene-d12	15.51	264	399827	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.52	112	1197024	116.40	ng	0.01
7) Phenol-d6	6.51	99	1351981	103.61	ng	0.00
23) Nitrobenzene-d5	7.44	82	964487	102.22	ng	-0.01
42) 2,4,6-Tribromophenol	10.71	330	452209	136.42	ng	0.00
45) 2-Fluorobiphenyl	9.24	172	1713189	105.59	ng	-0.01
79) Terphenyl-d14	12.99	244	1805023	95.53	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF071619\
Data File : BF115601.D
Acq On : 16 Jul 2019 17:03
Operator : HP/JU
Sample : K3620-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CL-01-071219-B

Quant Time: Jul 17 04:55:17 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF071219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 12 14:03:52 2019
Response via : Initial Calibration

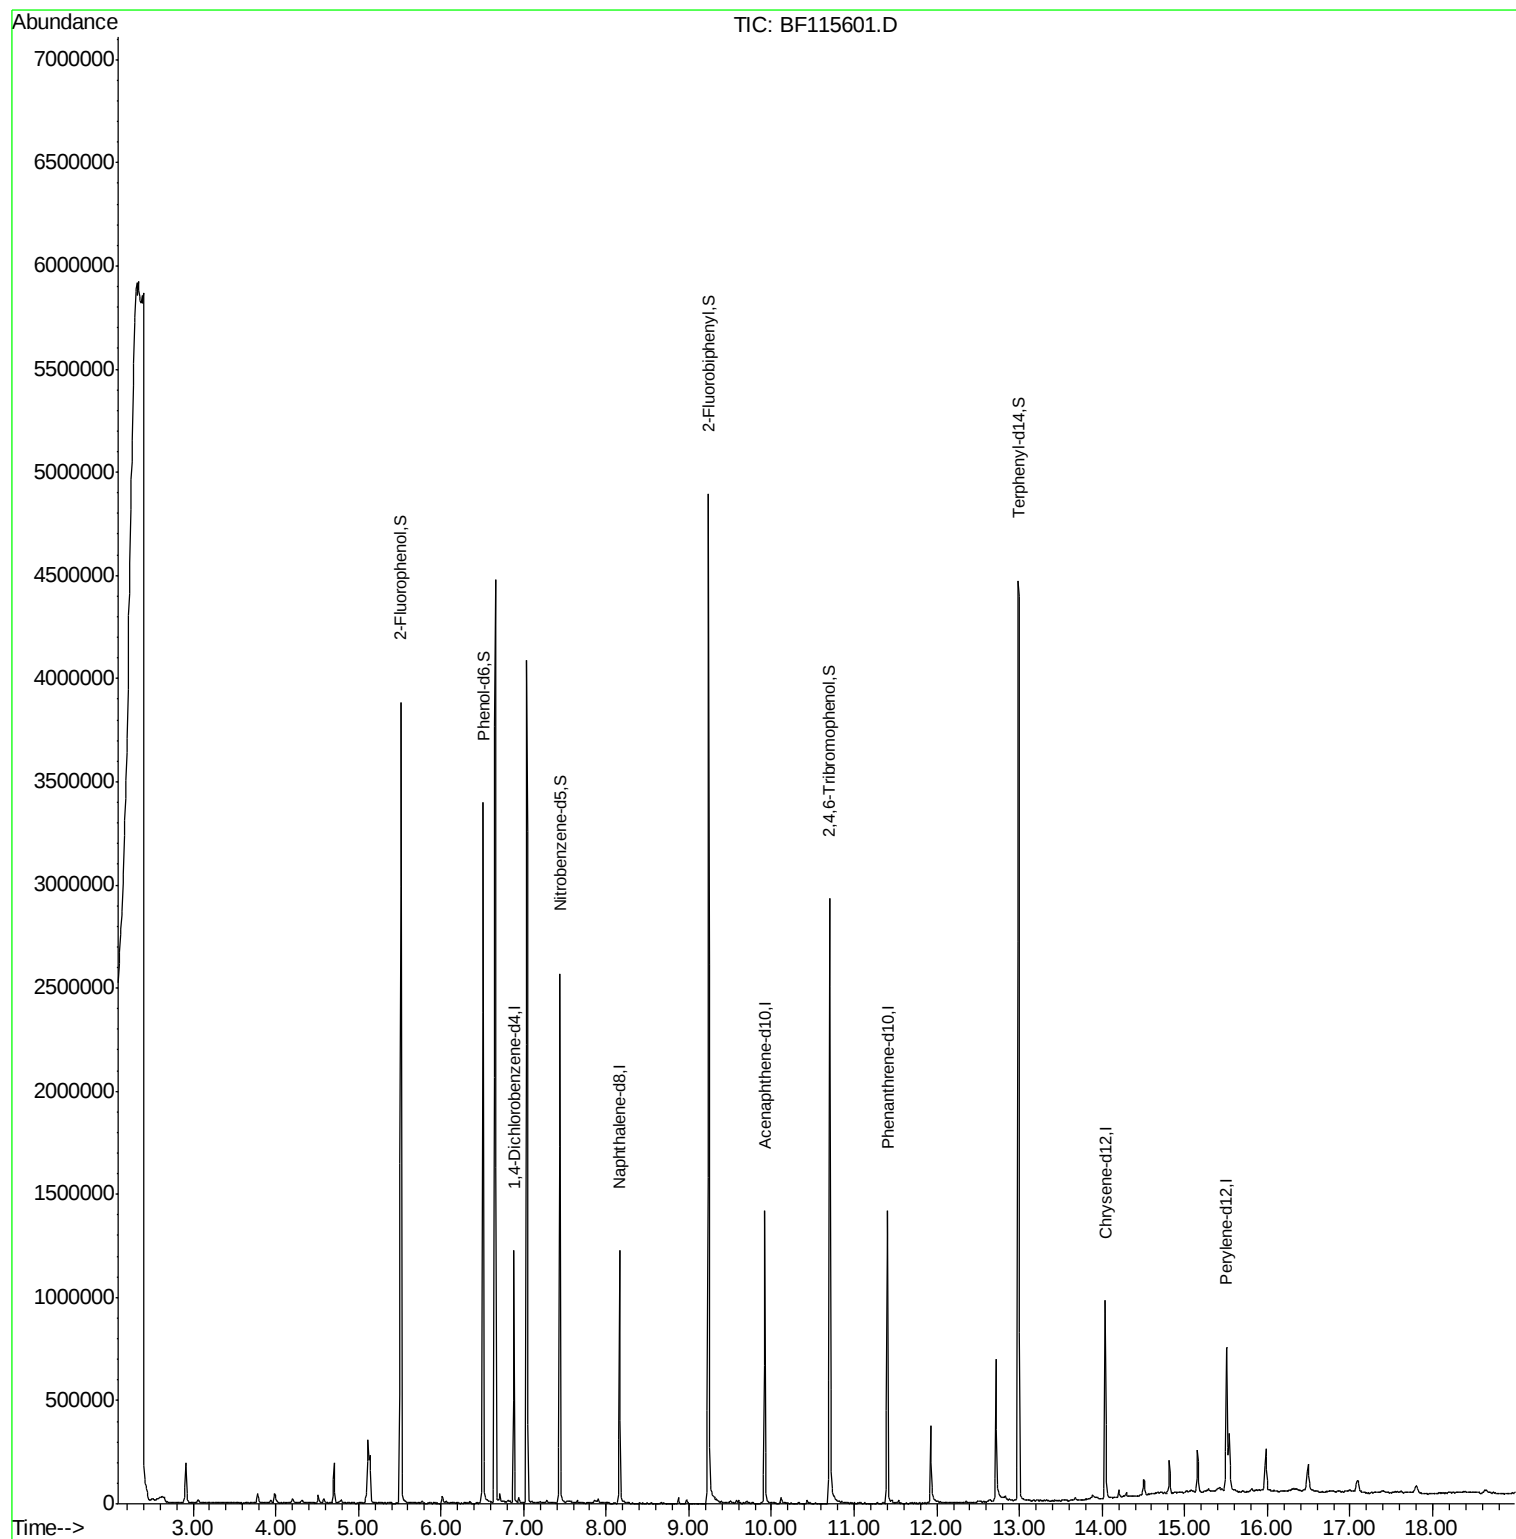

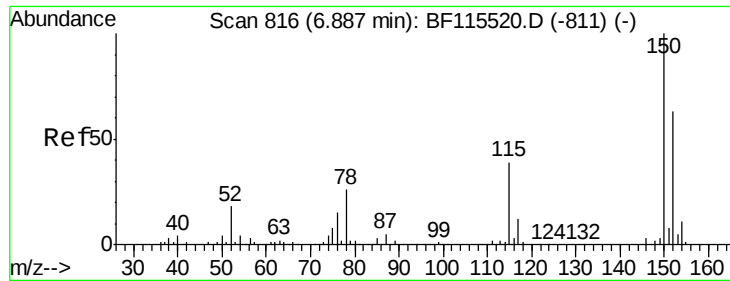


#1



1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.88 min Scan# 815
Delta R.T. -0.01 min
Lab File: BF115601.D
Acq: 16 Jul 2019 17:03

Instrument :
BNA_F
ClientSampleId :
CL-01-071219-B

Tot Ion:152 Resp: 168206
Ion Ratio Lower Upper
152 100
150 155.9 129.7 194.5
115 62.2 48.2 72.4

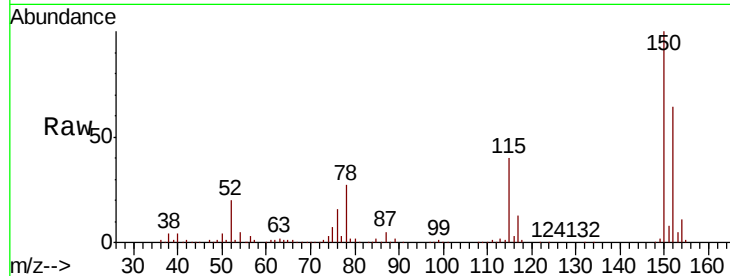


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

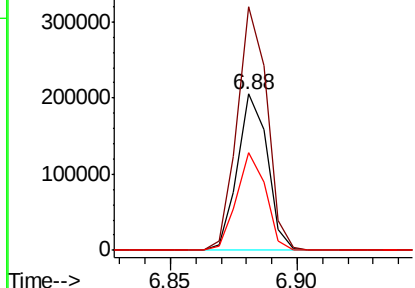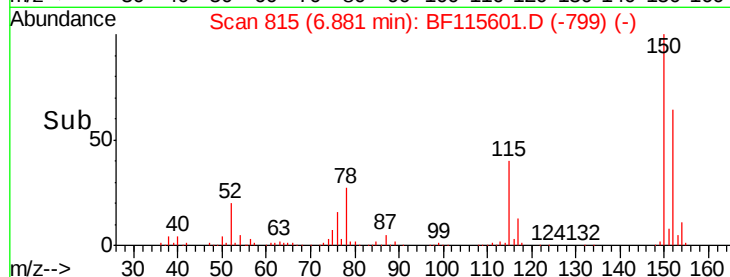



#5


2-Fluorophenol
Concen: 116.404 ng
RT: 5.52 min Scan# 583
Delta R.T. 0.01 min
Lab File: BF115601.D
Acq: 16 Jul 2019 17:03

Tgt Ion:112 Resp: 1197024
Ion Ratio Lower Upper
112 100
64 57.4 46.8 70.2
63 29.6 24.1 36.1

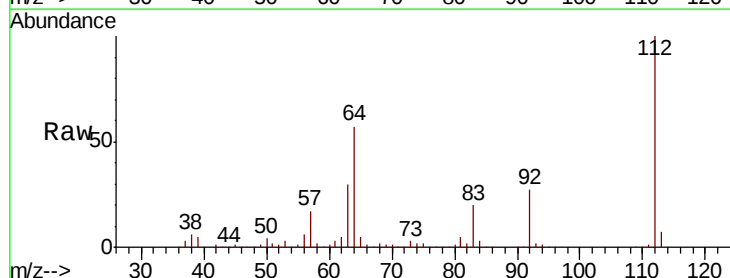

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

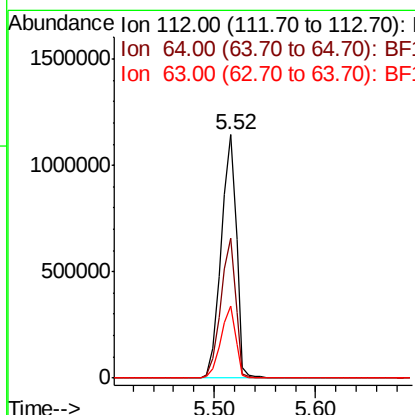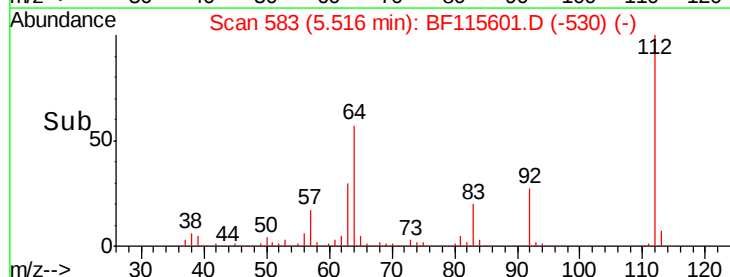

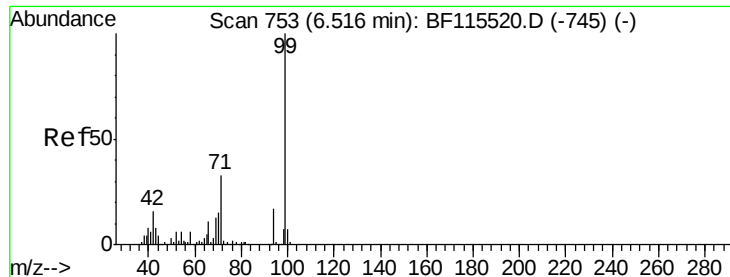

#7

Phenol-d6

Concen: 103.613 ng

RT: 6.51 min Scan# 752

Delta R.T. -0.01 min

Lab File: BF115601.D

Acq: 16 Jul 2019 17:03

Instrument :


BNA_F

ClientSampleId :

CL-01-071219-B

Tot Ion: 99 Resp: 1351981

Ion	Ratio	Lower	Upper
99	100		
42	16.6	13.6	20.4
71	34.9	28.5	42.7



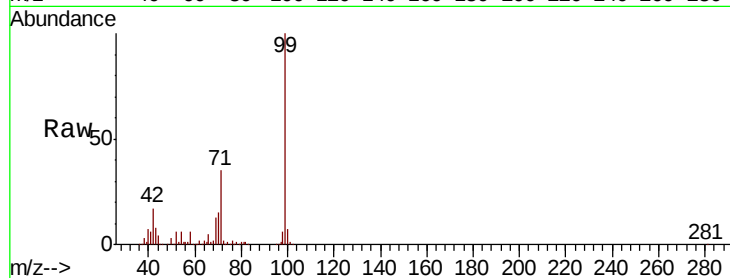


Abundance

Ion 99.00 (98.70 to 99.70): BF1

Ion 42.00 (41.70 to 42.70): BF1

Ion 71.00 (70.70 to 71.70): BF1

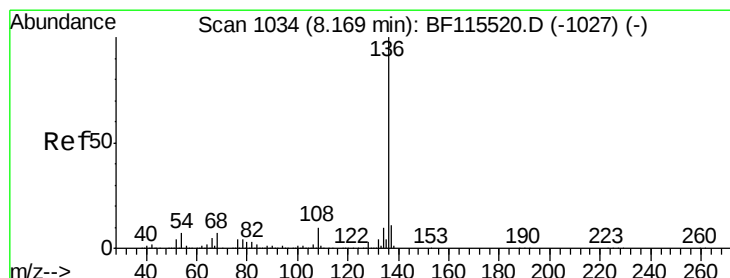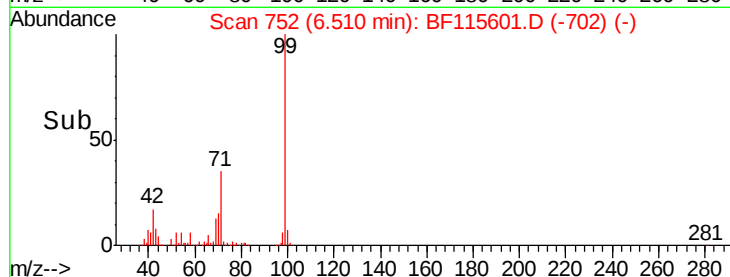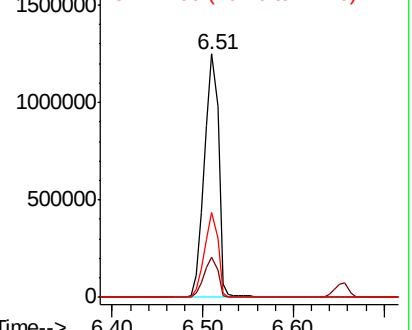

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.16 min Scan# 1033


Delta R.T. -0.01 min

Lab File: BF115601.D

Acq: 16 Jul 2019 17:03

Tgt Ion: 136 Resp: 548623

Ion	Ratio	Lower	Upper
136	100		
137	10.9	9.0	13.4
54	6.1	5.6	8.4
68	5.6	5.0	7.6

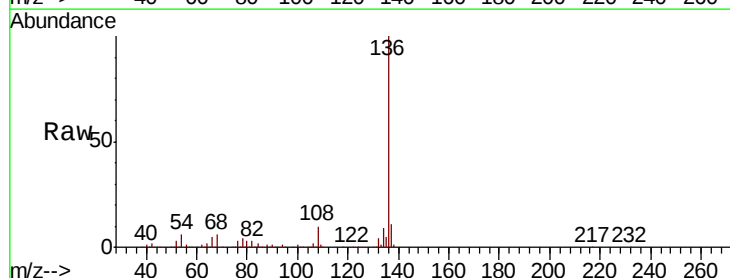



Abundance

Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF1

Ion 68.00 (67.70 to 68.70): BF1



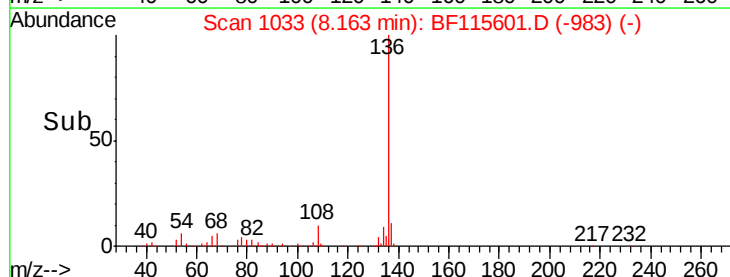
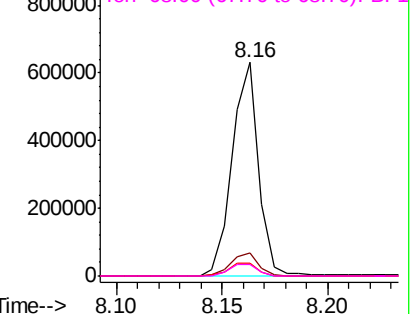




#23
 Nitrobenzene-d5
 Concen: 102.223 ng
 RT: 7.44 min Scan# 910
 Delta R.T. -0.01 min
 Lab File: BF115601.D
 Acq: 16 Jul 2019 17:03




Instrument :
 BNA_F
 ClientSampleId :
 CL-01-071219-B

Tot Ion: 82 Resp: 964487
 Ion Ratio Lower Upper
 82 100
 128 46.0 38.6 57.8
 54 44.0 35.6 53.4

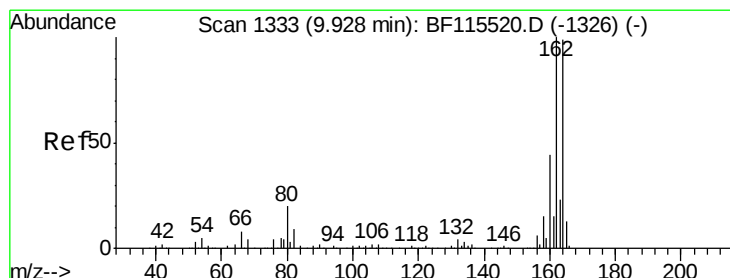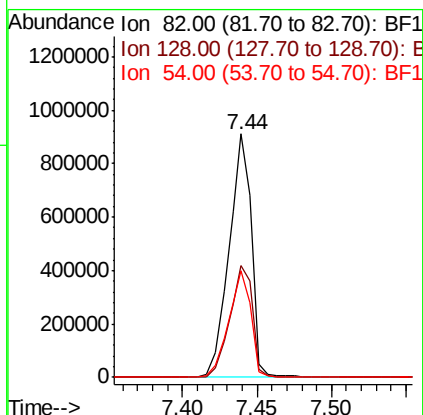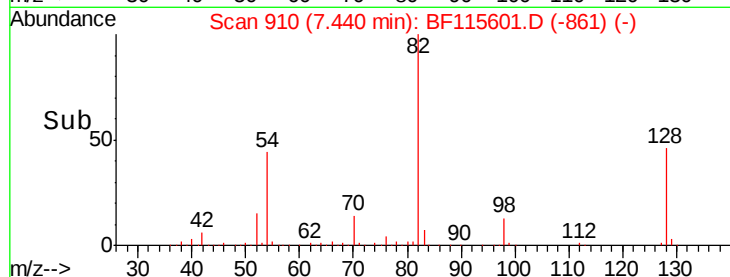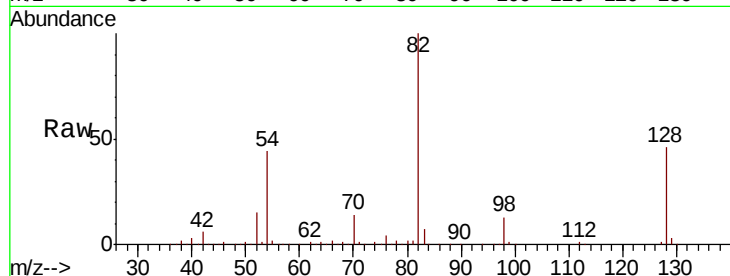

#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 9.92 min Scan# 1331
 Delta R.T. -0.01 min
 Lab File: BF115601.D
 Acq: 16 Jul 2019 17:03

Tgt Ion:164 Resp: 283993
 Ion Ratio Lower Upper
 164 100
 162 103.3 82.9 124.3
 160 46.3 36.8 55.2

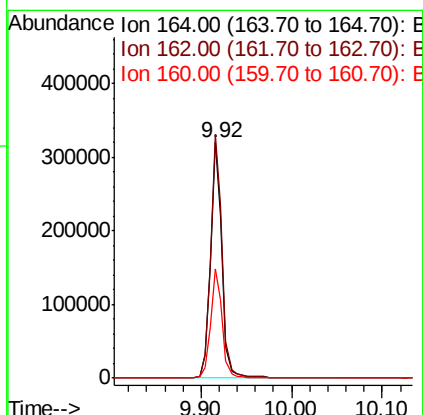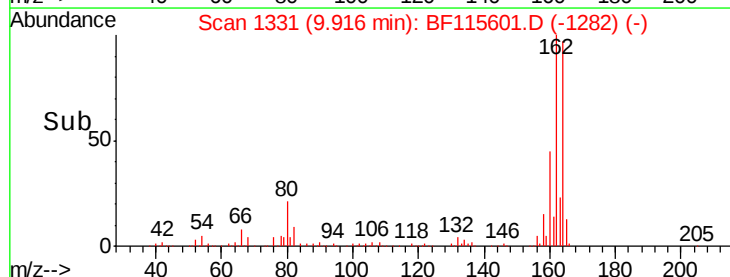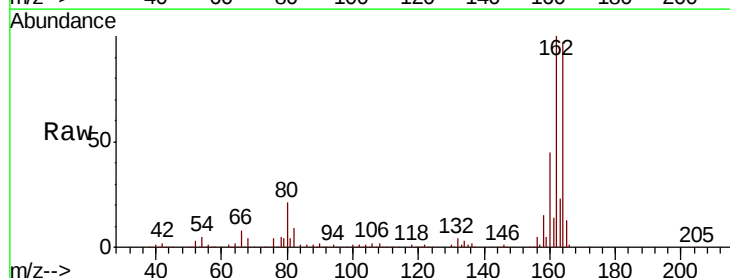







#42
 2,4,6-Tribromophenol
 Concen: 136.418 ng
 RT: 10.71 min Scan# 1466
 Delta R.T. -0.01 min
 Lab File: BF115601.D
 Acq: 16 Jul 2019 17:03

Instrument :
 BNA_F
 ClientSampleId :
 CL-01-071219-B

Tot Ion	Ratio	Lower	Upper
330	100		
332	95.8	77.4	116.2
141	30.3	22.4	33.6

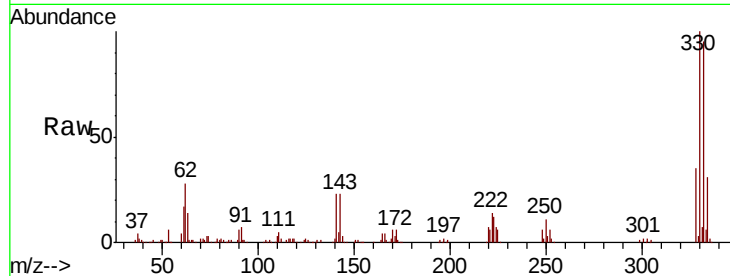


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

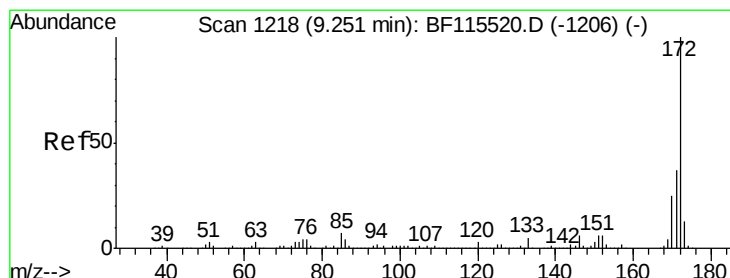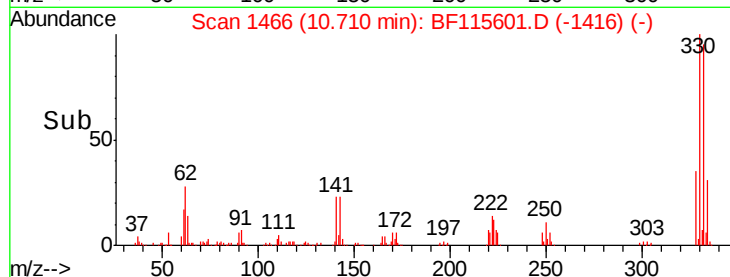
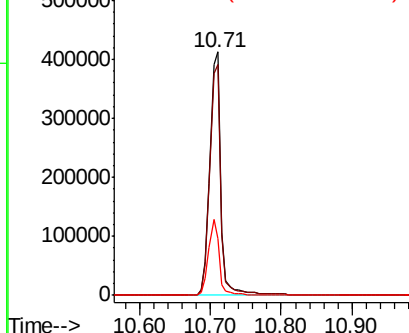



#45
 2-Fluorobiphenyl
 Concen: 105.586 ng
 RT: 9.24 min Scan# 1216
 Delta R.T. -0.01 min
 Lab File: BF115601.D
 Acq: 16 Jul 2019 17:03

Tgt Ion	Ratio	Lower	Upper
172	100		
171	37.3	30.6	46.0
170	25.0	20.5	30.7

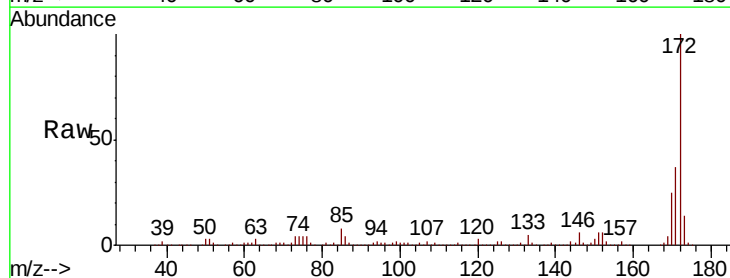

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E



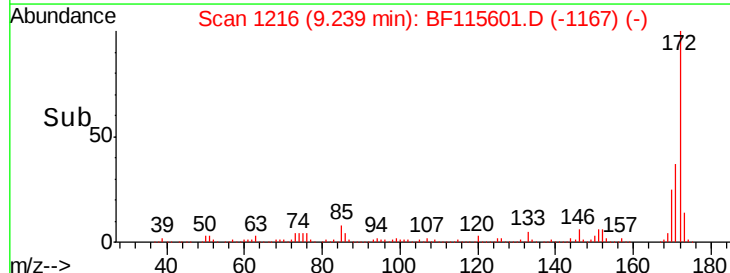
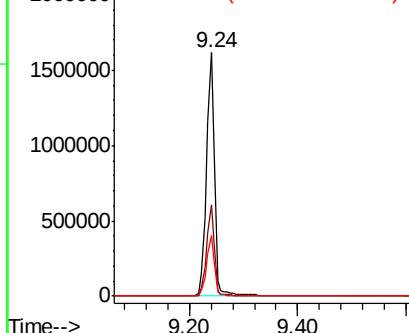


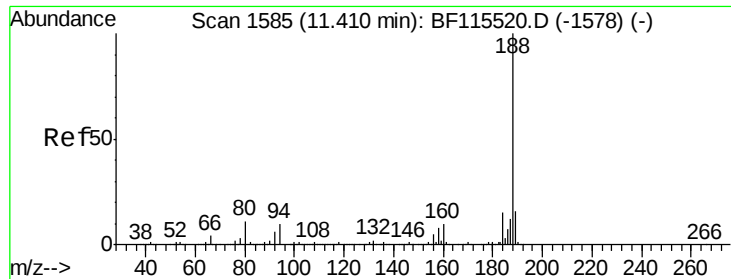

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.40 min Scan# 1584
Delta R.T. -0.01 min
Lab File: BF115601.D
Acq: 16 Jul 2019 17:03




Instrument :
BNA_F
ClientSampleId :
CL-01-071219-B


Tot Ion:188 Resp: 544803
Ion Ratio Lower Upper
188 100
94 8.7 7.8 11.6
80 9.2 8.6 13.0

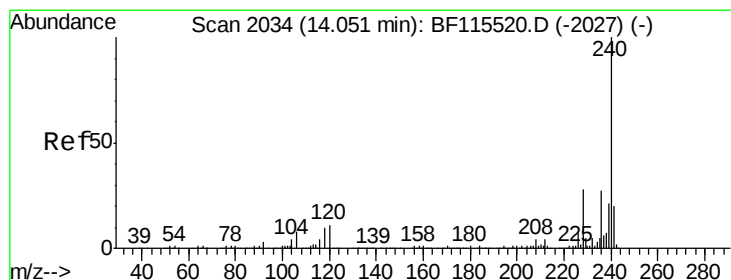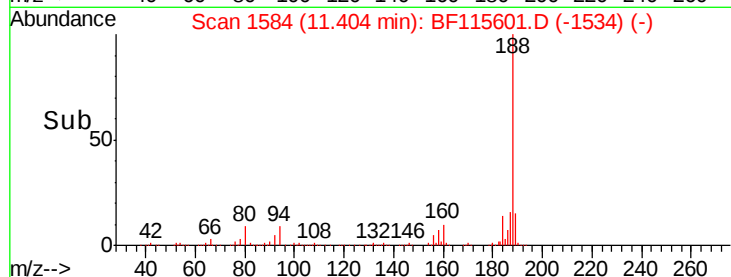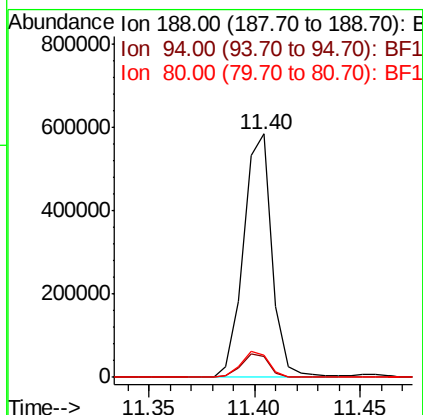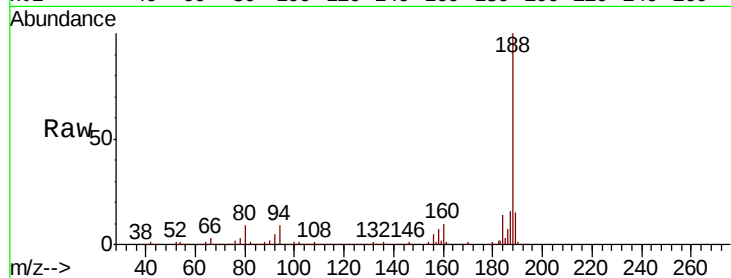

#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.04 min Scan# 2032
Delta R.T. -0.01 min
Lab File: BF115601.D
Acq: 16 Jul 2019 17:03

Tgt Ion:240 Resp: 348644
Ion Ratio Lower Upper
240 100
120 10.0 8.6 13.0
236 26.4 21.3 31.9

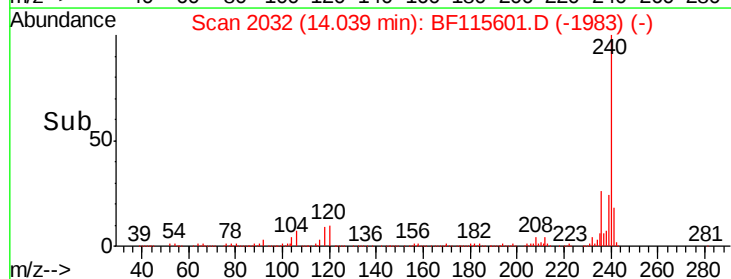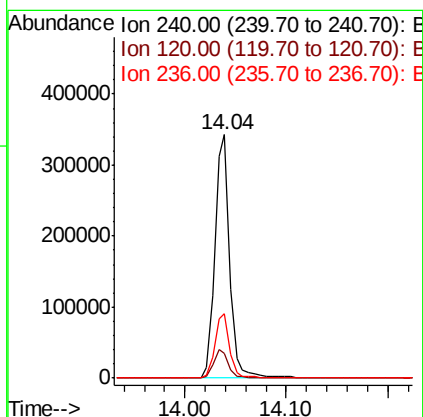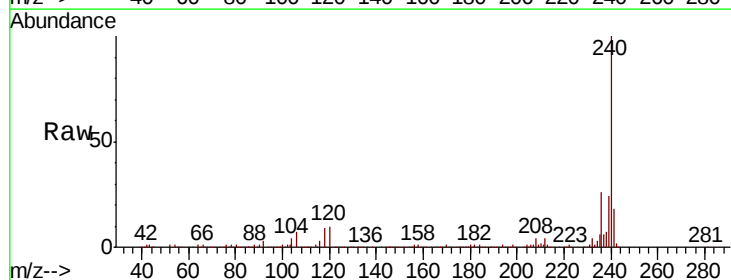

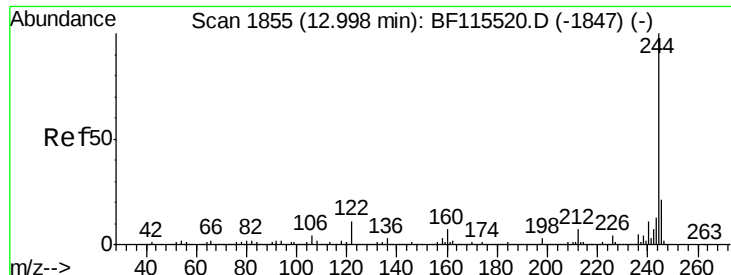

#79

Terphenyl-d14

Concen: 95.529 ng

RT: 12.99 min Scan# 1854

Delta R.T. -0.01 min

Lab File: BF115601.D

Acq: 16 Jul 2019 17:03

Instrument :

BNA_F

ClientSampleId :

CL-01-071219-B


Tot Ion:244 Resp: 1805023

Ion Ratio Lower Upper

244 100

212 6.8 6.0 9.0




122 9.9 8.6 12.8

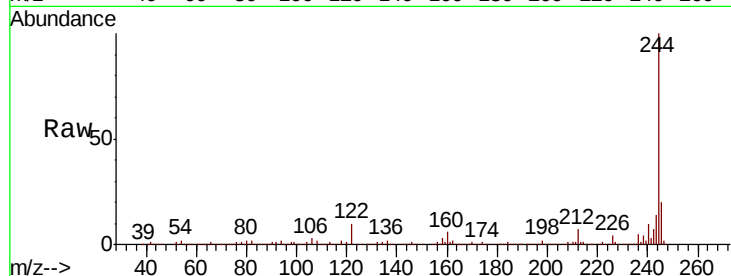

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

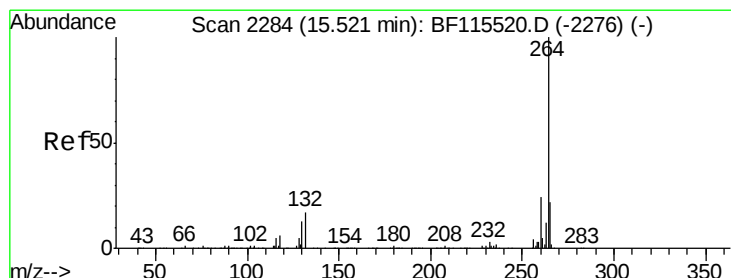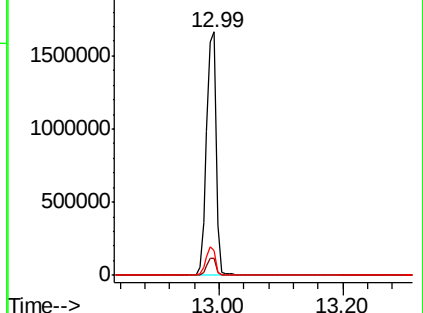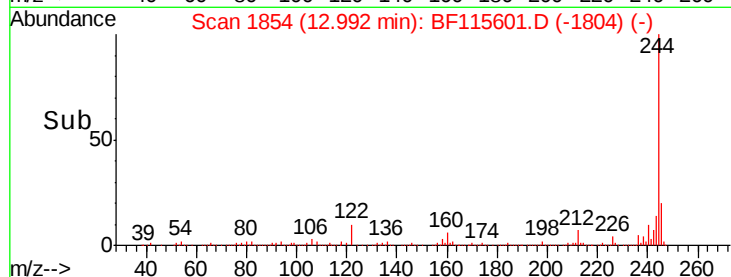

#87

Perylene-d12

Concen: 20.000 ng

RT: 15.51 min Scan# 2282

Delta R.T. -0.01 min

Lab File: BF115601.D

Acq: 16 Jul 2019 17:03


Tgt Ion:264 Resp: 399827

Ion Ratio Lower Upper

264 100

260 24.6 19.8 29.8

265 21.8 17.7 26.5

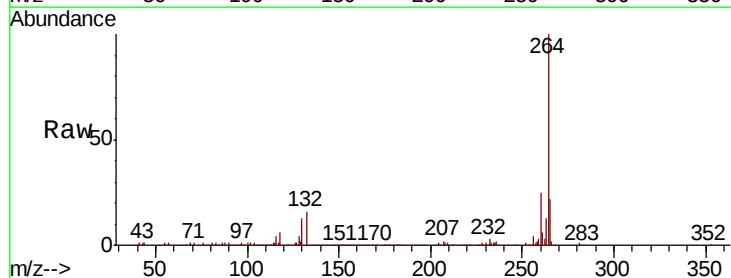

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

