

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF071619\
 Data File : BF115587.D
 Acq On : 16 Jul 2019 10:26
 Operator : HP/JU
 Sample : PB121365BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB121365BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF071219.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.299	24	36	45	rVB	234343	348668	6.12%	0.828%
2	5.516	578	583	586	rBV	3560437	4084887	71.68%	9.700%
3	6.516	746	753	755	rBV	3595175	4253826	74.65%	10.101%
4	6.657	771	777	780	rBV	4146799	4421987	77.60%	10.500%
5	6.881	811	815	819	rBV	1244967	1037832	18.21%	2.464%
6	7.039	837	842	846	rBV	3691952	3614049	63.42%	8.582%
7	7.439	904	910	913	rBV	2535671	2907213	51.02%	6.903%
8	8.163	1027	1033	1039	rBV	1401720	1341518	23.54%	3.185%
9	9.239	1209	1216	1219	rBV	4869597	5469993	95.99%	12.988%
10	9.916	1325	1331	1345	rBV	1499896	1582391	27.77%	3.757%
11	10.704	1459	1465	1487	rBV	2944837	3475563	60.99%	8.253%
12	11.404	1578	1584	1591	rBV	1804946	1657110	29.08%	3.935%
13	12.992	1848	1854	1857	rBV	5306675	5698485	100.00%	13.531%
14	14.039	2028	2032	2045	rBV	1150759	1228411	21.56%	2.917%
15	15.509	2276	2282	2303	rBV	533540	992449	17.42%	2.357%


Sum of corrected areas: 42114382

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF071619\
Data File : BF115587.D
Acq On : 16 Jul 2019 10:26
Operator : HP/JU
Sample : PB121365BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB121365BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF071219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

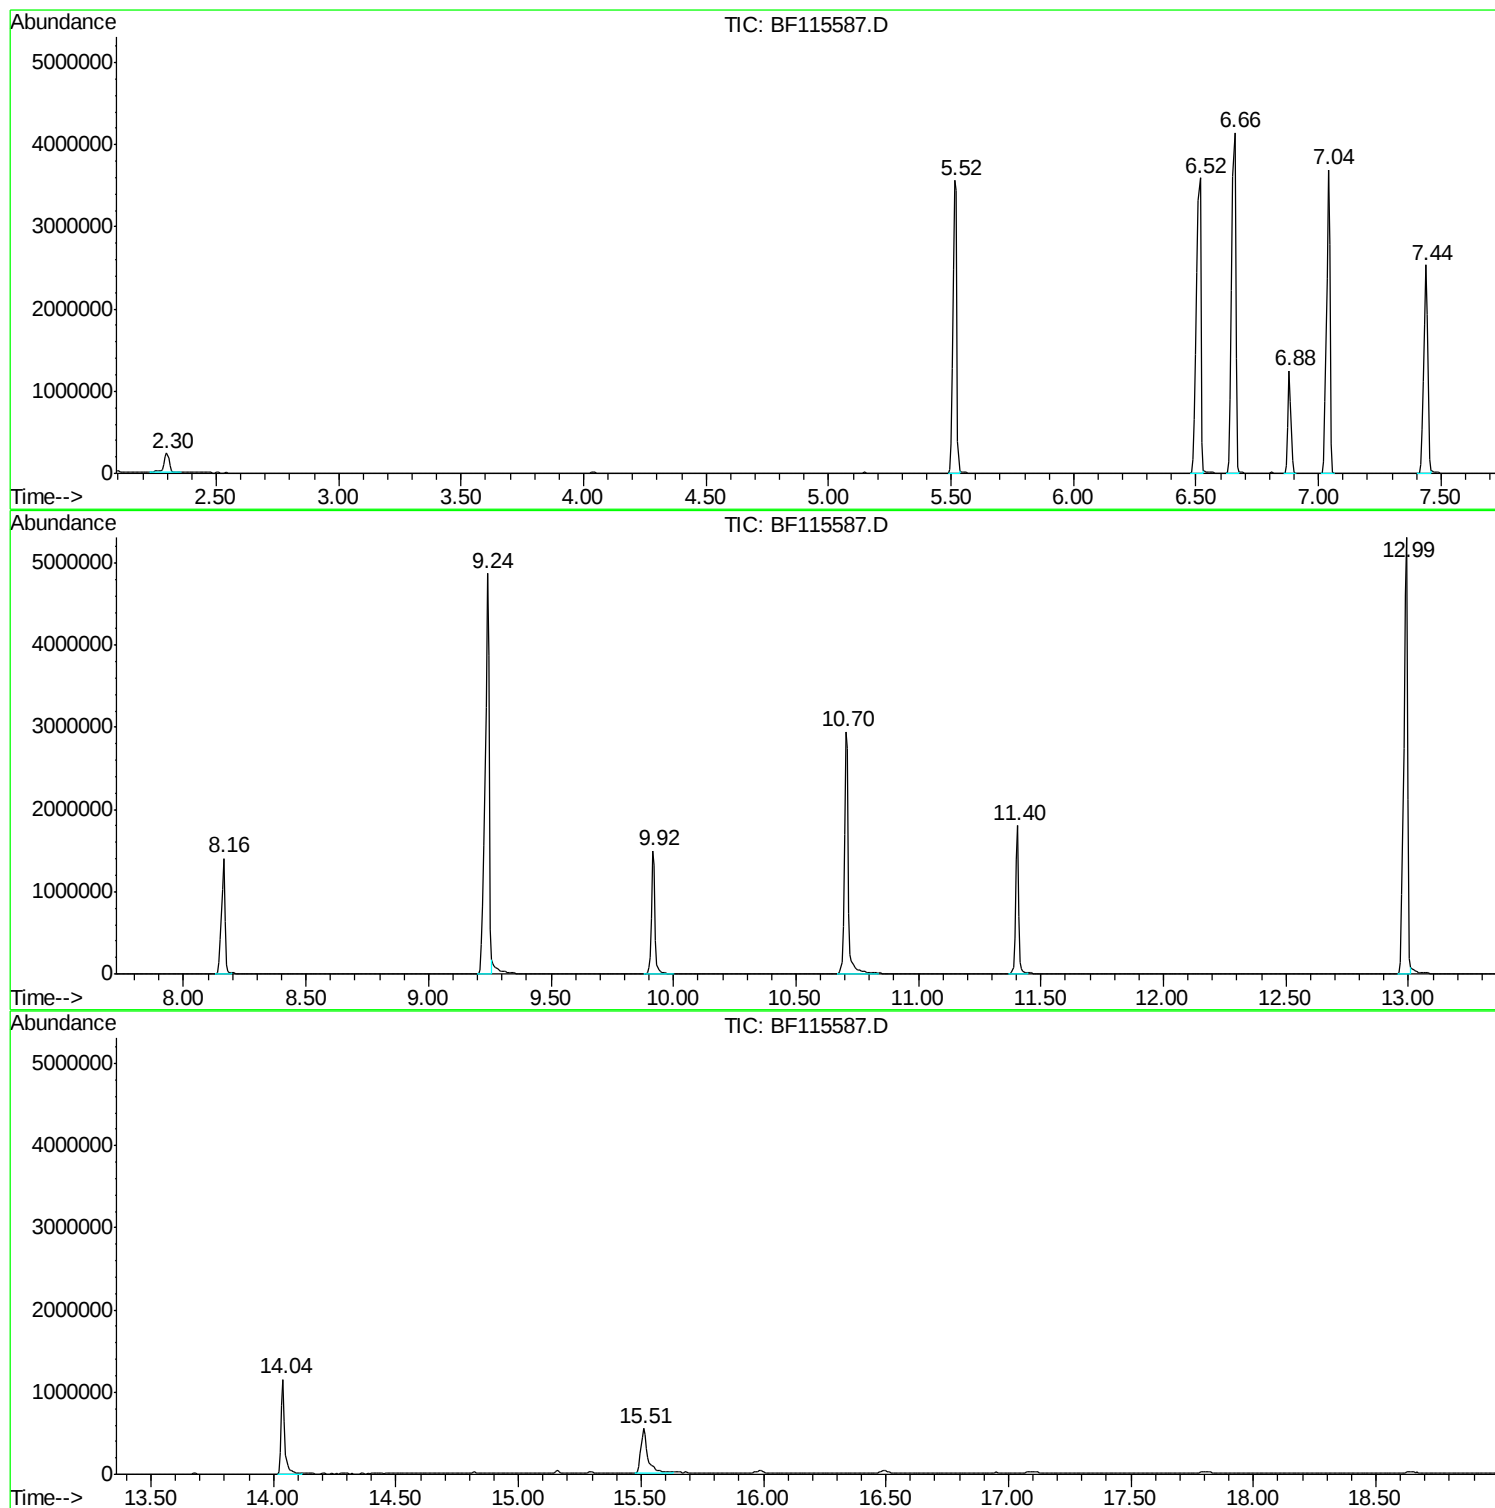

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF071619\
Data File : BF115587.D
Acq On : 16 Jul 2019 10:26
Operator : HP/JU
Sample : PB121365BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB121365BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF071219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.30	6.72 ng	348668	1,4-Dichlorobenzene-d4	6.88

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	83
2		2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	56
3		Silane, ethyltrimethyl-	102	C5H14Si	003439-38-1	33
4		Pentane, 3-methoxy-	102	C6H14O	036839-67-5	23
5		Acetamide, N-ethyl-	87	C4H9NO	000625-50-3	10

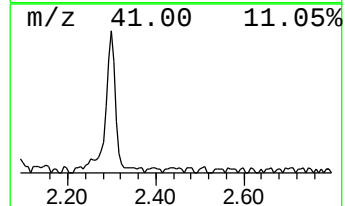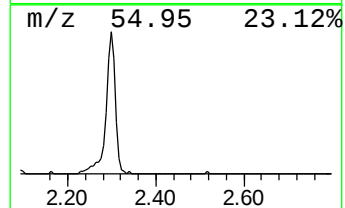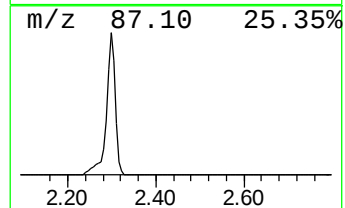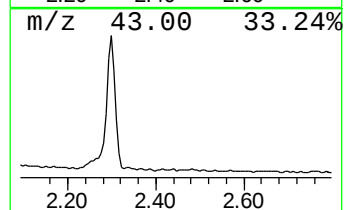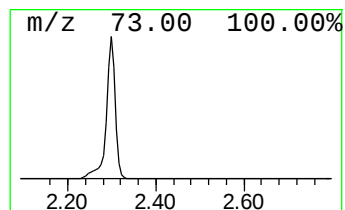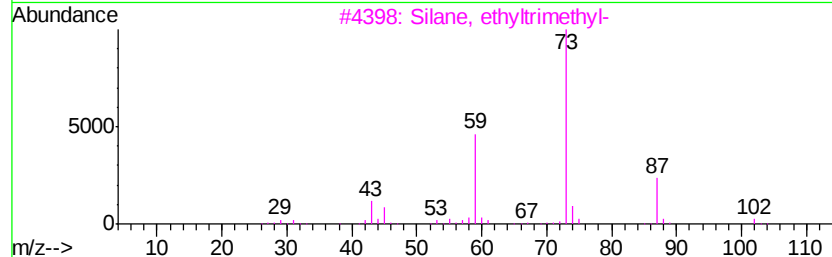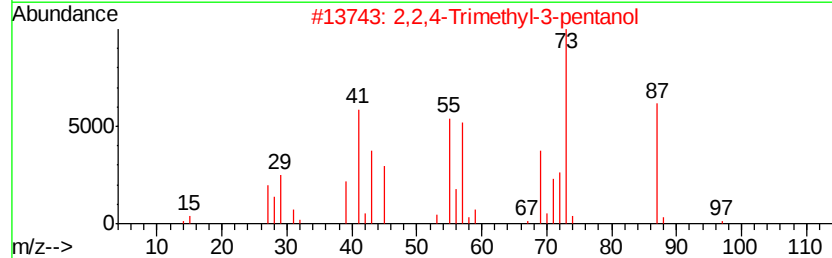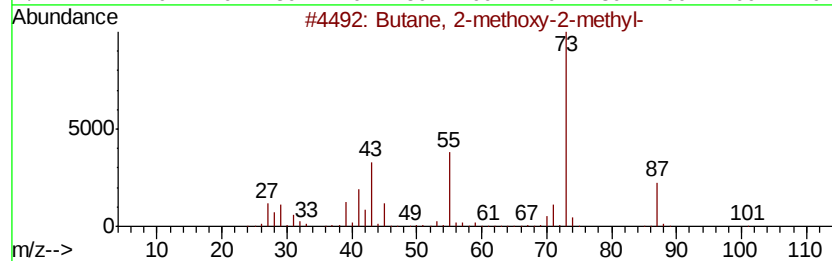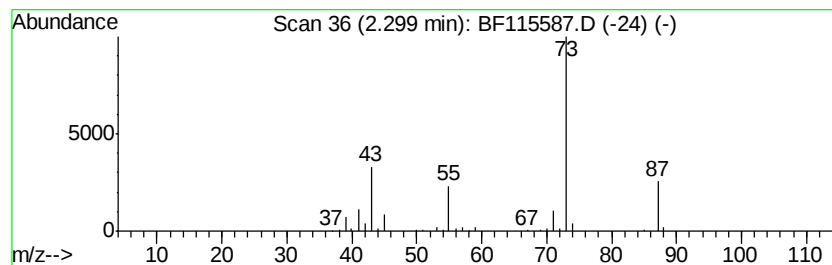

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF071619\
Data File : BF115587.D
Acq On : 16 Jul 2019 10:26
Operator : HP/JU
Sample : PB121365BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB121365BL









Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF071219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown6.66 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.66	85.22 ng	4421990	1,4-Dichlorobenzene-d4	6.88

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		Tranvlcypropine-propionyl	189	C12H15NO	1000123-86-3	12
3		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	9
4		Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9
5		4-Chloro-2-fluoro-pyrimidine	132	C4H2ClFN2	051422-00-5	9

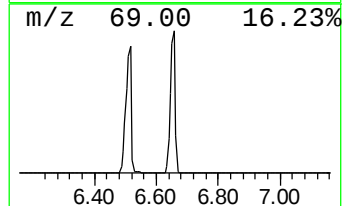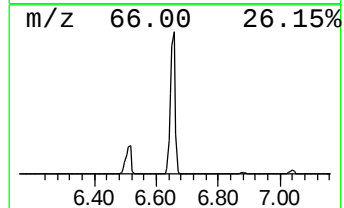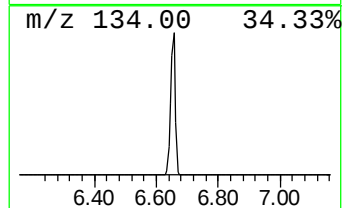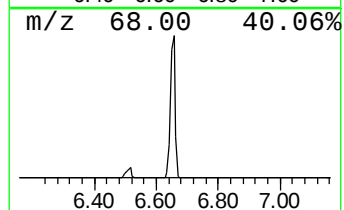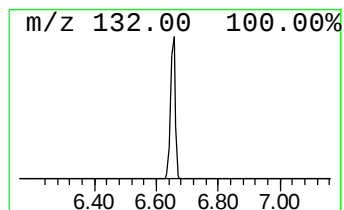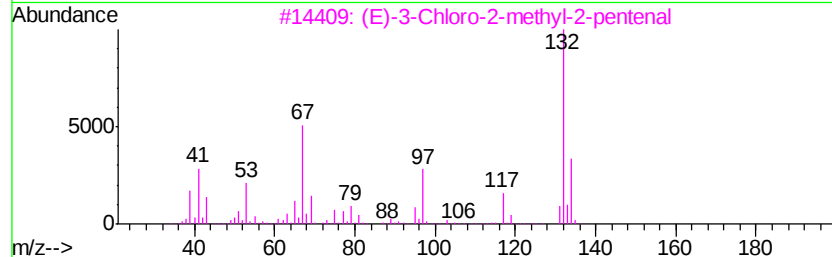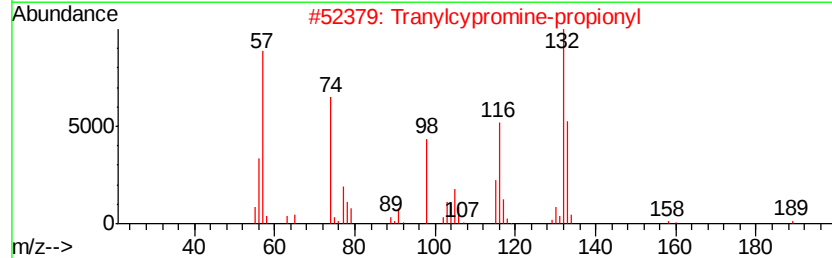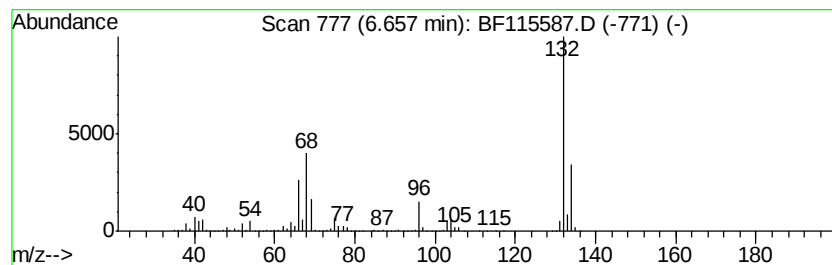

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF071619\
Data File : BF115587.D
Acq On : 16 Jul 2019 10:26
Operator : HP/JU
Sample : PB121365BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB121365BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF071219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-methoxy...	2.30	6.7	ng	348668	1	6.88	1037830	20.0
unknown6.66	6.66	85.2	ng	4421990	1	6.88	1037830	20.0