

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF071619\
 Data File : BF115591.D
 Acq On : 16 Jul 2019 12:13
 Operator : HP/JU
 Sample : PB121222BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB121222BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF071219.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.522	578	584	587	rBV	4213030	4849930	86.84%	11.460%
2	6.510	746	752	755	rBV	3437833	4348584	77.87%	10.275%
3	6.657	771	777	780	rBV	4021380	4470449	80.05%	10.563%
4	6.881	811	815	819	rBV	1208962	992969	17.78%	2.346%
5	7.039	837	842	845	rBV	3867962	3703707	66.32%	8.752%
6	7.439	904	910	913	rBV	2524879	2959183	52.99%	6.992%
7	8.163	1027	1033	1036	rBV	1249121	1256448	22.50%	2.969%
8	9.239	1209	1216	1219	rBV	4881613	5584585	100.00%	13.196%
9	9.916	1325	1331	1346	rBV	1443137	1480916	26.52%	3.499%
10	10.704	1458	1465	1491	rBV	2868367	3244270	58.09%	7.666%
11	11.404	1577	1584	1600	rBV	1581288	1578607	28.27%	3.730%
12	12.992	1848	1854	1857	rBV	5254435	5548757	99.36%	13.111%
13	14.039	2027	2032	2043	rBV	1048831	1148308	20.56%	2.713%
14	15.509	2276	2282	2300	rBV	494323	920892	16.49%	2.176%
15	15.980	2357	2362	2371	rVB	59719	90429	1.62%	0.214%
16	16.492	2443	2449	2458	rVB2	47971	85014	1.52%	0.201%
17	17.092	2546	2551	2558	rVB2	28383	57483	1.03%	0.136%


Sum of corrected areas: 42320531

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF071619\
Data File : BF115591.D
Acq On : 16 Jul 2019 12:13
Operator : HP/JU
Sample : PB121222BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB121222BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF071219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

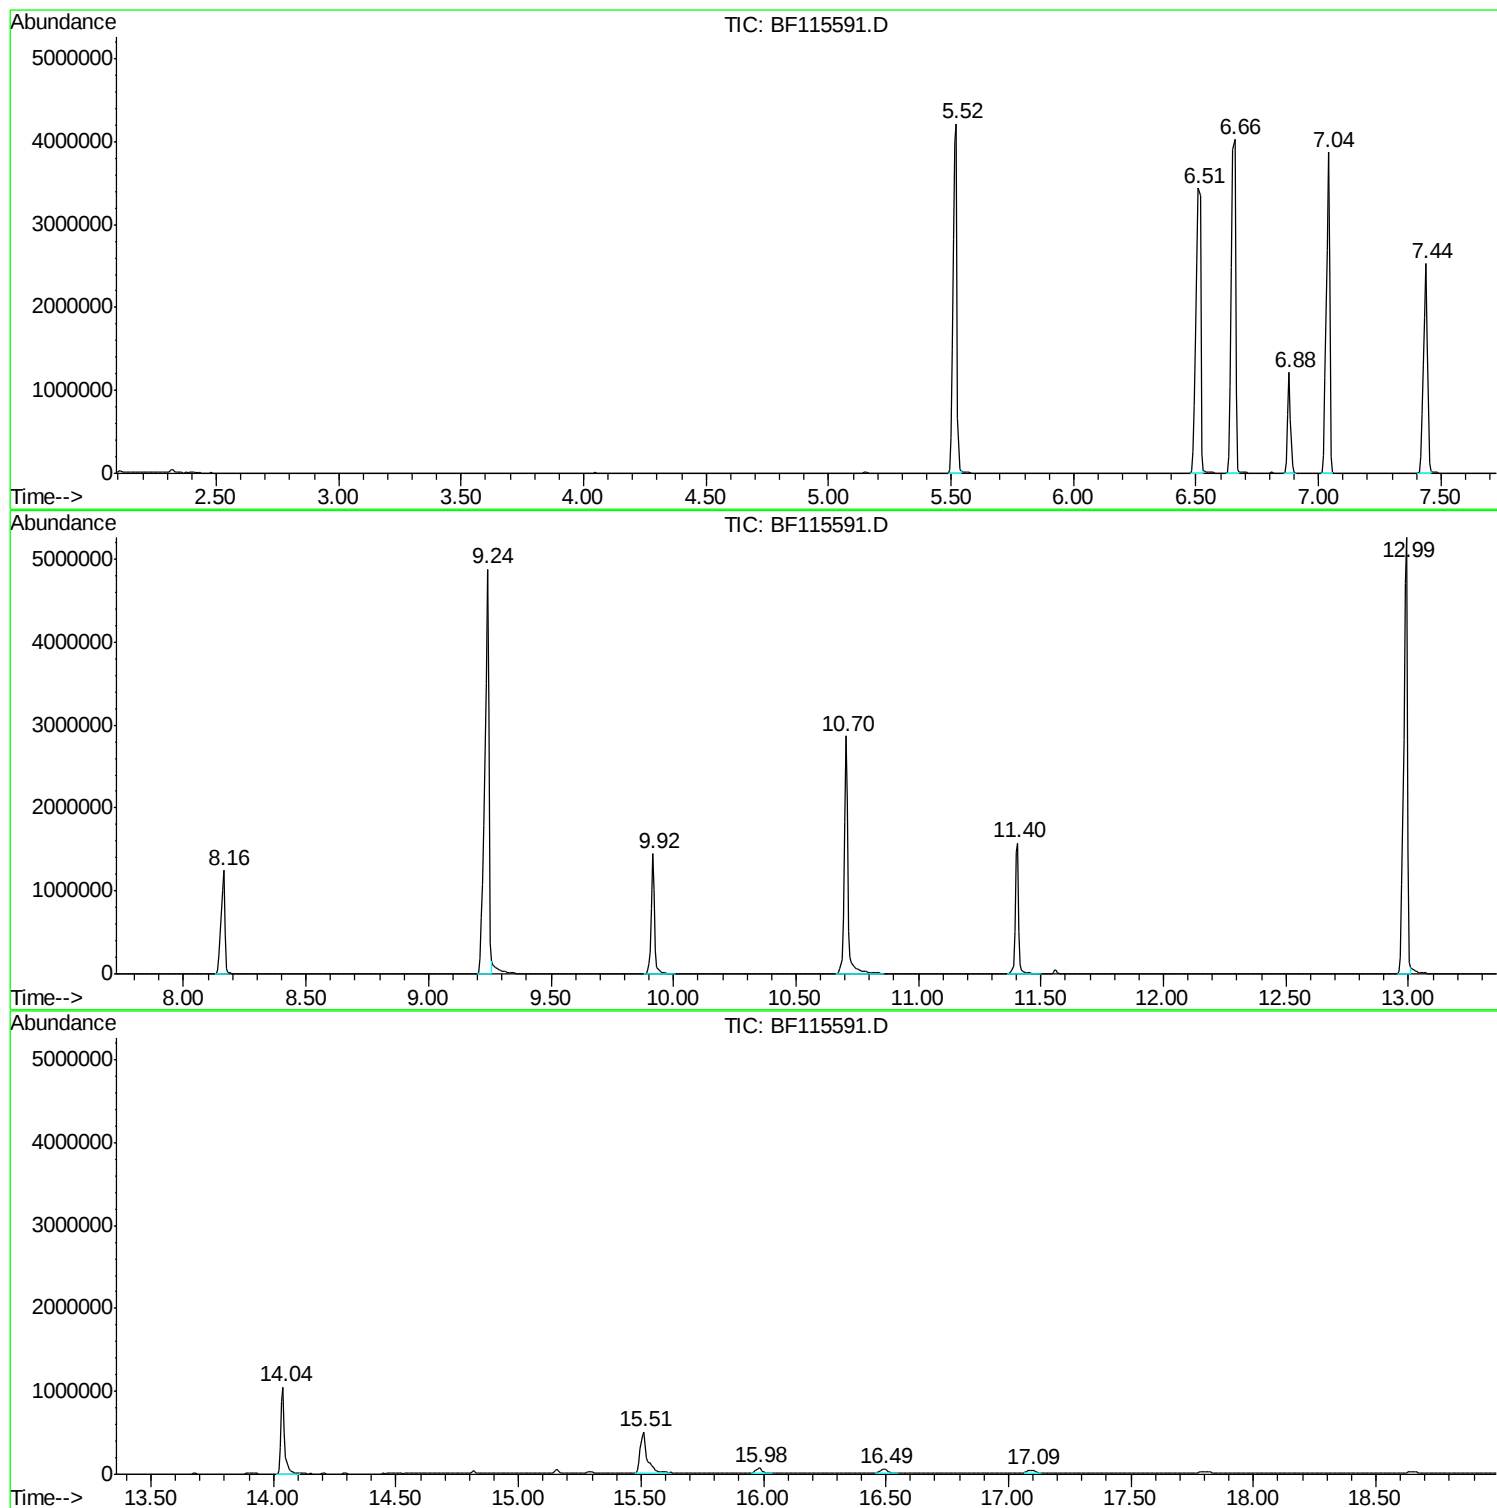

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF071619\
Data File : BF115591.D
Acq On : 16 Jul 2019 12:13
Operator : HP/JU
Sample : PB121222BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB121222BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF071219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.66 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.66	90.04 ng	4470450	1,4-Dichlorobenzene-d4	6.88

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	1,3-Cyclopentanedione, 2-chloro-	132	C5H5ClO2	014203-19-1	37
2		3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
3		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	16
4		Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	12
5		5-Aminoindole	132	C8H8N2	005192-03-0	12

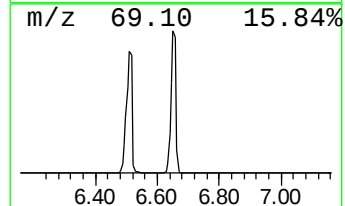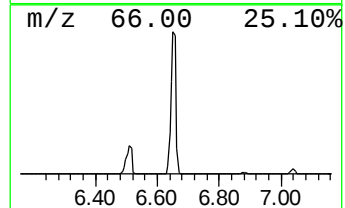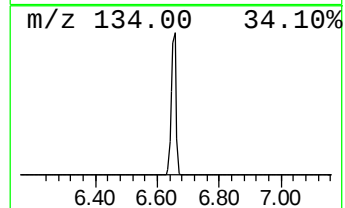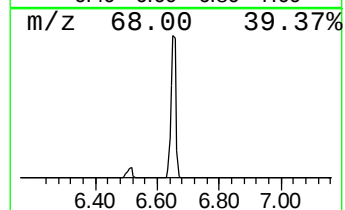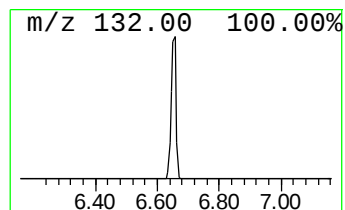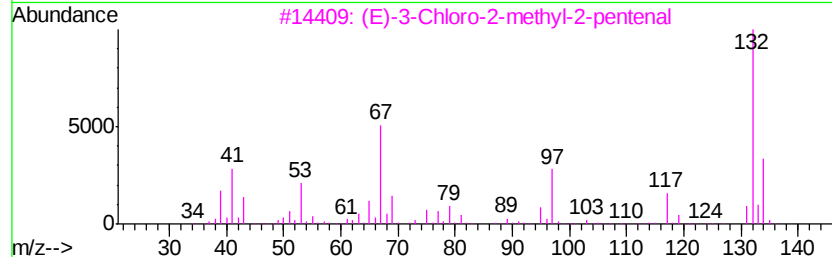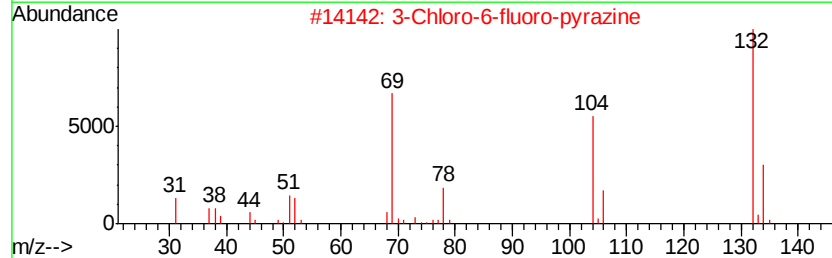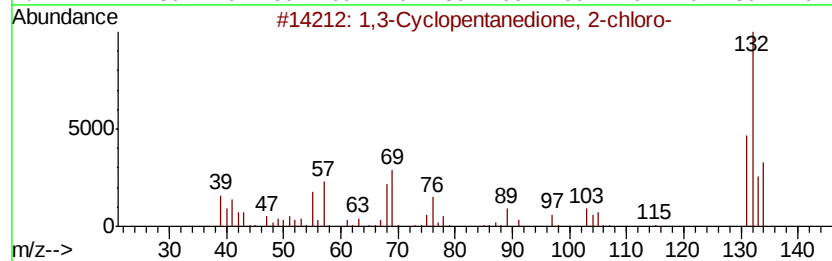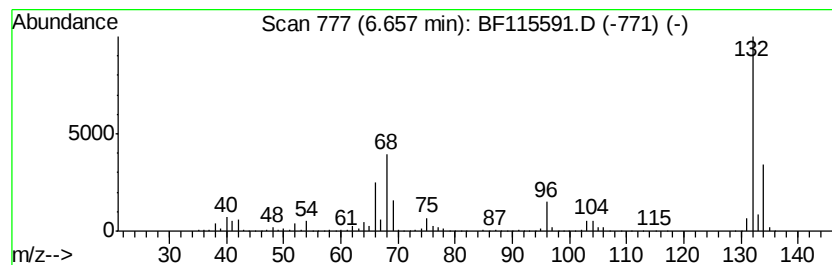

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF071619\
Data File : BF115591.D
Acq On : 16 Jul 2019 12:13
Operator : HP/JU
Sample : PB121222BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB121222BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF071219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.66	6.66	90.0	ng	4470450	1	6.88	992969	20.0