

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF071619\
 Data File : BF115593.D
 Acq On : 16 Jul 2019 13:06
 Operator : HP/JU
 Sample : PB121412BL
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB121412BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF071219.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.287	23	34	40	rVB	161426	233036	4.01%	0.491%
2	5.516	578	583	586	rBV	4351652	5039816	86.76%	10.614%
3	6.516	746	753	755	rBV	4366550	5325154	91.67%	11.215%
4	6.657	771	777	780	rBV	4857244	5338213	91.89%	11.242%
5	6.881	811	815	819	rBV	1560142	1258135	21.66%	2.650%
6	7.040	837	842	845	rBV	4507921	4395006	75.66%	9.256%
7	7.440	904	910	913	rBV	3151063	3607363	62.10%	7.597%
8	8.163	1027	1033	1036	rBV	1637536	1604450	27.62%	3.379%
9	9.239	1209	1216	1219	rBV	5181275	5682141	97.81%	11.967%
10	9.916	1325	1331	1355	rBV	1652052	1610801	27.73%	3.392%
11	10.704	1459	1465	1499	rBV	3110182	3699863	63.69%	7.792%
12	11.404	1578	1584	1592	rBV	1738341	1694498	29.17%	3.569%
13	12.992	1848	1854	1857	rBV	5417199	5809158	100.00%	12.234%
14	14.039	2027	2032	2051	rBV	1039078	1256592	21.63%	2.646%
15	15.510	2276	2282	2300	rBV	484936	928340	15.98%	1.955%


Sum of corrected areas: 47482566

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF071619\
Data File : BF115593.D
Acq On : 16 Jul 2019 13:06
Operator : HP/JU
Sample : PB121412BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB121412BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF071219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

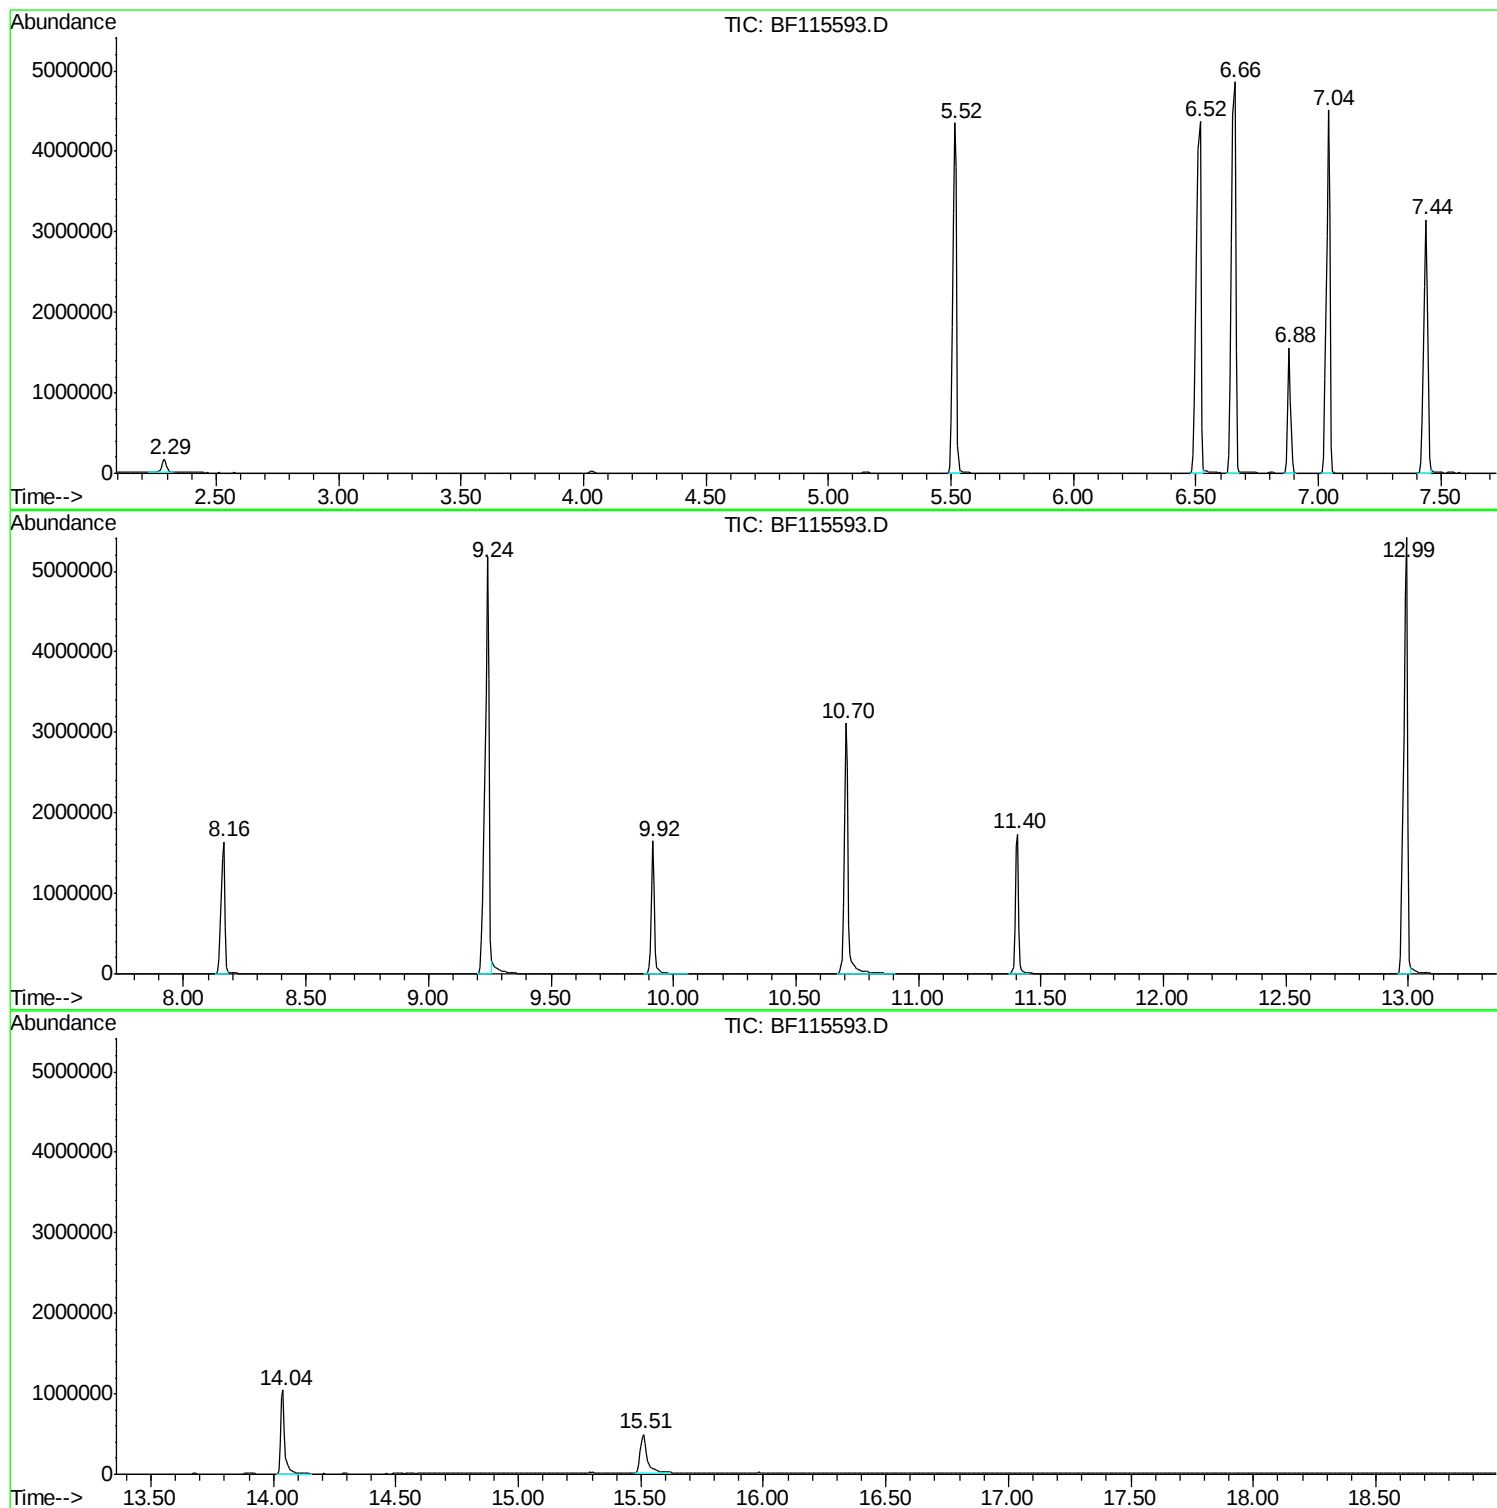

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF071619\
Data File : BF115593.D
Acq On : 16 Jul 2019 13:06
Operator : HP/JU
Sample : PB121412BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB121412BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF071219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.29	3.70 ng	233036	1,4-Dichlorobenzene-d4	6.88

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	78
2			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	40
3			Silane, ethyltrimethyl-	102	C5H14Si	003439-38-1	36
4			Pentane, 3-methoxy-	102	C6H14O	036839-67-5	17
5			3-Hexanol, 2-methyl-	116	C7H16O	000617-29-8	17

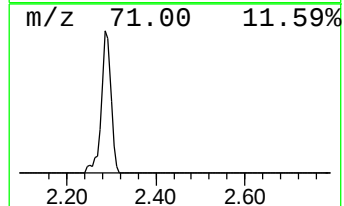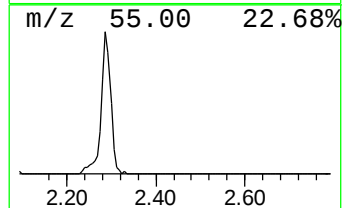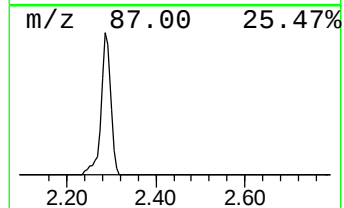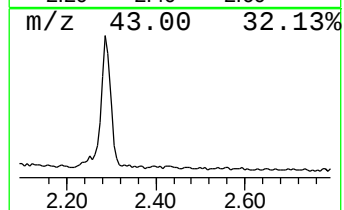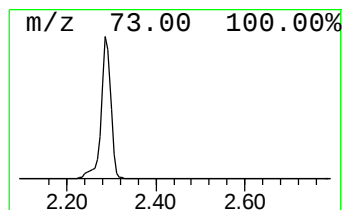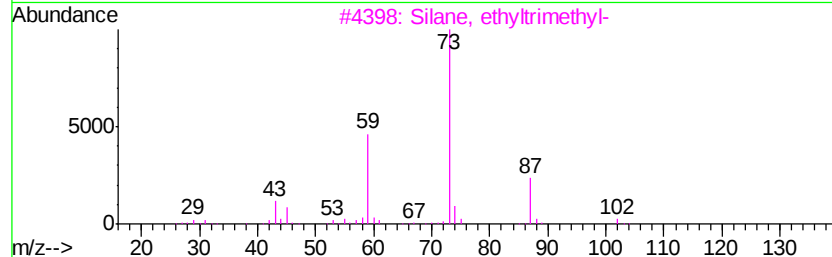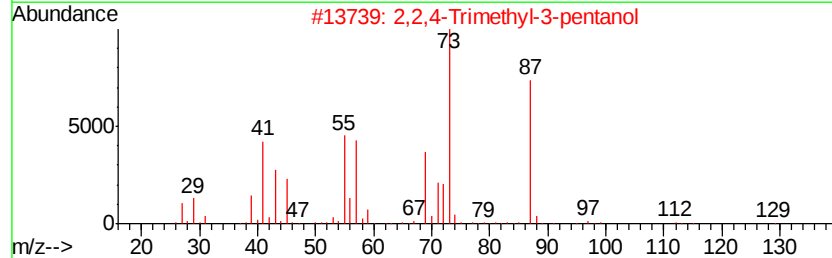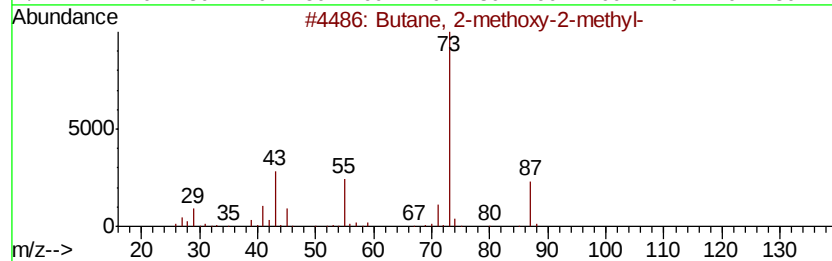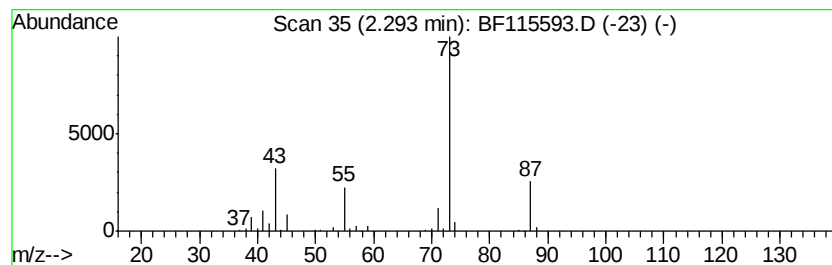

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF071619\
Data File : BF115593.D
Acq On : 16 Jul 2019 13:06
Operator : HP/JU
Sample : PB121412BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB121412BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF071219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown6.66 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.66	84.86 ng	5338210	1,4-Dichlorobenzene-d4	6.88

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			1,3-Cyclopentanedione, 2-chloro-	132	C5H5ClO2	014203-19-1	47
2			Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	12
3			5-Aminoindole	132	C8H8N2	005192-03-0	12
4			4-Chloro-2-fluoro-pyrimidine	132	C4H2ClFN2	051422-00-5	9
5			Xenon	132	Xe	007440-63-3	9

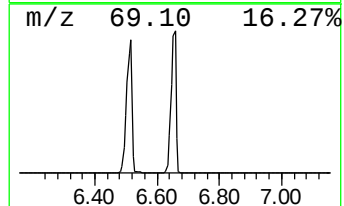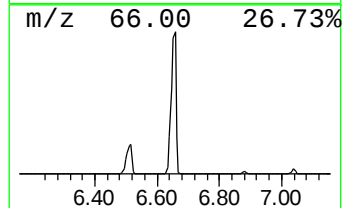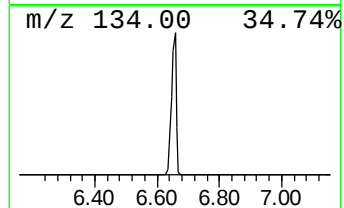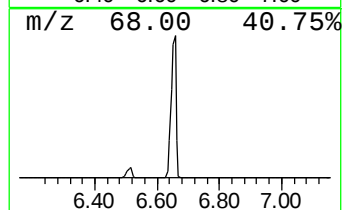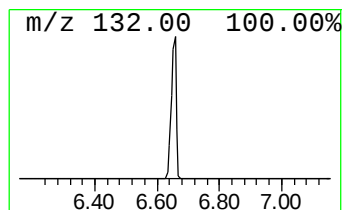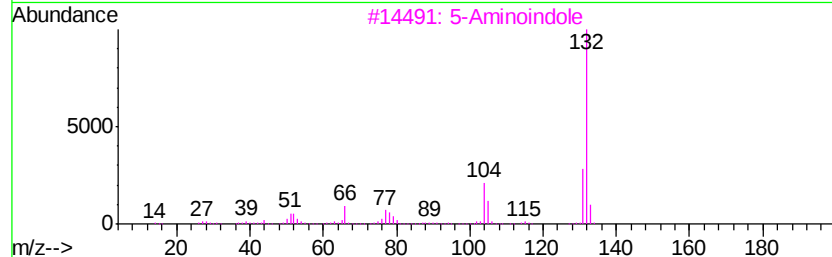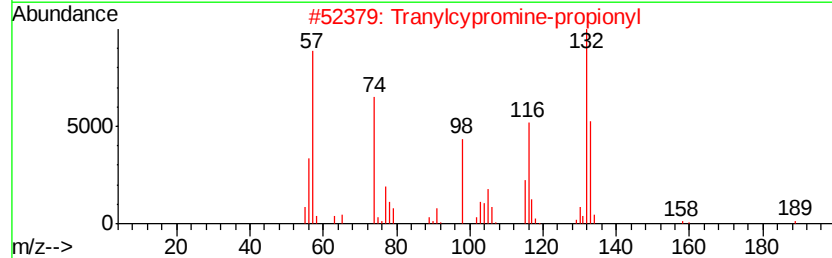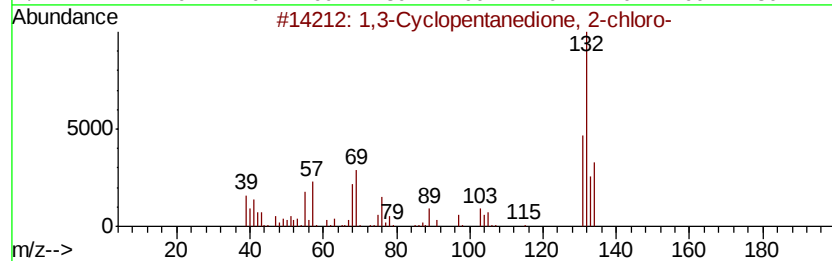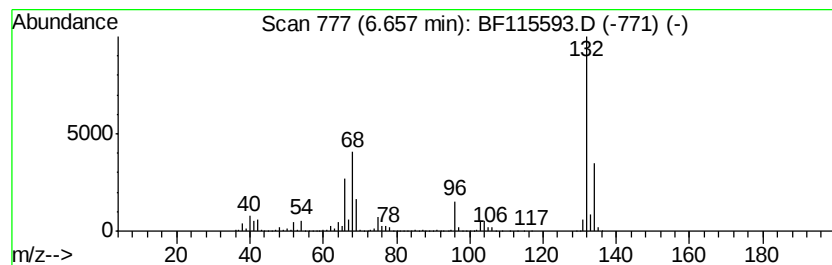

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF071619\
Data File : BF115593.D
Acq On : 16 Jul 2019 13:06
Operator : HP/JU
Sample : PB121412BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB121412BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF071219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---			
					#	RT	Resp	Conc
Butane, 2-methoxy...	2.29	3.7	ng	233036	1	6.88	1258140	20.0
unknown6.66	6.66	84.9	ng	5338210	1	6.88	1258140	20.0