


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF071619\
 Data File : BF115595.D
 Acq On : 16 Jul 2019 14:15
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF071219.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jul 12 14:03:52 2019

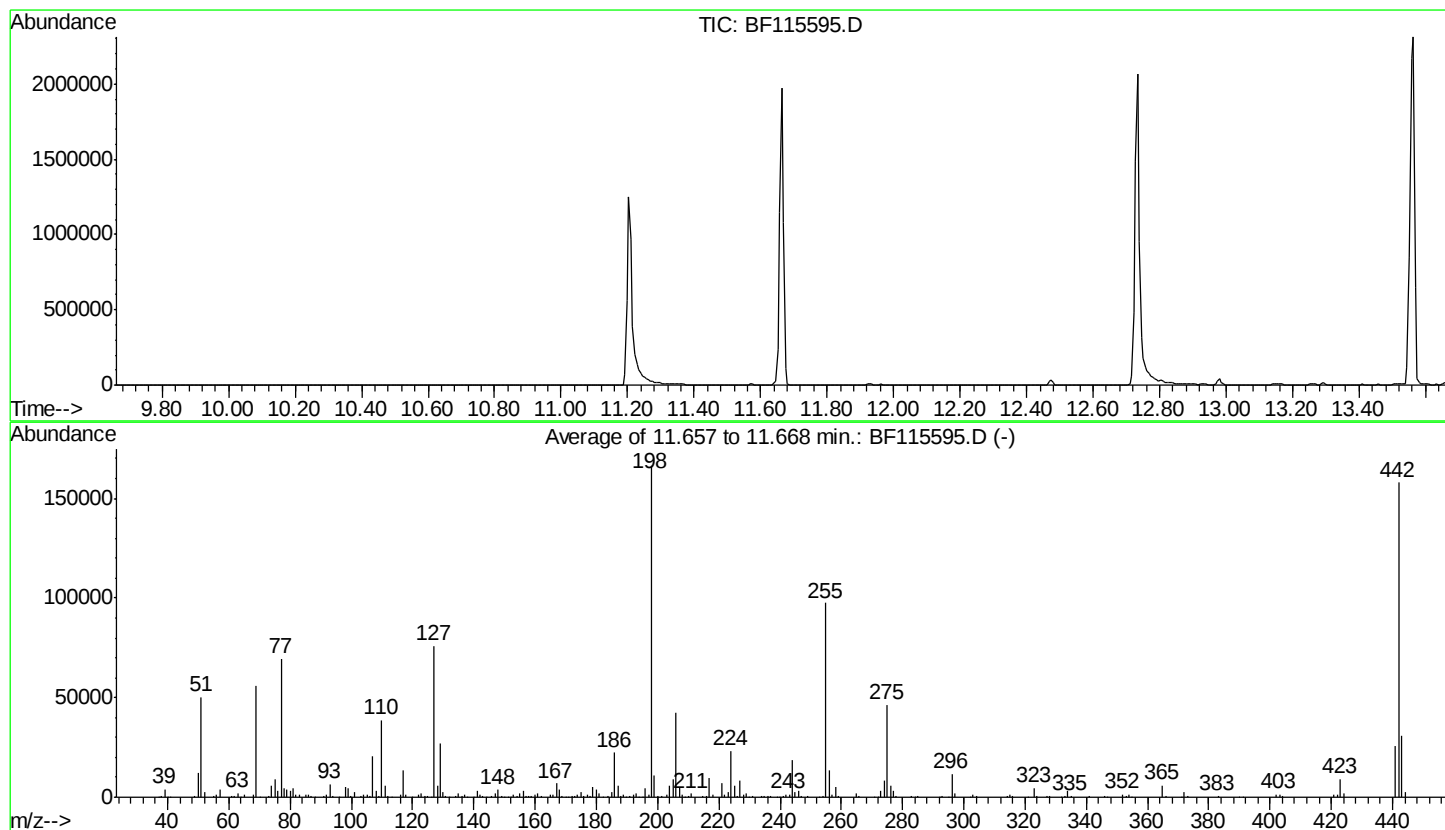

AutoFind: Scans 1627, 1628, 1629; Background Corrected with Scan 1621

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.2	50197	PASS
68	69	0.00	2	1.8	988	PASS
69	198	0.00	100	33.5	55829	PASS
70	69	0.00	2	0.5	298	PASS
127	198	10	80	45.6	75858	PASS
197	198	0.00	2	0.6	1068	PASS
198	198	100	100	100.0	166434	PASS
199	198	5	9	6.5	10875	PASS
275	198	10	60	28.0	46597	PASS
365	198	1	100	3.5	5811	PASS
441	198	0.01	100	15.3	25512	PASS
442	198	50	100	94.9	157970	PASS
443	442	15	24	19.4	30642	PASS