
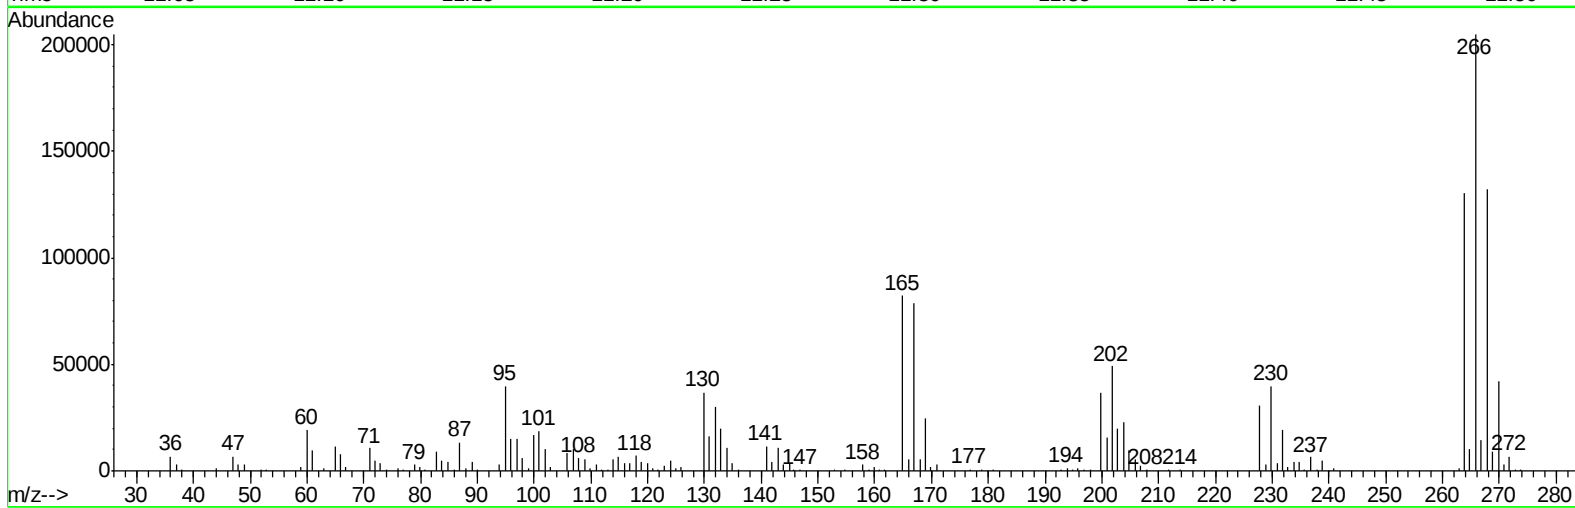


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF071719\
Data File : BF115620.D
Acq On : 17 Jul 2019 12:42
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 18 09:37:29 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF071219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 12 14:03:52 2019
Response via : Initial Calibration

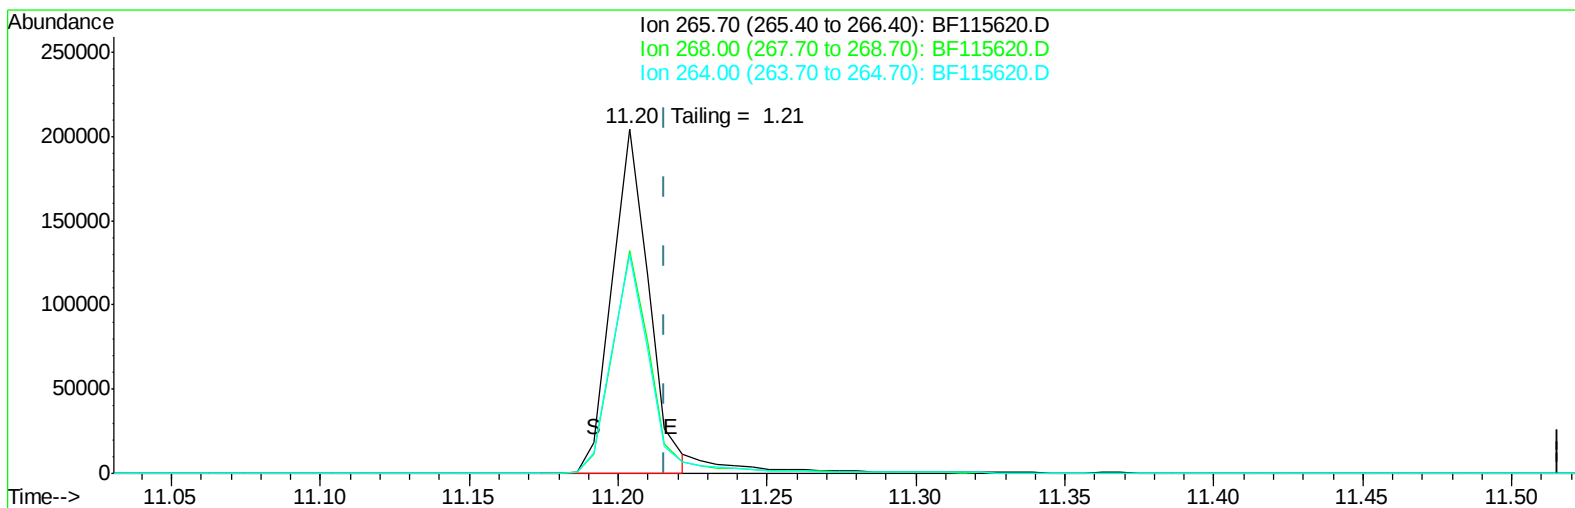

TIC: BF115620.D

(70) Pentachlorophenol (C)



11.204min (-0.012) 35300.67ng

response 187938

Ion	Exp%	Act%
265.70	100	100
268.00	64.50	64.59
264.00	63.30	63.50
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF071719\
Data File : BF115620.D
Acq On : 17 Jul 2019 12:42
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 18 09:37:29 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF071219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 12 14:03:52 2019
Response via : Initial Calibration

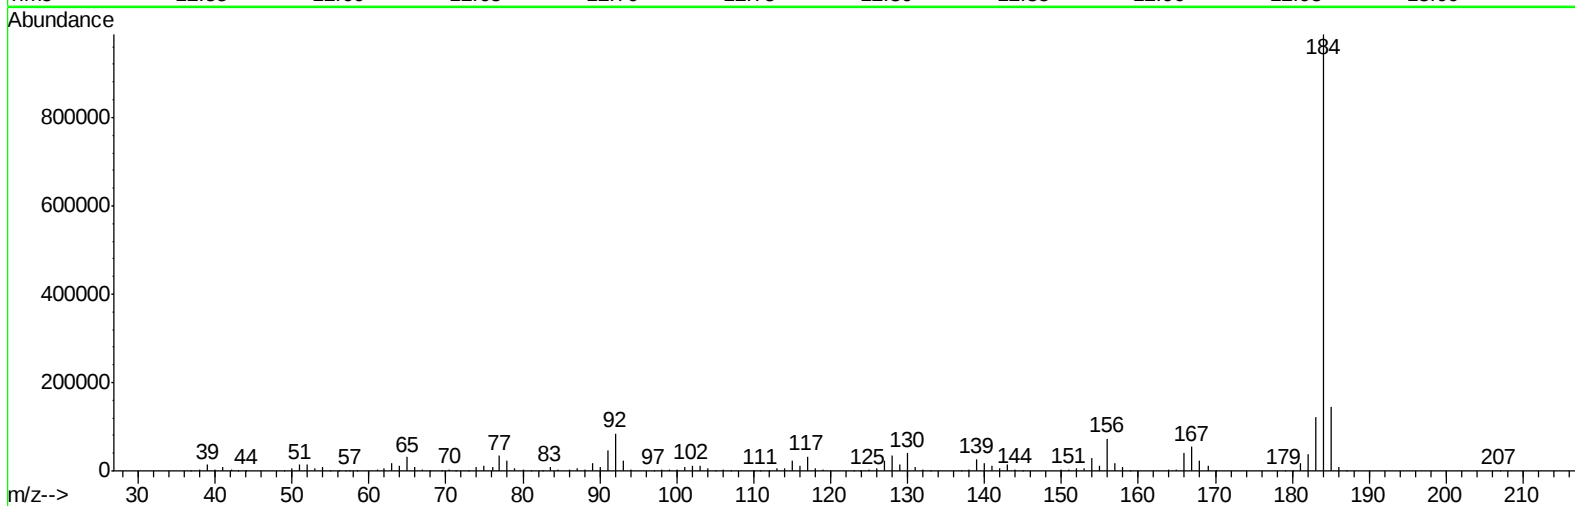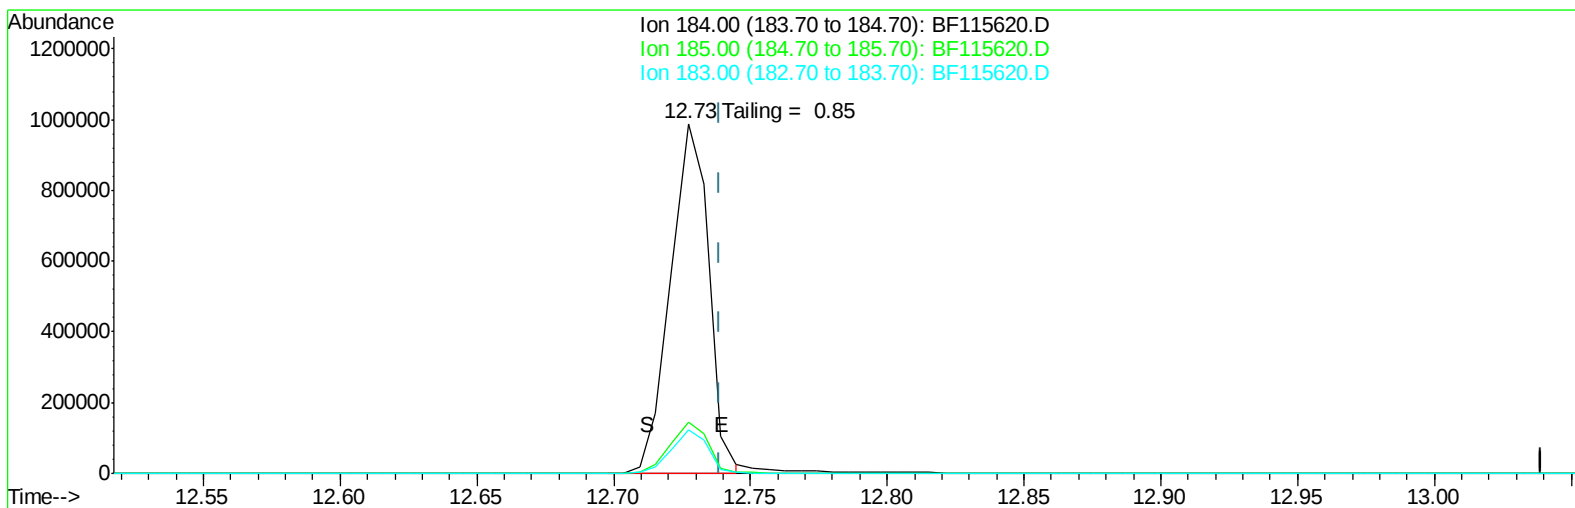

TIC: BF115620.D

(77) Benzidine

12.727min (-0.012) 0.00ng

response 990449

Ion	Exp%	Act%
184.00	100	100
185.00	15.00	14.58
183.00	11.60	12.31
0.00	0.00	0.00