


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF071719\
 Data File : BF115620.D
 Acq On : 17 Jul 2019 12:42
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF071219.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jul 12 14:03:52 2019

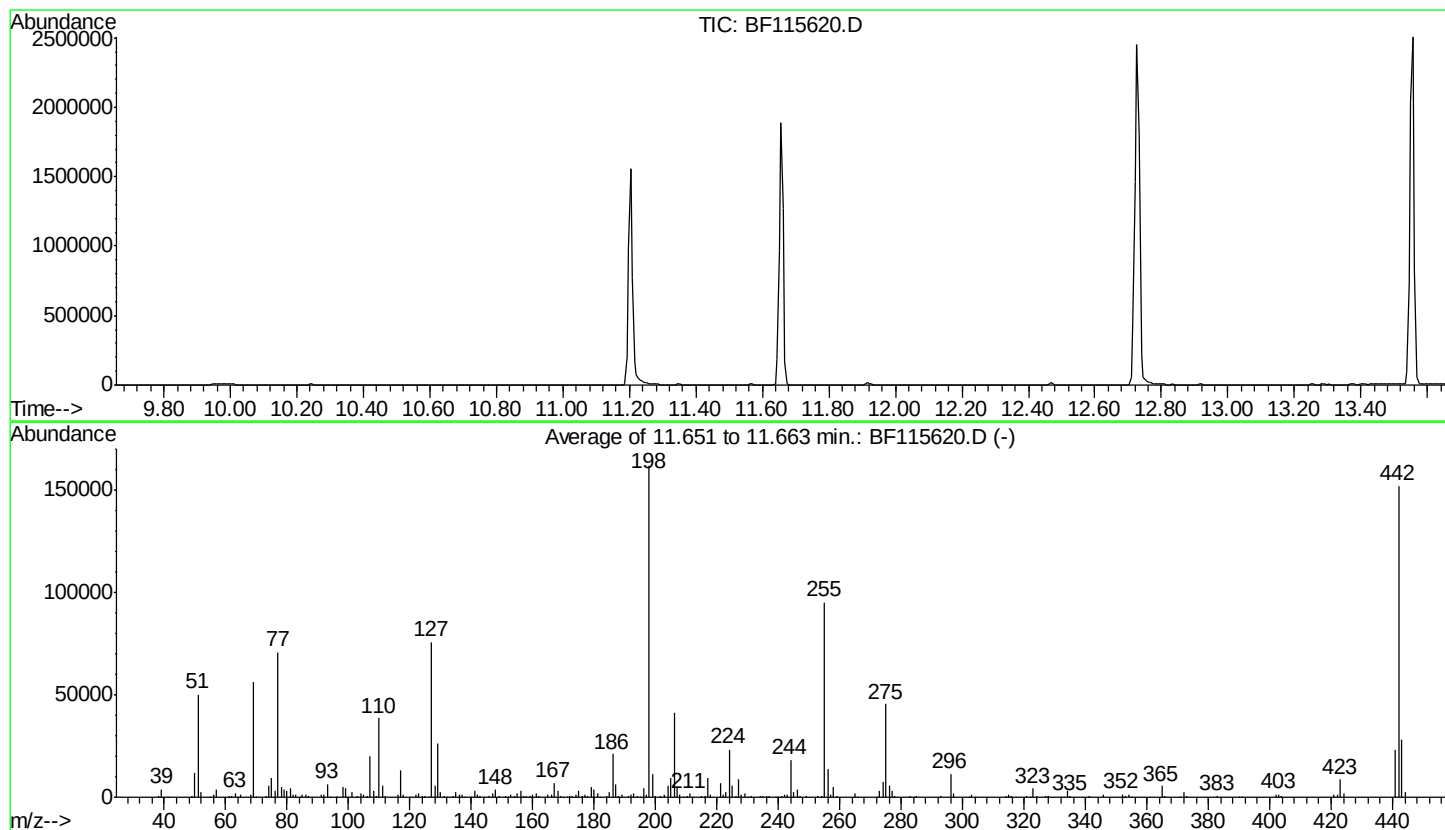

AutoFind: Scans 1626, 1627, 1628; Background Corrected with Scan 1621

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.9	50144	PASS
68	69	0.00	2	1.7	971	PASS
69	198	0.00	100	34.8	56397	PASS
70	69	0.00	2	0.3	160	PASS
127	198	10	80	46.9	75970	PASS
197	198	0.00	2	0.6	1004	PASS
198	198	100	100	100.0	162029	PASS
199	198	5	9	6.8	11021	PASS
275	198	10	60	28.1	45552	PASS
365	198	1	100	3.4	5491	PASS
441	198	0.01	100	14.5	23472	PASS
442	198	50	100	94.0	152320	PASS
443	442	15	24	18.5	28118	PASS