


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071723\
Data File : BF134313.D
Acq On : 17 Jul 2023 12:52
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Jul 14 22:51:27 2023

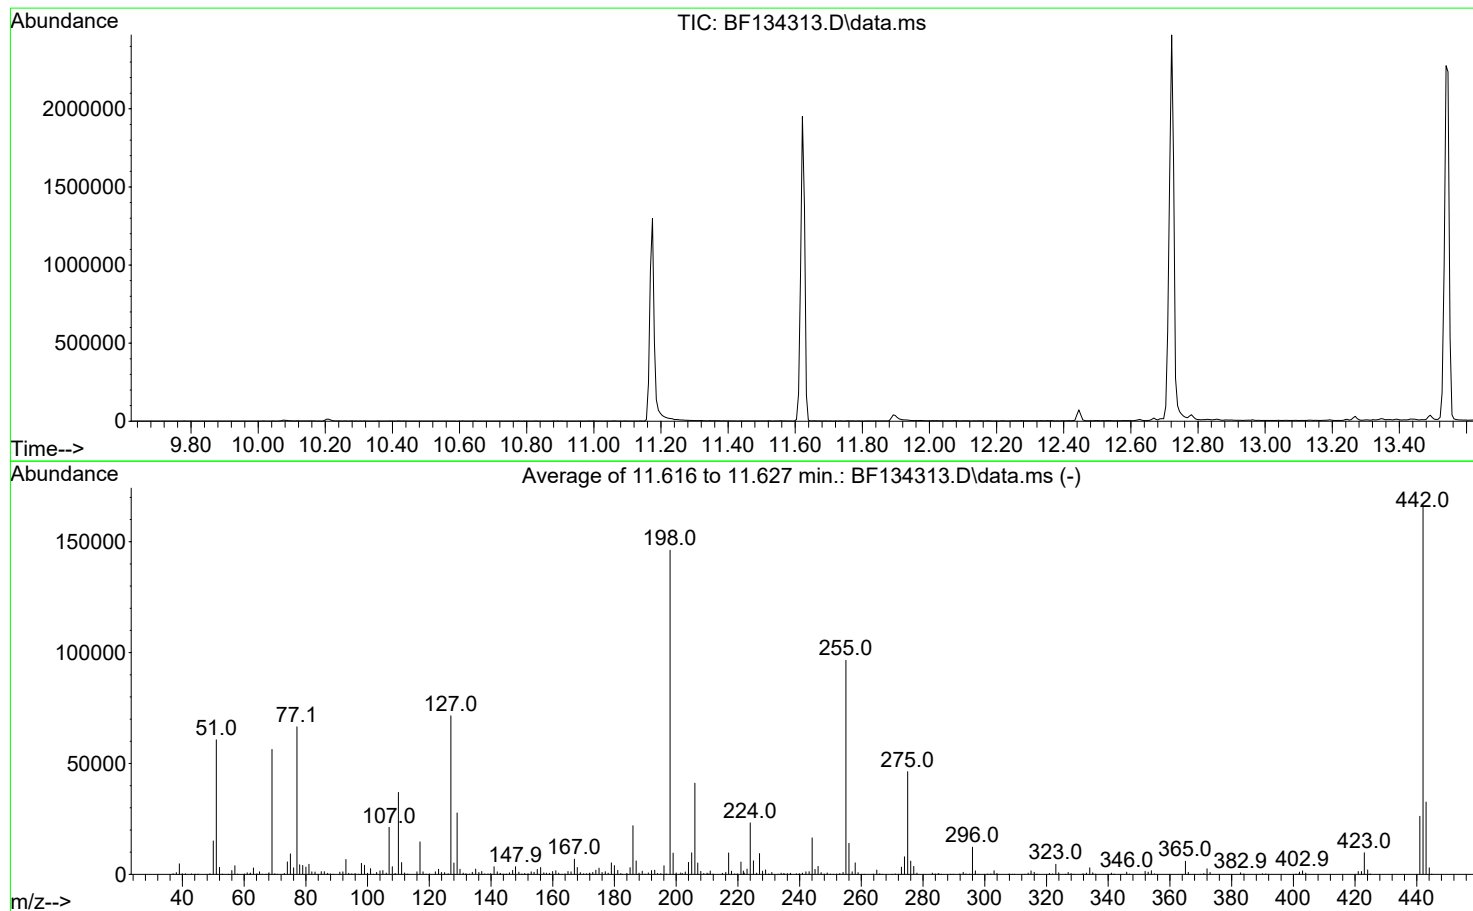




AutoFind: Scans 1620, 1621, 1622; Background Corrected with Scan 1615

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.5	60672	PASS
68	69	0.00	2	1.2	698	PASS
69	198	0.00	100	38.6	56363	PASS
70	69	0.00	2	0.6	313	PASS
127	198	10	80	49.0	71541	PASS
197	198	0.00	2	0.2	246	PASS
198	198	100	100	100.0	146144	PASS
199	198	5	9	6.6	9631	PASS
275	198	10	60	31.7	46293	PASS
365	198	1	100	4.1	5930	PASS
441	198	0.01	100	17.9	26186	PASS
442	442	50	100	100.0	165877	PASS
443	442	15	24	19.7	32619	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071723\
 Data File : BF134313.D
 Acq On : 17 Jul 2023 12:52
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Jul 17 16:23:29 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 14 22:51:27 2023
 Response via : Initial Calibration

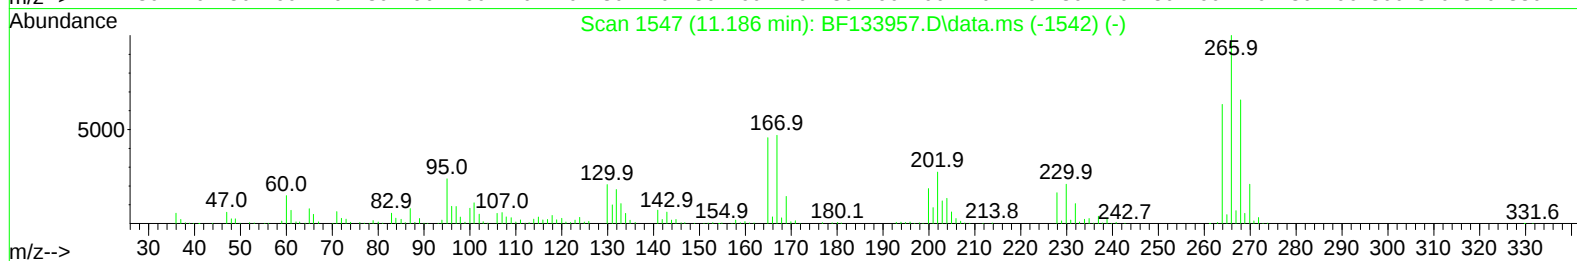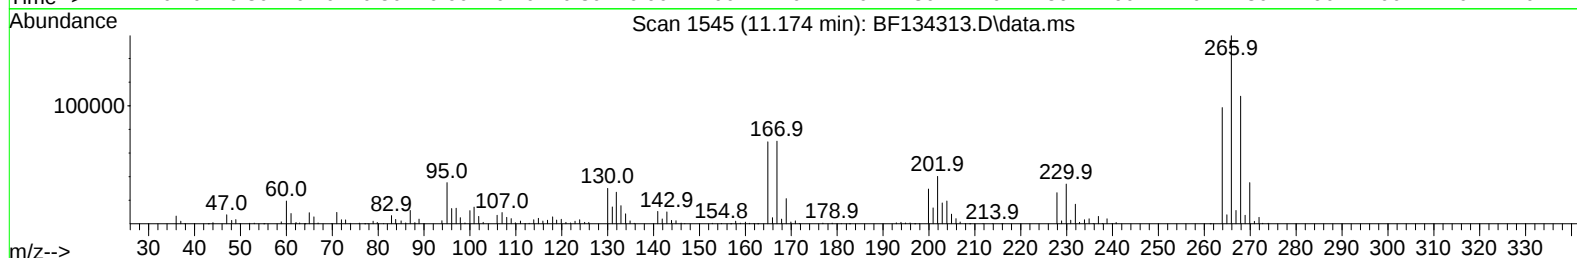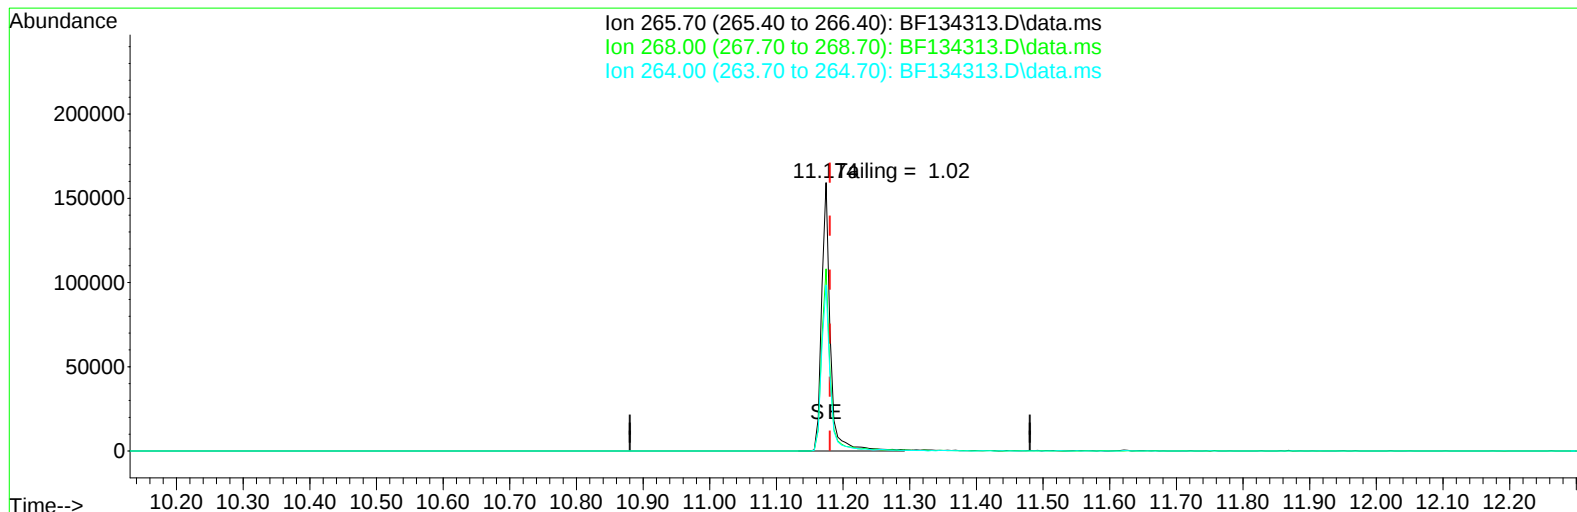

TIC: BF134313.D\data.ms

(70) Pentachlorophenol (C)

11.174min (-0.006) 326355.12 ng




response 145341

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.80	67.85
264.00	63.30	61.82
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071723\
Data File : BF134313.D
Acq On : 17 Jul 2023 12:52
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 17 16:23:29 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 14 22:51:27 2023
Response via : Initial Calibration

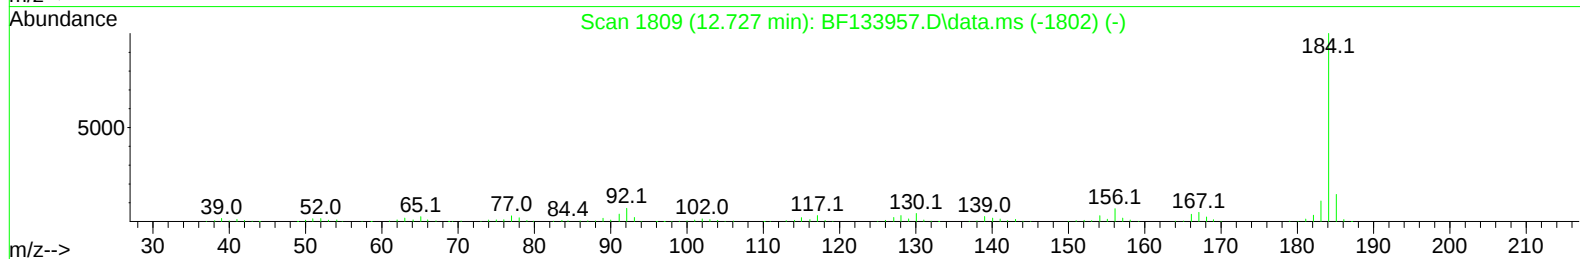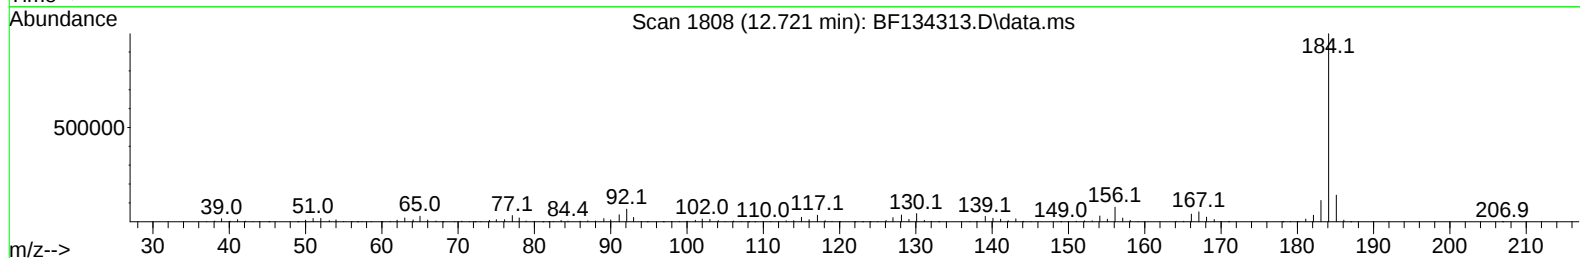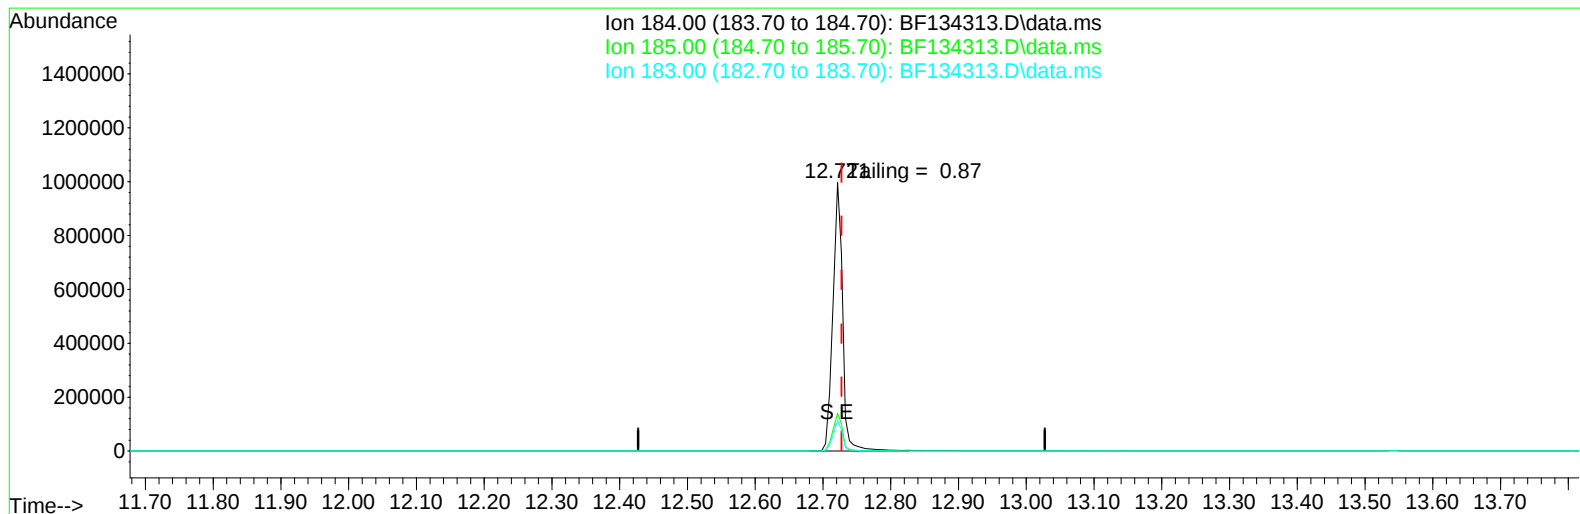

TIC: BF134313.D\data.ms

(77) Benzidine

12.721min (-0.006) 122939.96 ng

response 1000444

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.15
183.00	11.00	11.35
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/17/2023	BNA_F	BF134313.D
Compound Name	Response	Retention Time
DDT	437307	13.545
DDD	6499	13.268
DDE	272	12.909
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6771	444078	1.52

Instrument :
BNA_F
ClientSampleId :
DFTPP