
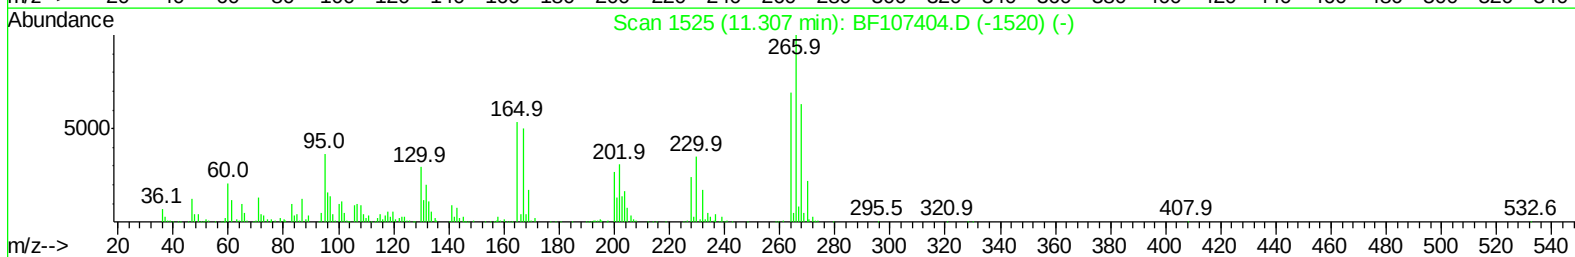
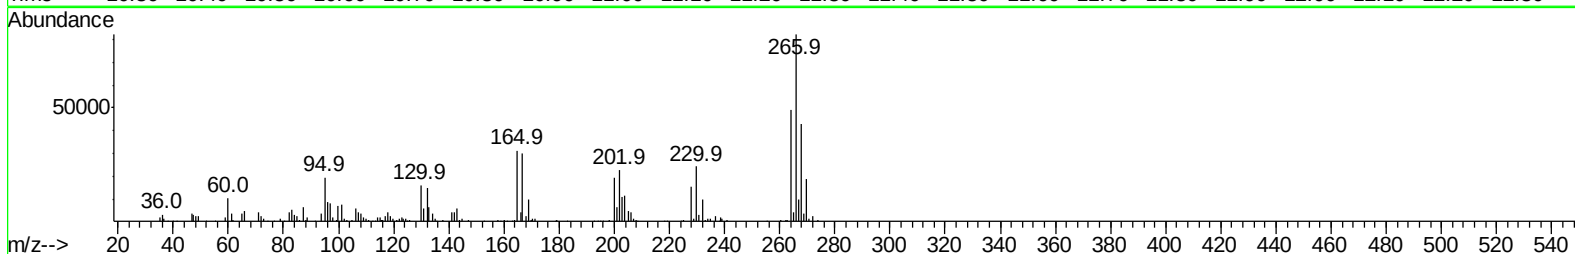


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF071818\
Data File : BF107490.D
Acq On : 19 Jul 2018 2:32
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 19 04:40:53 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF071618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 18 11:55:34 2018
Response via : Initial Calibration

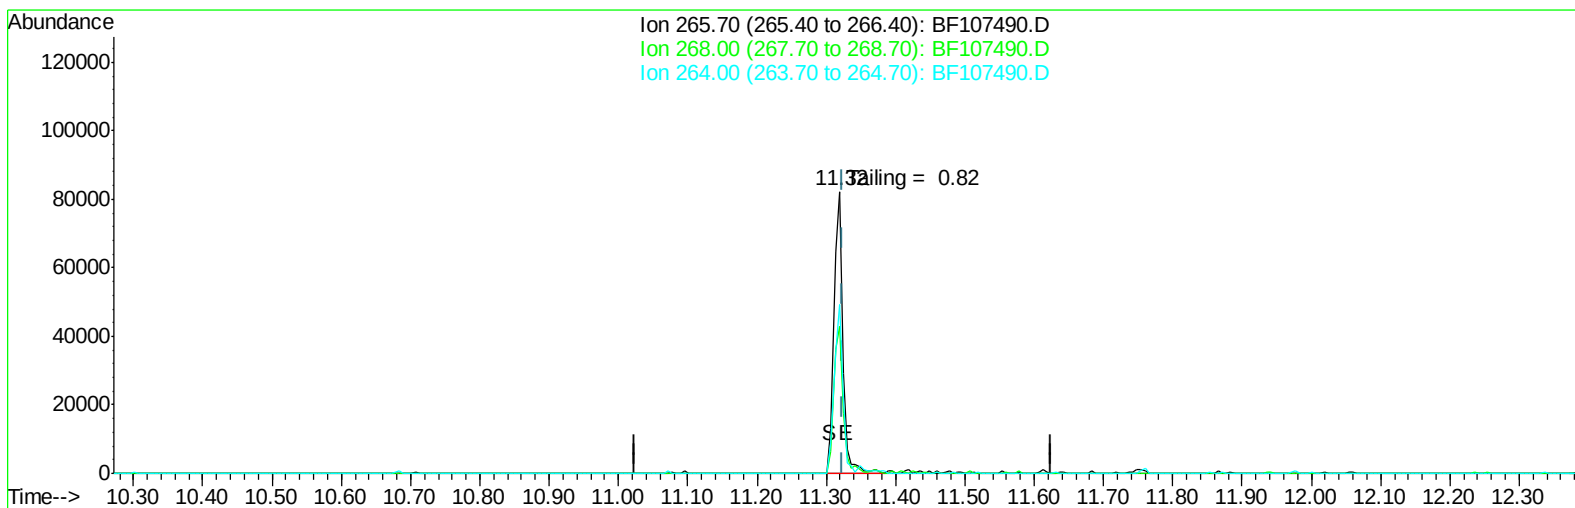

TIC: BF107490.D

(69) Pentachlorophenol (C)




11.319min (-0.006) 87367.89ng

response 73163

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	52.16
264.00	61.90	60.00
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF071818\
Data File : BF107490.D
Acq On : 19 Jul 2018 2:32
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 19 04:40:53 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF071618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 18 11:55:34 2018
Response via : Initial Calibration

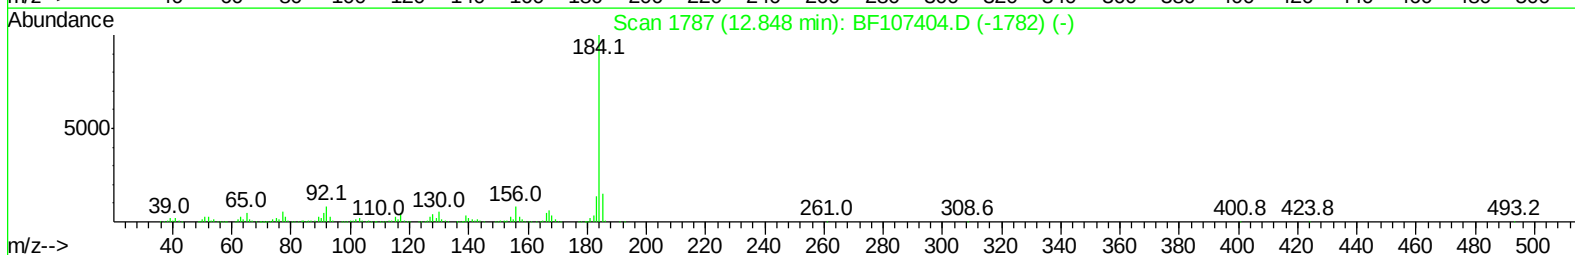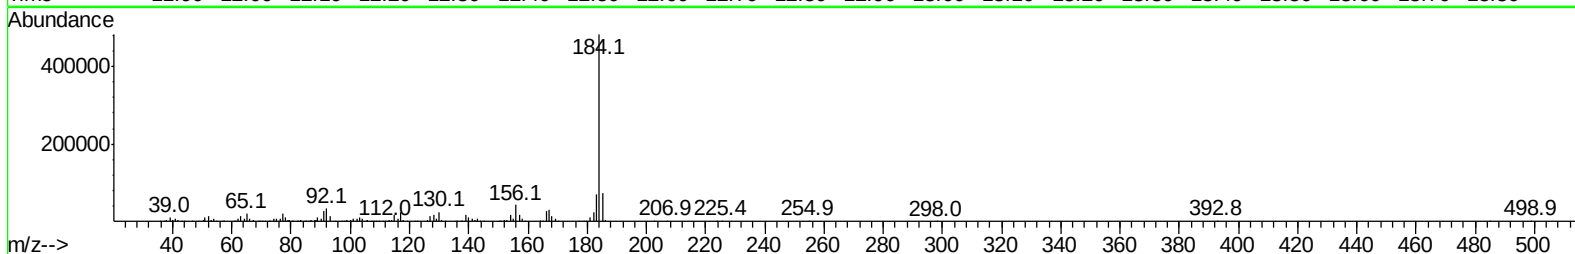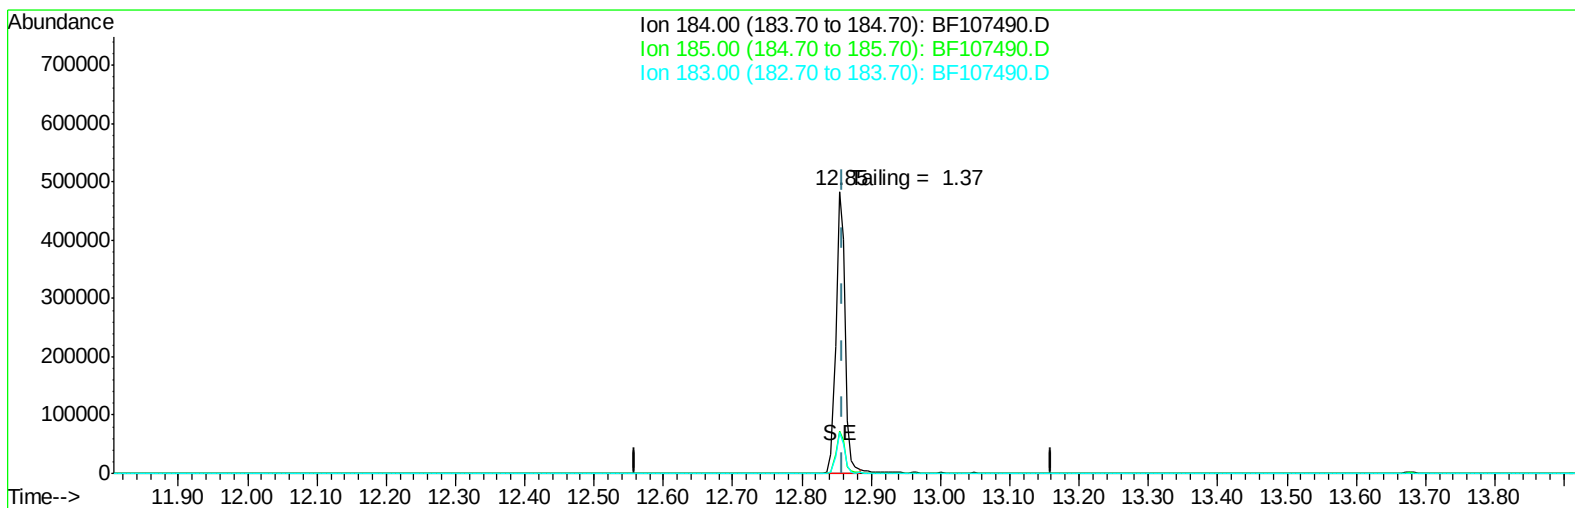

TIC: BF107490.D

(76) Benzidine

12.854min (-0.006) 55796.66ng

response 454746

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.87
183.00	11.60	14.44#
0.00	0.00	0.00