

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF071818\
 Data File : BF107466.D
 Acq On : 18 Jul 2018 10:14
 Operator : JU/SJ
 Sample : PB111180BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB111180BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF071618.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.407	7	12	16	rVB3	43934	68872	1.30%	0.180%
2	5.237	486	493	500	rVB	424051	552372	10.46%	1.443%
3	5.619	553	558	561	rBV	3310179	3704516	70.17%	9.681%
4	6.613	721	727	730	rBV	3642102	3833289	72.61%	10.017%
5	6.754	746	751	755	rBV	3600762	3903409	73.94%	10.200%
6	6.984	786	790	794	rBV	1116045	937392	17.76%	2.450%
7	7.142	812	817	820	rBV	3293354	3043652	57.65%	7.954%
8	7.548	880	886	889	rBV	2374557	2577299	48.82%	6.735%
9	8.266	1003	1008	1012	rBV	1170471	1118668	21.19%	2.923%
10	9.342	1185	1191	1194	rBV	4378597	4569382	86.56%	11.941%
11	10.025	1302	1307	1311	rBV	1301715	1382078	26.18%	3.612%
12	10.825	1433	1443	1446	rBV	2730844	3052912	57.83%	7.978%
13	11.525	1556	1562	1565	rBV	1641703	1618270	30.65%	4.229%
14	13.113	1825	1832	1835	rBV	4988224	5279118	100.00%	13.795%
15	14.171	2007	2012	2017	rBV	1543199	1551557	29.39%	4.055%
16	14.618	2085	2088	2092	rBV6	41629	57663	1.09%	0.151%
17	15.707	2268	2273	2282	rVB	727980	1016579	19.26%	2.657%


Sum of corrected areas: 38267028

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF071818\
Data File : BF107466.D
Acq On : 18 Jul 2018 10:14
Operator : JU/SJ
Sample : PB111180BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB111180BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF071618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

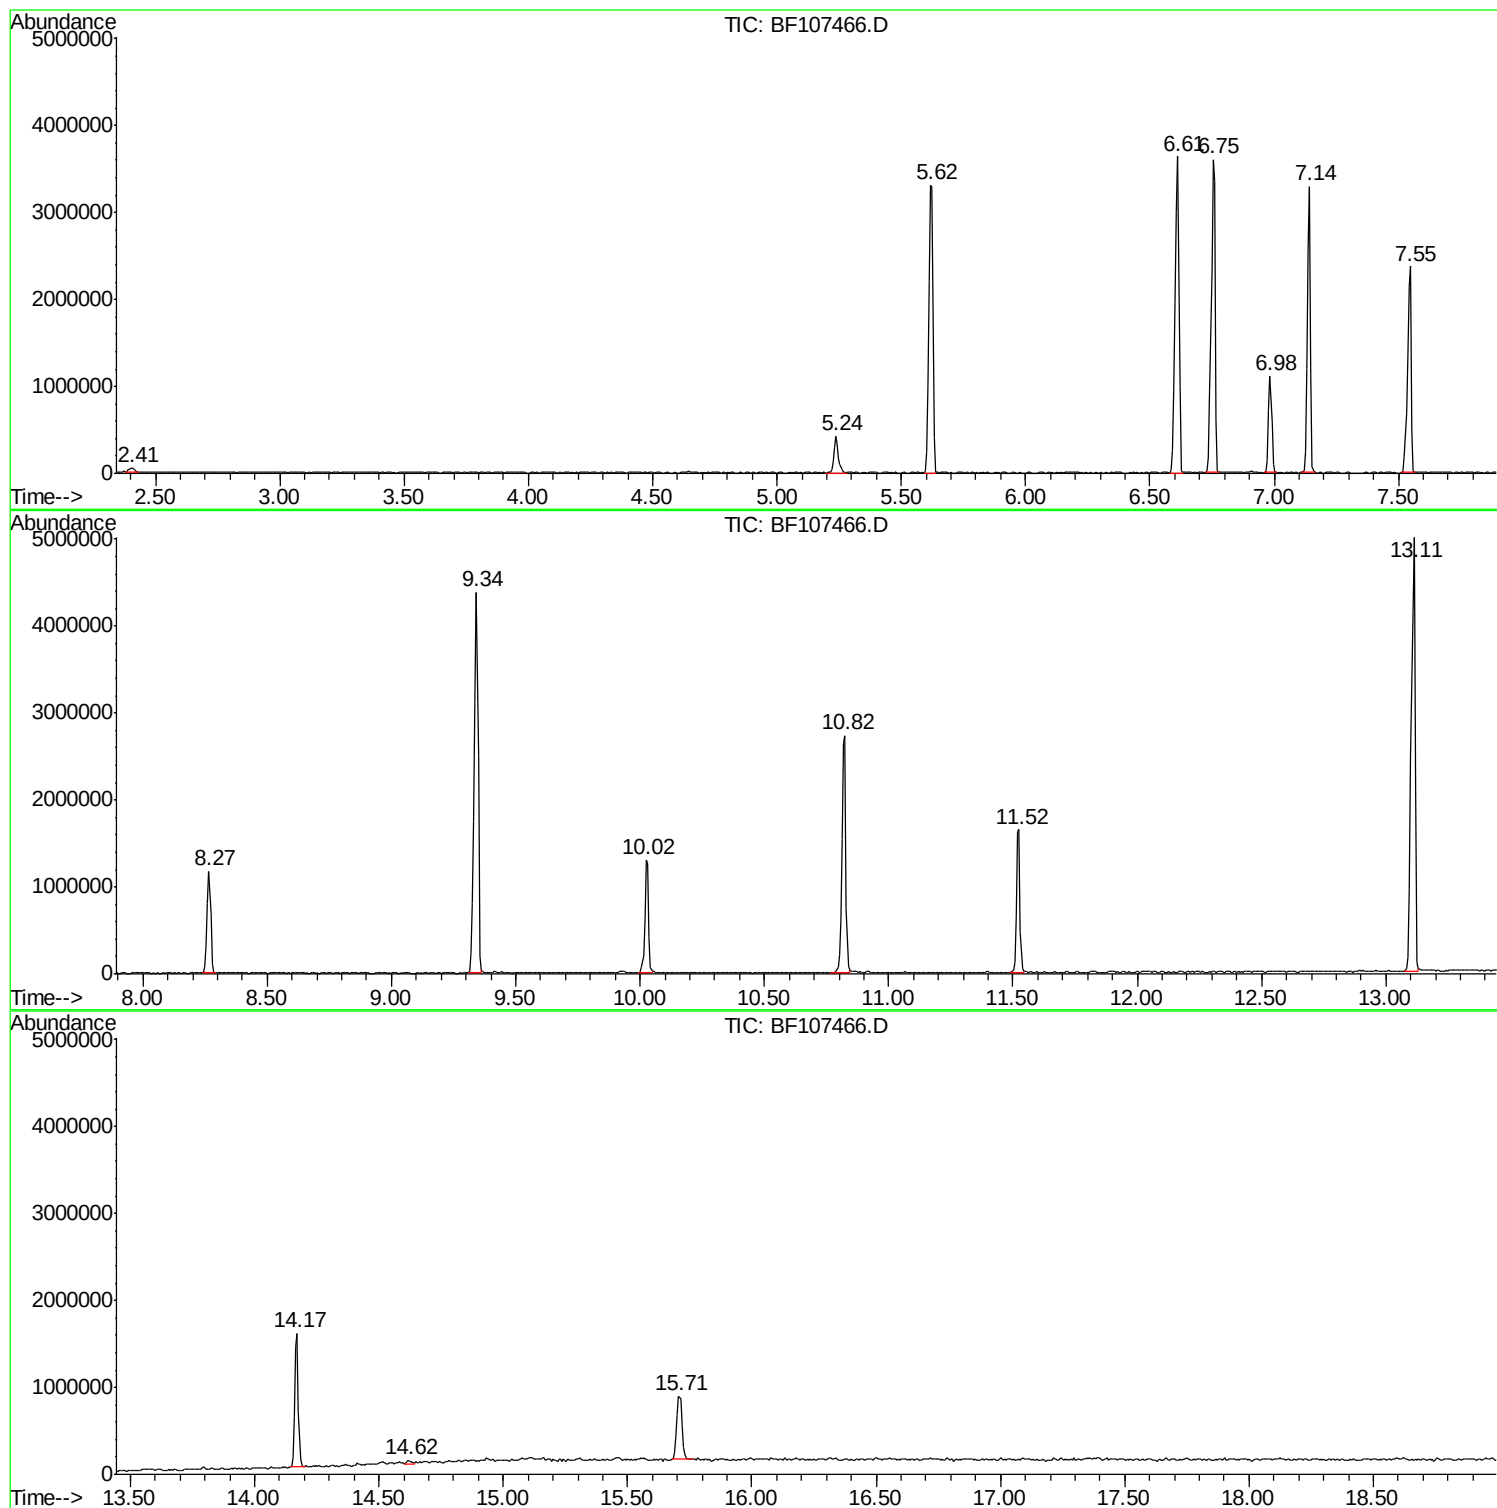

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF071818\
Data File : BF107466.D
Acq On : 18 Jul 2018 10:14
Operator : JU/SJ
Sample : PB111180BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB111180BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF071618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.24	11.79 ng	552372	1,4-Dichlorobenzene-d4	6.98

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	45
2			Butane, 1-(1-methylethoxy)-	116	C7H16O	001860-27-1	32
3			2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	16
4			Butyl aldoxime, 3-methyl-, syn-	101	C5H11NO	005780-40-5	12
5			Acetone	58	C3H6O	000067-64-1	9

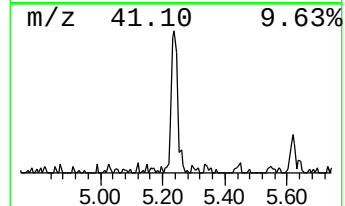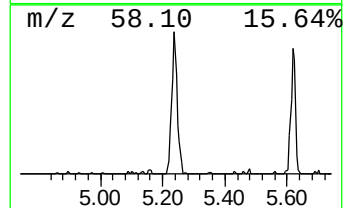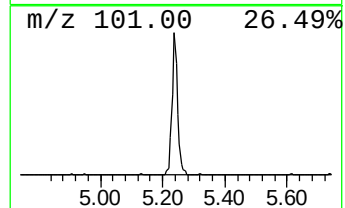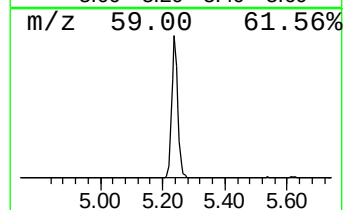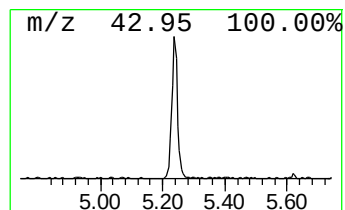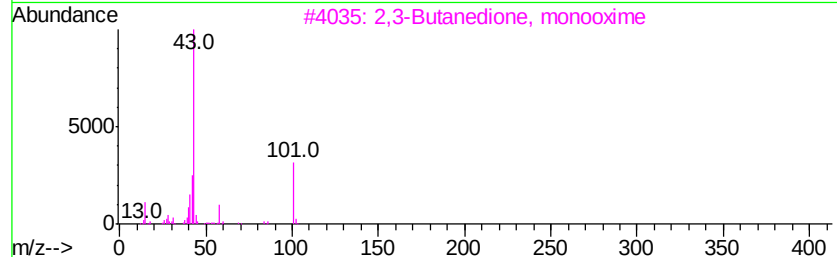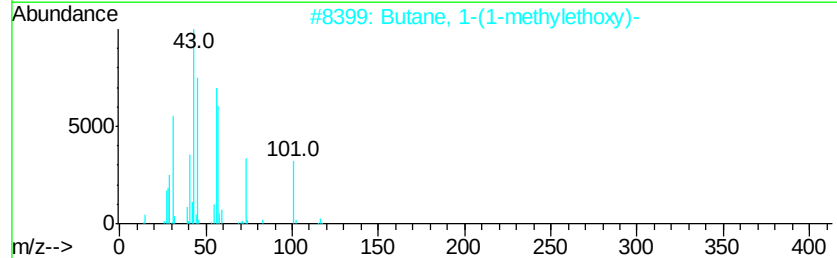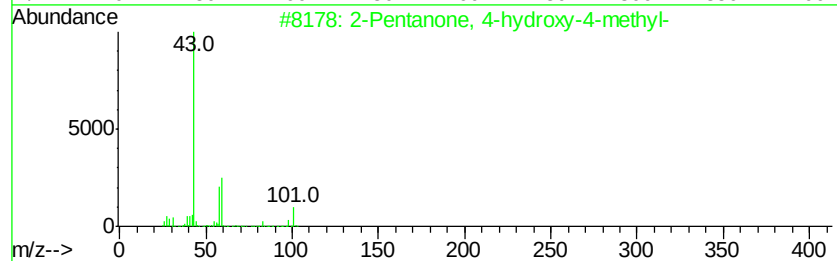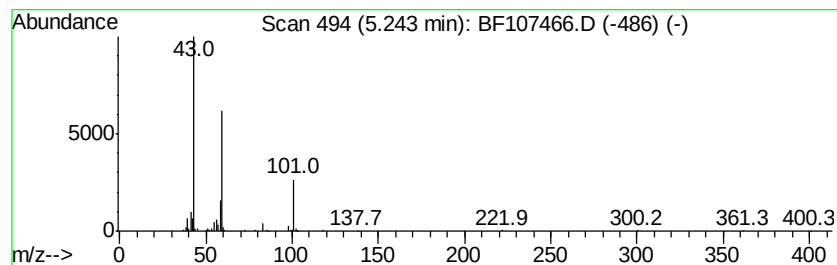

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF071818\
Data File : BF107466.D
Acq On : 18 Jul 2018 10:14
Operator : JU/SJ
Sample : PB111180BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB111180BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF071618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown6.75 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.75	83.28 ng	3903410	1,4-Dichlorobenzene-d4	6.98

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	14
2		Tranlycypromine-propionyl	189	C12H15NO	1000123-86-3	10
3		Cyclopropanamine, 1-phenyl-	133	C9H11N	1000351-26-2	10
4		1,3-Cyclopentanedione, 2-chloro-	132	C5H5ClO2	014203-19-1	10
5		1,3,5-Trifluorobenzene	132	C6H3F3	000372-38-3	9

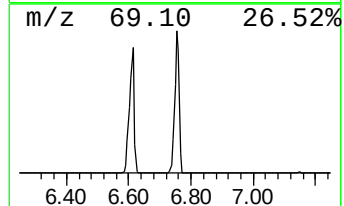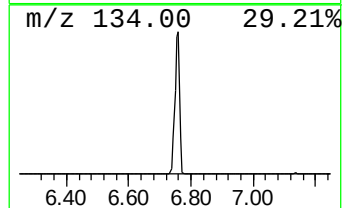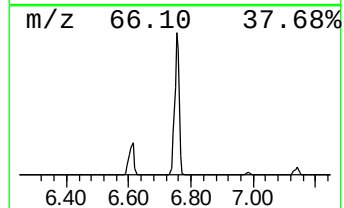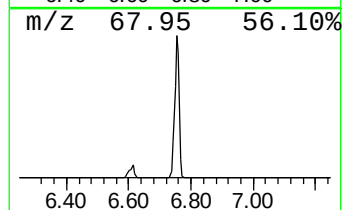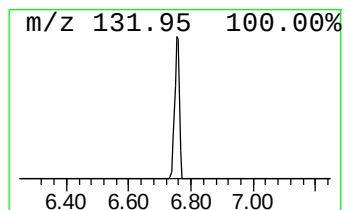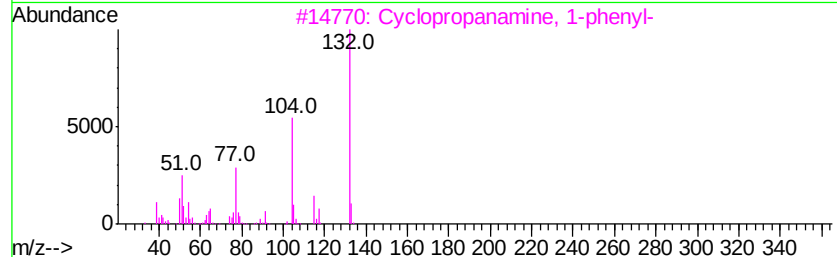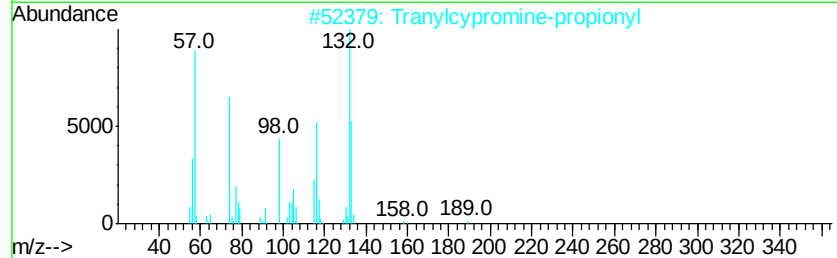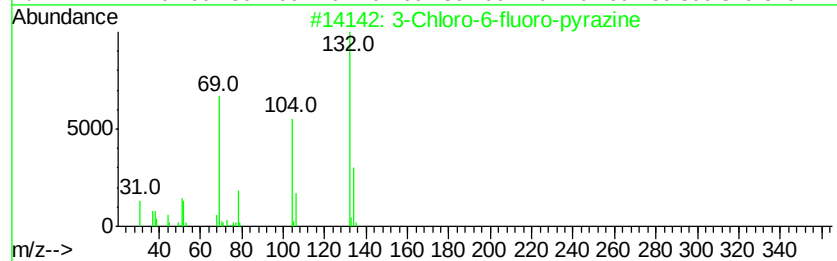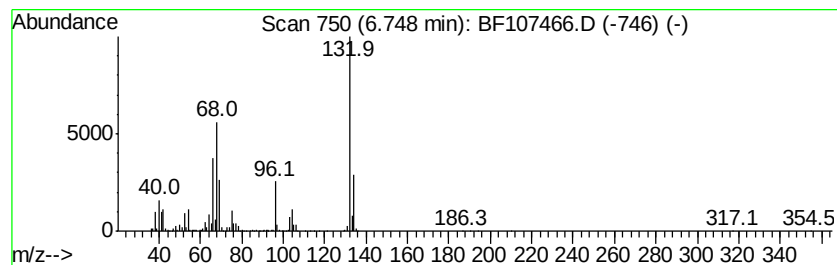

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF071818\
Data File : BF107466.D
Acq On : 18 Jul 2018 10:14
Operator : JU/SJ
Sample : PB111180BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB111180BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF071618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-hy...	5.24	11.8	ng	552372	1	6.98	937392	20.0
unknown6.75	6.75	83.3	ng	3903410	1	6.98	937392	20.0