


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071818\
 Data File : BF107490.D
 Acq On : 19 Jul 2018 2:32
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF071618.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jul 18 11:55:34 2018

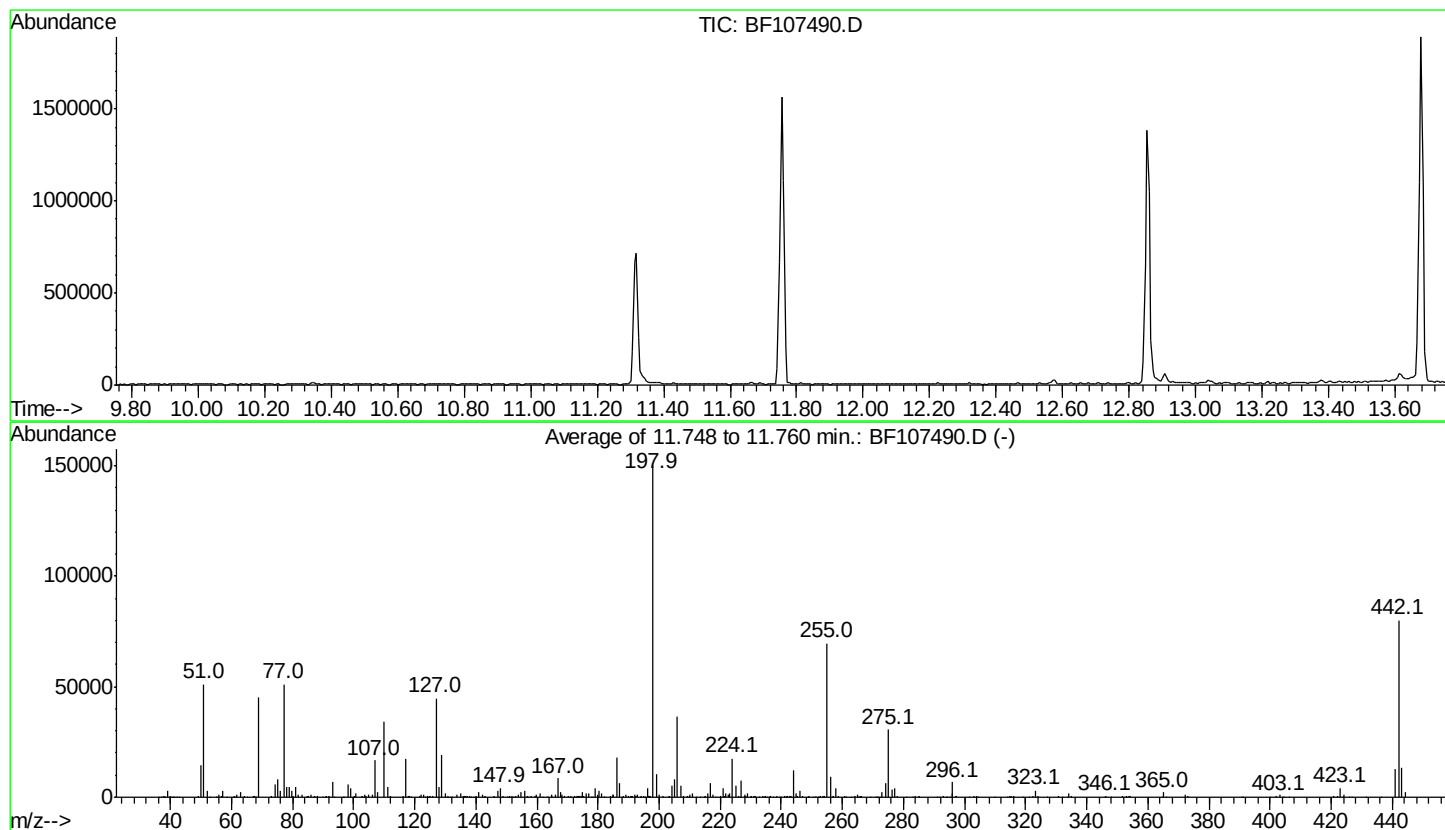

AutoFind: Scans 1600, 1601, 1602; Background Corrected with Scan 1596

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.1	51141	PASS
68	69	0.00	2	0.9	424	PASS
69	198	0.00	100	30.2	45256	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	29.7	44608	PASS
197	198	0.00	2	0.4	526	PASS
198	198	100	100	100.0	150040	PASS
199	198	5	9	6.9	10350	PASS
275	198	10	60	20.4	30649	PASS
365	198	1	100	1.4	2076	PASS
441	198	0.01	100	8.5	12814	PASS
442	198	50	100	53.3	80026	PASS
443	442	15	24	16.8	13457	PASS