
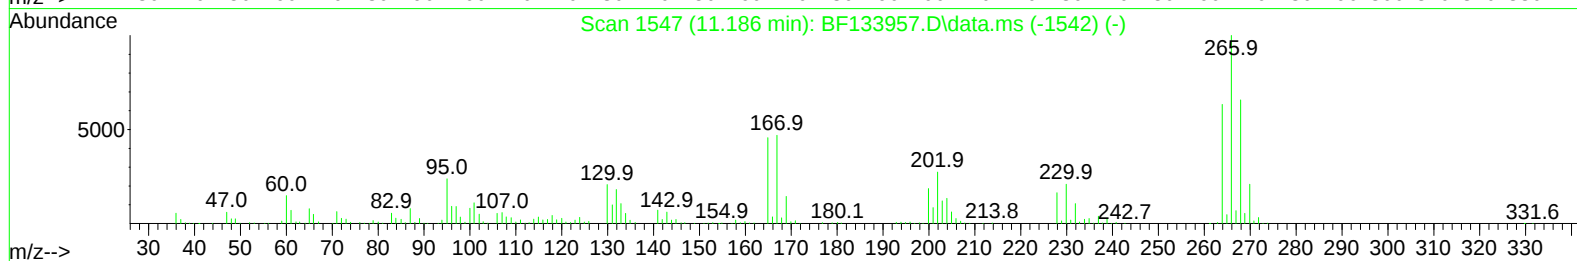
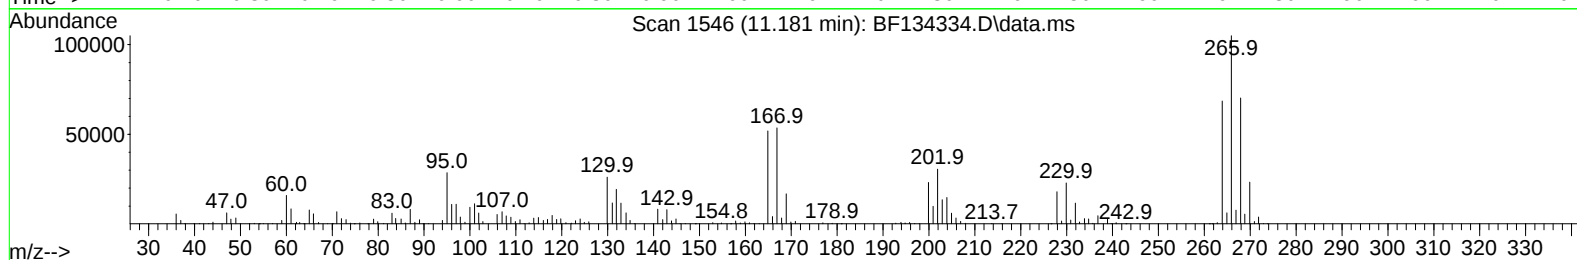


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071823\
Data File : BF134334.D
Acq On : 18 Jul 2023 12:11
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 18 14:03:17 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 14 22:51:27 2023
Response via : Initial Calibration

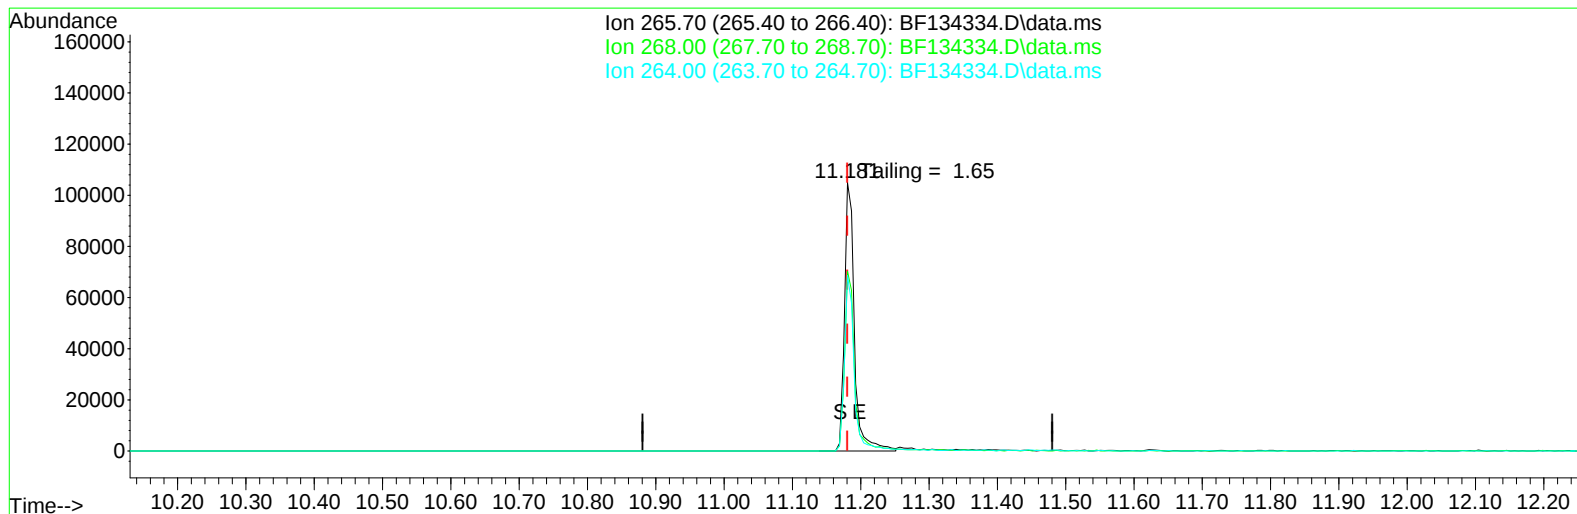

TIC: BF134334.D\data.ms

(70) Pentachlorophenol (C)




11.181min (+ 0.000) 24933.83 ng

response 105658

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.80	66.95
264.00	63.30	65.35
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071823\
Data File : BF134334.D
Acq On : 18 Jul 2023 12:11
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 18 14:03:17 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 14 22:51:27 2023
Response via : Initial Calibration

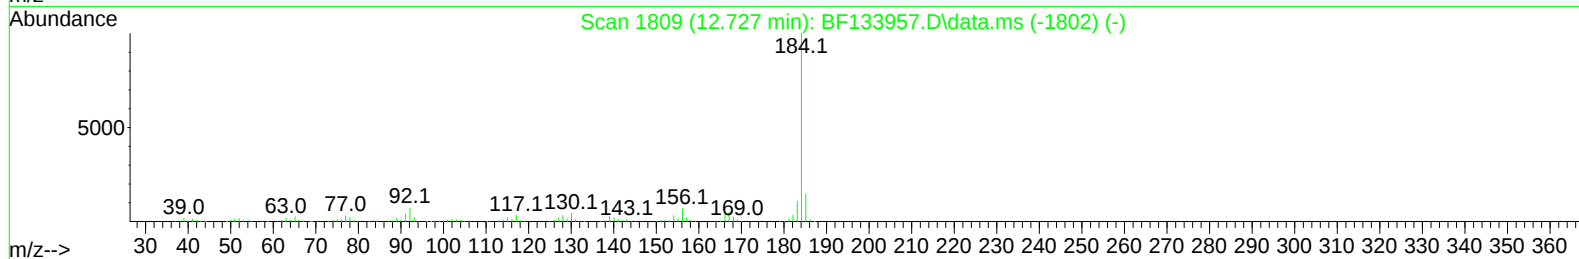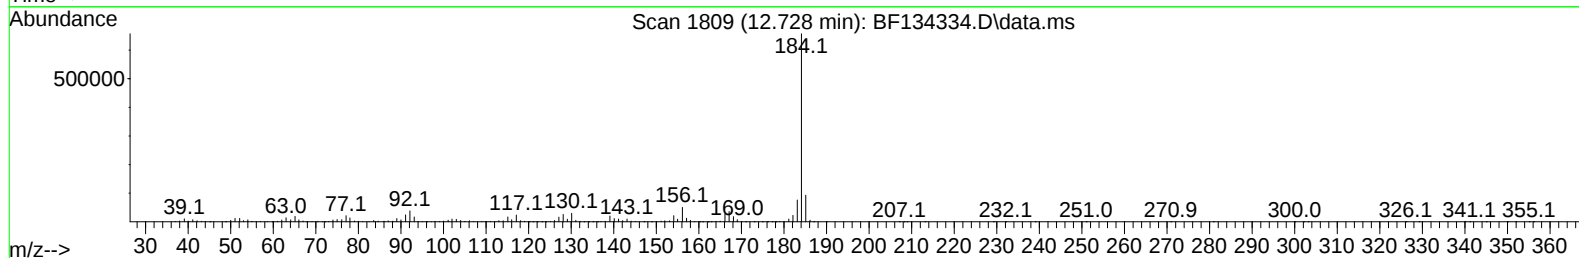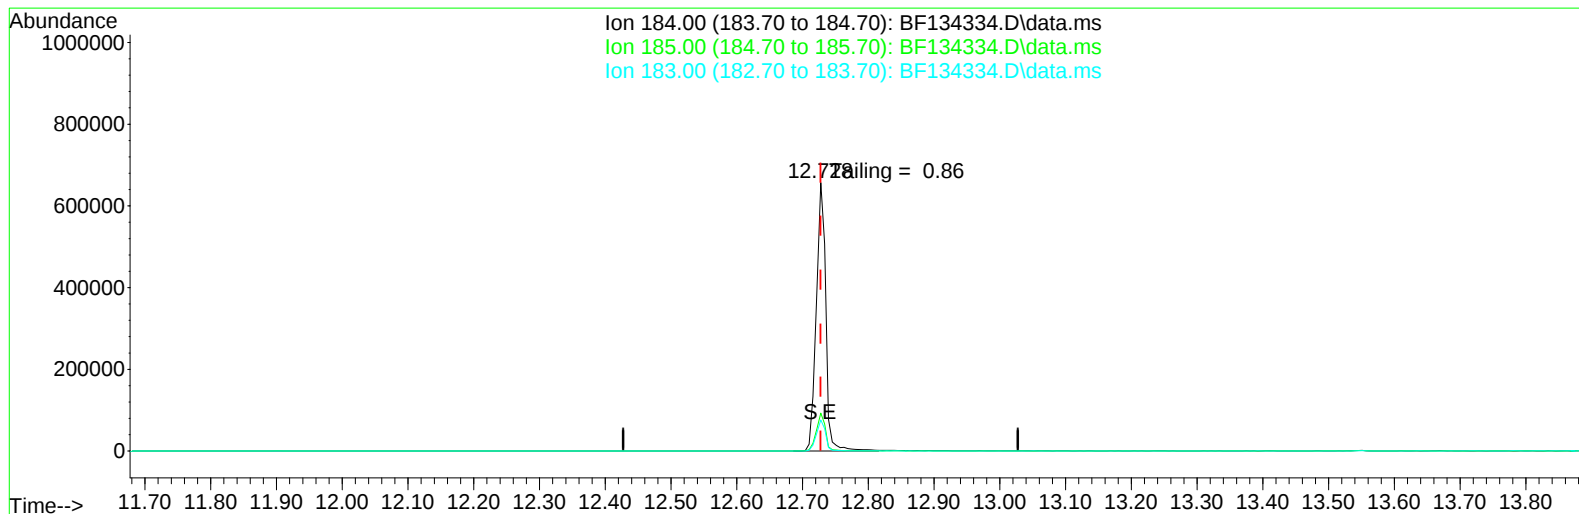

TIC: BF134334.D\data.ms

(77) Benzidine

12.728min (+ 0.000) 42781.30 ng

response 601610

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.15
183.00	11.00	11.56
0.00	0.00	0.00