
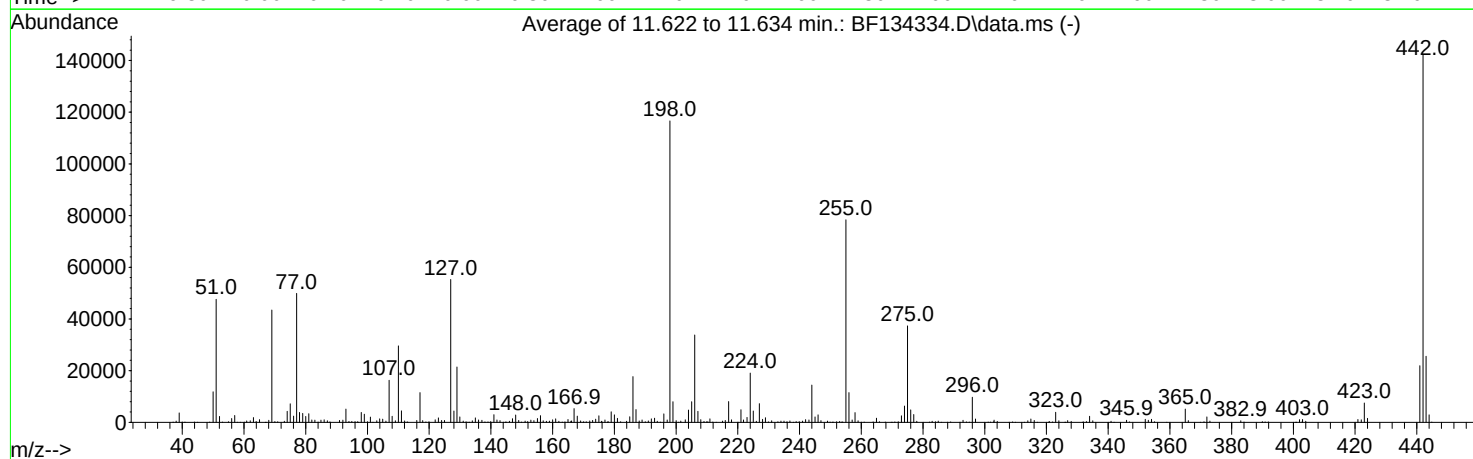


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071823\
Data File : BF134334.D
Acq On : 18 Jul 2023 12:11
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Jul 14 22:51:27 2023

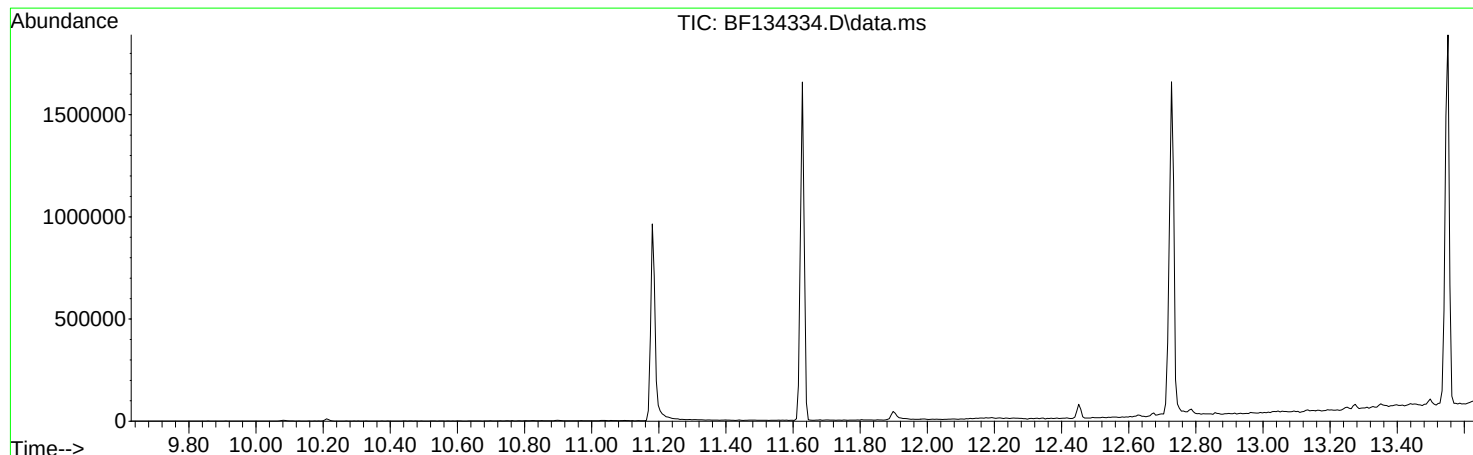

AutoFind: Scans 1621, 1622, 1623; Background Corrected with Scan 1616

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.8	47637	PASS
68	69	0.00	2	1.8	779	PASS
69	198	0.00	100	37.3	43483	PASS
70	69	0.00	2	0.7	288	PASS
127	198	10	80	47.4	55288	PASS
197	198	0.00	2	0.8	908	PASS
198	198	100	100	100.0	116619	PASS
199	198	5	9	6.9	8005	PASS
275	198	10	60	32.0	37347	PASS
365	198	1	100	4.4	5129	PASS
441	198	0.01	100	18.8	21931	PASS
442	442	50	100	100.0	142317	PASS
443	442	15	24	18.0	25593	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
7/18/2023	BNA_F	<u>BF134334.D</u>
Compound Name	Response	Retention Time
DDT	302531	13.551
DDD	6800	13.275
DDE	595	12.904
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7395	309926	2.39

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071823\
Data File : BF134334.D
Acq On : 18 Jul 2023 12:11
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 18 14:03:17 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 14 22:51:27 2023
Response via : Initial Calibration

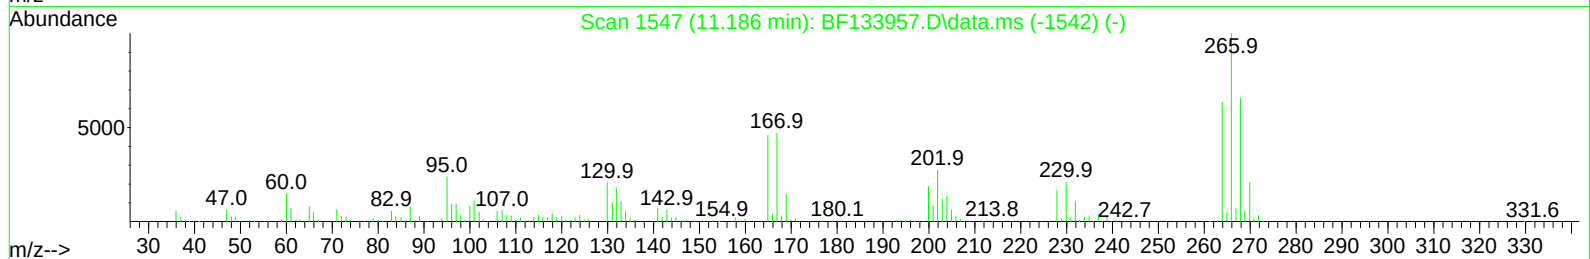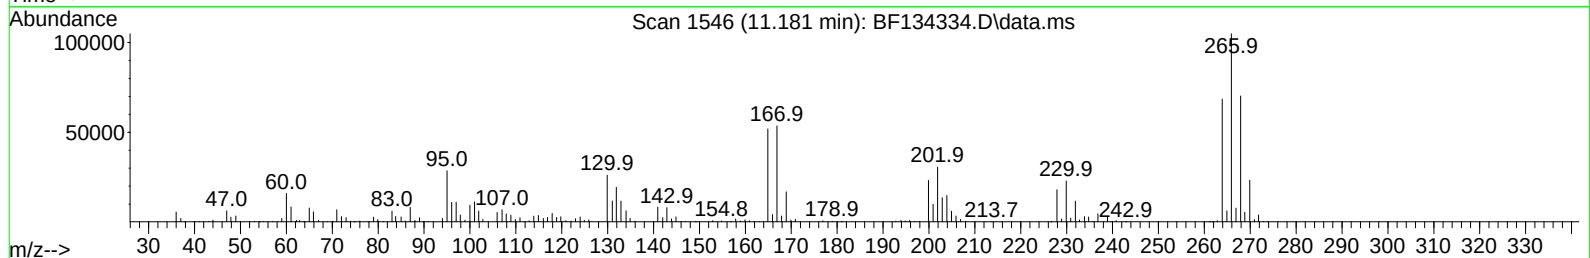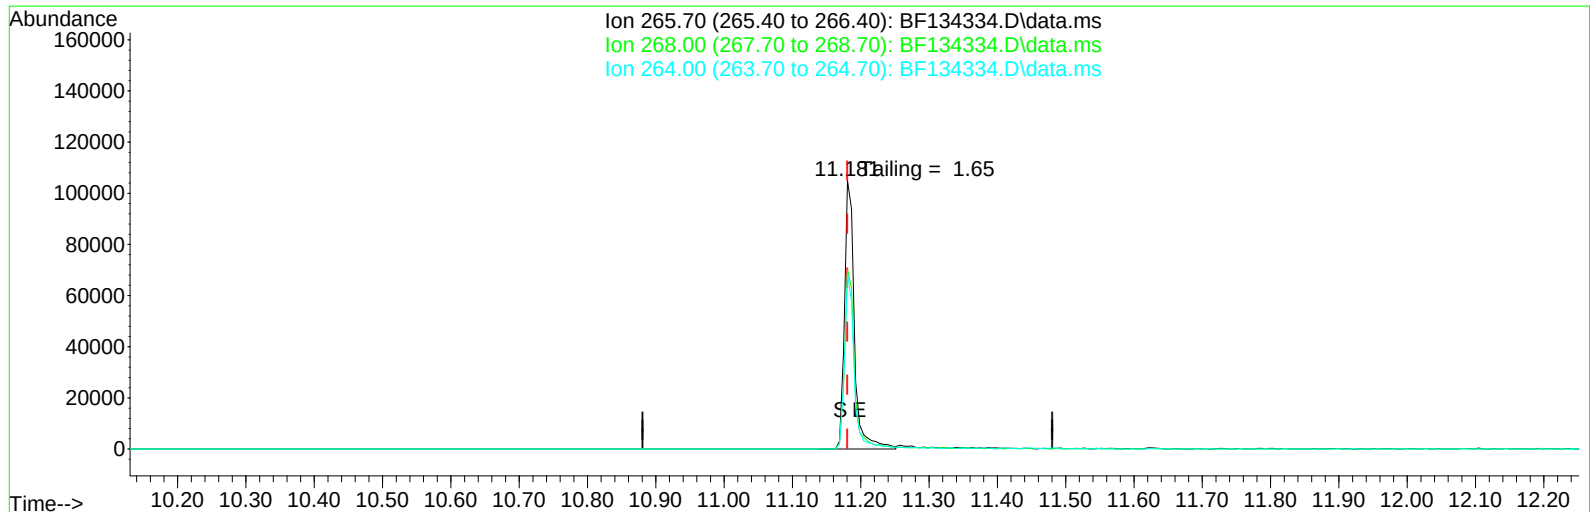

TIC: BF134334.D\data.ms

(70) Pentachlorophenol (C)

11.181min (+ 0.000) 24933.83 ng




response 105658

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.80	66.95
264.00	63.30	65.35
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071823\
Data File : BF134334.D
Acq On : 18 Jul 2023 12:11
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 18 14:03:17 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 14 22:51:27 2023
Response via : Initial Calibration

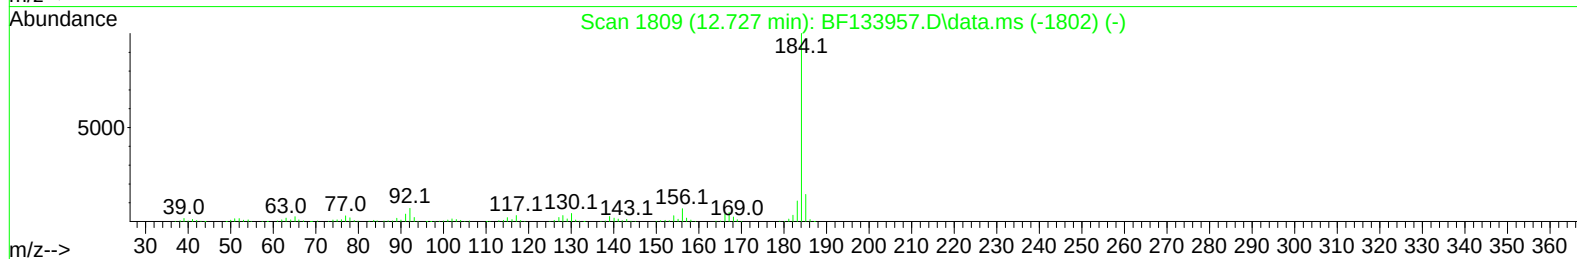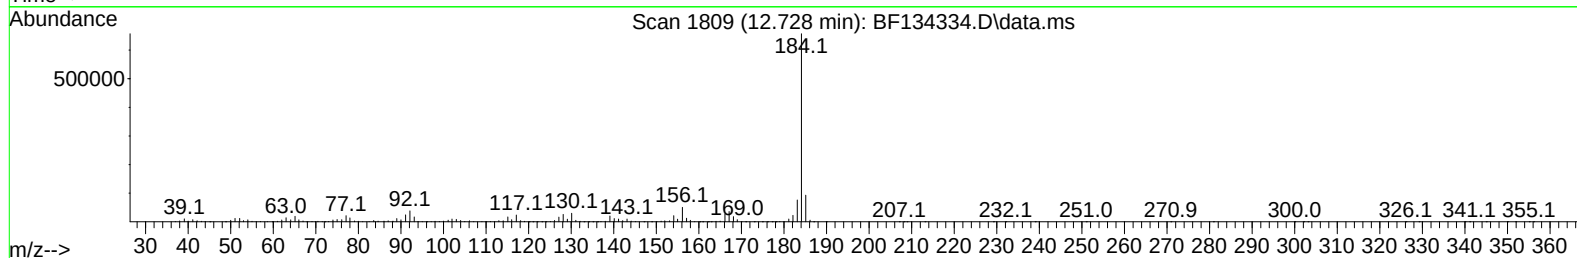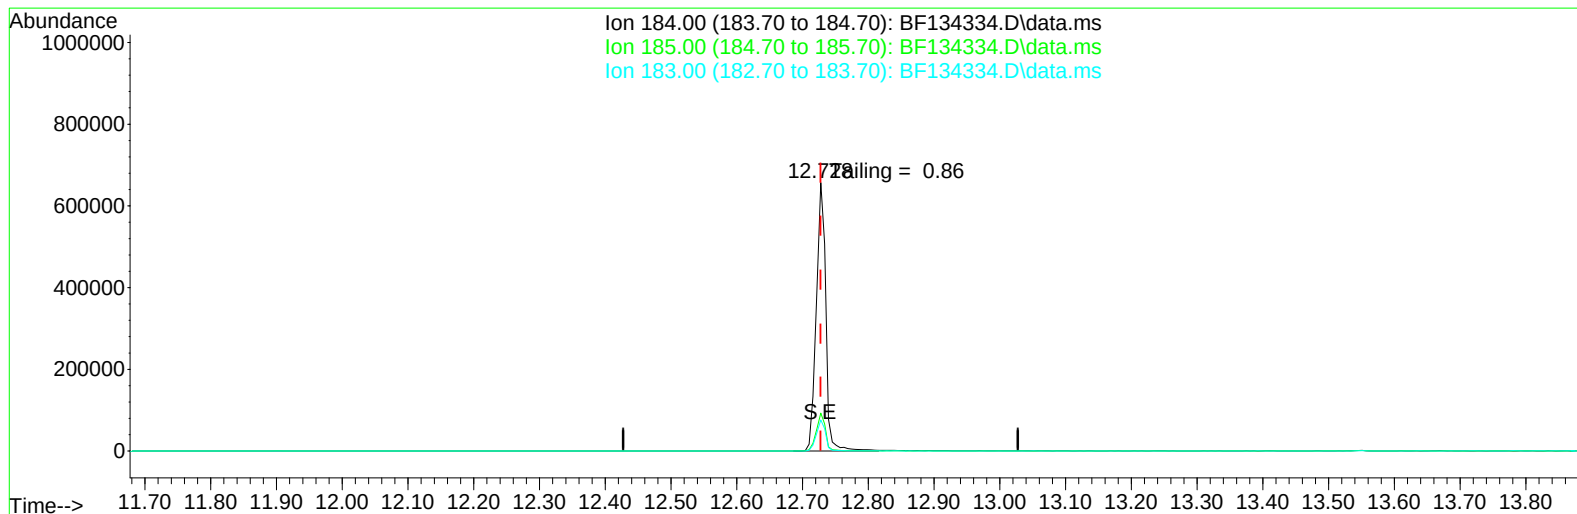

TIC: BF134334.D\data.ms

(77) Benzidine

12.728min (+ 0.000) 42781.30 ng

response 601610

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.15
183.00	11.00	11.56
0.00	0.00	0.00