


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071918\
 Data File : BF107512.D
 Acq On : 19 Jul 2018 16:41
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF071618.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jul 18 11:55:34 2018

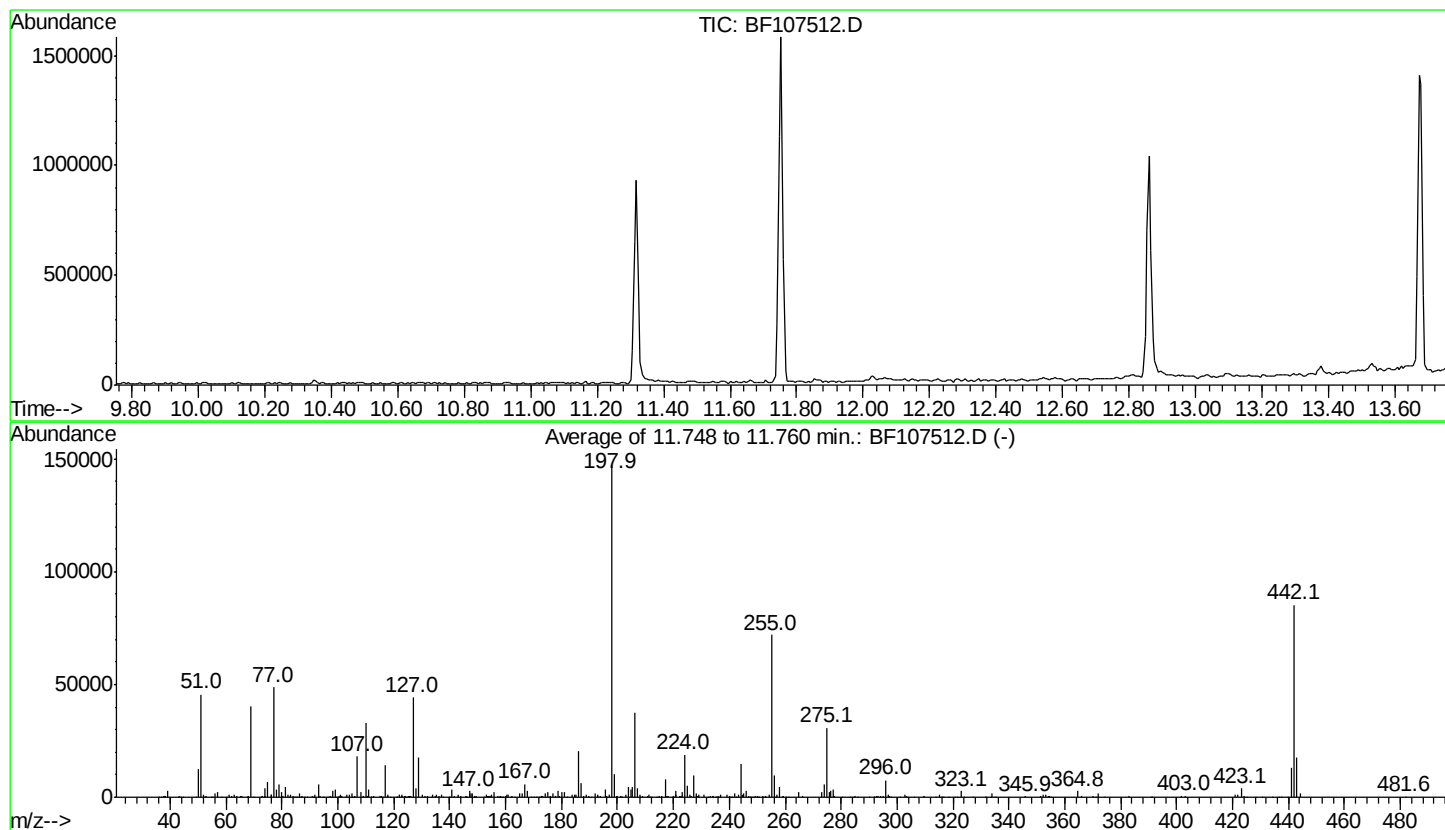

AutoFind: Scans 1600, 1601, 1602; Background Corrected with Scan 1592

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.0	45536	PASS
68	69	0.00	2	1.6	625	PASS
69	198	0.00	100	27.4	40261	PASS
70	69	0.00	2	0.3	106	PASS
127	198	10	80	30.0	44178	PASS
197	198	0.00	2	0.9	1272	PASS
198	198	100	100	100.0	147050	PASS
199	198	5	9	6.8	9970	PASS
275	198	10	60	20.9	30784	PASS
365	198	1	100	1.9	2741	PASS
441	198	0.01	100	9.0	13224	PASS
442	198	50	100	57.9	85154	PASS
443	442	15	24	20.4	17405	PASS