

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF071919\
 Data File : BF115680.D
 Acq On : 19 Jul 2019 19:07
 Operator : HP/JU
 Sample : K3887-02
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Quant Time: Jul 20 01:40:32 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF071219.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 12 14:03:52 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.88	152	210189	20.00	ng	0.00
21) Naphthalene-d8	8.16	136	821410	20.00	ng	0.00
39) Acenaphthene-d10	9.92	164	391351	20.00	ng	-0.01
64) Phenanthrene-d10	11.40	188	668273	20.00	ng	0.00
76) Chrysene-d12	14.04	240	407757	20.00	ng	0.00
87) Perylene-d12	15.52	264	335481	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.53	112	1332014	103.66	ng	0.02
7) Phenol-d6	6.52	99	1581485	96.99	ng	0.00
23) Nitrobenzene-d5	7.45	82	1249080	88.42	ng	0.00
42) 2,4,6-Tribromophenol	10.71	330	510095	111.67	ng	0.00
45) 2-Fluorobiphenyl	9.24	172	2120715	94.85	ng	-0.01
79) Terphenyl-d14	12.99	244	1924626	87.09	ng	0.00
Target Compounds						
19) n-Nitroso-di-n-propylamine	7.45	70	167964	15.795	ng	# 77
25) Isophorone	7.45	82	1230903	43.545	ng	# 64
51) 2,6-Dinitrotoluene	9.92	165	50677	7.574	ng	# 27
57) 2,4-Dinitrotoluene	9.92	165	50677	5.846	ng	# 24
67) 4-Bromophenyl-phenylether	10.71	248	30503	3.994	ng	# 1

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF071919\
Data File : BF115680.D
Acq On : 19 Jul 2019 19:07
Operator : HP/JU
Sample : K3887-02
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: Jul 20 01:40:32 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF071219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 12 14:03:52 2019
Response via : Initial Calibration




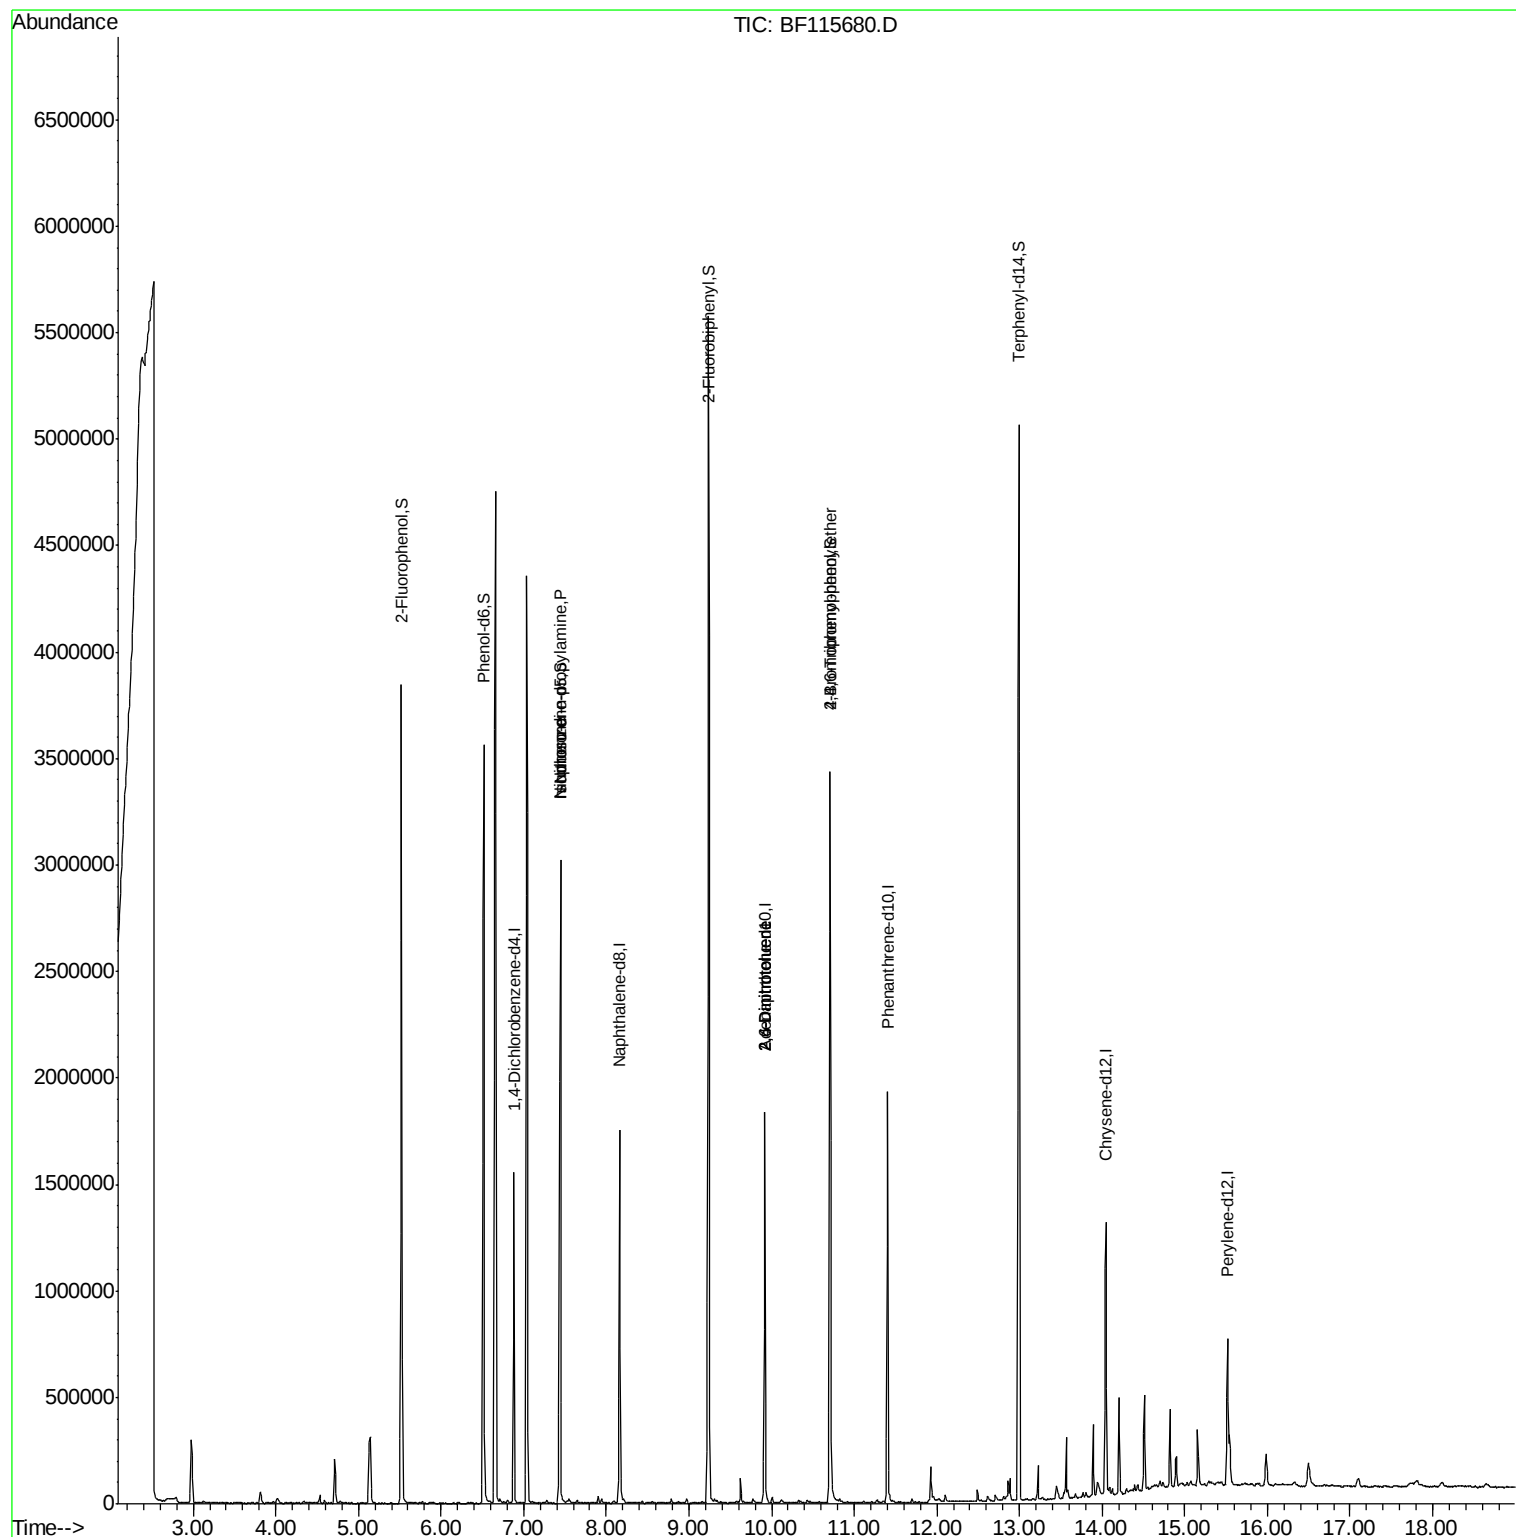




#1
 1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 6.88 min Scan# 815
 Delta R.T. -0.01 min
 Lab File: BF115680.D
 Acq: 19 Jul 2019 19:07




Instrument :
 BNA_F
 ClientSampleId :




Tot Ion:152 Resp: 210189
 Ion Ratio Lower Upper
 152 100
 150 156.0 129.7 194.5
 115 61.8 48.2 72.4

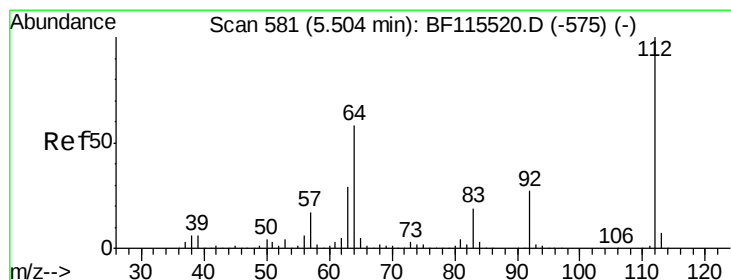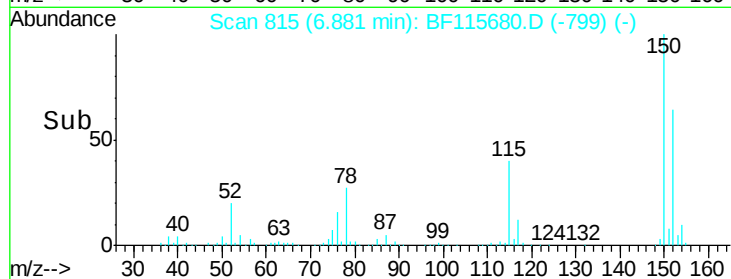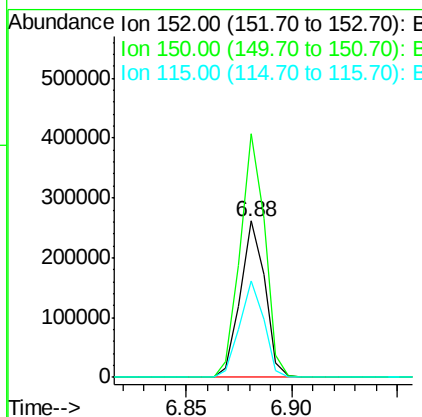

#5
 2-Fluorophenol
 Concen: 103.659 ng
 RT: 5.53 min Scan# 585
 Delta R.T. 0.02 min
 Lab File: BF115680.D
 Acq: 19 Jul 2019 19:07

Tgt Ion:112 Resp: 1332014
 Ion Ratio Lower Upper
 112 100
 64 54.9 46.8 70.2
 63 28.1 24.1 36.1

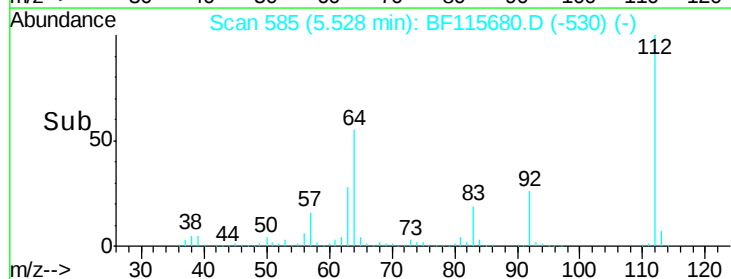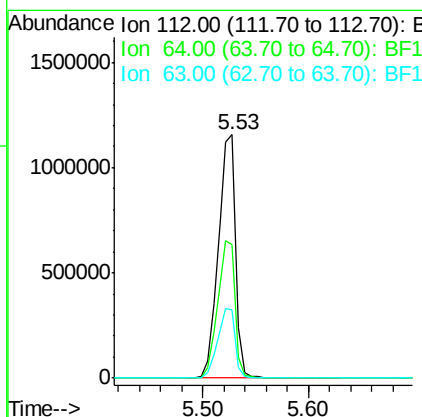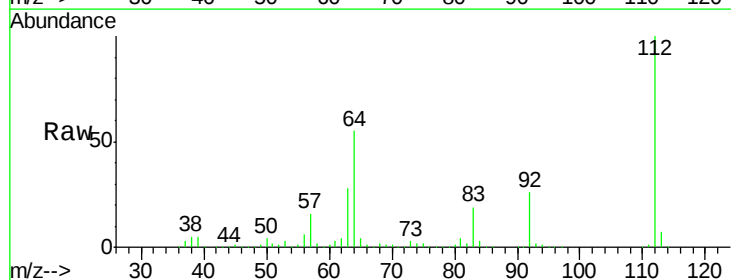

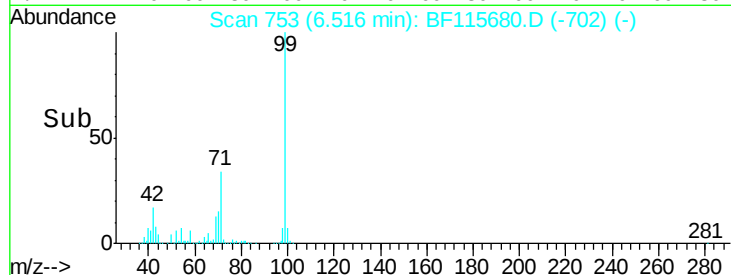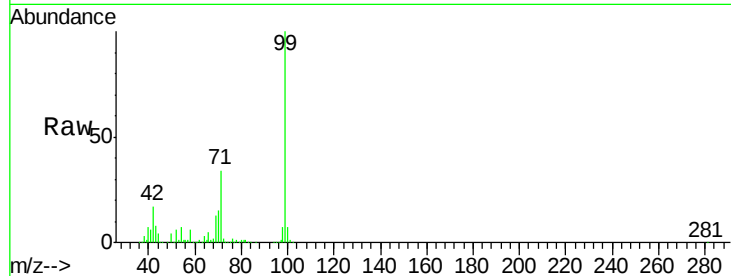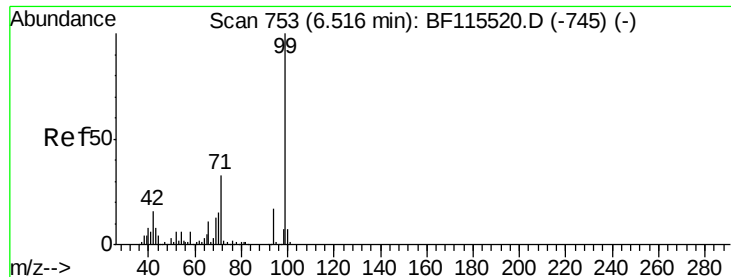

#7

Phenol-d6

Concen: 96.993 ng

RT: 6.52 min Scan# 753

Delta R.T. 0.00 min

Lab File: BF115680.D

Acq: 19 Jul 2019 19:07

Instrument :

BNA_F

ClientSampleId :





Tot Ion: 99 Resp: 1581485

Ion Ratio Lower Upper

99 100

42 16.9 13.6 20.4

71 34.2 28.5 42.7

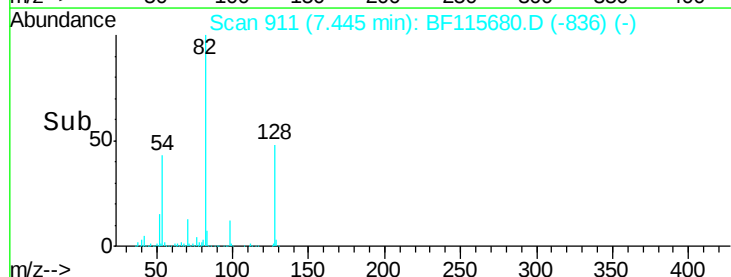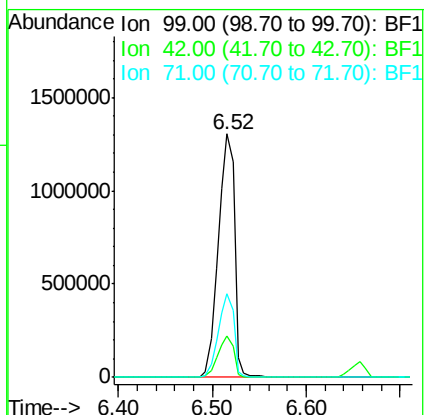

#19

n-Nitroso-di-n-propylamine

Concen: 15.795 ng

RT: 7.45 min Scan# 911

Delta R.T. 0.14 min

Lab File: BF115680.D

Acq: 19 Jul 2019 19:07

Tgt Ion: 70 Resp: 167964


Ion Ratio Lower Upper


70 100

42 40.8 39.6 59.4

101 0.0 8.1 12.1#

130 2.6 18.2 27.2#

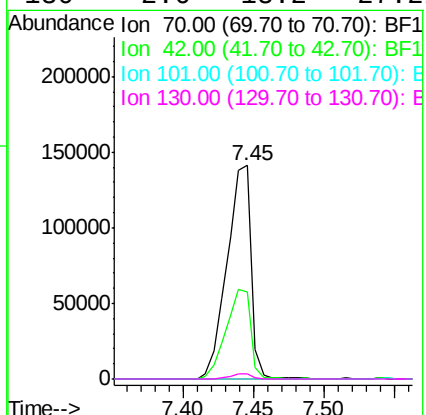

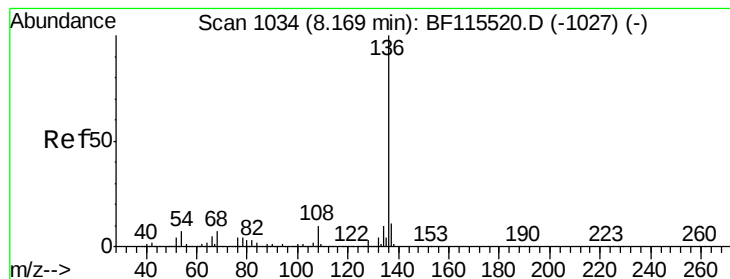

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.16 min Scan# 1033

Delta R.T. -0.01 min

Lab File: BF115680.D

Acq: 19 Jul 2019 19:07

Instrument :
BNA_F
ClientSampled :

Tot Ion:136 Resp: 821410



Ion Ratio Lower Upper

136 100

137 11.2 9.0 13.4

54 6.8 5.6 8.4

68 6.2 5.0 7.6

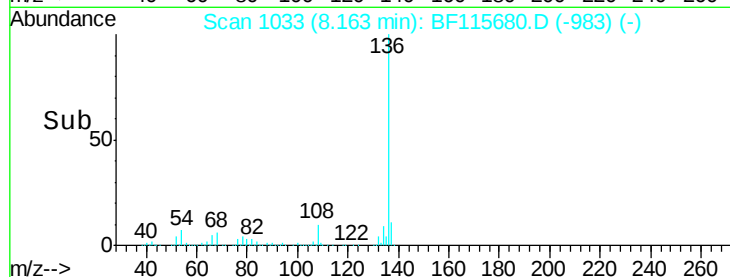
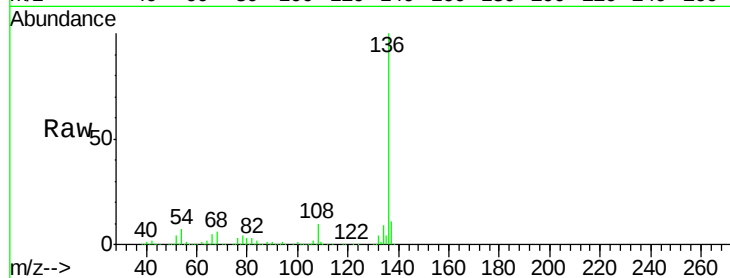


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF1

Ion 68.00 (67.70 to 68.70): BF1

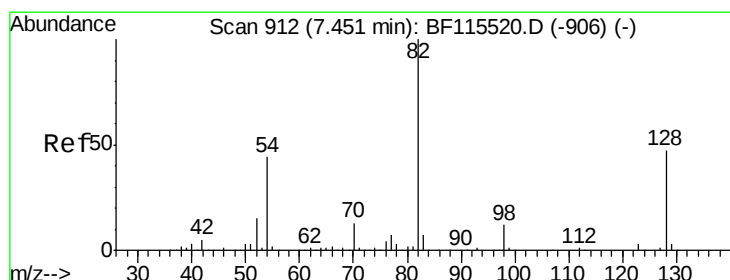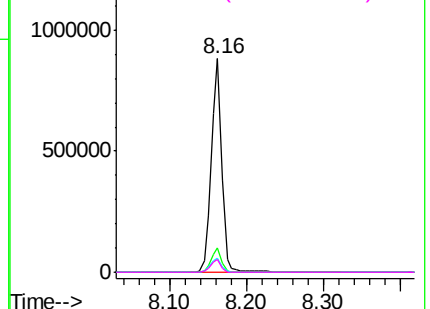

#23

Nitrobenzene-d5

Concen: 88.421 ng

RT: 7.45 min Scan# 911

Delta R.T. -0.01 min

Lab File: BF115680.D

Acq: 19 Jul 2019 19:07



Tgt Ion: 82 Resp: 1249080

Ion Ratio Lower Upper

82 100

128 48.4 38.6 57.8


54 43.4 35.6 53.4

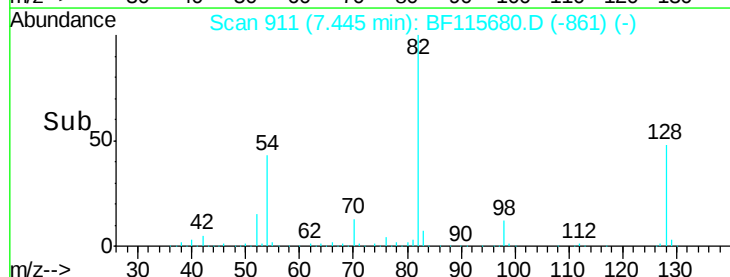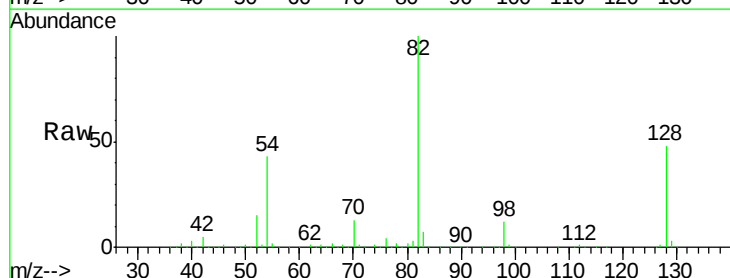


Abundance Ion 82.00 (81.70 to 82.70): BF1

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BF1

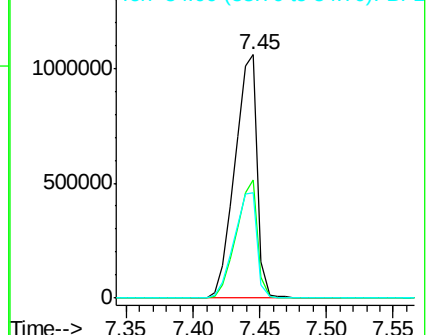

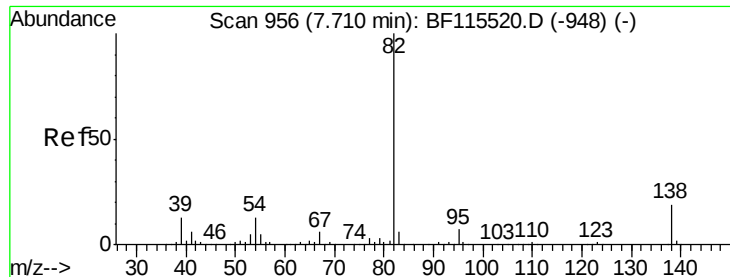

#25

Isophorone

Concen: 43.545 ng

RT: 7.45 min Scan# 911

Delta R.T. -0.26 min

Lab File: BF115680.D

Acq: 19 Jul 2019 19:07

Instrument :

BNA_F

ClientSampleId :


Tot Ion: 82 Resp: 1230903

Ion Ratio Lower Upper

82 100

95 0.0 5.5 8.3#




138 0.0 14.9 22.3#

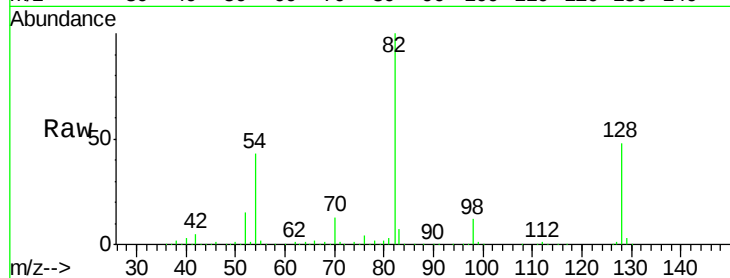

Abundance Ion 82.00 (81.70 to 82.70): BF1

Ion 95.00 (94.70 to 95.70): BF1

Ion 138.00 (137.70 to 138.70): BF1

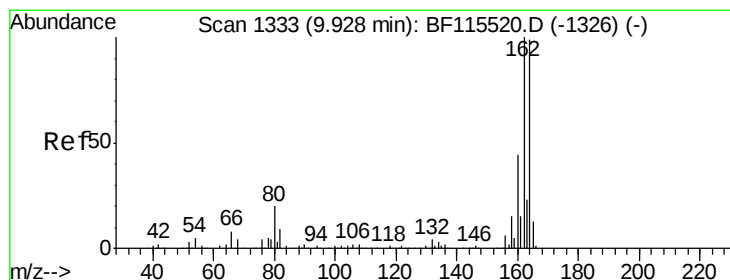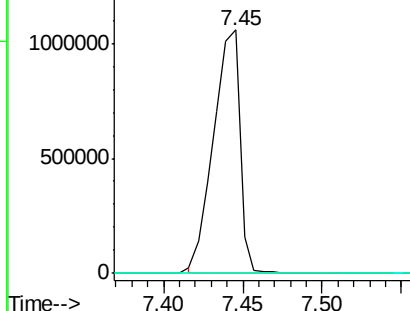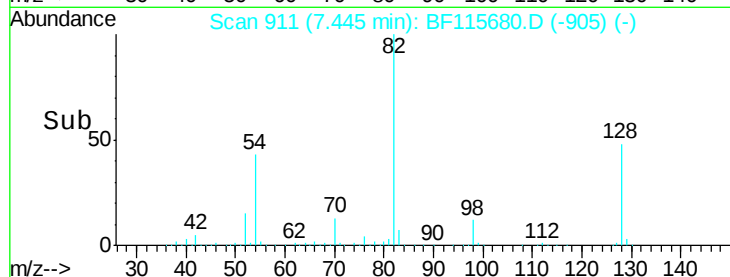

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.92 min Scan# 1331

Delta R.T. -0.01 min

Lab File: BF115680.D

Acq: 19 Jul 2019 19:07


Tgt Ion: 164 Resp: 391351

Ion Ratio Lower Upper

164 100

162 102.2 82.9 124.3



160 45.7 36.8 55.2

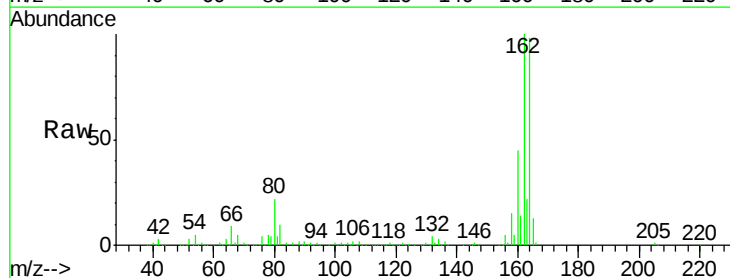


Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

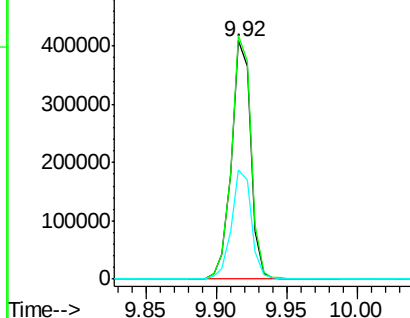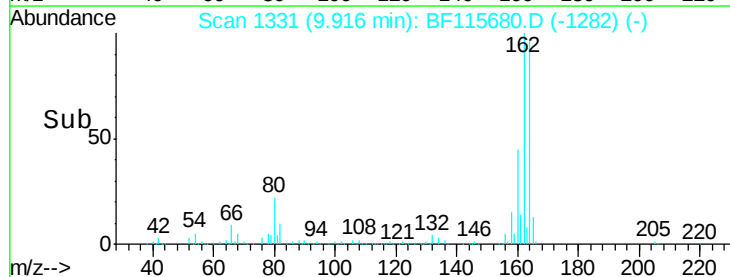

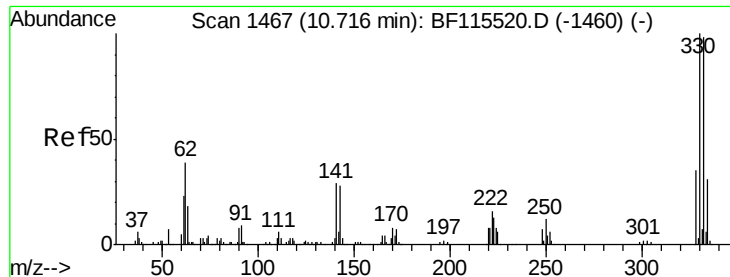

#42

2,4,6-Tribromophenol

Concen: 111.667 ng

RT: 10.71 min Scan# 1466

Delta R.T. -0.01 min

Lab File: BF115680.D

Acq: 19 Jul 2019 19:07

Instrument :

BNA_F

ClientSampleId :


Tot Ion:330 Resp: 510095

Ion Ratio Lower Upper

330 100

332 95.5 77.4 116.2




141 30.9 22.4 33.6

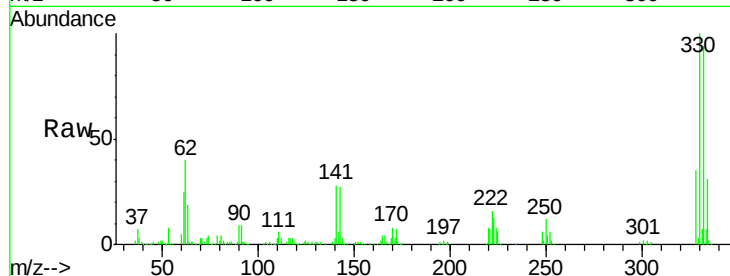

Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

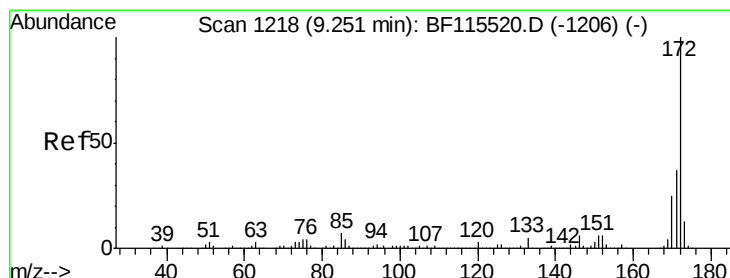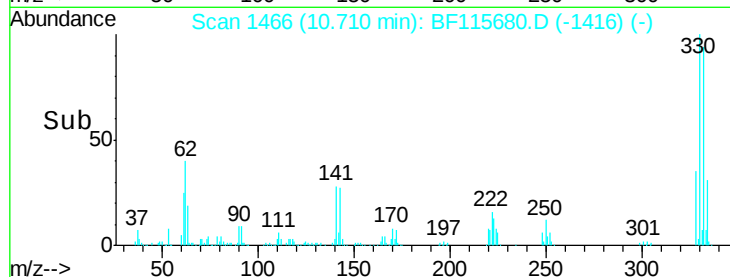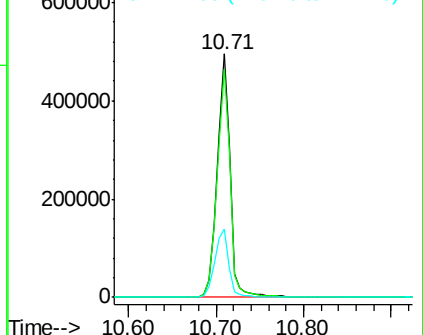

#45

2-Fluorobiphenyl

Concen: 94.847 ng

RT: 9.24 min Scan# 1216

Delta R.T. -0.01 min

Lab File: BF115680.D

Acq: 19 Jul 2019 19:07


Tgt Ion:172 Resp: 2120715

Ion Ratio Lower Upper

172 100

171 37.1 30.6 46.0



170 25.3 20.5 30.7

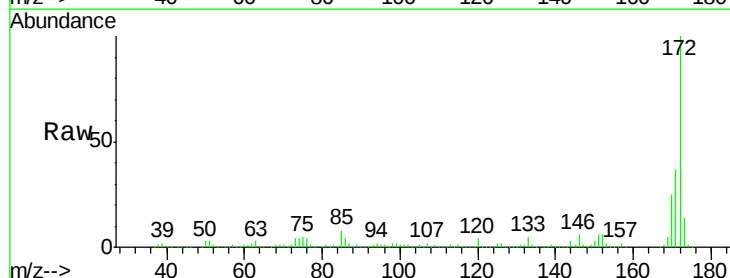


Abundance Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

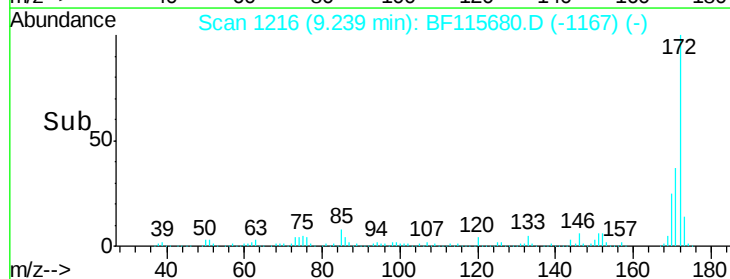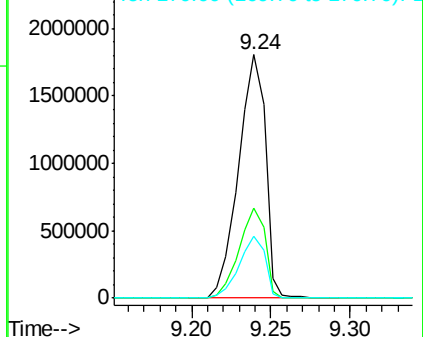

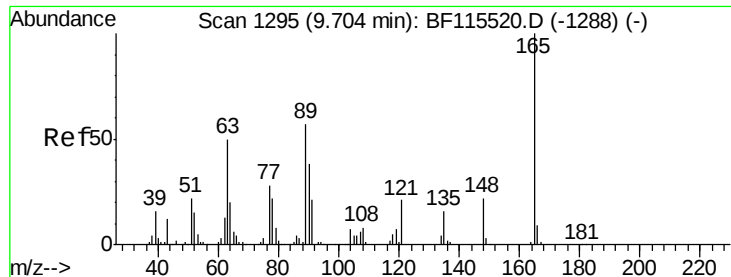

#51

2,6-Dinitrotoluene

Concen: 7.574 ng

RT: 9.92 min Scan# 1331

Delta R.T. 0.21 min

Lab File: BF115680.D

Acq: 19 Jul 2019 19:07

Instrument :

BNA_F

ClientSampleId :


Tot Ion:165 Resp: 50677

Ion Ratio Lower Upper

165 100

63 0.8 40.6 61.0#




89 1.6 43.9 65.9#



Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BF1

Ion 89.00 (88.70 to 89.70): BF1

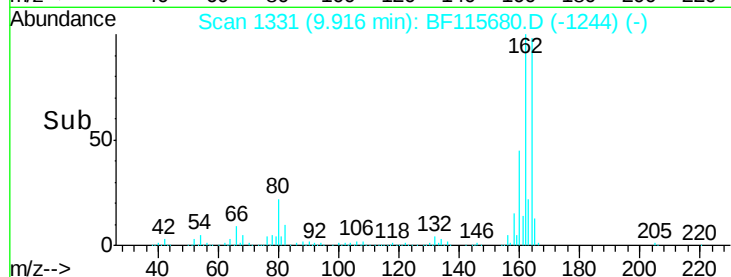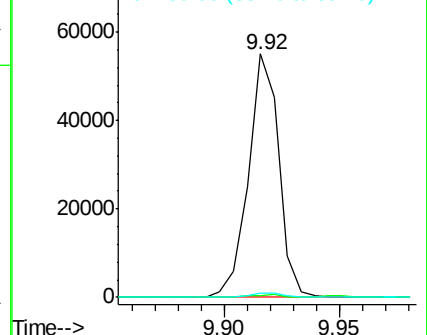

#57

2,4-Dinitrotoluene

Concen: 5.846 ng

RT: 9.92 min Scan# 1331

Delta R.T. -0.19 min

Lab File: BF115680.D

Acq: 19 Jul 2019 19:07

Tgt Ion:165 Resp: 50677


Ion Ratio Lower Upper

165 100

63 0.8 34.9 52.3#

89 1.6 57.5 86.3#

182 0.0 2.2 3.4#






Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BF1

Ion 89.00 (88.70 to 89.70): BF1

Ion 182.00 (181.70 to 182.70): E



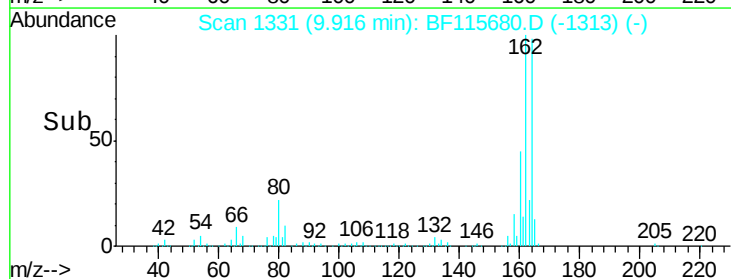
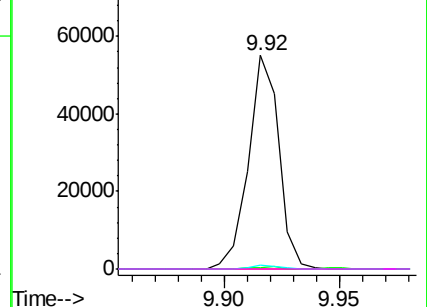


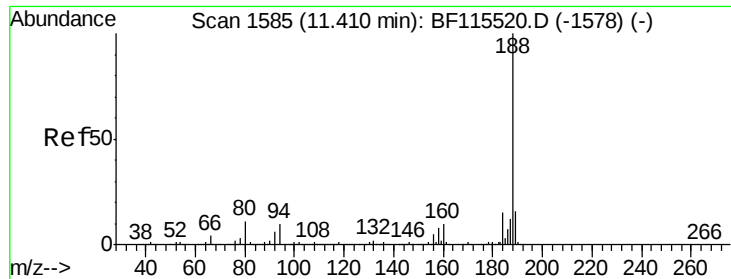

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.40 min Scan# 1584
Delta R.T. -0.01 min
Lab File: BF115680.D
Acq: 19 Jul 2019 19:07




Instrument :
BNA_F
ClientSampleId :


Tot Ion:188 Resp: 668273
Ion Ratio Lower Upper
188 100
94 9.7 7.8 11.6
80 10.5 8.6 13.0

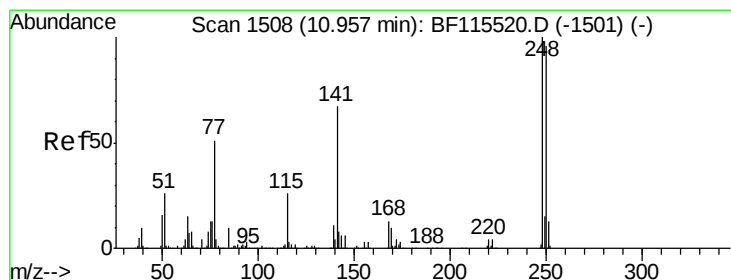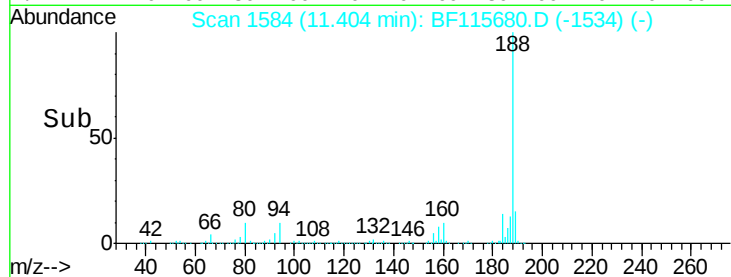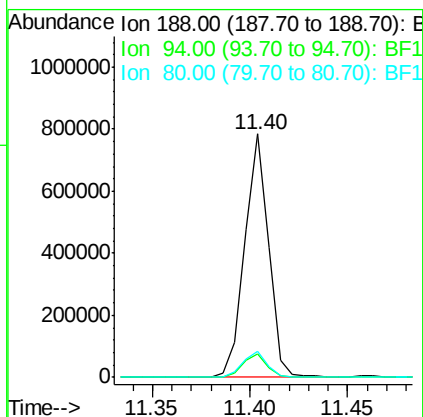

#67
4-Bromophenyl-phenylether
Concen: 3.994 ng
RT: 10.71 min Scan# 1466
Delta R.T. -0.25 min
Lab File: BF115680.D
Acq: 19 Jul 2019 19:07

Tgt Ion:248 Resp: 30503
Ion Ratio Lower Upper
248 100
250 204.4 78.0 117.0#
141 464.6 57.7 86.5#


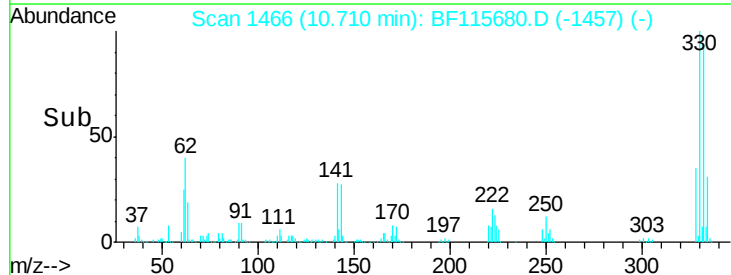
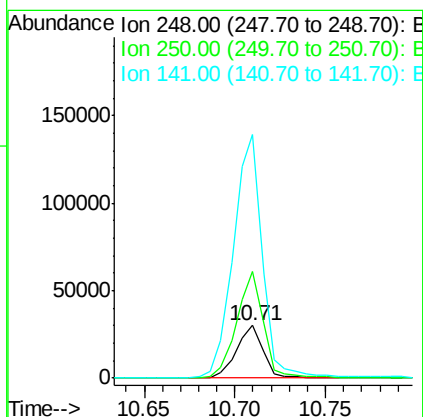



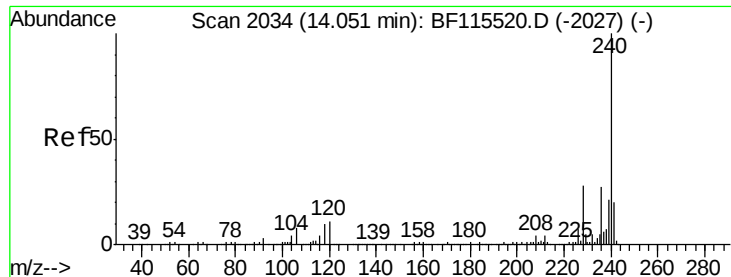

#76
 Chrysene-d12
 Concen: 20.000 ng
 RT: 14.04 min Scan# 2033
 Delta R.T. -0.01 min
 Lab File: BF115680.D
 Acq: 19 Jul 2019 19:07




Instrument :
 BNA_F
 ClientSampleId :


Tot Ion:240 Resp: 407757
 Ion Ratio Lower Upper
 240 100
 120 10.6 8.6 13.0
 236 26.2 21.3 31.9

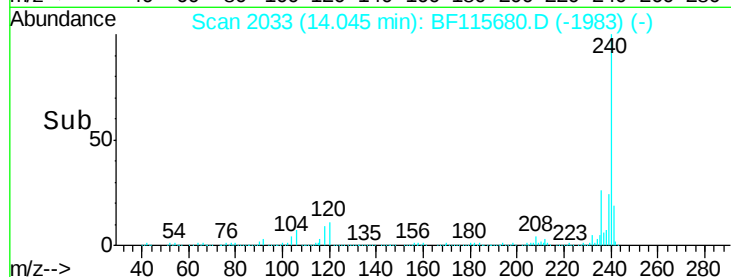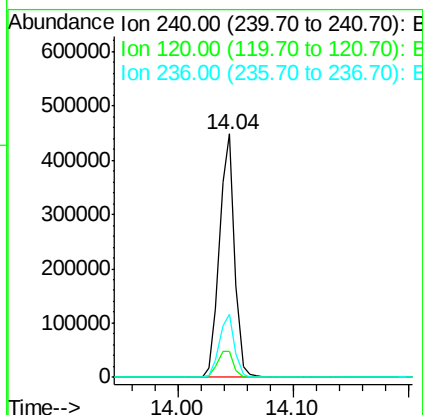

#79
 Terphenyl-d14
 Concen: 87.093 ng
 RT: 12.99 min Scan# 1854
 Delta R.T. -0.01 min
 Lab File: BF115680.D
 Acq: 19 Jul 2019 19:07

Tgt Ion:244 Resp: 1924626
 Ion Ratio Lower Upper
 244 100
 212 7.1 6.0 9.0
 122 11.8 8.6 12.8

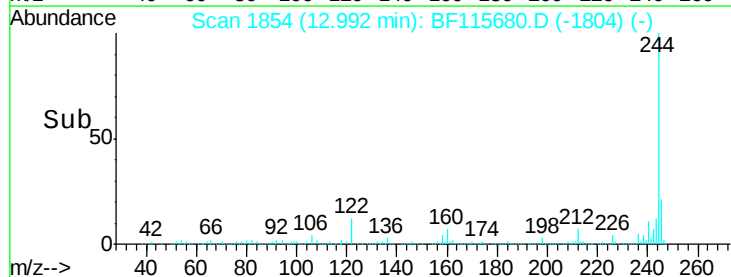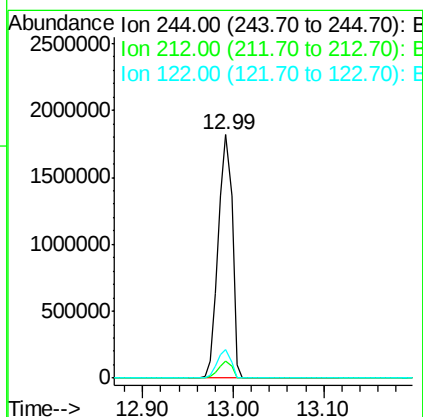


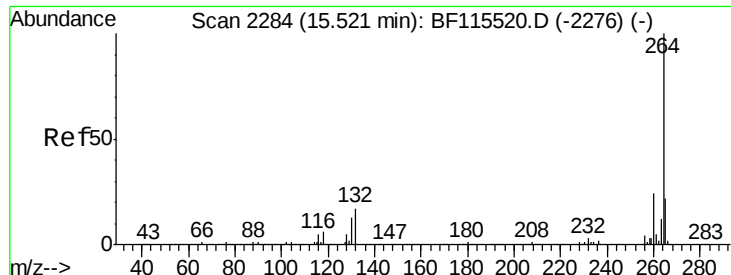

#87
 Pervlene-d12
 Concen: 20.000 ng
 RT: 15.52 min Scan# 2284
 Delta R.T. 0.00 min
 Lab File: BF115680.D
 Acq: 19 Jul 2019 19:07

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
264	100		
260	23.7	19.8	29.8
265	21.5	17.7	26.5

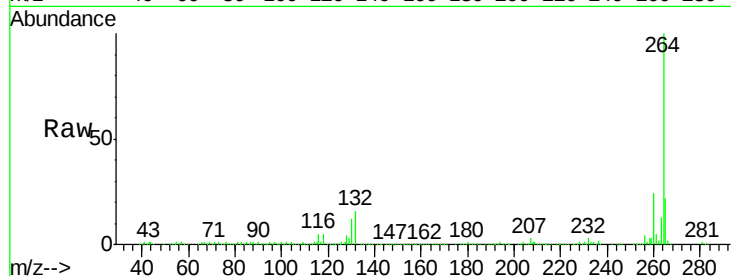

Abundance

Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

