
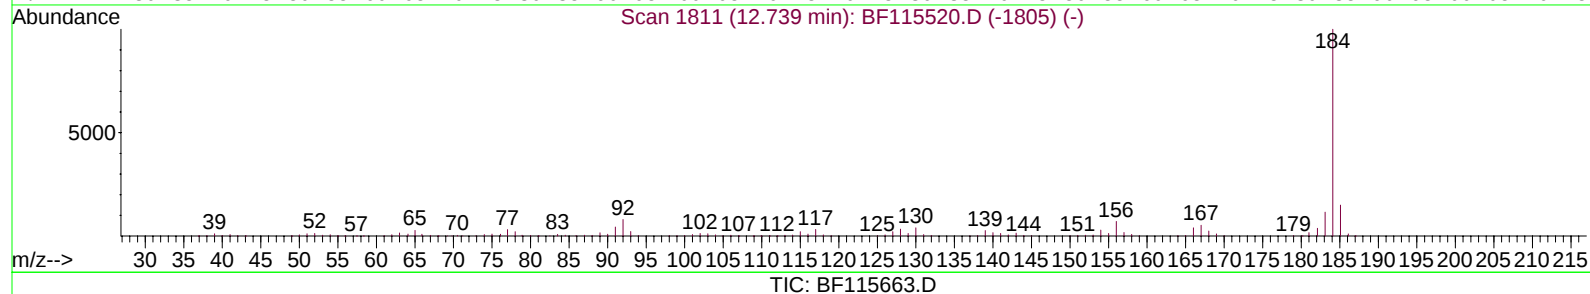
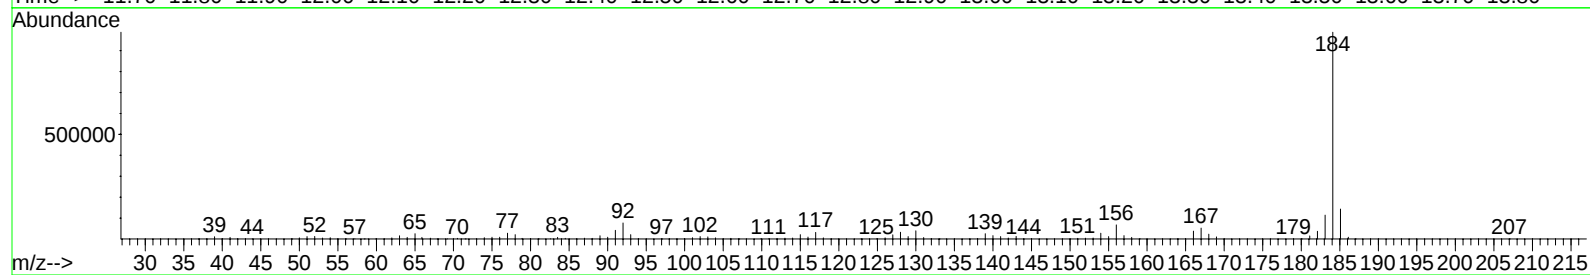


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF071919\
Data File : BF115663.D
Acq On : 19 Jul 2019 8:14
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 19 18:30:03 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF071219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 12 14:03:52 2019
Response via : Initial Calibration

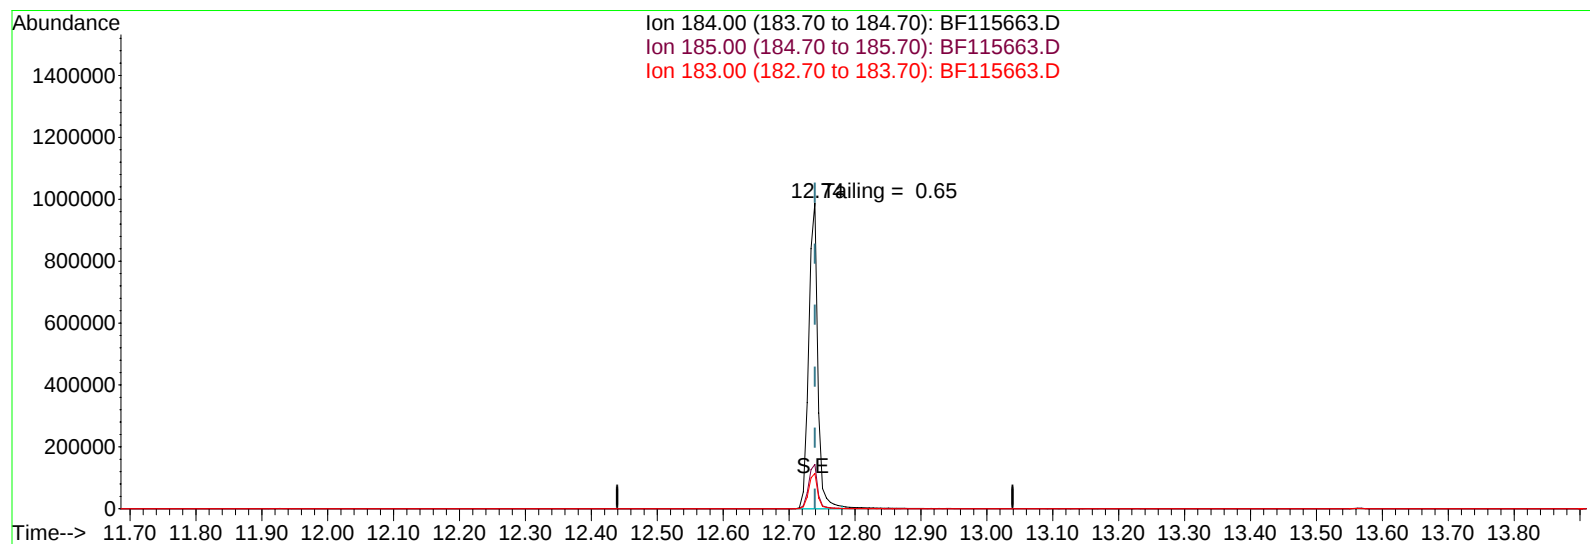

(77) Benzidine




12.739min (+0.000) 0.00ng

response 967342

Ion	Exp%	Act%
184.00	100	100
185.00	15.00	14.48
183.00	11.60	11.59
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF071919\
Data File : BF115663.D
Acq On : 19 Jul 2019 8:14
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 19 18:30:03 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF071219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 12 14:03:52 2019
Response via : Initial Calibration

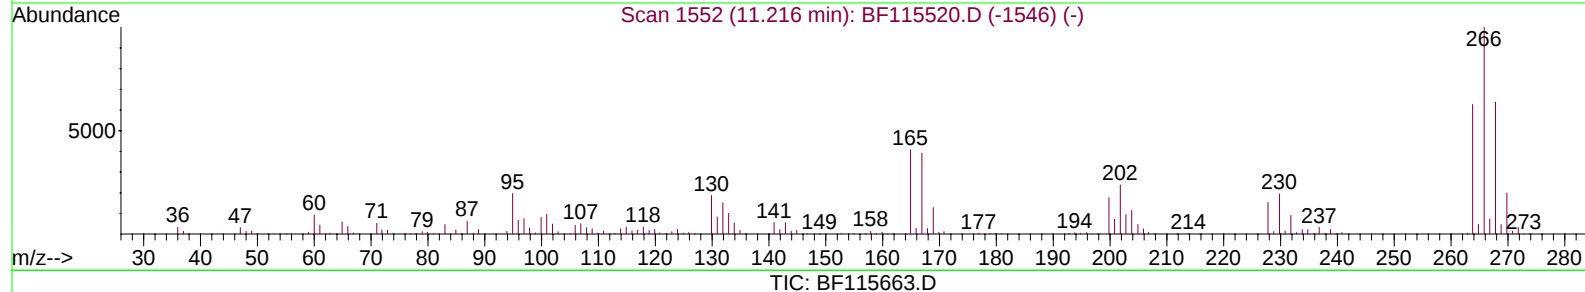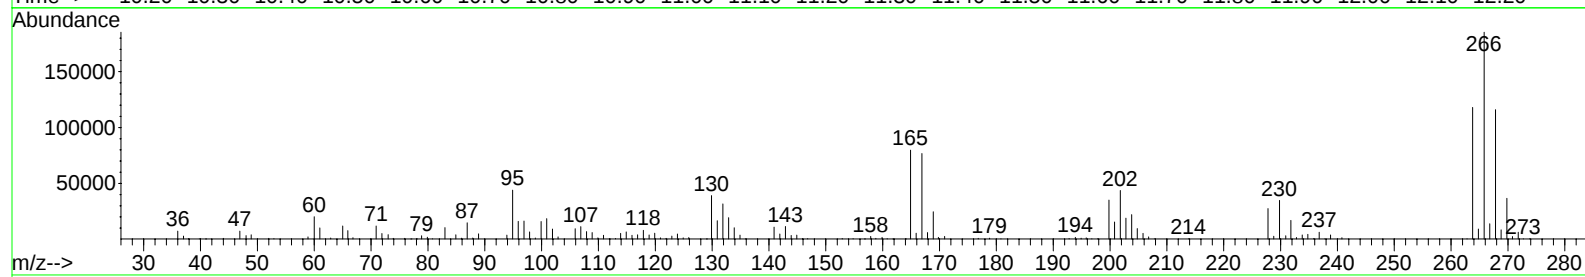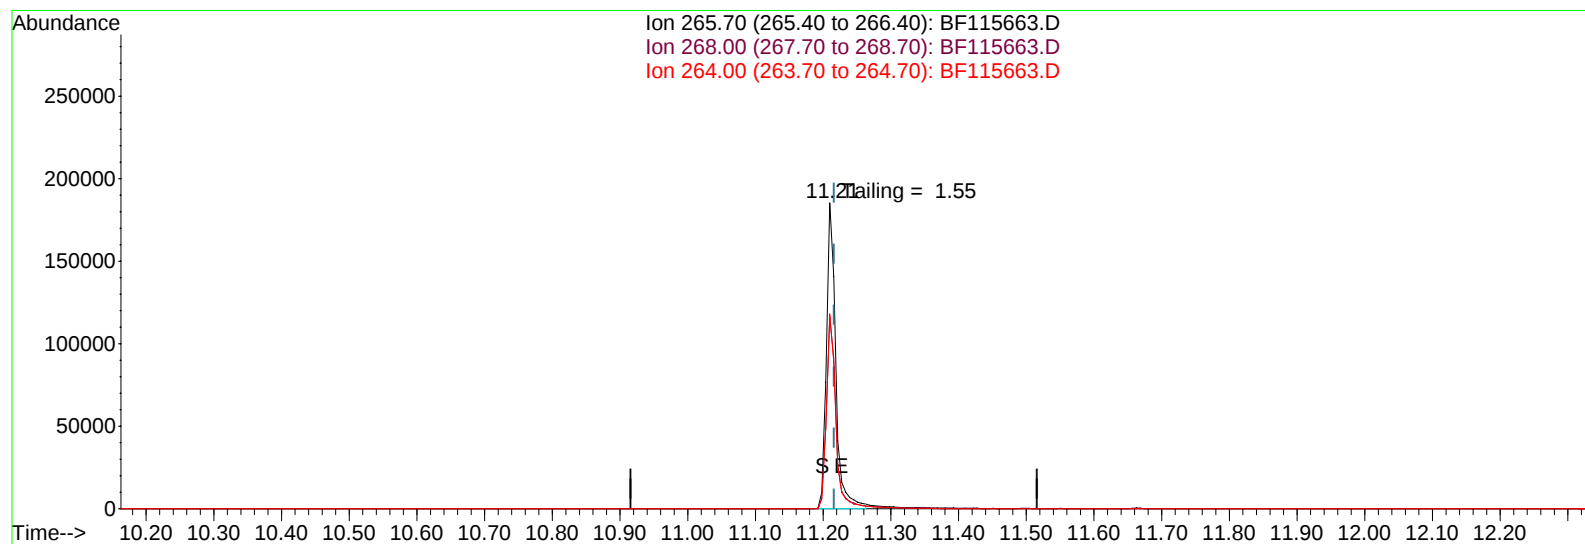

(70) Pentachlorophenol (C)

11.210min (-0.006) 38964.26ng

response 182251

Ion	Exp%	Act%
265.70	100	100
268.00	64.50	62.57
264.00	63.30	63.70
0.00	0.00	0.00