
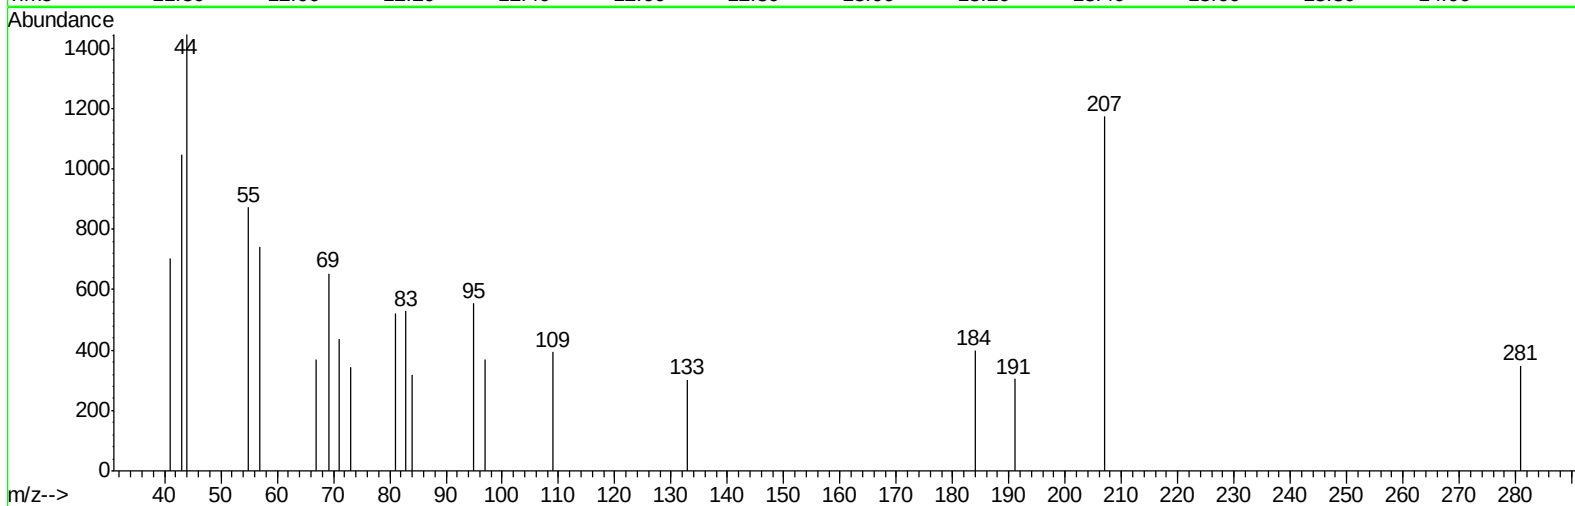


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF071919\
Data File : BF115676.D
Acq On : 19 Jul 2019 16:39
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 20 05:51:02 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF071219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 12 14:03:52 2019
Response via : Initial Calibration

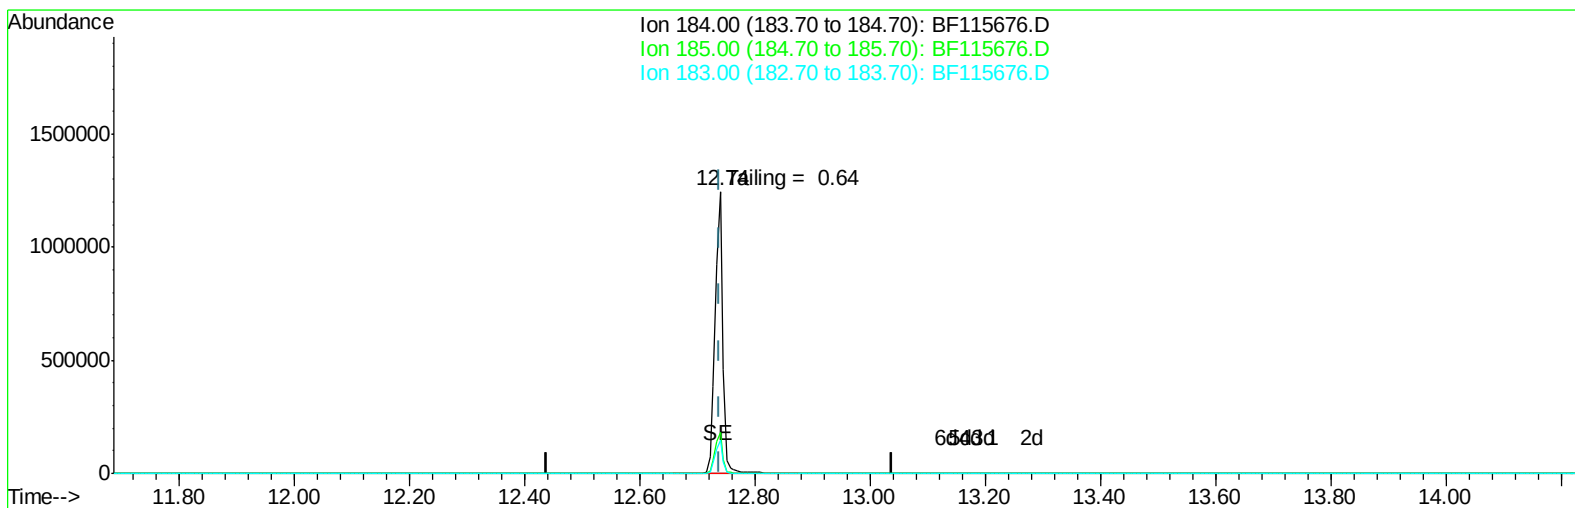

TIC: BF115676.D

(77) Benzidine



13.216min (+0.476) 32.66ng

response 140

Ion	Exp%	Act%
184.00	100	100
185.00	15.00	0.00#
183.00	11.60	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF071919\
Data File : BF115676.D
Acq On : 19 Jul 2019 16:39
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 20 05:51:02 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF071219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 12 14:03:52 2019
Response via : Initial Calibration

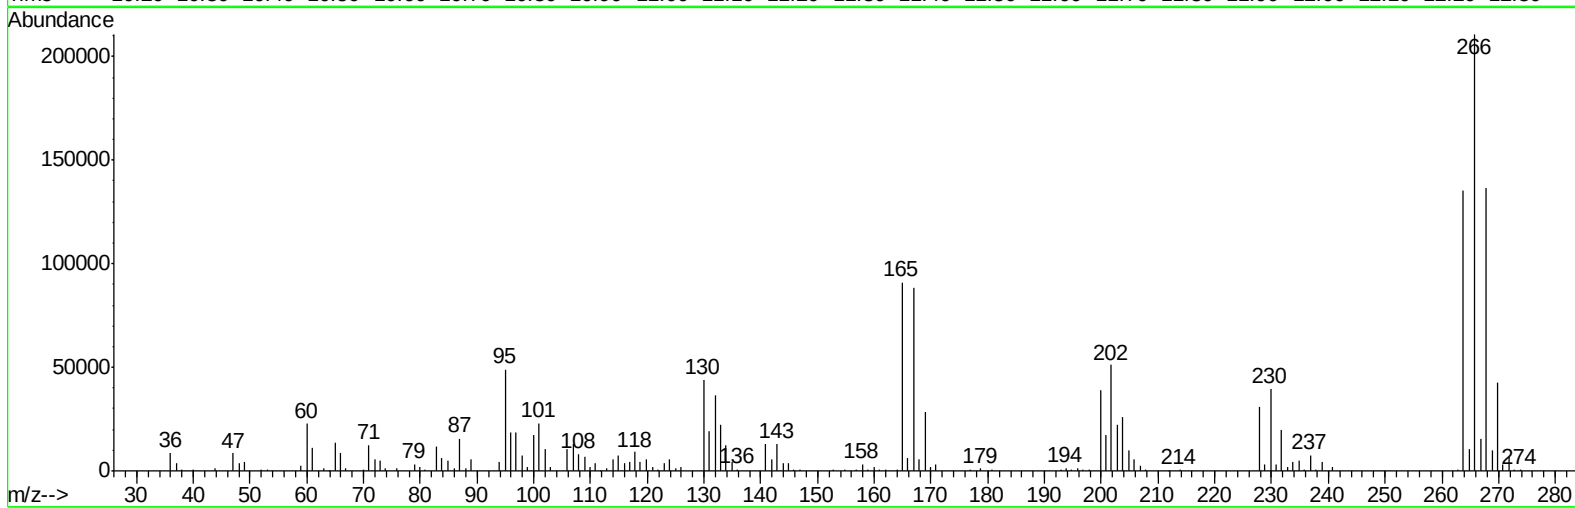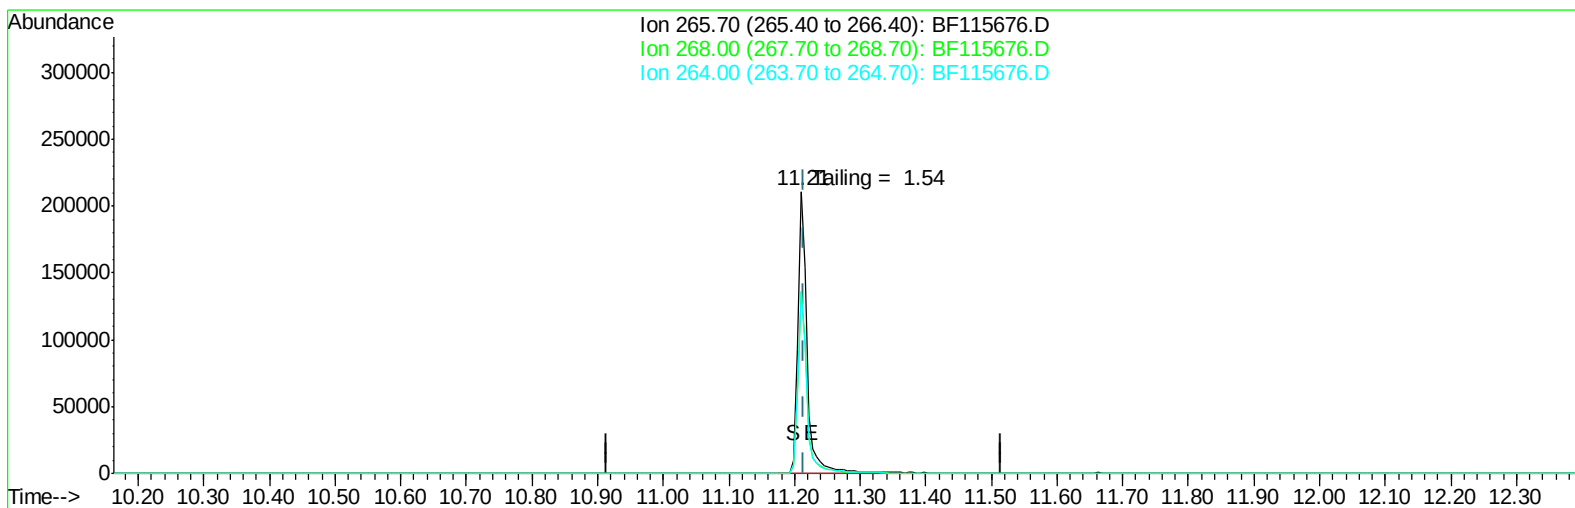

TIC: BF115676.D

(70) Pentachlorophenol (C)

11.210min (-0.006) 30005.27ng

response 209322

Ion	Exp%	Act%
265.70	100	100
268.00	64.50	64.70
264.00	63.30	64.37
0.00	0.00	0.00