


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF071919\
 Data File : BF115676.D
 Acq On : 19 Jul 2019 16:39
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF071219.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jul 12 14:03:52 2019

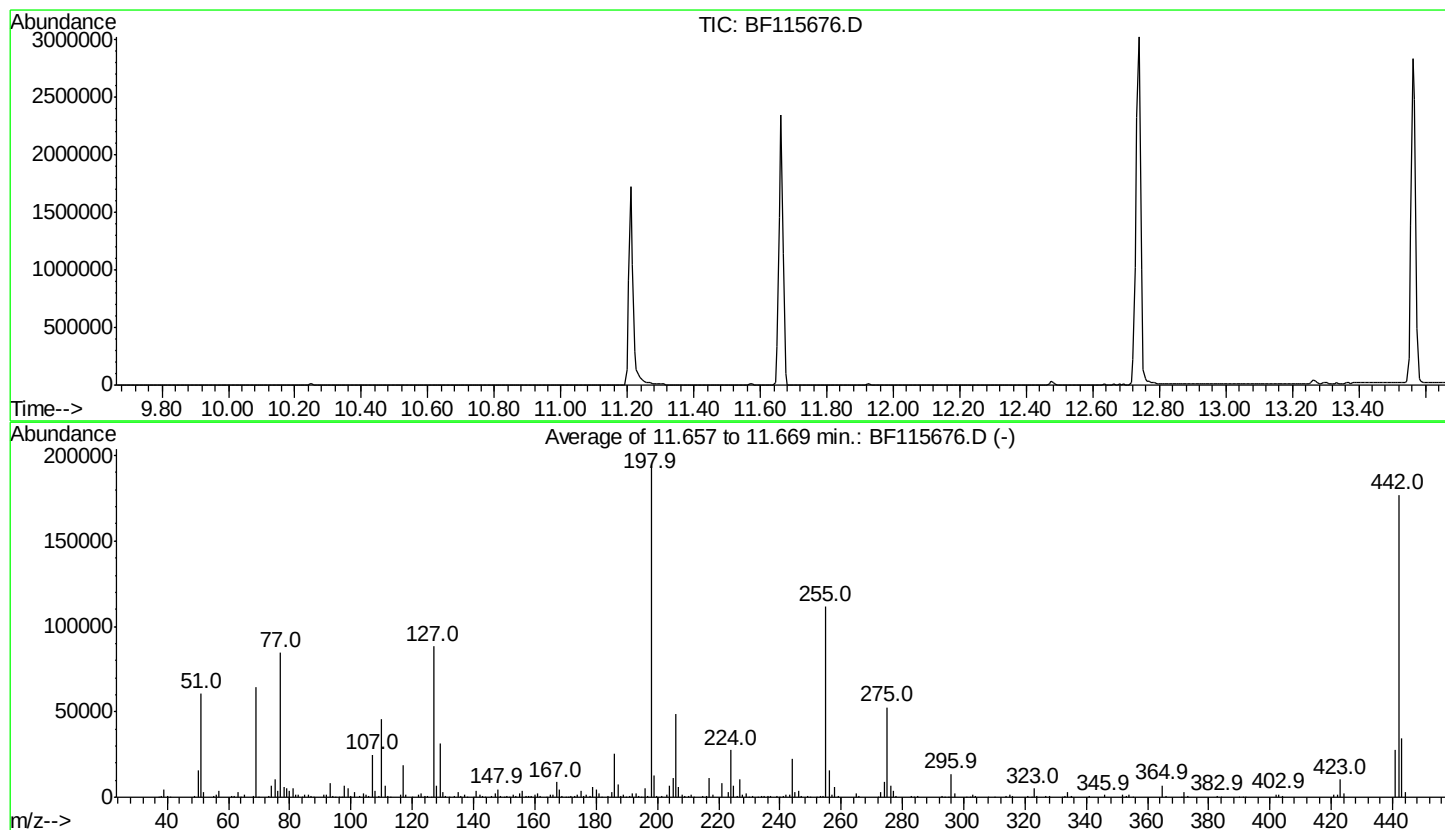

AutoFind: Scans 1627, 1628, 1629; Background Corrected with Scan 1622

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.3	60672	PASS
68	69	0.00	2	1.8	1131	PASS
69	198	0.00	100	33.2	64376	PASS
70	69	0.00	2	0.6	359	PASS
127	198	10	80	45.5	88256	PASS
197	198	0.00	2	0.6	1088	PASS
198	198	100	100	100.0	194104	PASS
199	198	5	9	6.6	12891	PASS
275	198	10	60	27.0	52472	PASS
365	198	1	100	3.5	6862	PASS
441	198	0.01	100	14.3	27736	PASS
442	198	50	100	91.2	176944	PASS
443	442	15	24	19.3	34162	PASS