
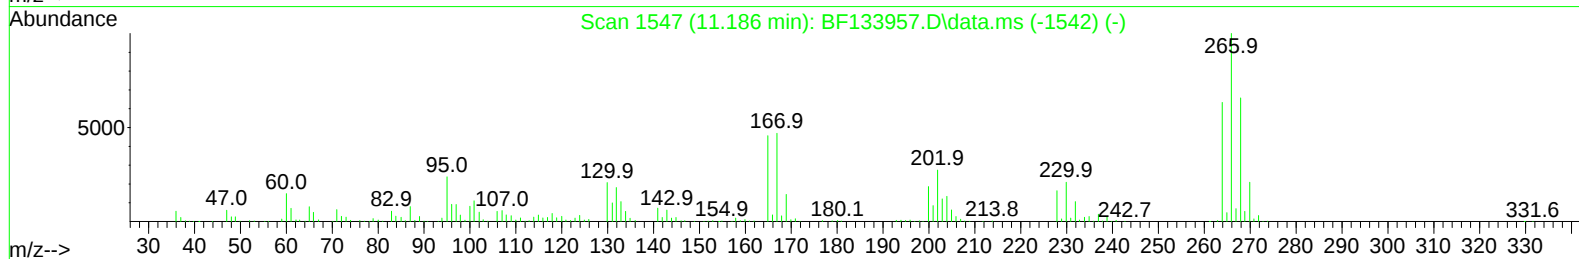
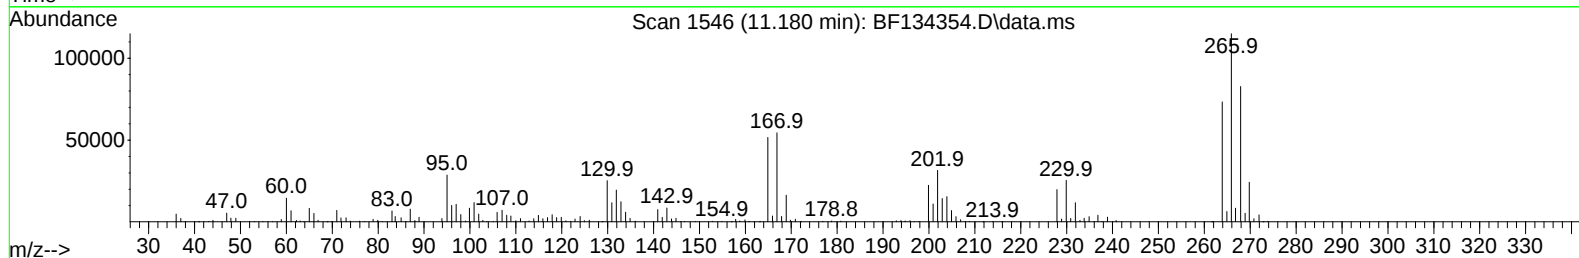


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071923\
Data File : BF134354.D
Acq On : 19 Jul 2023 12:29
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 19 14:08:20 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 14 22:51:27 2023
Response via : Initial Calibration

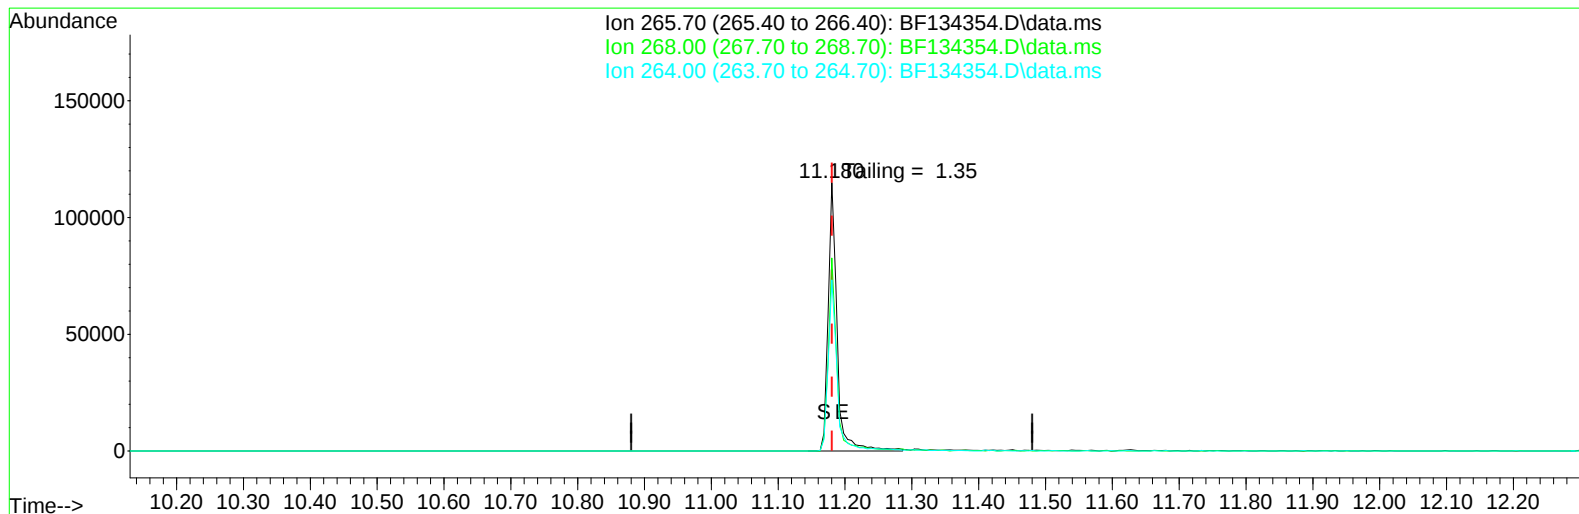

TIC: BF134354.D\data.ms

(70) Pentachlorophenol (C)




11.180min (0.000) 24915.29 ng

response 107765

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.80	71.93
264.00	63.30	63.77
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071923\
Data File : BF134354.D
Acq On : 19 Jul 2023 12:29
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 19 14:08:20 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 14 22:51:27 2023
Response via : Initial Calibration

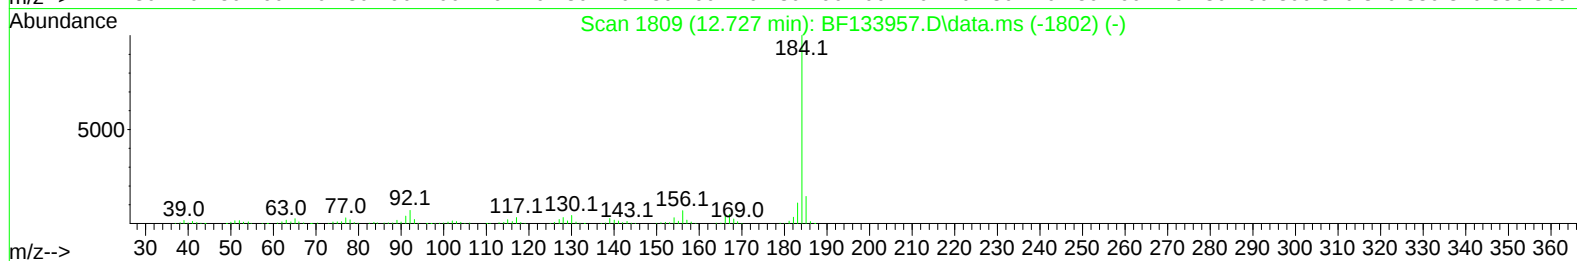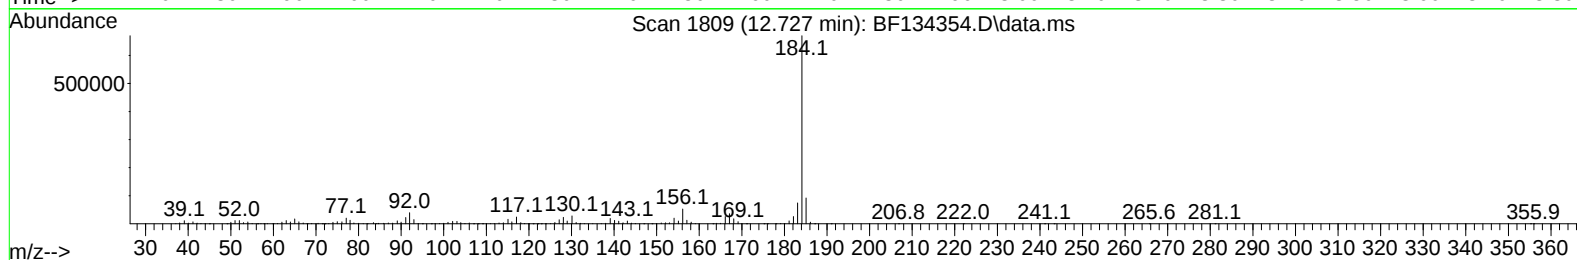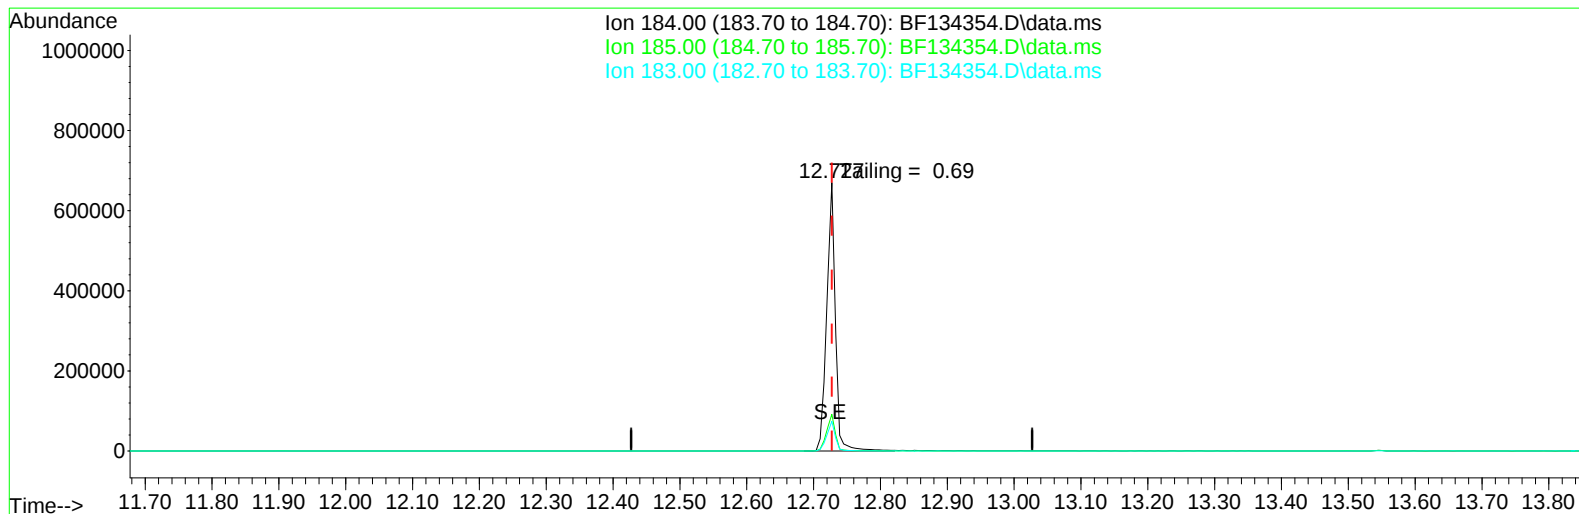

TIC: BF134354.D\data.ms

(77) Benzidine

12.727min (0.000) 426374.76 ng

response 598573

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	13.69
183.00	11.00	11.08
0.00	0.00	0.00