

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF072018\
 Data File : BF107567.D
 Acq On : 21 Jul 2018 11:10
 Operator : JU/SJ
 Sample : J4061-10
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 071718-TIPC-F-U-S

Quant Time: Jul 23 03:27:59 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072018.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 20 16:29:27 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.97	152	303833	20.00	ng	0.00
21) Naphthalene-d8	8.25	136	1080414	20.00	ng	0.00
38) Acenaphthene-d10	10.01	164	387967	20.00	ng	0.00
63) Phenanthrene-d10	11.51	188	684470	20.00	ng	0.00
75) Chrysene-d12	14.16	240	706380	20.00	ng	0.00
86) Perylene-d12	15.69	264	587891	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.60	112	790376	41.82	ng	0.00
7) Phenol-d6	6.60	99	699911	30.85	ng	-0.01
23) Nitrobenzene-d5	7.54	82	1710423	106.84	ng	-0.01
41) 2,4,6-Tribromophenol	10.81	330	378579	85.81	ng	-0.01
44) 2-Fluorobiphenyl	9.33	172	2609551	135.09	ng	0.00
78) Terphenyl-d14	13.10	244	2213650	80.23	ng	0.00
Target Compounds						
19) n-Nitroso-di-n-propylamine	7.54	70	224835	15.338	ng	# 79
25) Isophorone	7.54	82	1710414	50.038	ng	# 64
50) 2,6-Dinitrotoluene	10.01	165	48284	8.317	ng	# 25
56) 2,4-Dinitrotoluene	10.01	165	48284	6.890	ng	# 23
64) 4,6-Dinitro-2-methylphenol	10.81	198	778	8.874	ng	# 1
66) 4-Bromophenyl-phenylether	10.81	248	22940	2.847	ng	# 1
73) Di-n-butylphthalate	12.05	149	889	Below Cal		# 78


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF072018\
Data File : BF107567.D
Acq On : 21 Jul 2018 11:10
Operator : JU/SJ
Sample : J4061-10
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
071718-TIPC-F-U-S

Quant Time: Jul 23 03:27:59 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 20 16:29:27 2018
Response via : Initial Calibration

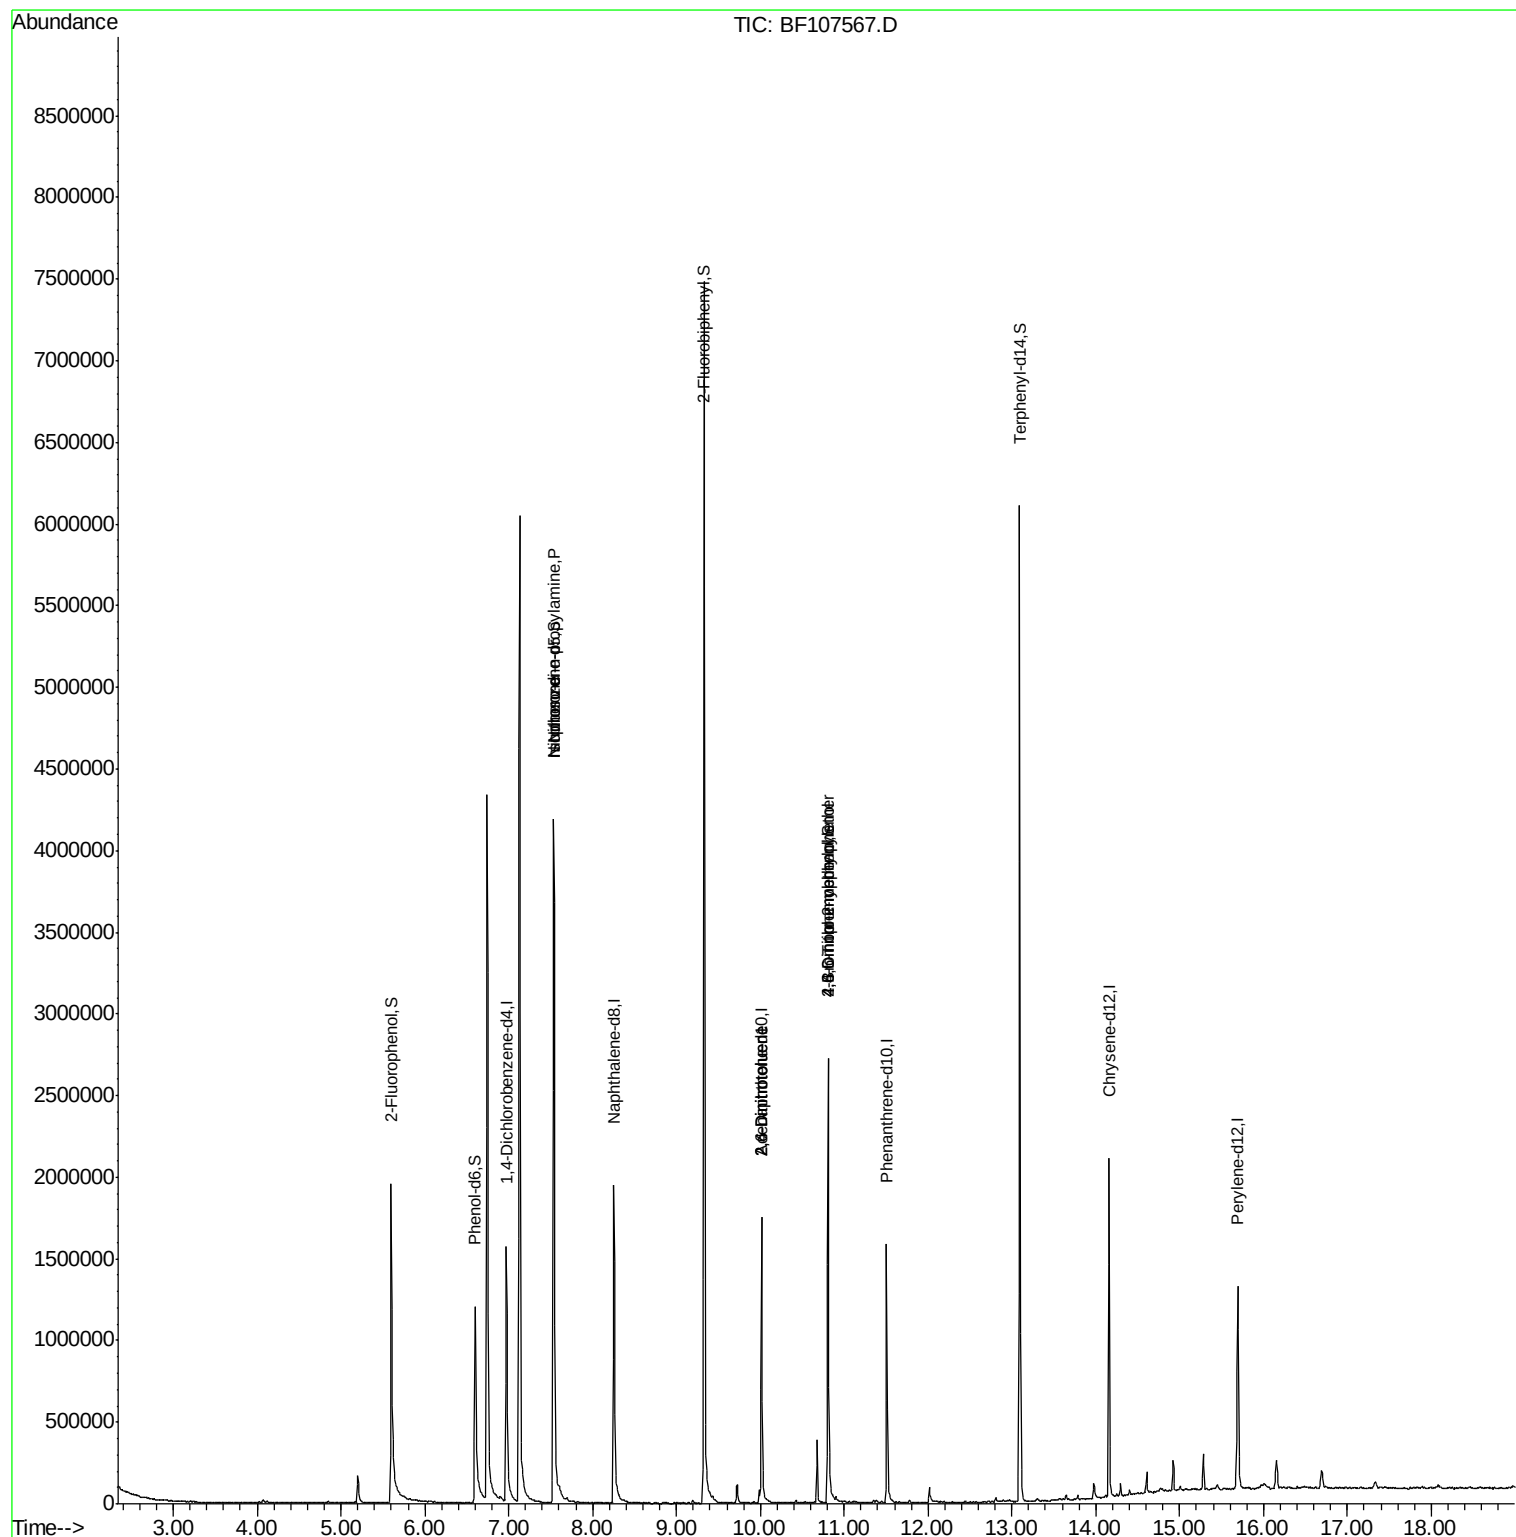

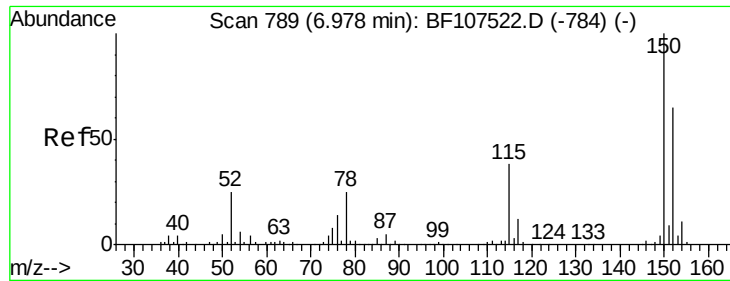


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.97 min Scan# 788
Delta R.T. -0.01 min
Lab File: BF107567.D
Acq: 21 Jul 2018 11:10

Instrument :
BNA_F
ClientSampleId :
071718-TIPC-F-U-S

Tgt Ion:152 Resp: 303833
Ion Ratio Lower Upper
152 100
150 156.1 124.6 186.8
115 60.7 50.1 75.1

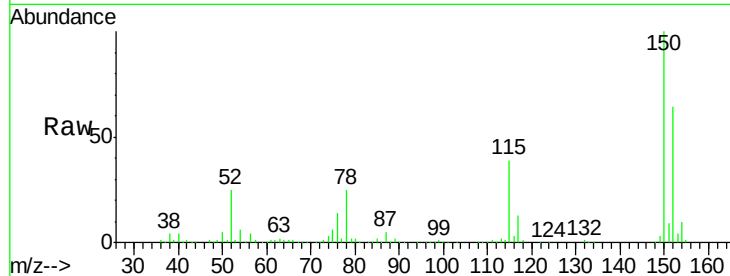


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

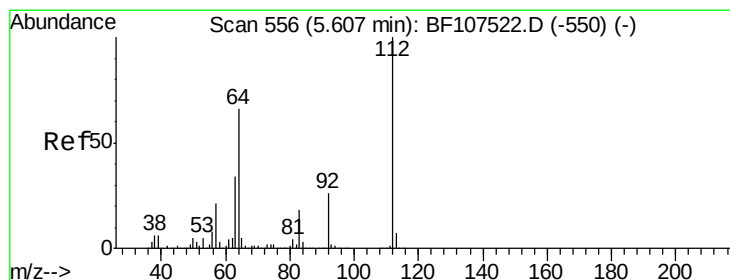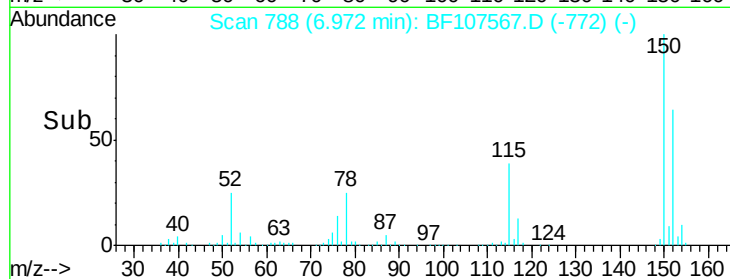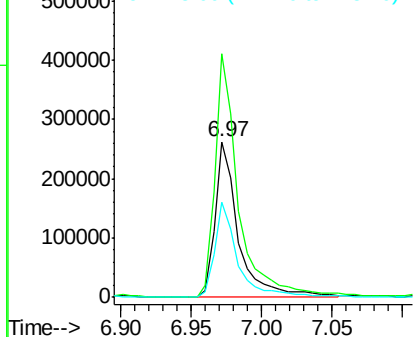



#5


2-Fluorophenol
Concen: 41.825 ng
RT: 5.60 min Scan# 555
Delta R.T. -0.01 min
Lab File: BF107567.D
Acq: 21 Jul 2018 11:10

Tgt Ion:112 Resp: 790376
Ion Ratio Lower Upper
112 100
64 65.0 47.9 71.9
63 33.1 23.7 35.5

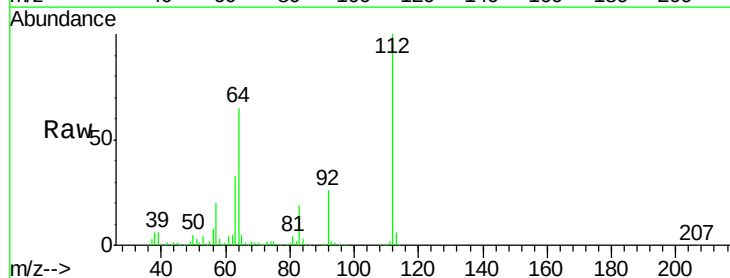

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

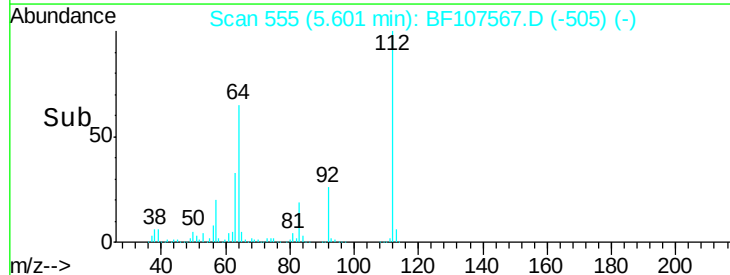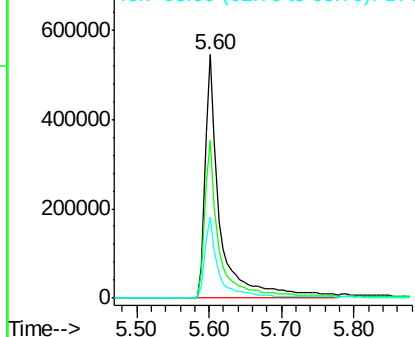

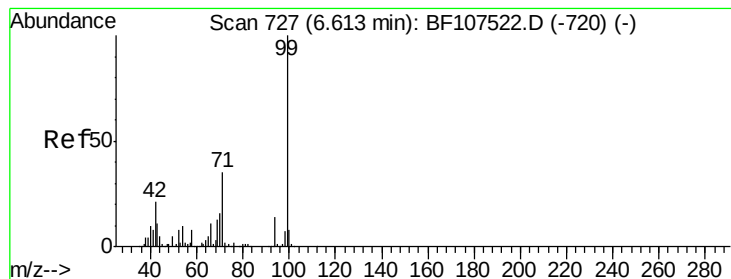

#7

Phenol-d6

Concen: 30.846 ng

RT: 6.60 min Scan# 725

Delta R.T. -0.01 min

Lab File: BF107567.D

Acq: 21 Jul 2018 11:10

Instrument :

BNA_F

ClientSampleId :

071718-TIPC-F-U-S





Tgt Ion: 99 Resp: 699911

Ion Ratio Lower Upper

99 100

42 18.9 14.5 21.7

71 30.9 25.4 38.0

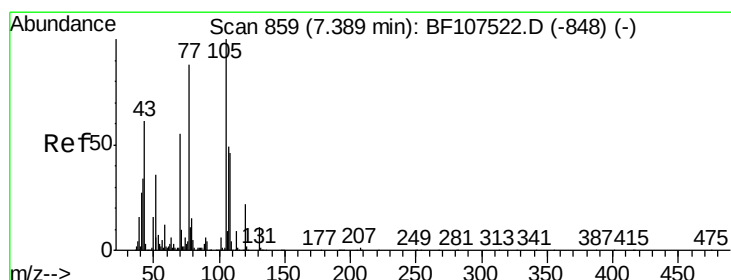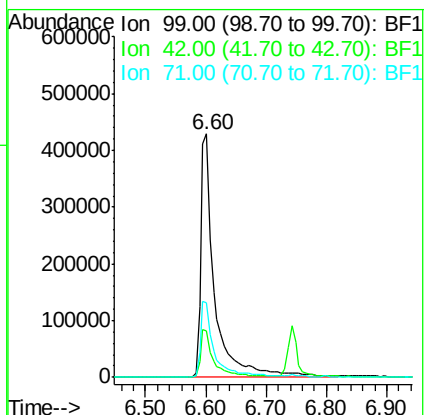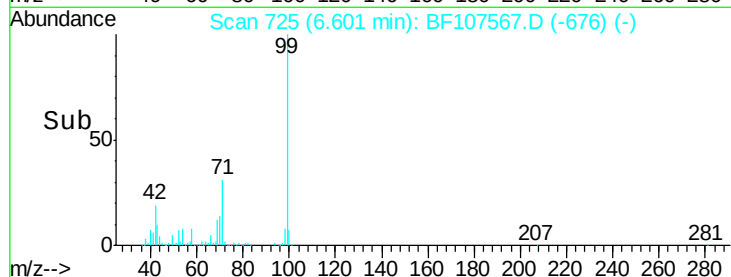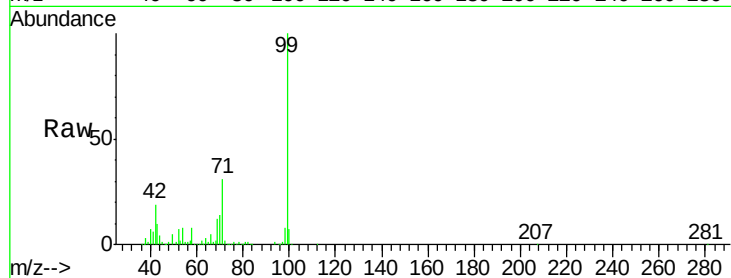

#19

n-Nitroso-di-n-propylamine

Concen: 15.338 ng

RT: 7.54 min Scan# 884

Delta R.T. 0.15 min

Lab File: BF107567.D

Acq: 21 Jul 2018 11:10

Tgt Ion: 70 Resp: 224835




Ion Ratio Lower Upper


70 100

42 49.7 47.5 71.3

101 0.0 7.4 11.2#

130 2.1 16.6 25.0#

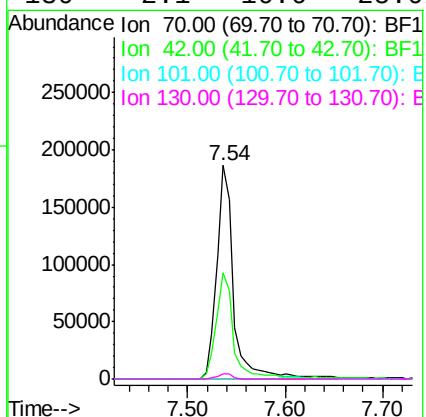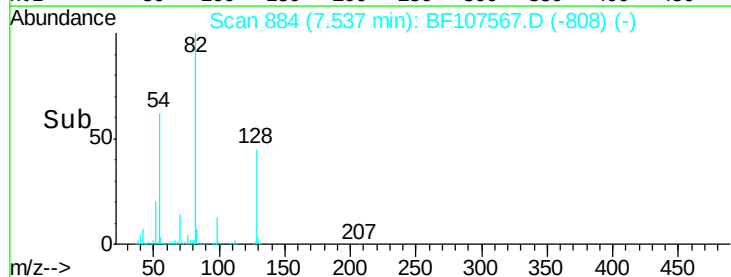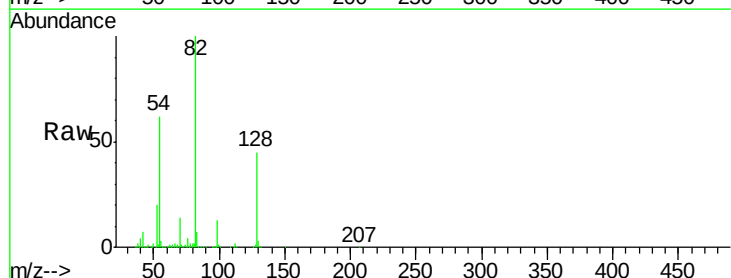


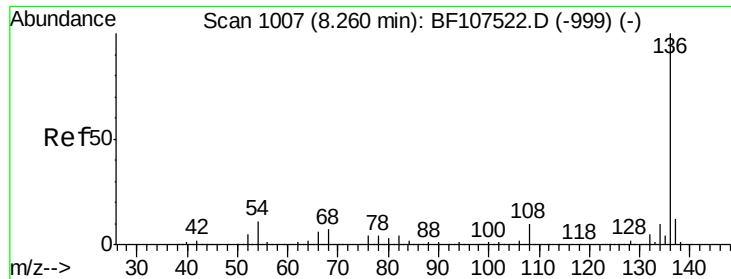




#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.25 min Scan# 1006
Delta R.T. -0.01 min
Lab File: BF107567.D
Acq: 21 Jul 2018 11:10

Instrument :
BNA_F
ClientSampleId :
071718-TIPC-F-U-S

Tgt Ion:136 Resp: 1080414
Ion Ratio Lower Upper
136 100
137 11.4 8.9 13.3
54 10.5 6.6 9.8#
68 6.5 5.0 7.4

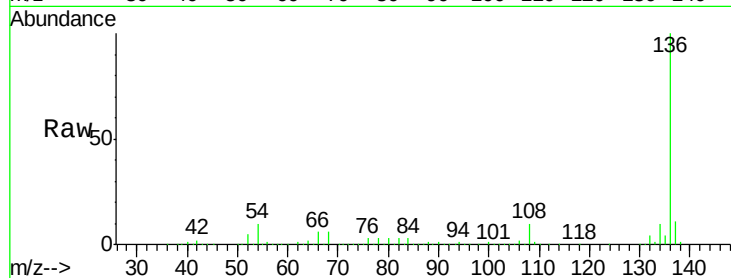


Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1

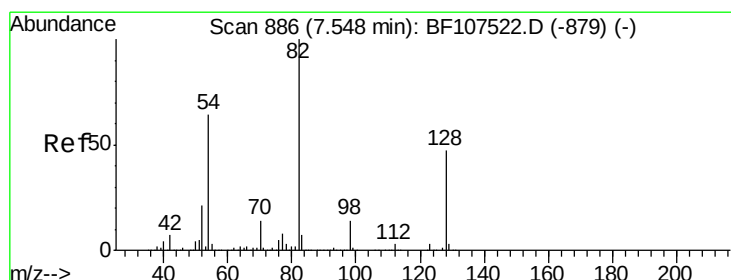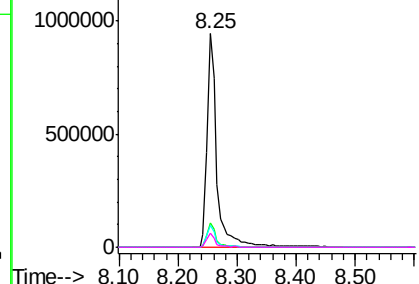
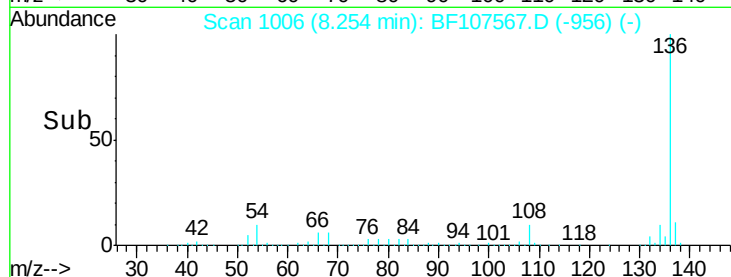



#23
Nitrobenzene-d5
Concen: 106.841 ng
RT: 7.54 min Scan# 884
Delta R.T. -0.01 min
Lab File: BF107567.D
Acq: 21 Jul 2018 11:10

Tgt Ion: 82 Resp: 1710423
Ion Ratio Lower Upper
82 100
128 45.5 36.1 54.1
54 62.1 41.4 62.2

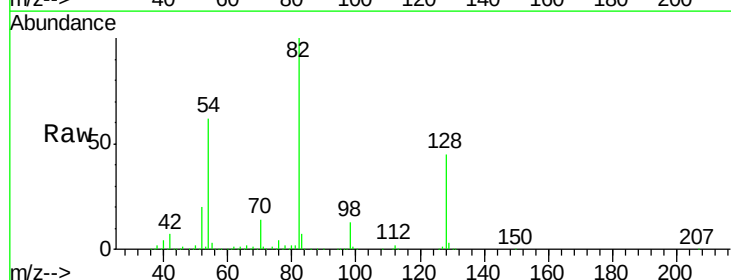

Abundance Ion 82.00 (81.70 to 82.70): BF1
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BF1

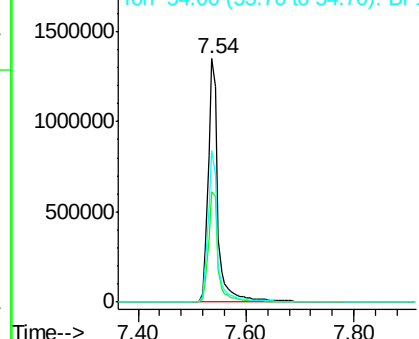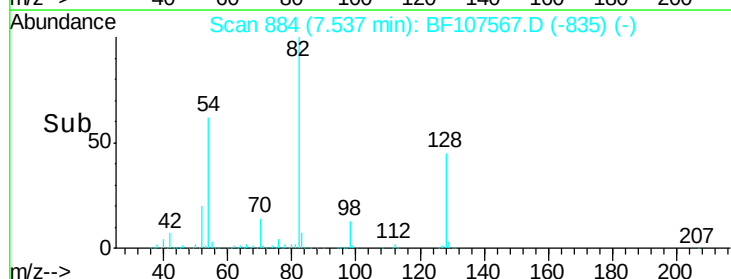


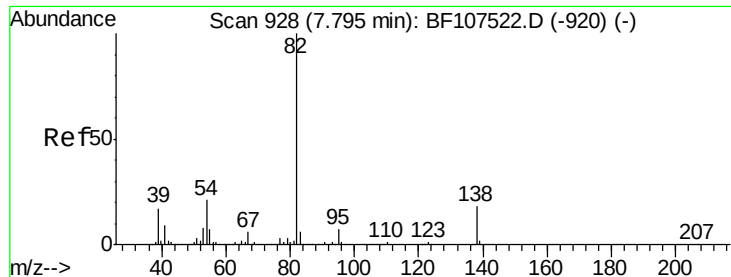




#25
Isophorone
Concen: 50.038 ng
RT: 7.54 min Scan# 884
Delta R.T. -0.26 min
Lab File: BF107567.D
Acq: 21 Jul 2018 11:10

Instrument :
BNA_F
ClientSampleId :
071718-TIPC-F-U-S

Tgt Ion: 82 Resp: 1710414
Ion Ratio Lower Upper
82 100
95 0.0 5.2 7.8#
138 0.0 14.9 22.3#

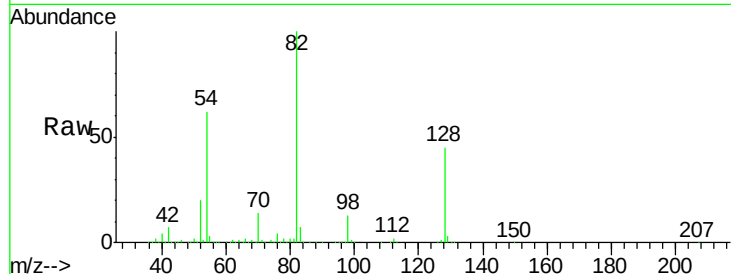


Abundance Ion 82.00 (81.70 to 82.70): BF1
Ion 95.00 (94.70 to 95.70): BF1
Ion 138.00 (137.70 to 138.70): BF1

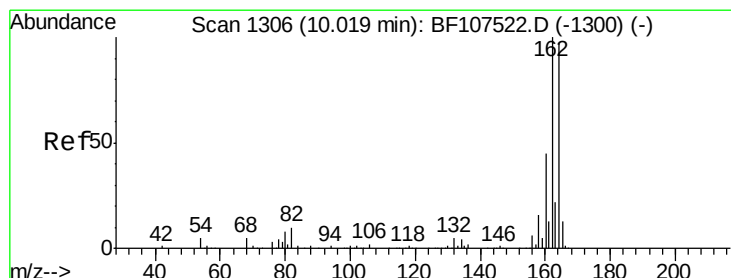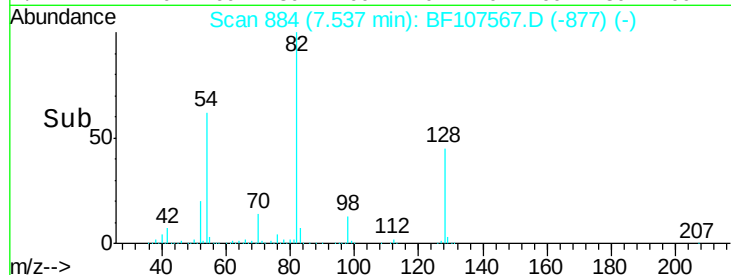
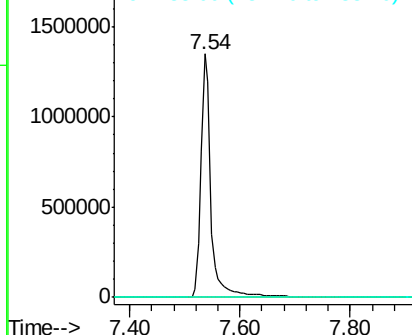



#38
Acenaphthene-d10
Concen: 20.000 ng
RT: 10.01 min Scan# 1305
Delta R.T. -0.01 min
Lab File: BF107567.D
Acq: 21 Jul 2018 11:10

Tgt Ion: 164 Resp: 387967
Ion Ratio Lower Upper
164 100
162 104.3 86.1 129.1
160 47.5 38.3 57.5

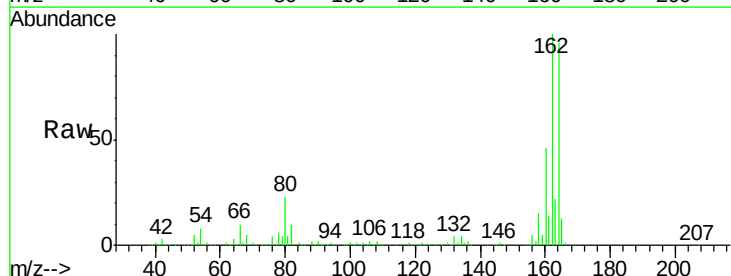

Abundance Ion 164.00 (163.70 to 164.70): BF1
Ion 162.00 (161.70 to 162.70): BF1
Ion 160.00 (159.70 to 160.70): BF1

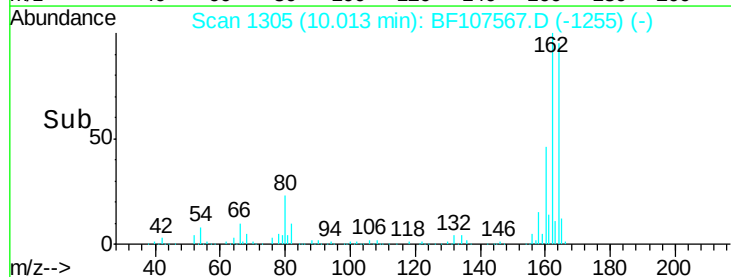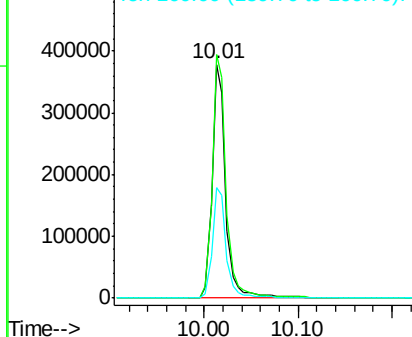


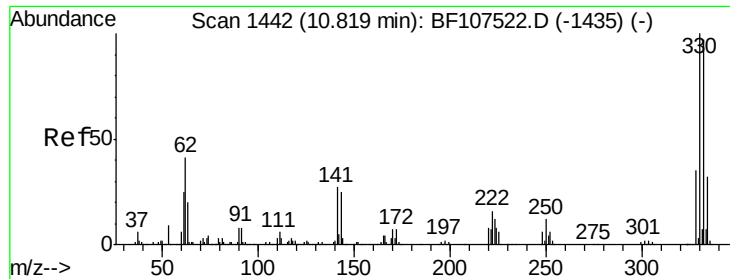




#41
 2,4,6-Tribromophenol
 Concen: 85.811 ng
 RT: 10.81 min Scan# 1440
 Delta R.T. -0.01 min
 Lab File: BF107567.D
 Acq: 21 Jul 2018 11:10

Instrument :
 BNA_F
 ClientSampleId :
 071718-TIPC-F-U-S

Tgt Ion:330 Resp: 378579
 Ion Ratio Lower Upper
 330 100
 332 97.0 77.0 115.6
 141 30.8 29.9 44.9

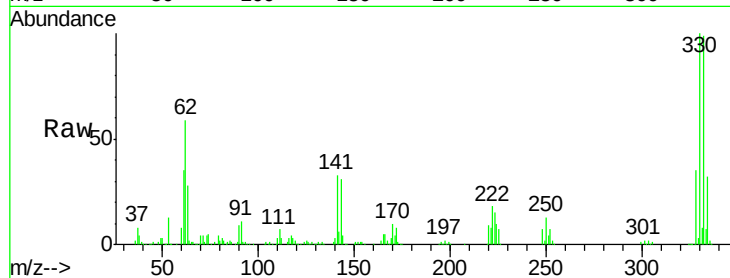


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

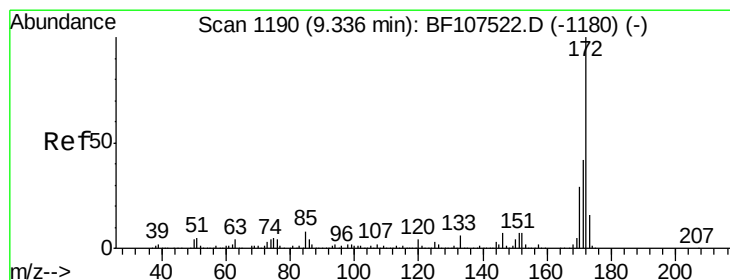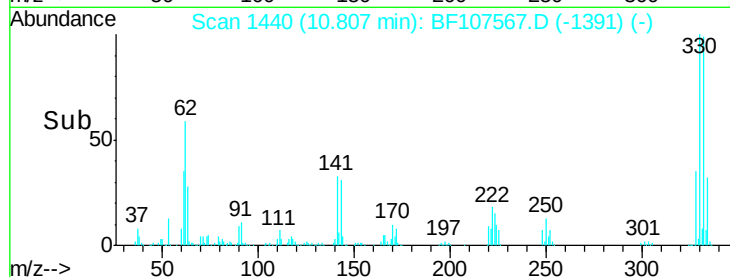
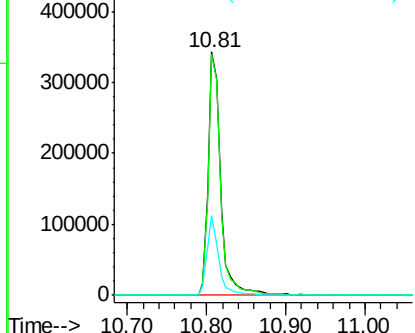



#44
 2-Fluorobiphenyl
 Concen: 135.092 ng
 RT: 9.33 min Scan# 1189
 Delta R.T. -0.01 min
 Lab File: BF107567.D
 Acq: 21 Jul 2018 11:10

Tgt Ion:172 Resp: 2609551
 Ion Ratio Lower Upper
 172 100
 171 40.0 29.7 44.5
 170 27.2 19.6 29.4

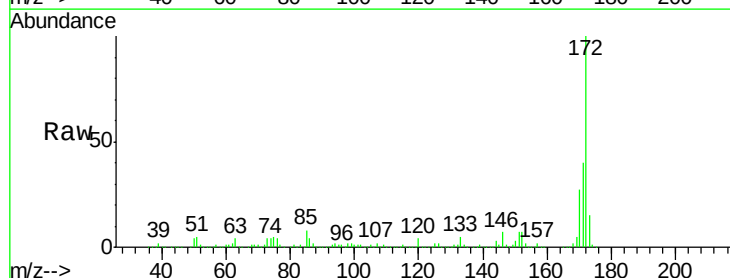

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E



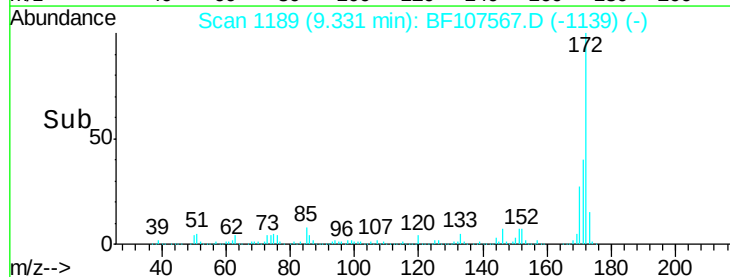
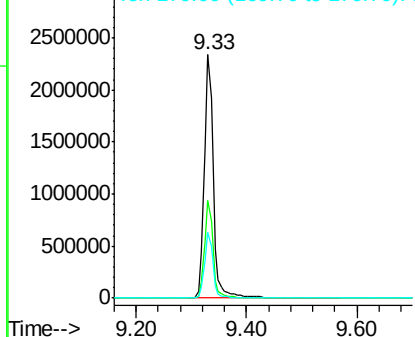


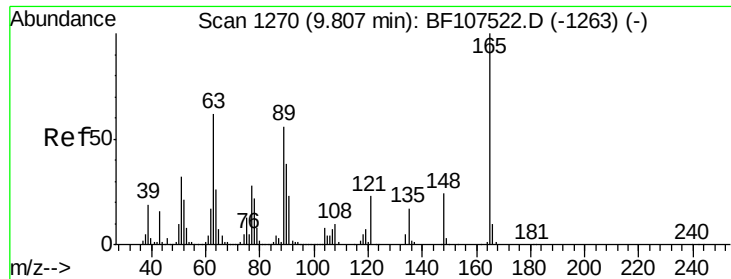

#50
 2,6-Dinitrotoluene
 Concen: 8.317 ng
 RT: 10.01 min Scan# 1305
 Delta R.T. 0.21 min
 Lab File: BF107567.D
 Acq: 21 Jul 2018 11:10




Instrument :
 BNA_F
 ClientSampleId :
 071718-TIPC-F-U-S


Tgt Ion:165 Resp: 48284
 Ion Ratio Lower Upper
 165 100
 63 1.0 44.7 67.1#
 89 1.6 44.0 66.0#

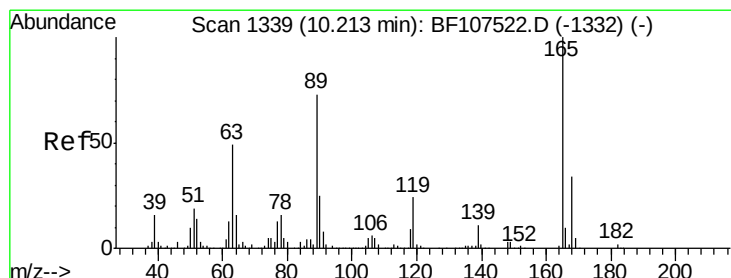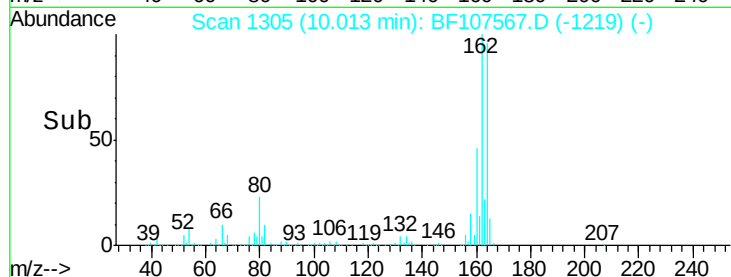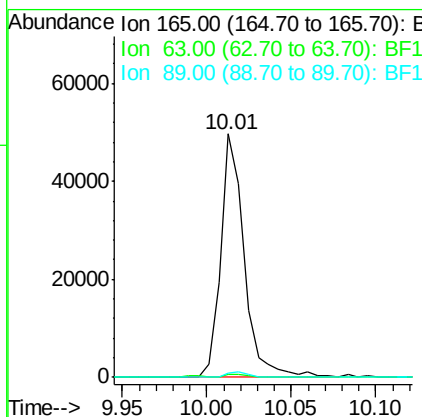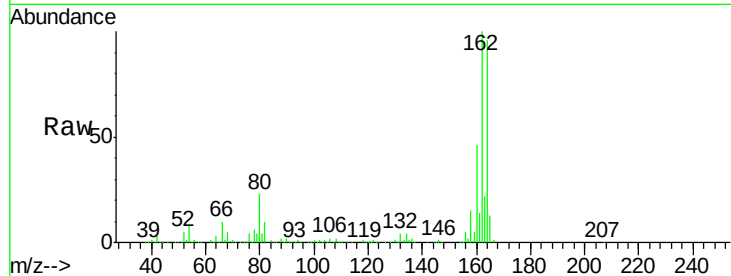

#56
 2,4-Dinitrotoluene
 Concen: 6.890 ng
 RT: 10.01 min Scan# 1305
 Delta R.T. -0.20 min
 Lab File: BF107567.D
 Acq: 21 Jul 2018 11:10

Tgt Ion:165 Resp: 48284
 Ion Ratio Lower Upper
 165 100
 63 1.0 36.4 54.6#
 89 1.6 57.8 86.6#
 182 0.0 1.6 2.4#

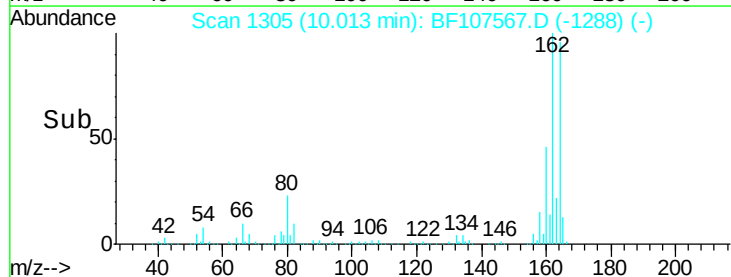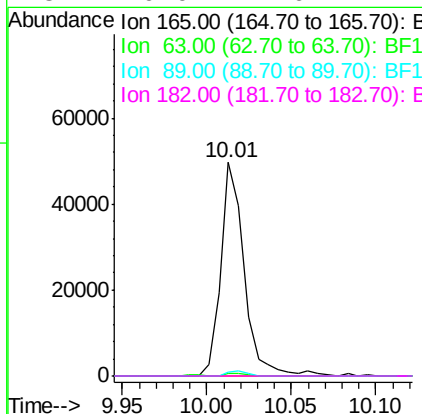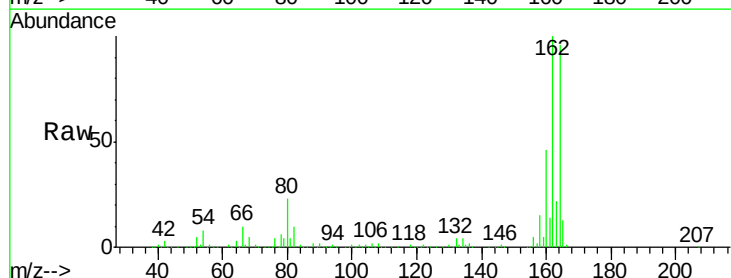

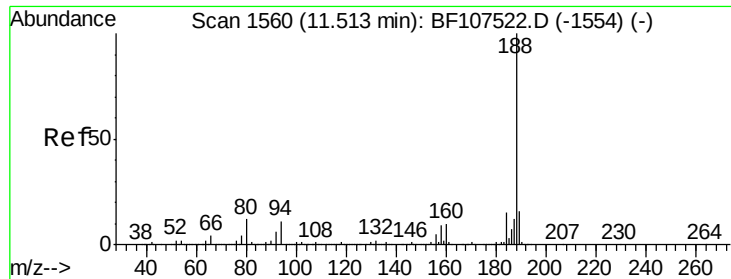

#63

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.51 min Scan# 1559

Delta R.T. -0.01 min

Lab File: BF107567.D

Acq: 21 Jul 2018 11:10

Instrument :

BNA_F

ClientSampleId :

071718-TIPC-F-U-S


Tgt Ion:188 Resp: 684470

Ion Ratio Lower Upper

188 100

94 10.8 8.5 12.7

80 11.8 9.2 13.8

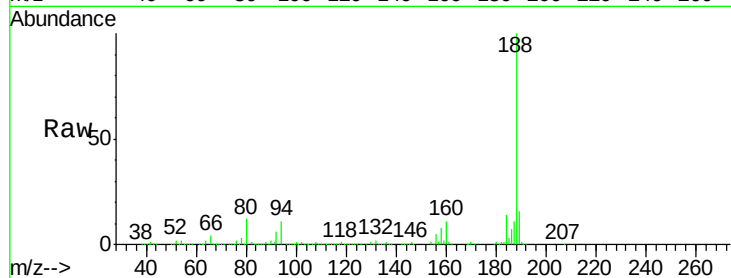

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF1

Ion 80.00 (79.70 to 80.70): BF1

11.51

800000



600000

400000

200000

0

Time--> 11.40 11.50 11.60 11.70

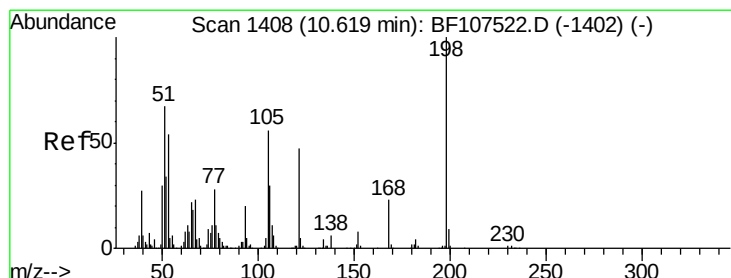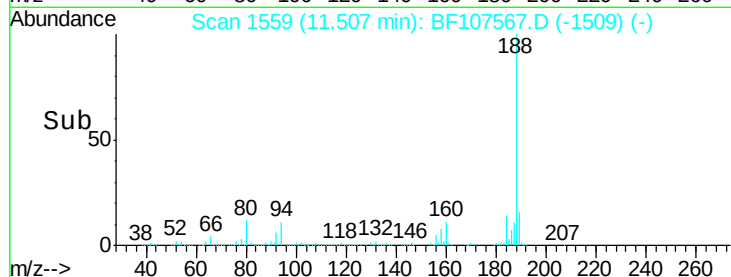

#64

4,6-Dinitro-2-methylphenol

Concen: 8.874 ng

RT: 10.81 min Scan# 1440

Delta R.T. 0.19 min

Lab File: BF107567.D

Acq: 21 Jul 2018 11:10


Tgt Ion:198 Resp: 778

Ion Ratio Lower Upper

198 100

51 129.2 37.7 77.7#

105 137.7 36.3 76.3#

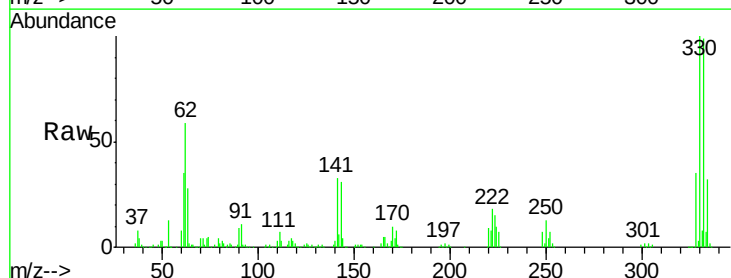

Abundance Ion 198.00 (197.70 to 198.70): E

Ion 51.00 (50.70 to 51.70): BF1

Ion 105.00 (104.70 to 105.70): E

10.81


1500


1000

500

0

Time--> 10.78 10.80 10.82

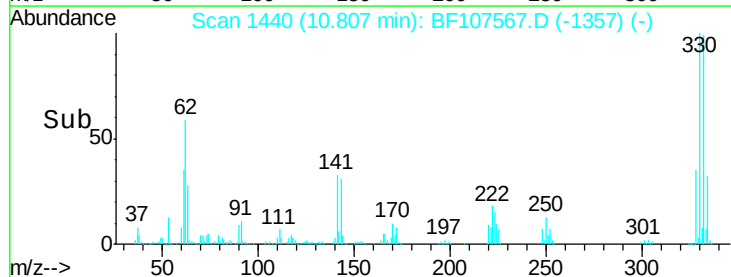


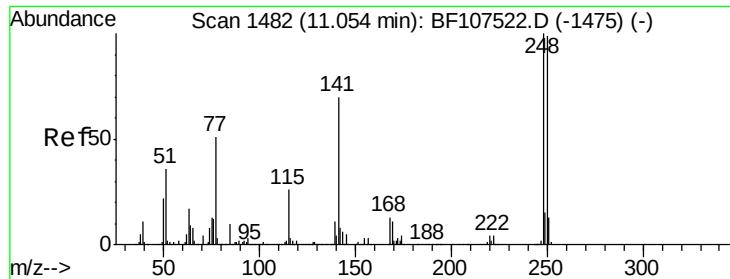




#66
4-Bromophenyl-phenylether
Concen: 2.847 ng
RT: 10.81 min Scan# 1440
Delta R.T. -0.25 min
Lab File: BF107567.D
Acq: 21 Jul 2018 11:10

Instrument :
BNA_F
ClientSampleId :
071718-TIPC-F-U-S

Tgt Ion:248 Resp: 22940
Ion Ratio Lower Upper
248 100
250 204.9 76.9 115.3#
141 499.5 74.4 111.6#

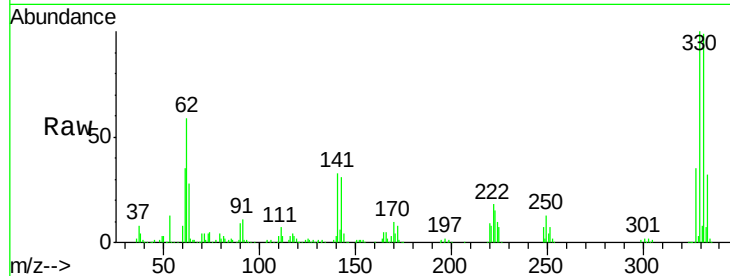


Abundance Ion 248.00 (247.70 to 248.70): E
Ion 250.00 (249.70 to 250.70): E
Ion 141.00 (140.70 to 141.70): E

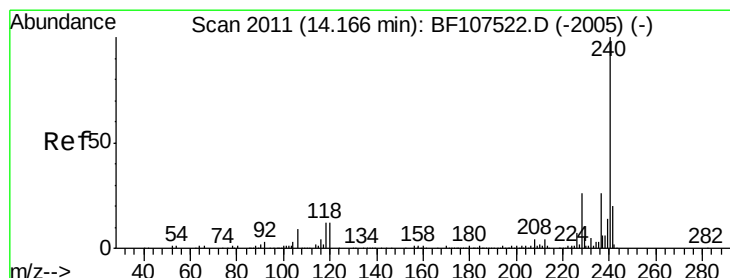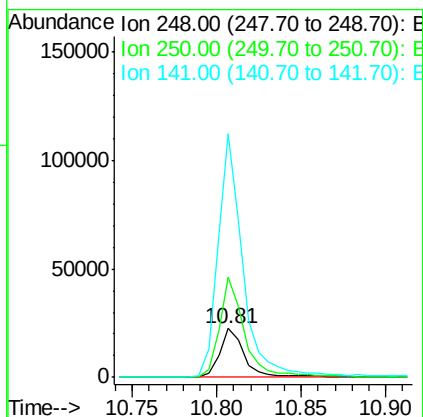
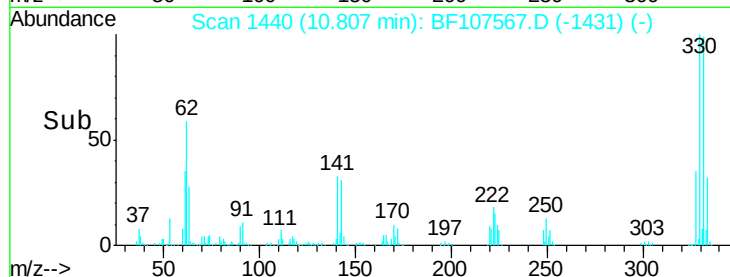



#75
Chrysene-d12
Concen: 20.000 ng
RT: 14.16 min Scan# 2010
Delta R.T. -0.01 min
Lab File: BF107567.D
Acq: 21 Jul 2018 11:10

Tgt Ion:240 Resp: 706380
Ion Ratio Lower Upper
240 100
120 12.0 9.5 14.3
236 25.7 20.7 31.1

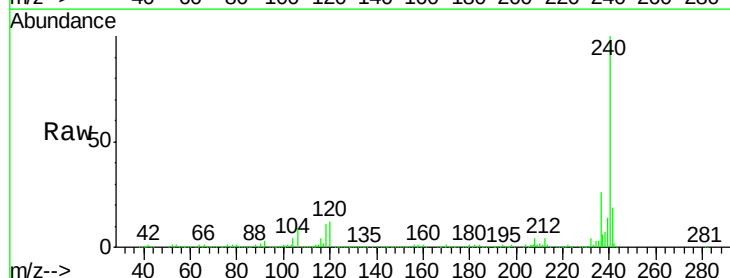

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

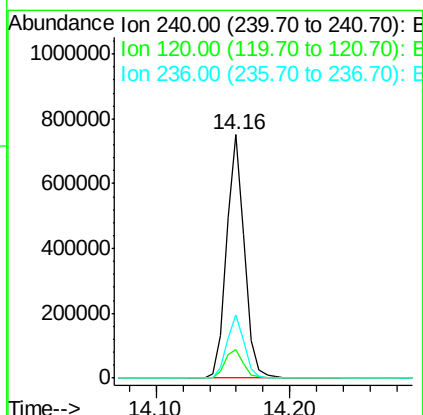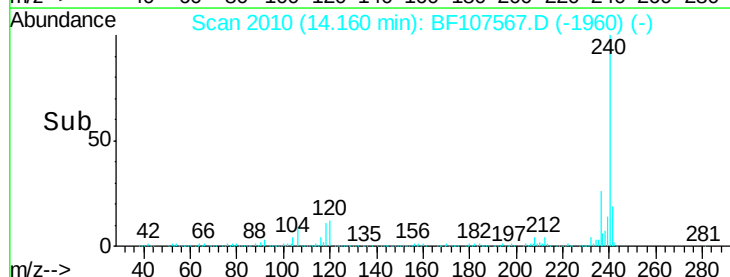

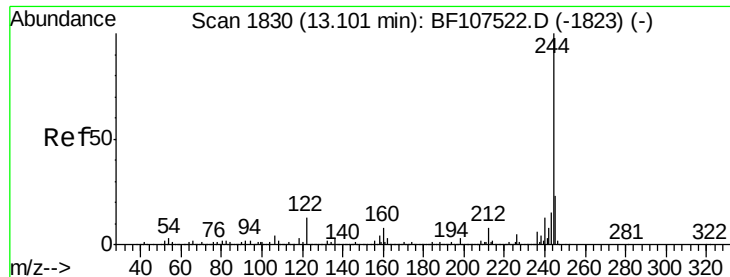

#78

Terphenyl-d14

Concen: 80.228 ng

RT: 13.10 min Scan# 1829

Delta R.T. -0.00 min

Lab File: BF107567.D

Acq: 21 Jul 2018 11:10

Instrument :

BNA_F

ClientSampleId :

071718-TIPC-F-U-S


Tgt Ion:244 Resp: 2213650

Ion Ratio Lower Upper

244 100

212 7.6 5.4 8.0




122 13.1 11.0 16.4

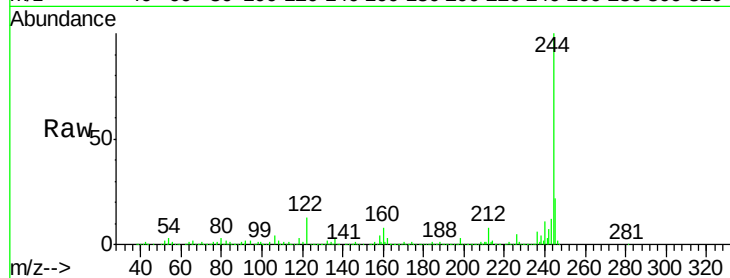

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

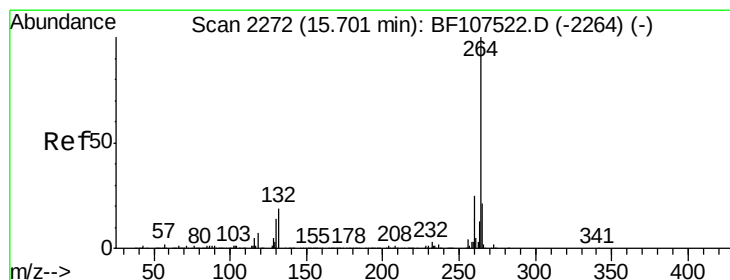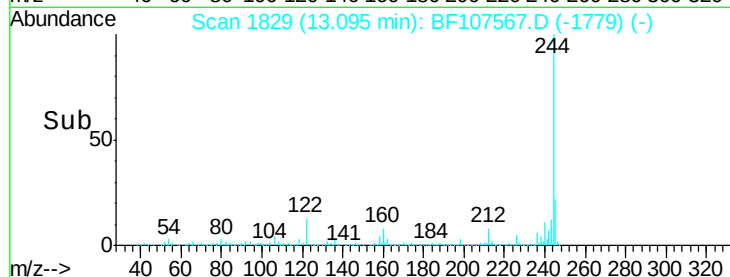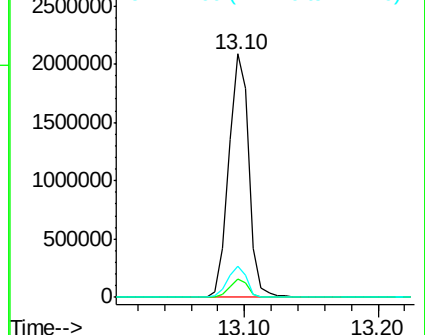

#86

Perylene-d12

Concen: 20.000 ng

RT: 15.69 min Scan# 2271

Delta R.T. -0.01 min

Lab File: BF107567.D

Acq: 21 Jul 2018 11:10


Tgt Ion:264 Resp: 587891

Ion Ratio Lower Upper

264 100

260 24.8 19.2 28.8

265 22.1 17.5 26.3

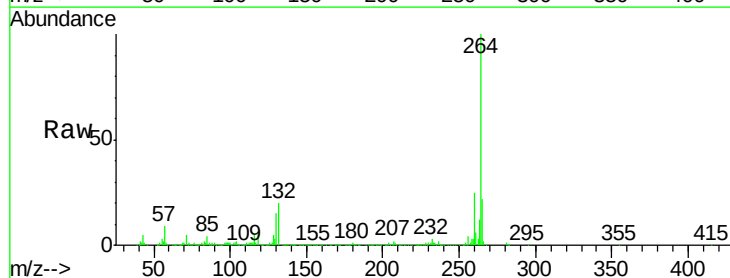

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

