

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF072018\
 Data File : BF107570.D
 Acq On : 21 Jul 2018 12:29
 Operator : JU/SJ
 Sample : J4094-03
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 071818-DBRI-E-D-S

Quant Time: Jul 23 03:28:32 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072018.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 20 16:29:27 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.97	152	345892	20.00	ng	0.00
21) Naphthalene-d8	8.25	136	1224518	20.00	ng	0.00
38) Acenaphthene-d10	10.01	164	448024	20.00	ng	0.00
63) Phenanthrene-d10	11.51	188	766759	20.00	ng	0.00
75) Chrysene-d12	14.16	240	777063	20.00	ng	0.00
86) Perylene-d12	15.69	264	598783	20.00	ng	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
5) 2-Fluorophenol	5.60	112	808846	37.60	ng	0.00
7) Phenol-d6	6.60	99	708257	27.42	ng	-0.02
23) Nitrobenzene-d5	7.54	82	1811571	99.84	ng	-0.01
41) 2,4,6-Tribromophenol	10.81	330	396813	77.89	ng	-0.01
44) 2-Fluorobiphenyl	9.33	172	2784418	118.27	ng	0.00
78) Terphenyl-d14	13.10	244	2171534	71.54	ng	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
9) Benzaldehyde	6.60	77	1467	Below Cal	#	1
19) n-Nitroso-di-n-propylamine	7.54	70	246745	14.786	ng	# 79
25) Isophorone	7.54	82	1811562	46.761	ng	# 64
32) Benzoic acid	8.26	122	120	7.908	ng	# 1
50) 2,6-Dinitrotoluene	10.01	165	57071	8.513	ng	# 26
56) 2,4-Dinitrotoluene	10.01	165	57507	7.106	ng	# 23
64) 4,6-Dinitro-2-methylphenol	10.81	198	832	8.865	ng	# 16
66) 4-Bromophenyl-phenylether	10.81	248	24022	2.661	ng	# 1
73) Di-n-butylphthalate	12.05	149	2668	Below Cal	#	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF072018\
Data File : BF107570.D
Acq On : 21 Jul 2018 12:29
Operator : JU/SJ
Sample : J4094-03
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
071818-DBRI-E-D-S

Quant Time: Jul 23 03:28:32 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 20 16:29:27 2018
Response via : Initial Calibration




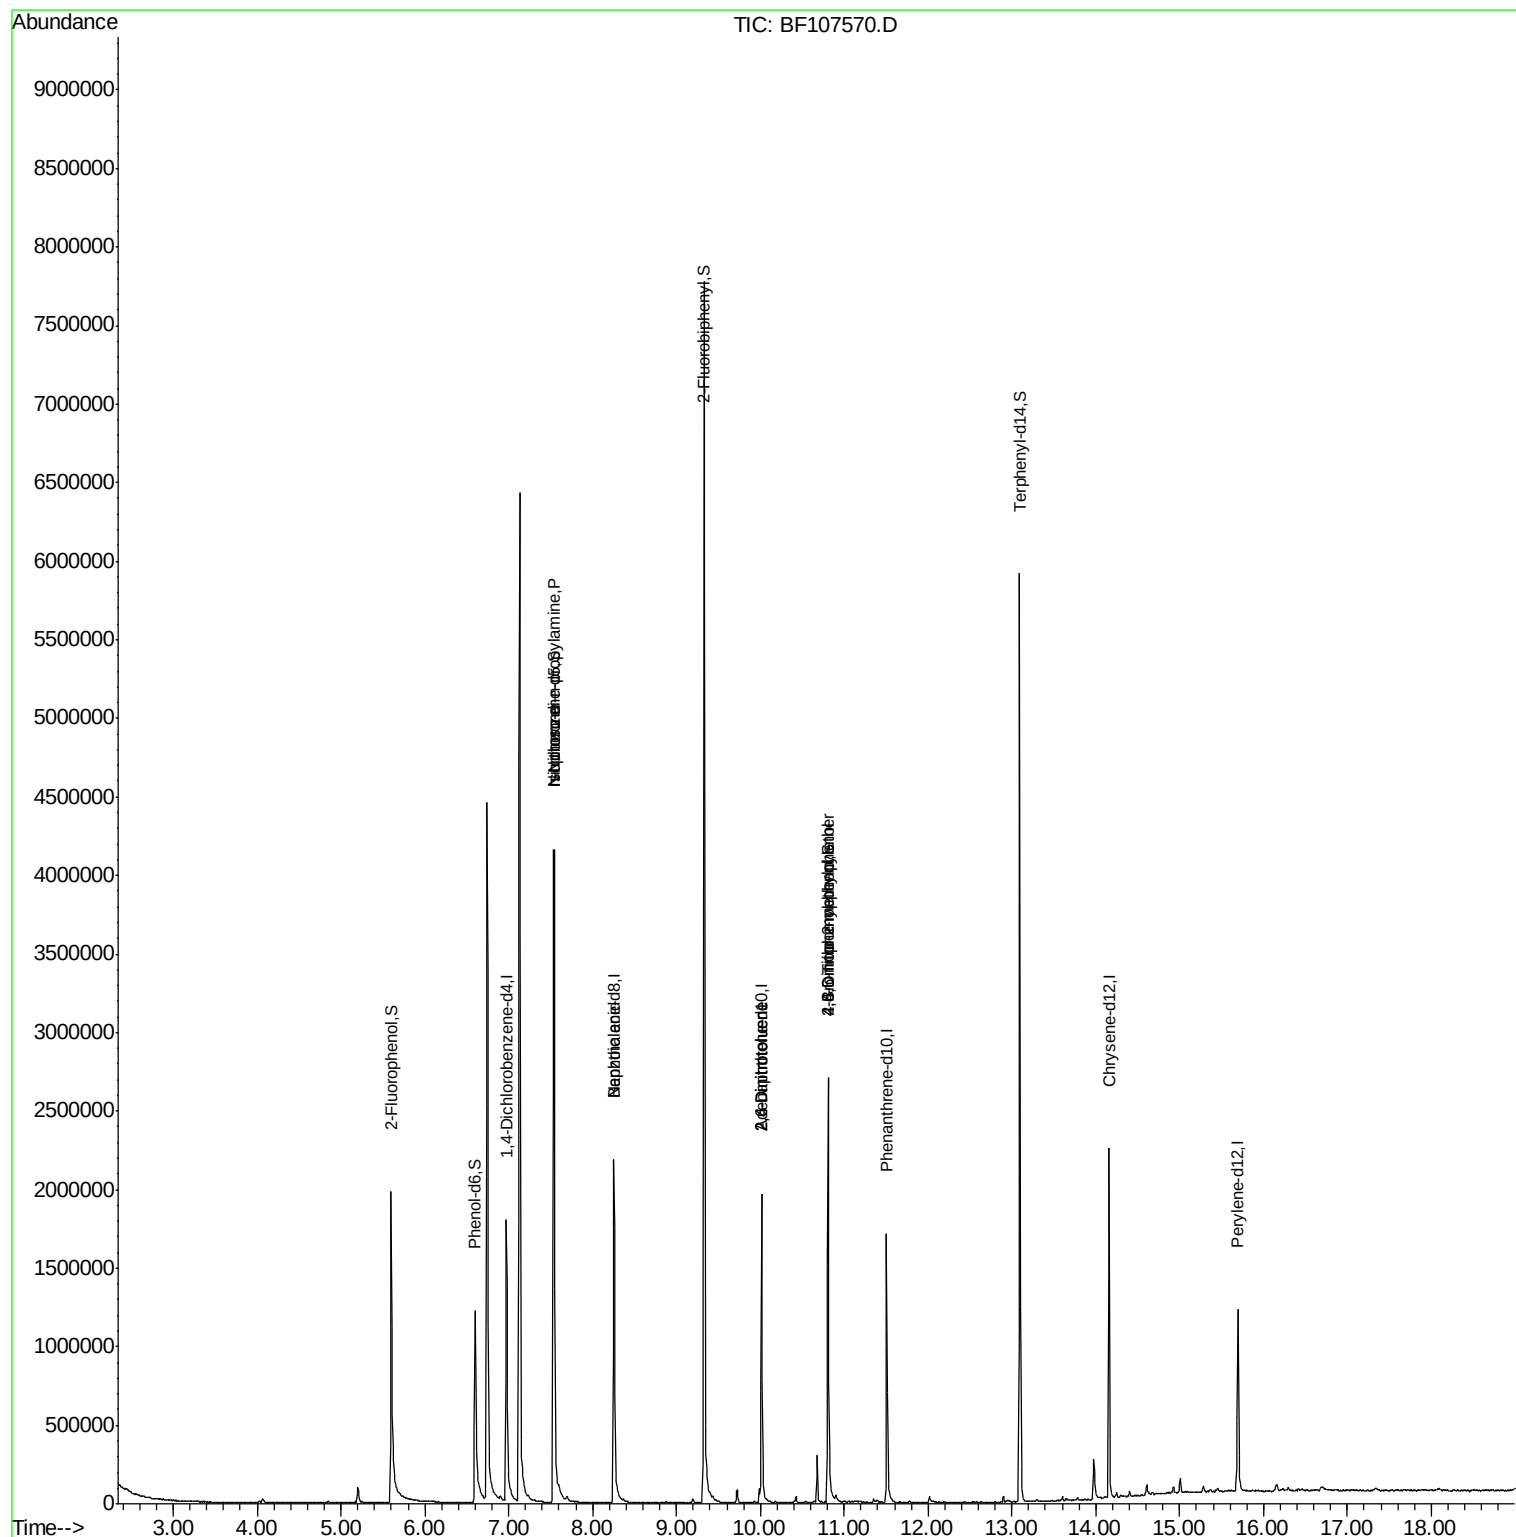


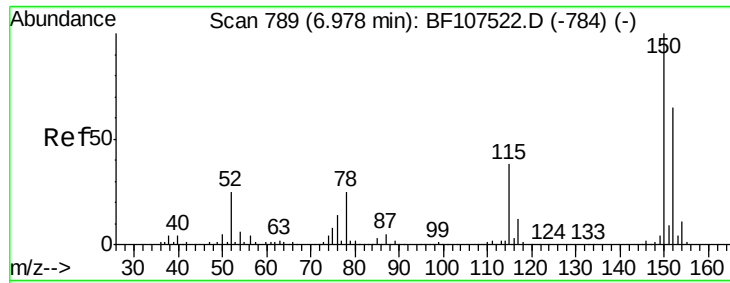

#1
 1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 6.97 min Scan# 788
 Delta R.T. -0.01 min
 Lab File: BF107570.D
 Acq: 21 Jul 2018 12:29




Instrument :
 BNA_F
 ClientSampleId :
 071818-DBRI-E-D-S


Tgt Ion:152 Resp: 345892
 Ion Ratio Lower Upper
 152 100
 150 152.3 124.6 186.8
 115 59.3 50.1 75.1

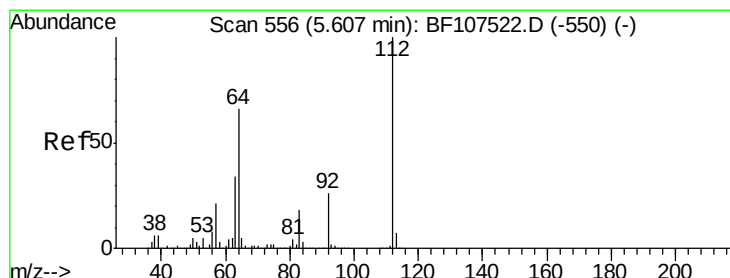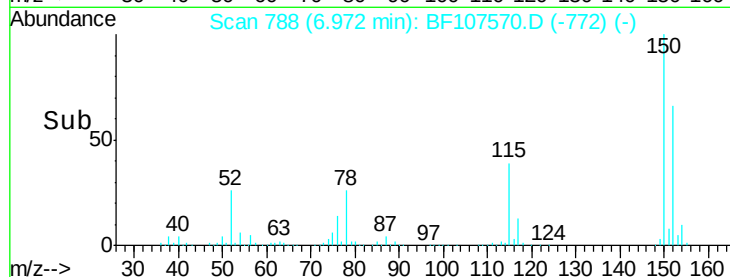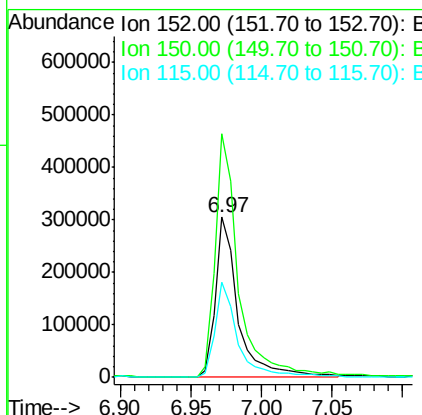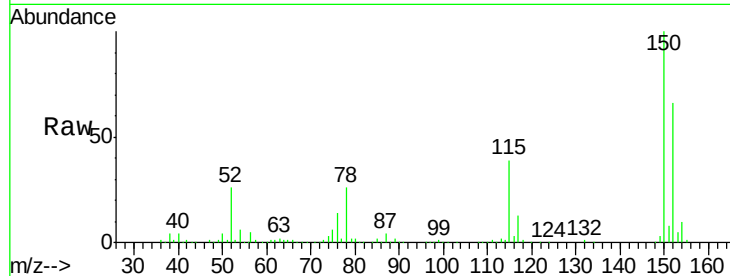

#5
 2-Fluorophenol
 Concen: 37.598 ng
 RT: 5.60 min Scan# 555
 Delta R.T. -0.01 min
 Lab File: BF107570.D
 Acq: 21 Jul 2018 12:29

Tgt Ion:112 Resp: 808846
 Ion Ratio Lower Upper
 112 100
 64 63.2 47.9 71.9
 63 32.7 23.7 35.5

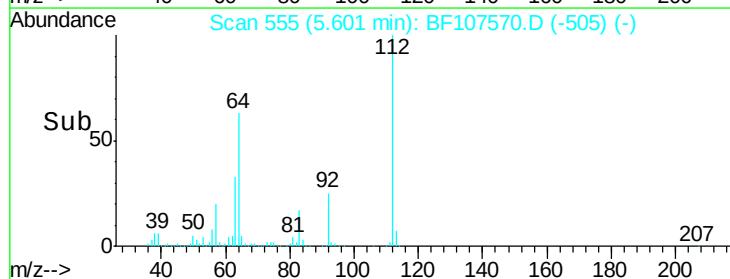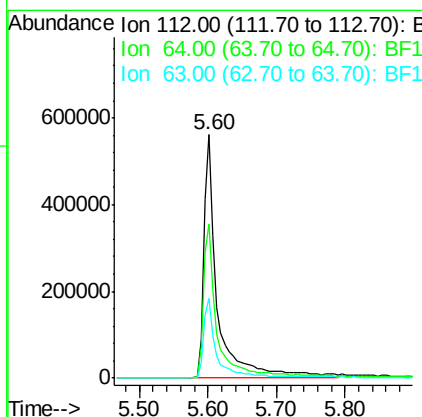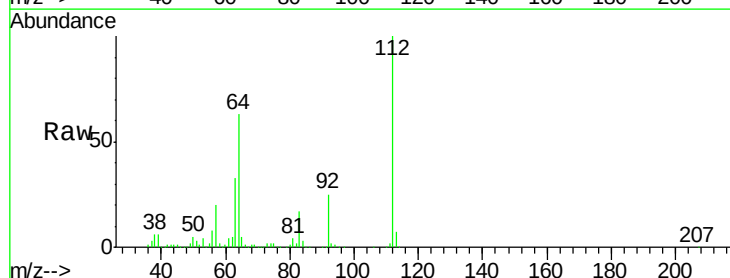

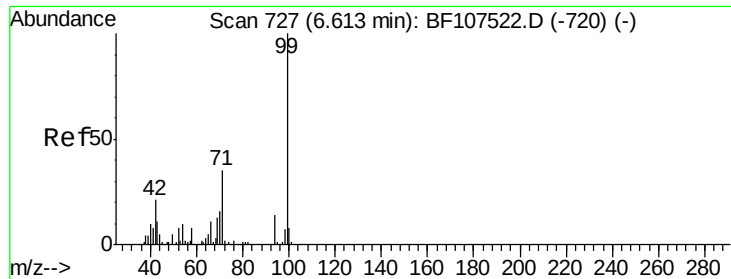

#7

Phenol-d6

Concen: 27.418 ng

RT: 6.60 min Scan# 724

Delta R.T. -0.02 min

Lab File: BF107570.D

Acq: 21 Jul 2018 12:29

Instrument :

BNA_F

ClientSampleId :

071818-DBRI-E-D-S





Tgt Ion: 99 Resp: 708257

Ion Ratio Lower Upper

99 100

42 19.5 14.5 21.7

71 31.2 25.4 38.0

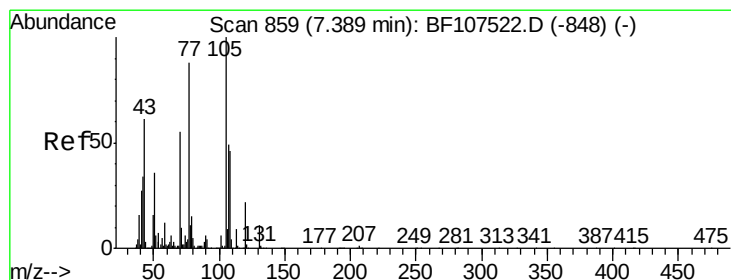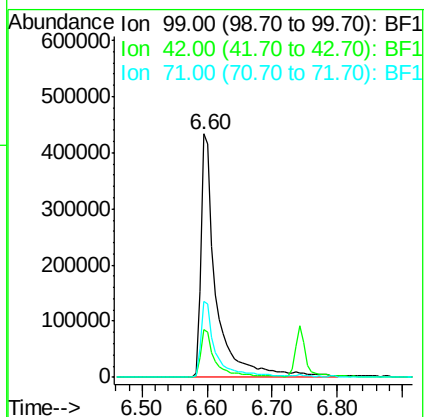

#19

n-Nitroso-di-n-propylamine

Concen: 14.786 ng

RT: 7.54 min Scan# 884

Delta R.T. 0.15 min

Lab File: BF107570.D

Acq: 21 Jul 2018 12:29

Tgt Ion: 70 Resp: 246745




Ion Ratio Lower Upper


70 100

42 49.2 47.5 71.3

101 0.0 7.4 11.2#

130 1.9 16.6 25.0#

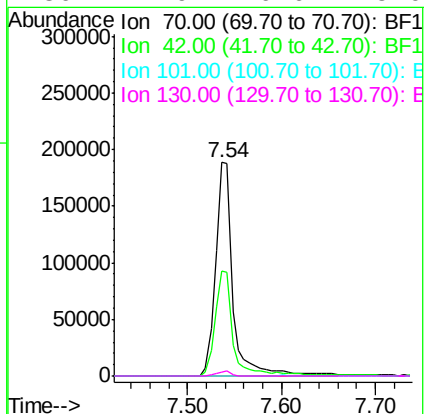


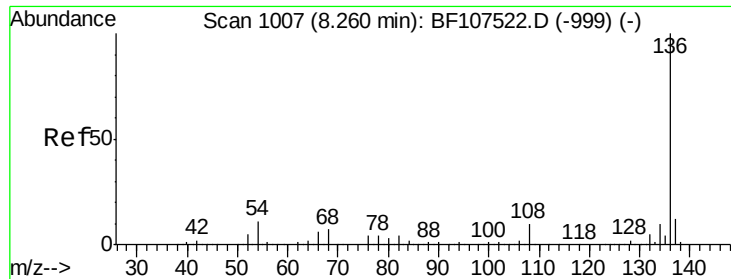




#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.25 min Scan# 1006
Delta R.T. -0.01 min
Lab File: BF107570.D
Acq: 21 Jul 2018 12:29

Instrument :
BNA_F
ClientSampleId :
071818-DBRI-E-D-S

Tgt Ion: 136 Resp: 1224518
Ion Ratio Lower Upper
136 100
137 11.4 8.9 13.3
54 10.4 6.6 9.8#
68 6.4 5.0 7.4




Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1

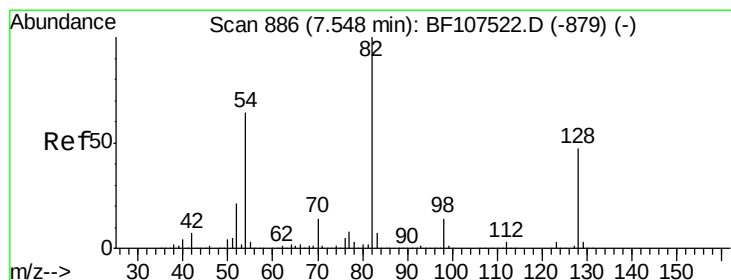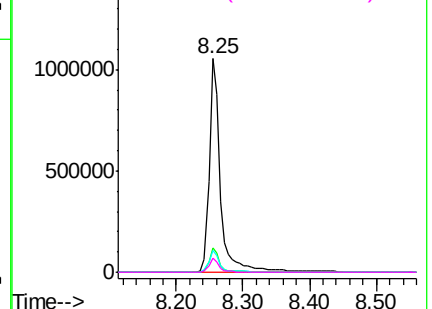




#23
Nitrobenzene-d5
Concen: 99.842 ng
RT: 7.54 min Scan# 884
Delta R.T. -0.01 min
Lab File: BF107570.D
Acq: 21 Jul 2018 12:29

Tgt Ion: 82 Resp: 1811571
Ion Ratio Lower Upper
82 100
128 45.0 36.1 54.1
54 62.6 41.4 62.2#

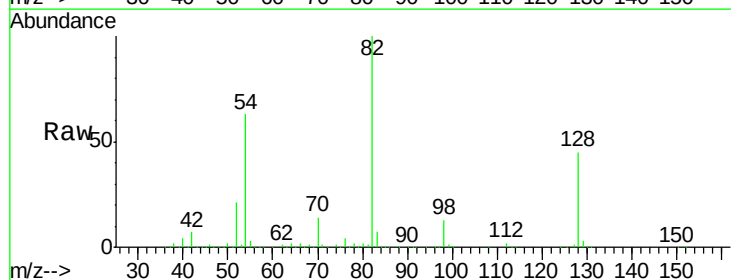

Abundance Ion 82.00 (81.70 to 82.70): BF1
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BF1

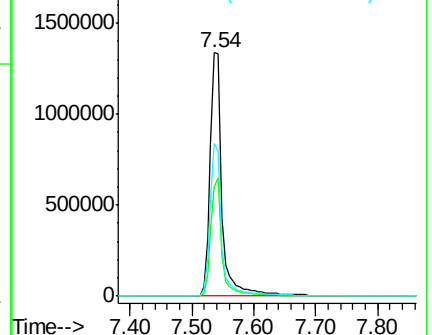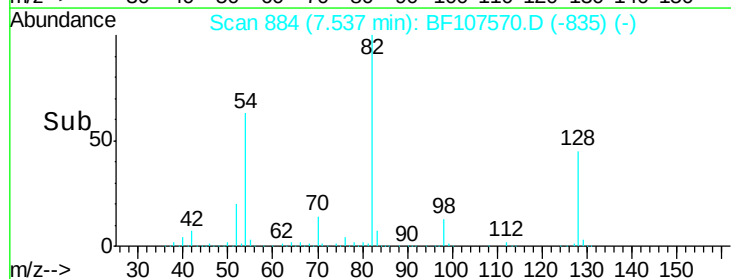



#25

Isophorone

Concen: 46.761 ng

RT: 7.54 min Scan# 884

Delta R.T. -0.26 min

Lab File: BF107570.D

Acq: 21 Jul 2018 12:29

Instrument :

BNA_F

ClientSampleId :

071818-DBRI-E-D-S


Tgt Ion: 82 Resp: 1811562

Ion Ratio Lower Upper

82 100

95 0.0 5.2 7.8#




138 0.0 14.9 22.3#



Abundance Ion 82.00 (81.70 to 82.70): BF1

Ion 95.00 (94.70 to 95.70): BF1

Ion 138.00 (137.70 to 138.70): BF1

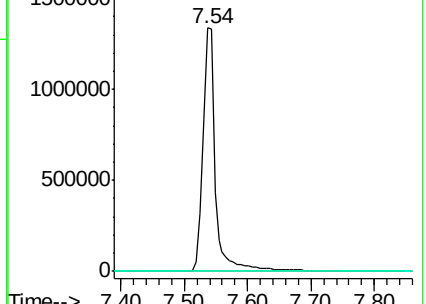

#32

Benzoic acid

Concen: 7.908 ng

RT: 8.26 min Scan# 1007

Delta R.T. 0.21 min

Lab File: BF107570.D

Acq: 21 Jul 2018 12:29


Tgt Ion: 122 Resp: 120

Ion Ratio Lower Upper

122 100

105 267.3 101.1 141.1#



77 740.4 70.7 110.7#




Abundance Ion 122.00 (121.70 to 122.70): E

Ion 105.00 (104.70 to 105.70): E

Ion 77.00 (76.70 to 77.70): BF1

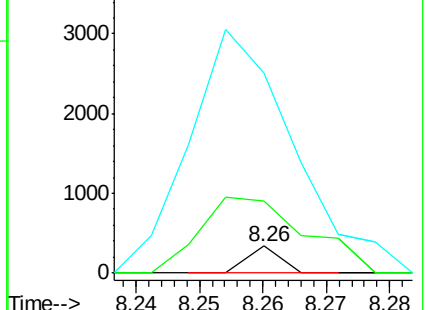

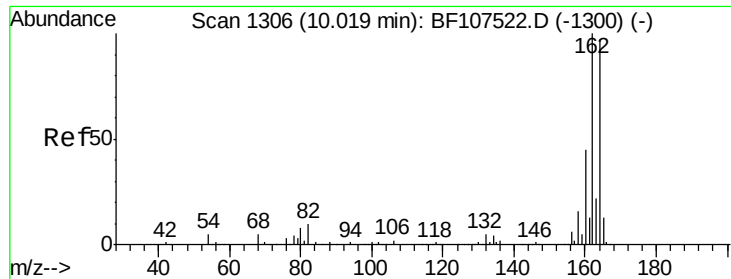

#38

Acenaphthene-d10

Concen: 20.000 ng

RT: 10.01 min Scan# 1305

Delta R.T. -0.01 min

Lab File: BF107570.D

Acq: 21 Jul 2018 12:29

Instrument :

BNA_F

ClientSampleId :

071818-DBRI-E-D-S


Tgt Ion:164 Resp: 448024

Ion Ratio Lower Upper

164 100

162 104.2 86.1 129.1




160 48.3 38.3 57.5

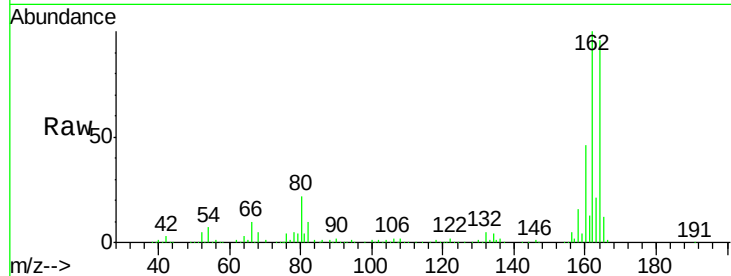

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

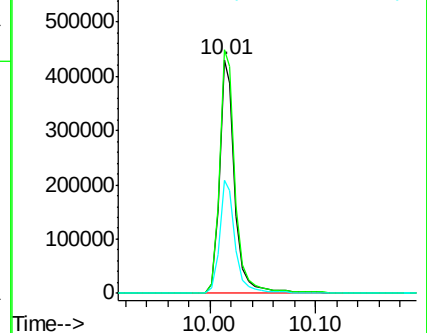

#41

2,4,6-Tribromophenol

Concen: 77.887 ng

RT: 10.81 min Scan# 1440

Delta R.T. -0.01 min

Lab File: BF107570.D

Acq: 21 Jul 2018 12:29


Tgt Ion:330 Resp: 396813

Ion Ratio Lower Upper

330 100

332 96.0 77.0 115.6



141 30.4 29.9 44.9




Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

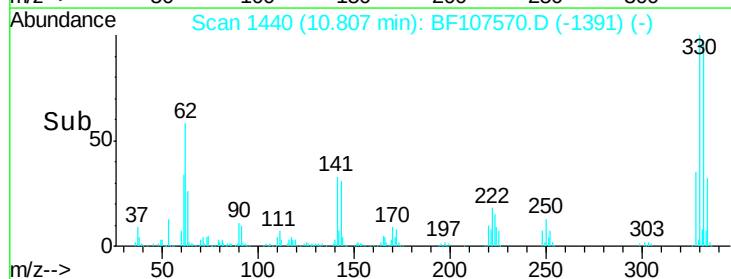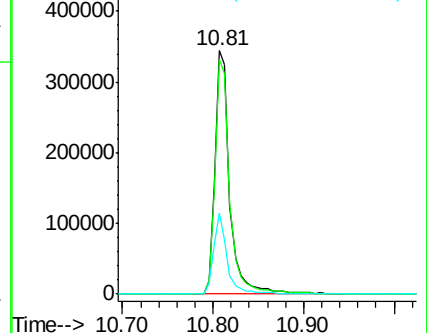

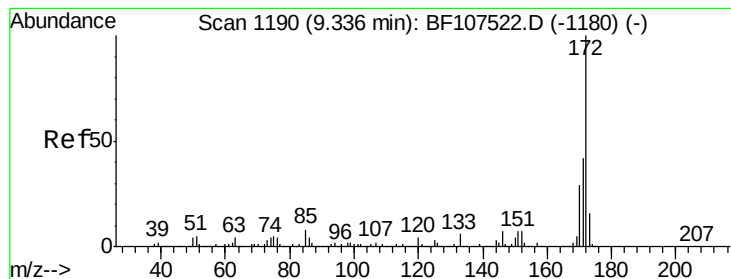

#44

2-Fluorobiphenyl

Concen: 118.266 ng

RT: 9.33 min Scan# 1189

Delta R.T. -0.01 min

Lab File: BF107570.D

Acq: 21 Jul 2018 12:29

Instrument :

BNA_F

ClientSampleId :

071818-DBRI-E-D-S


Tgt Ion:172 Resp: 2784418

Ion Ratio Lower Upper

172 100

171 40.7 29.7 44.5




170 27.8 19.6 29.4



Abundance Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

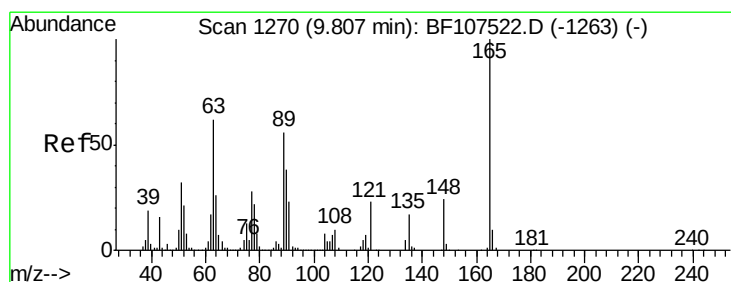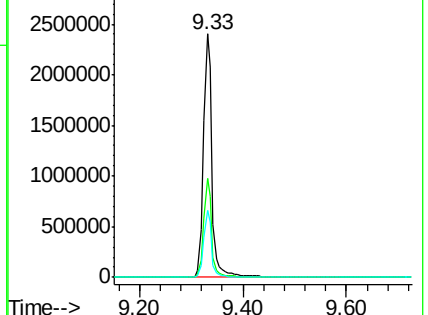

#50

2,6-Dinitrotoluene

Concen: 8.513 ng

RT: 10.01 min Scan# 1305

Delta R.T. 0.21 min

Lab File: BF107570.D

Acq: 21 Jul 2018 12:29


Tgt Ion:165 Resp: 57071

Ion Ratio Lower Upper

165 100

63 1.6 44.7 67.1#



89 1.4 44.0 66.0#

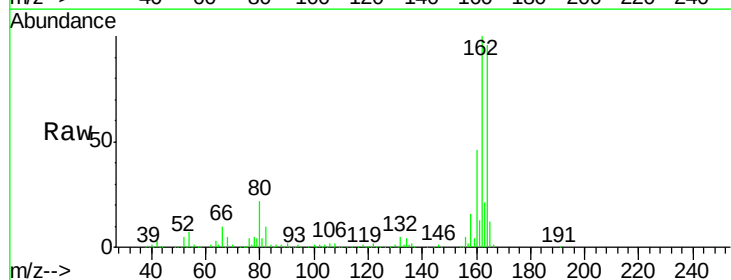


Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BF1

Ion 89.00 (88.70 to 89.70): BF1



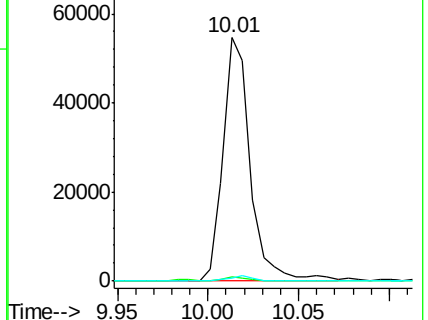





#56
2,4-Dinitrotoluene
Concen: 7.106 ng
RT: 10.01 min Scan# 1305
Delta R.T. -0.20 min
Lab File: BF107570.D
Acq: 21 Jul 2018 12:29




Instrument :
BNA_F
ClientSampleId :
071818-DBRI-E-D-S


Tgt Ion	Ratio	Lower	Upper
165	100		
63	1.6	36.4	54.6#
89	1.4	57.8	86.6#
182	0.0	1.6	2.4#

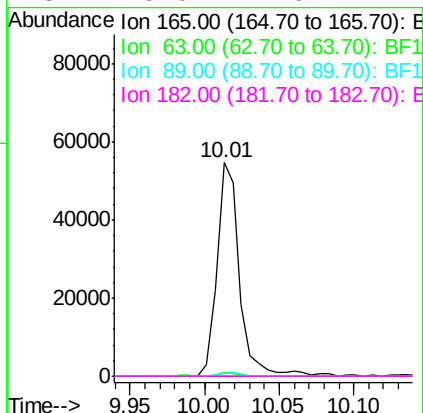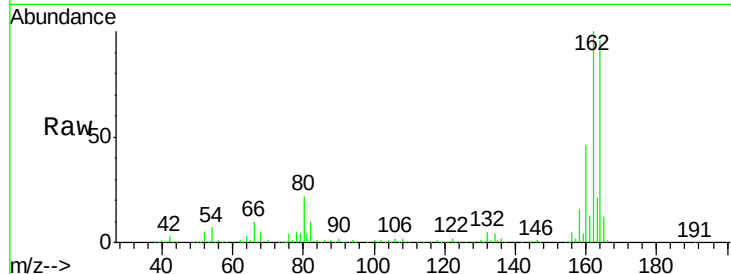

#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.51 min Scan# 1559
Delta R.T. -0.01 min
Lab File: BF107570.D
Acq: 21 Jul 2018 12:29

Tgt Ion	Ratio	Lower	Upper
188	100		
94	10.4	8.5	12.7
80	11.7	9.2	13.8

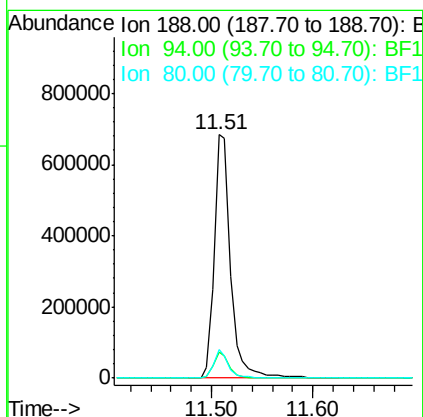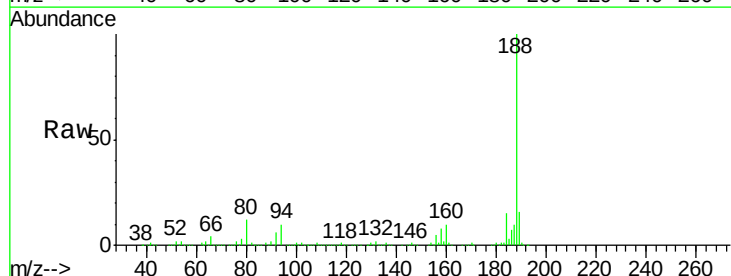


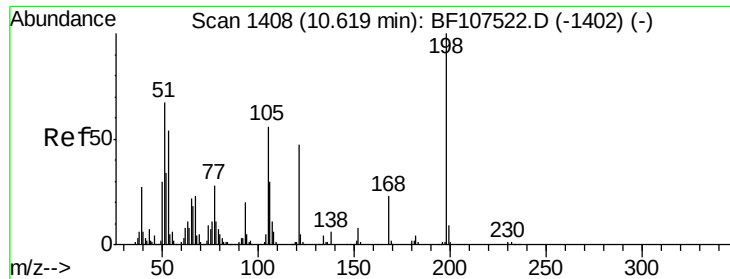




#64
 4,6-Dinitro-2-methylphenol
 Concen: 8.865 ng
 RT: 10.81 min Scan# 1440
 Delta R.T. 0.19 min
 Lab File: BF107570.D
 Acq: 21 Jul 2018 12:29

Instrument :
 BNA_F
 ClientSampleId :
 071818-DBRI-E-D-S

Tgt Ion:198 Resp: 832
 Ion Ratio Lower Upper
 198 100
 51 130.2 37.7 77.7#
 105 107.2 36.3 76.3#

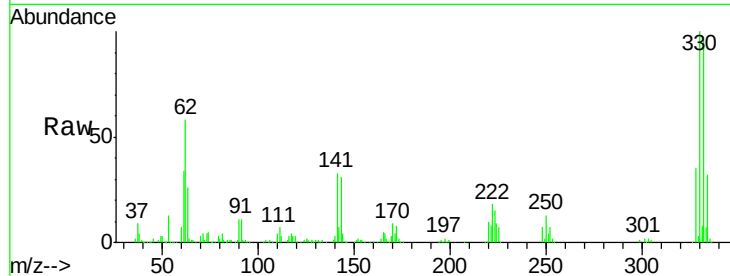


Abundance Ion 198.00 (197.70 to 198.70): E
 Ion 51.00 (50.70 to 51.70): BF1
 Ion 105.00 (104.70 to 105.70): E

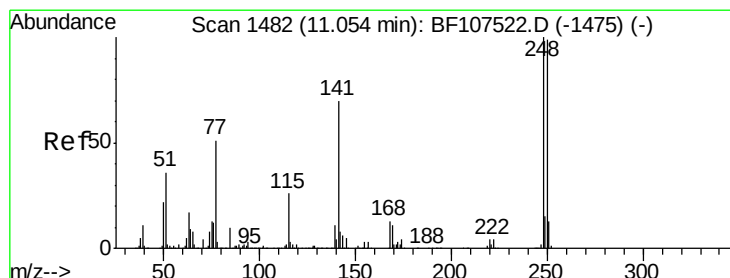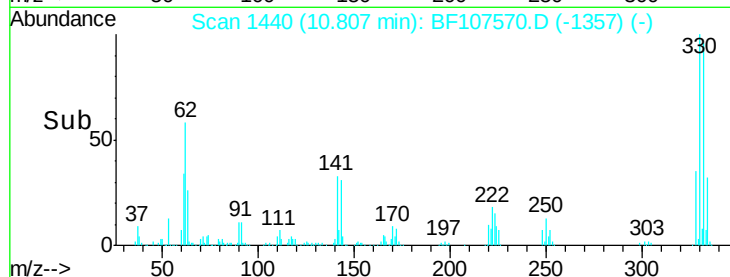
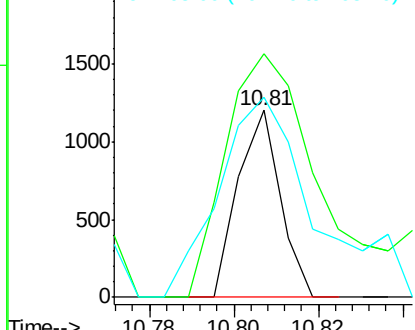



#66
 4-Bromophenyl-phenylether
 Concen: 2.661 ng
 RT: 10.81 min Scan# 1440
 Delta R.T. -0.25 min
 Lab File: BF107570.D
 Acq: 21 Jul 2018 12:29

Tgt Ion:248 Resp: 24022
 Ion Ratio Lower Upper
 248 100
 250 192.1 76.9 115.3#
 141 509.5 74.4 111.6#

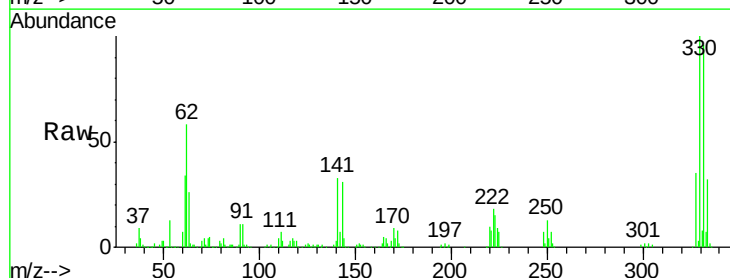

Abundance Ion 248.00 (247.70 to 248.70): E
 Ion 250.00 (249.70 to 250.70): E
 Ion 141.00 (140.70 to 141.70): E

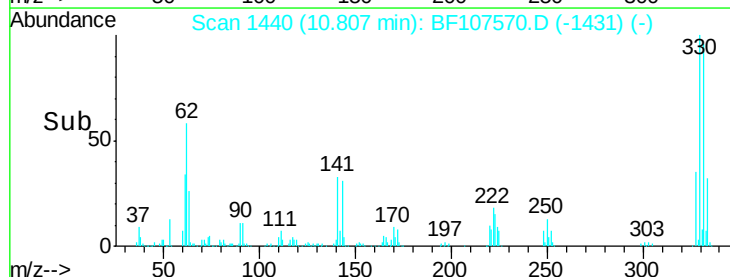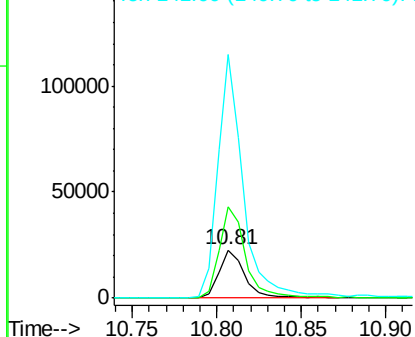

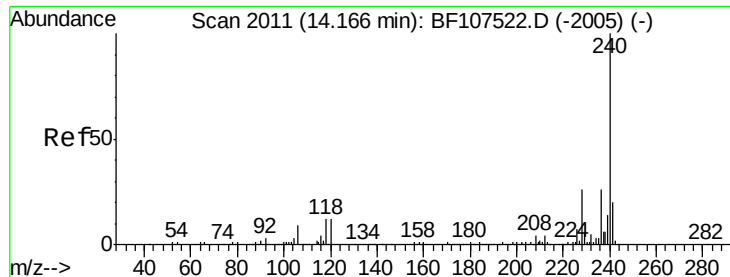

#75

Chrysene-d12

Concen: 20.000 ng

RT: 14.16 min Scan# 2010

Delta R.T. -0.01 min

Lab File: BF107570.D

Acq: 21 Jul 2018 12:29

Instrument :

BNA_F

ClientSampleId :

071818-DBRI-E-D-S


Tgt Ion:240 Resp: 777063

Ion Ratio Lower Upper

240 100

120 12.4 9.5 14.3




236 26.0 20.7 31.1

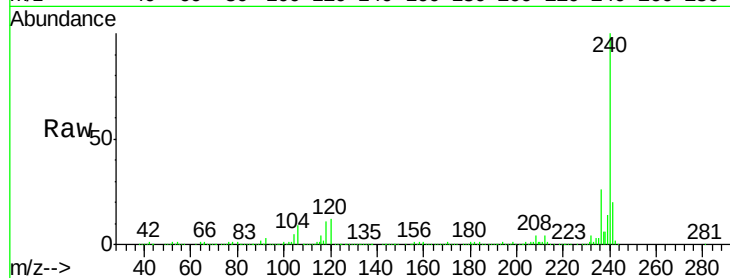

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

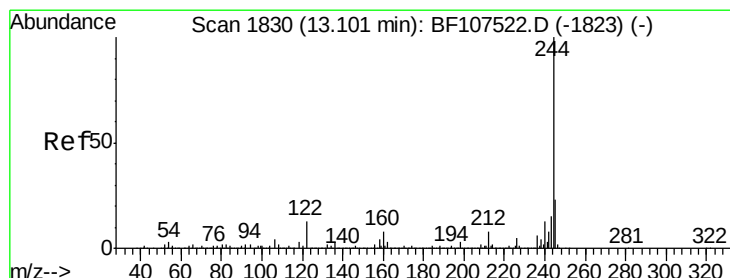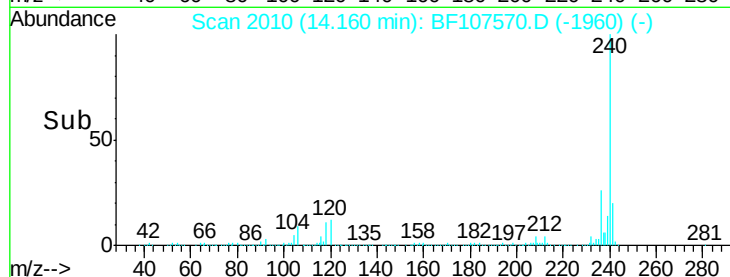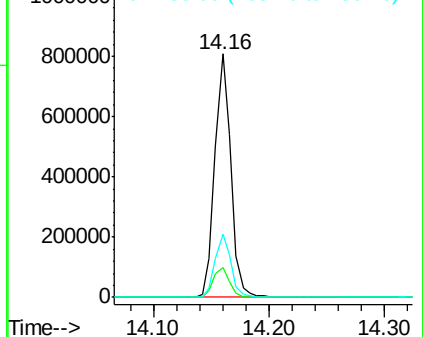

#78

Terphenyl-d14

Concen: 71.543 ng

RT: 13.10 min Scan# 1829

Delta R.T. -0.00 min

Lab File: BF107570.D

Acq: 21 Jul 2018 12:29


Tgt Ion:244 Resp: 2171534

Ion Ratio Lower Upper

244 100

212 7.5 5.4 8.0



122 13.2 11.0 16.4



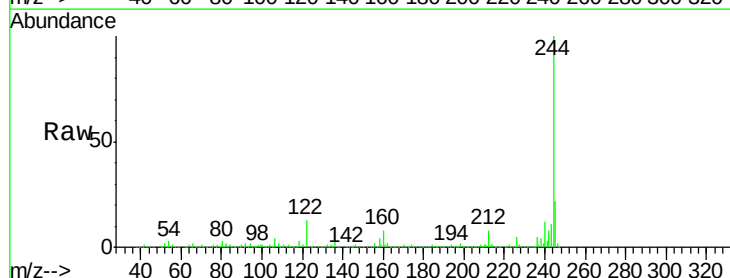


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

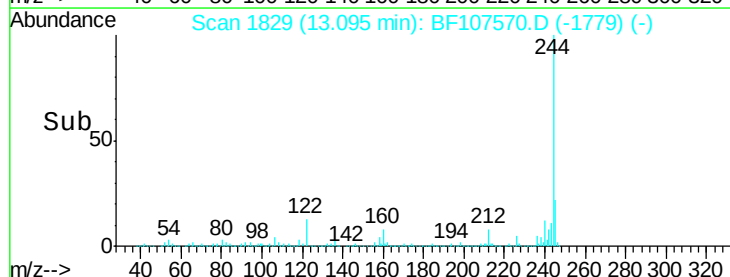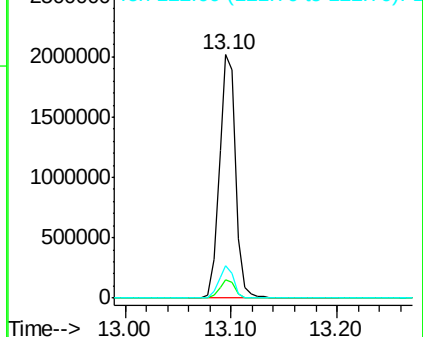

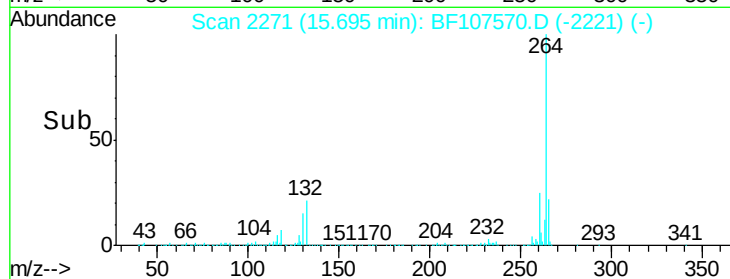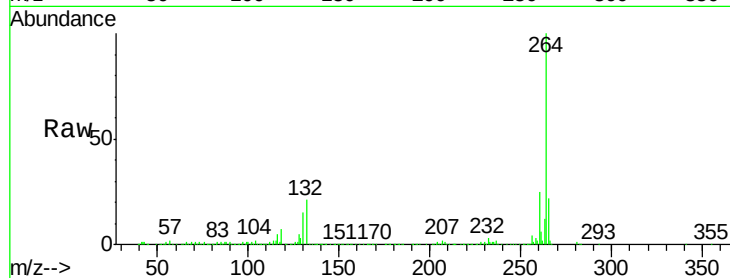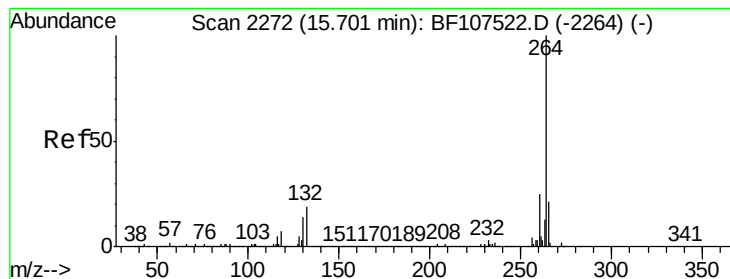

#86

Perylene-d12

Concen: 20.000 ng

RT: 15.69 min Scan# 2271

Delta R.T. -0.01 min

Lab File: BF107570.D

Acq: 21 Jul 2018 12:29

Instrument :

BNA_F

ClientSampleId :

071818-DBRI-E-D-S

Tgt Ion: 264 Resp: 598783

Ion Ratio Lower Upper

264 100

260 24.9 19.2 28.8

265 22.2 17.5 26.3

