



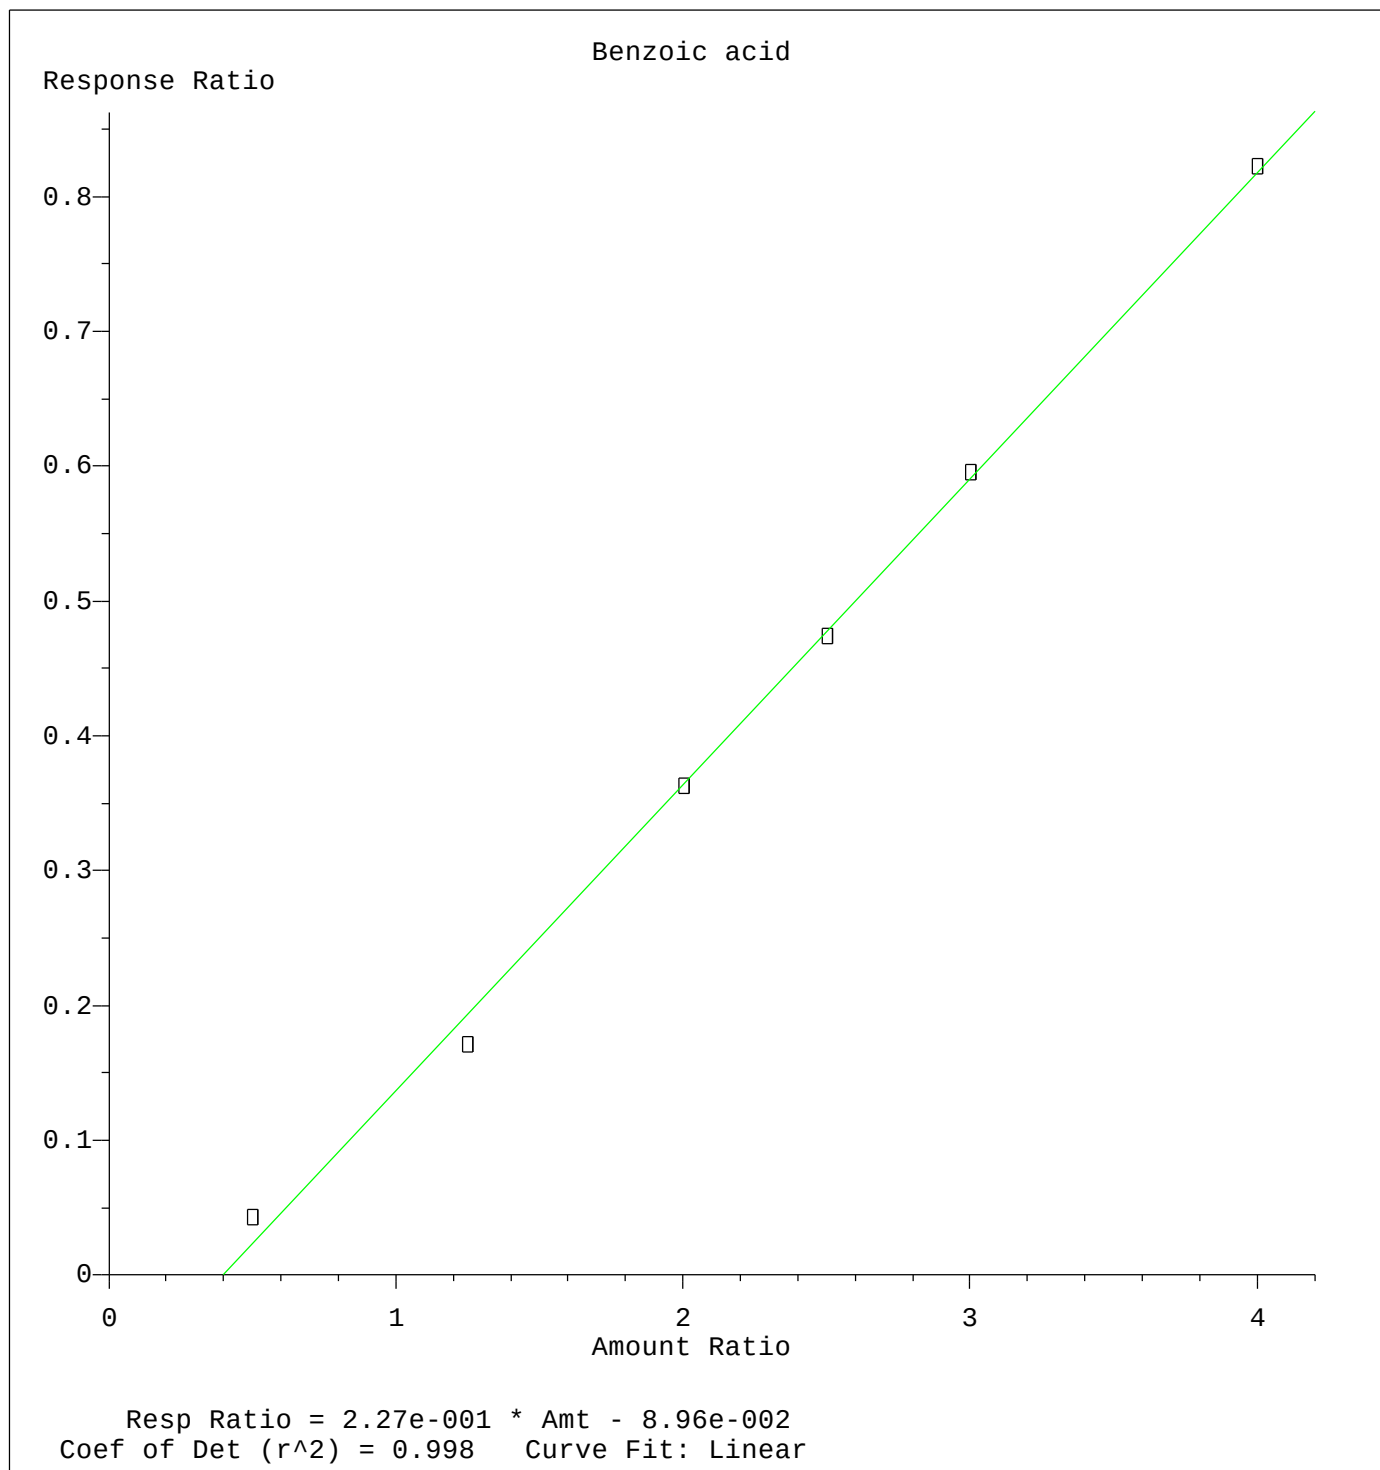


Method Name: Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072018.M
Calibration Table Last Updated: Fri Jul 20 16:29:27 2018

4,6-Dinitro-2-methylphenol

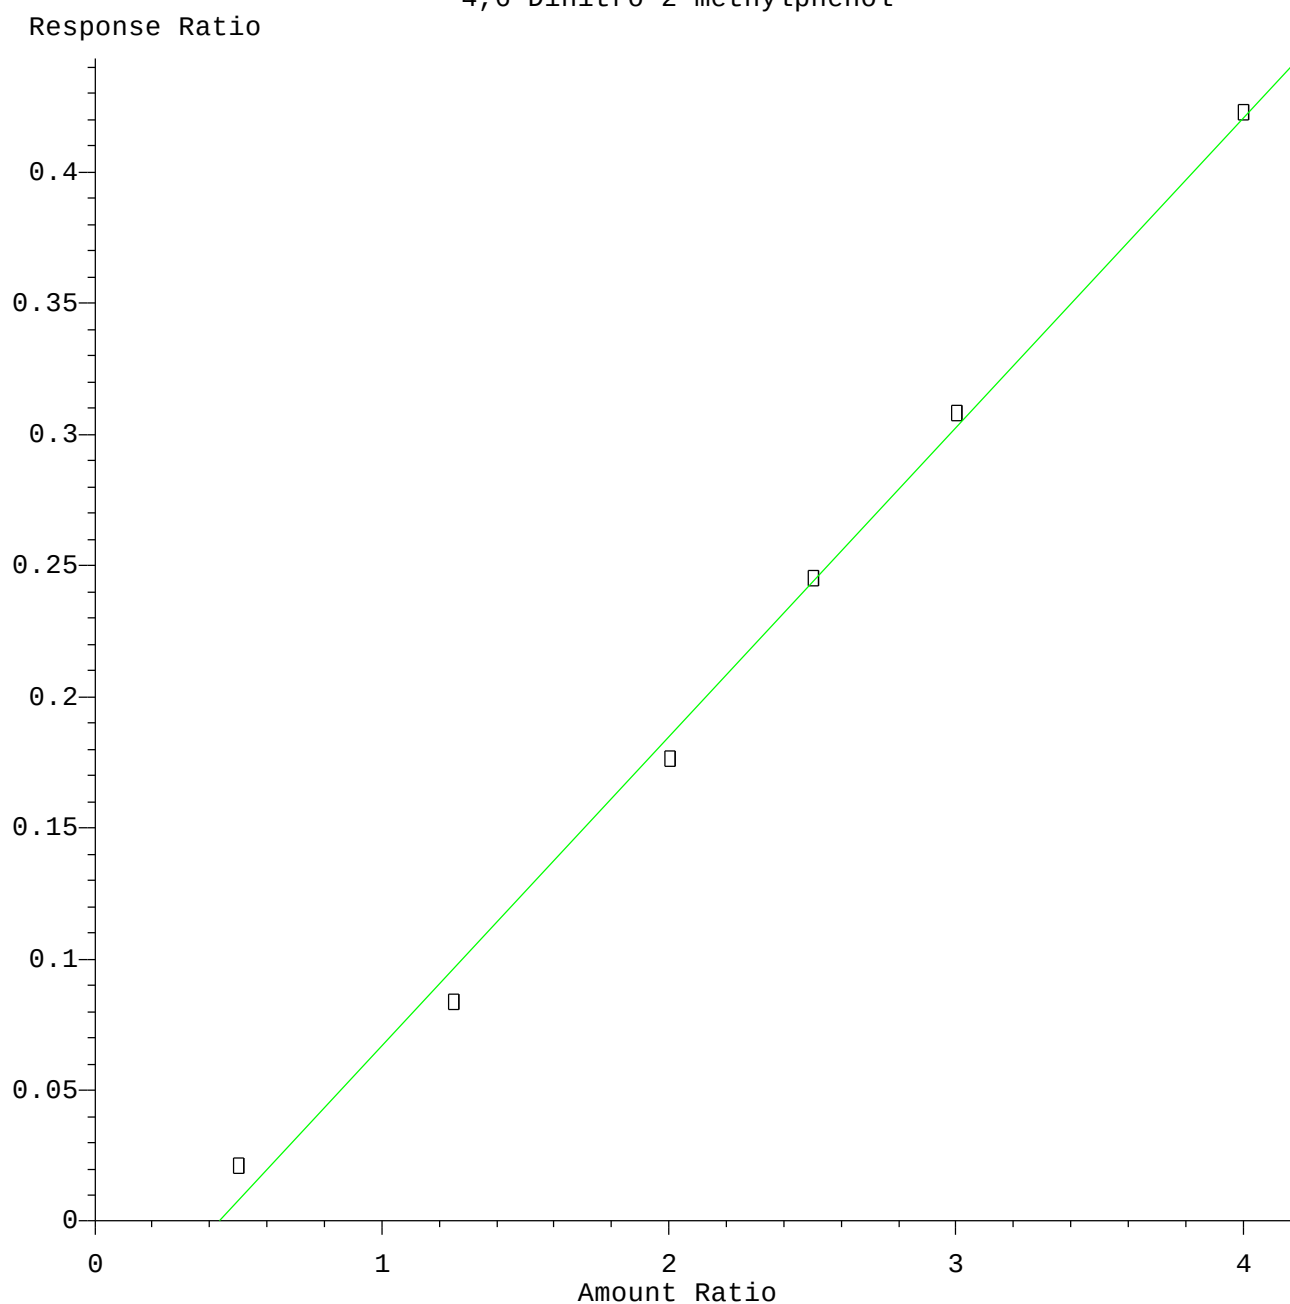

Resp Ratio = $1.18 \times 10^{-1} \times \text{Amt} - 5.12 \times 10^{-2}$
Coef of Det (r^2) = 0.996 Curve Fit: Linear


Method Name: Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072018.M
Calibration Table Last Updated: Fri Jul 20 16:29:27 2018

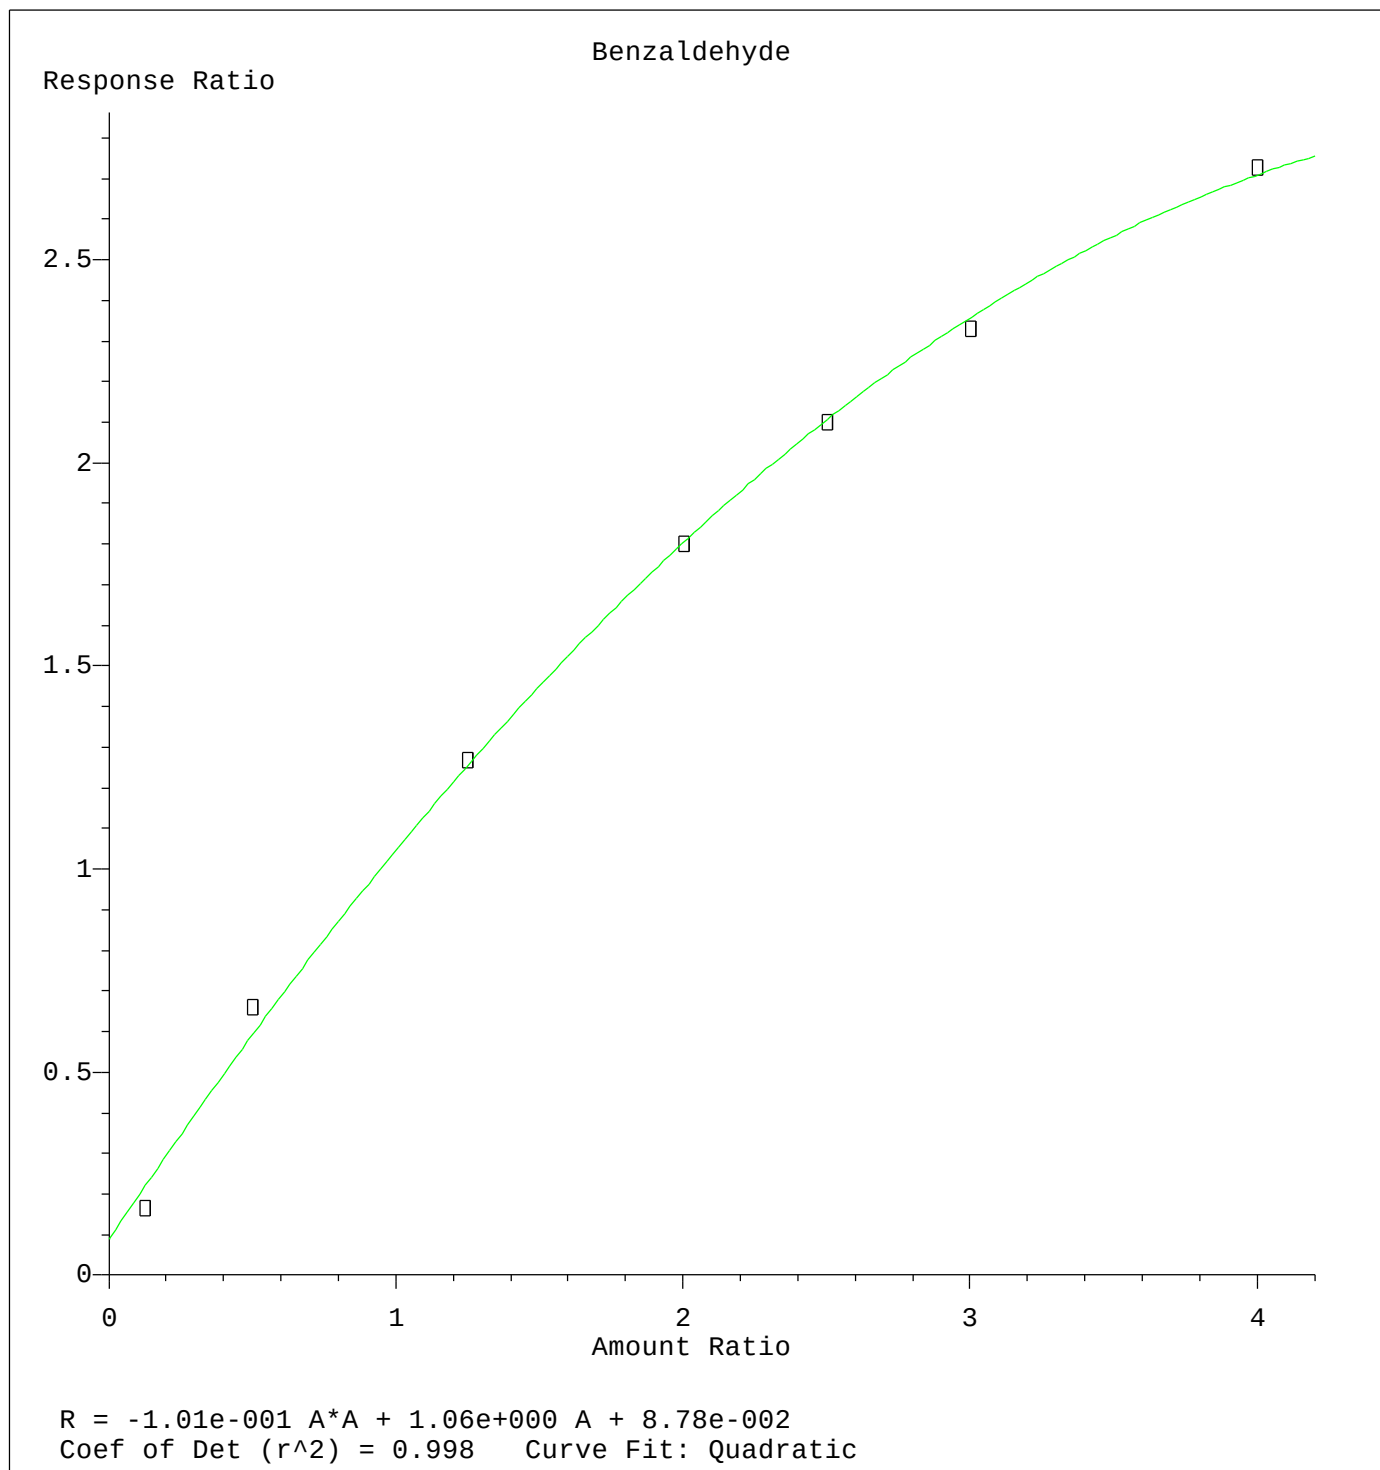

Method Name: Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072018.M
Calibration Table Last Updated: Fri Jul 20 16:29:27 2018


2-Fluorobiphenyl

Response Ratio

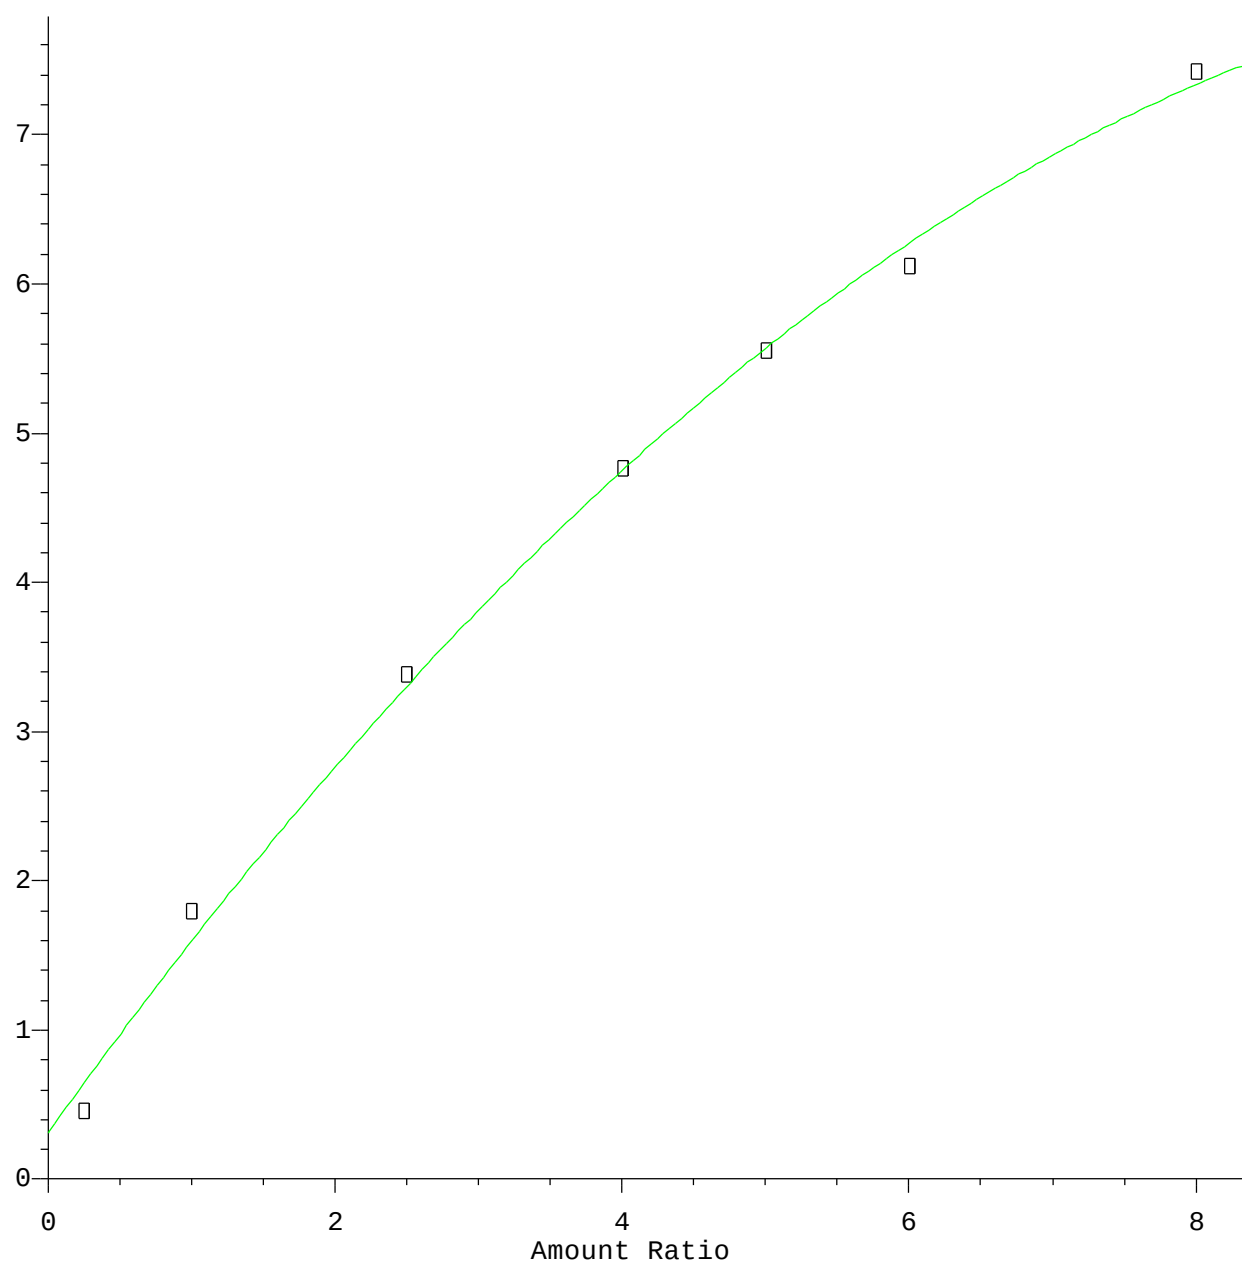


$R = -5.78e-002 A^2 + 1.34e+000 A + 3.12e-001$
Coef of Det (r^2) = 0.997 Curve Fit: Quadratic

Method Name: Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072018.M
Calibration Table Last Updated: Fri Jul 20 16:29:27 2018

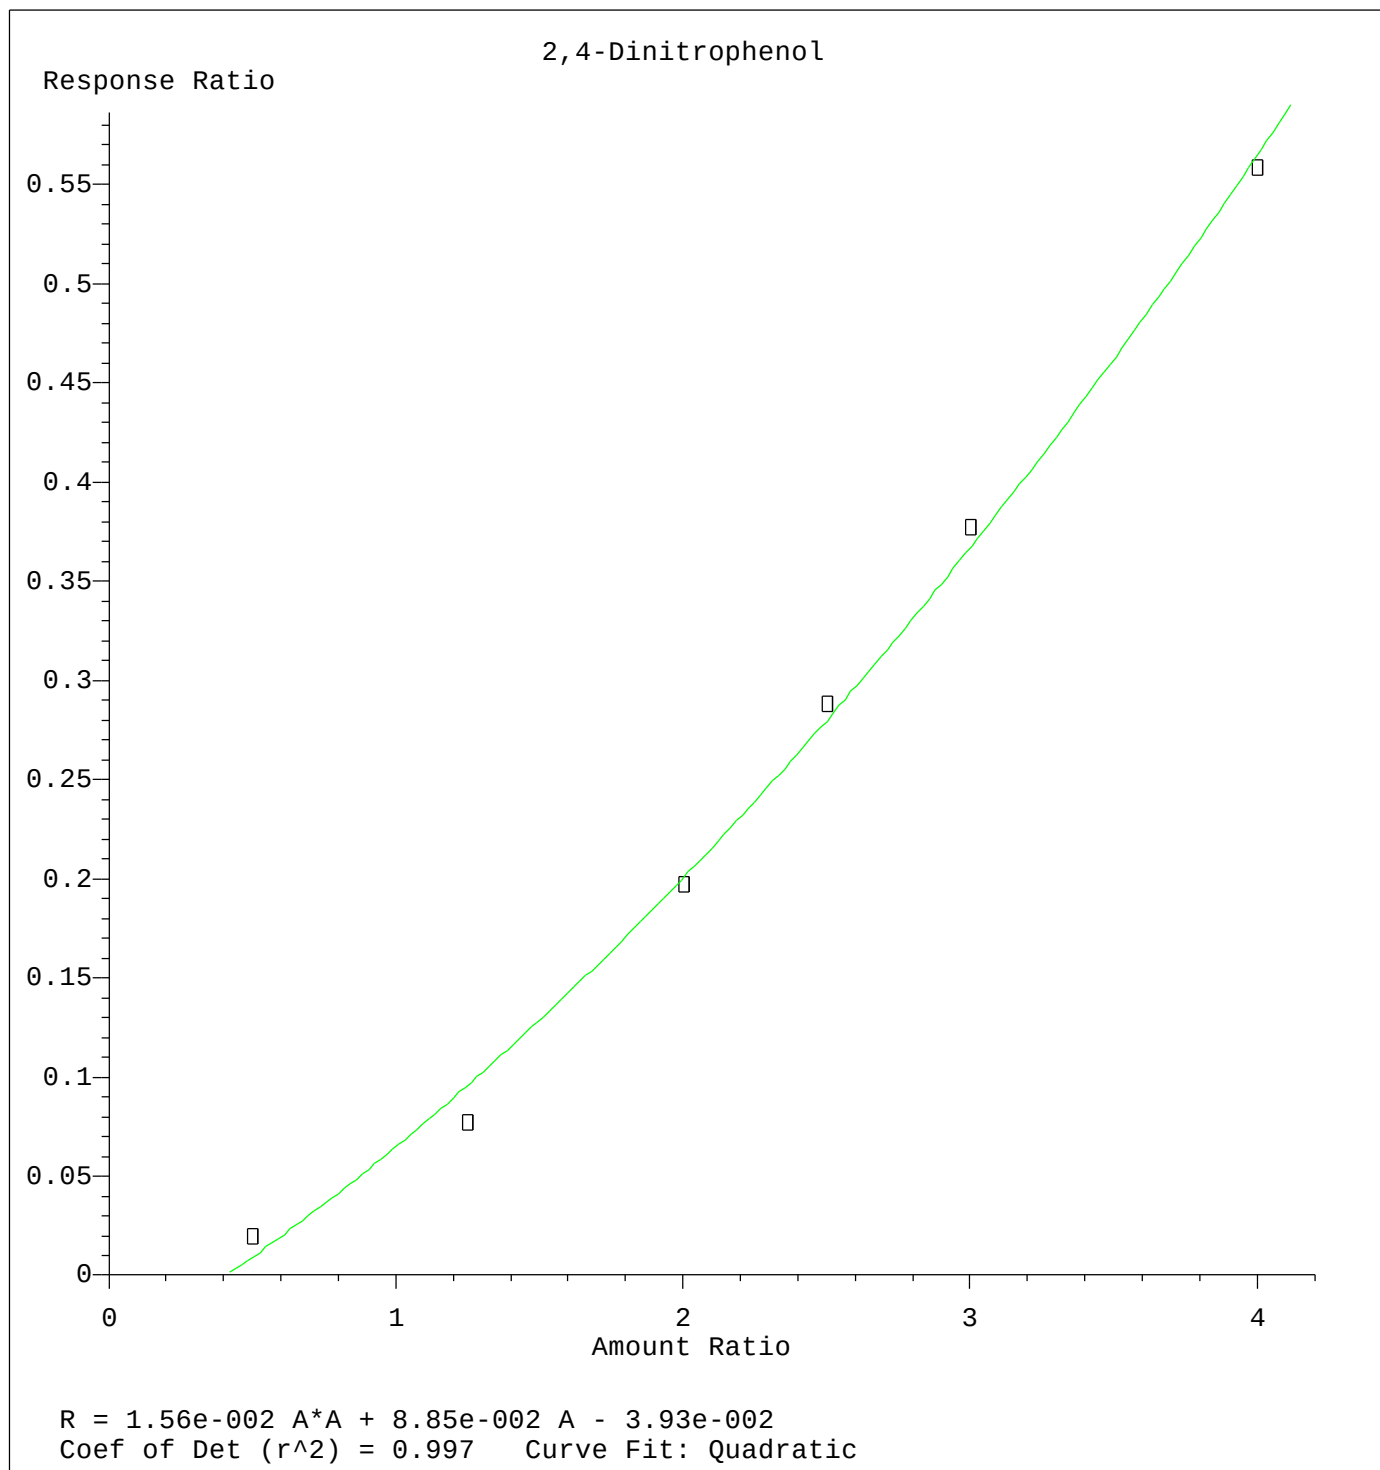


Method Name: Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072018.M
Calibration Table Last Updated: Fri Jul 20 16:29:27 2018

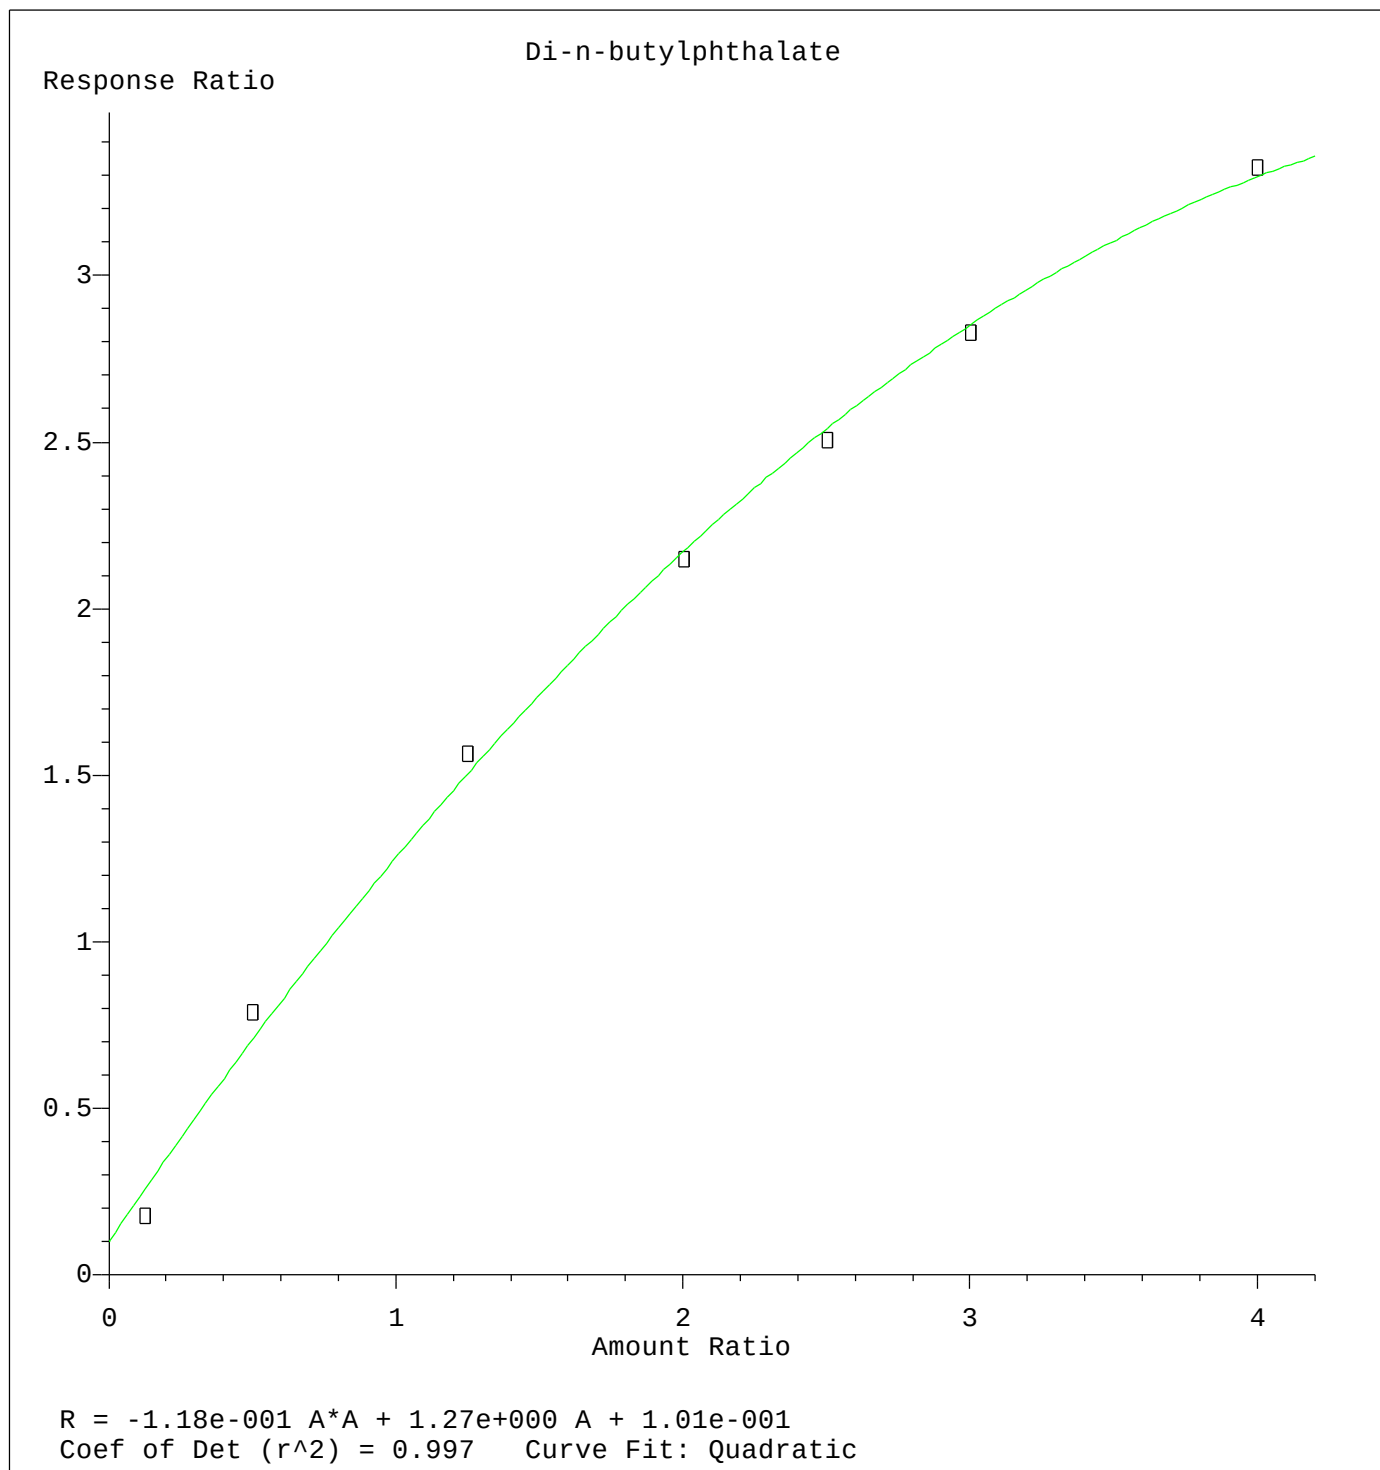

Method Name: Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072018.M
Calibration Table Last Updated: Fri Jul 20 16:29:27 2018

3,3'-Dichlorobenzidine

Response Ratio

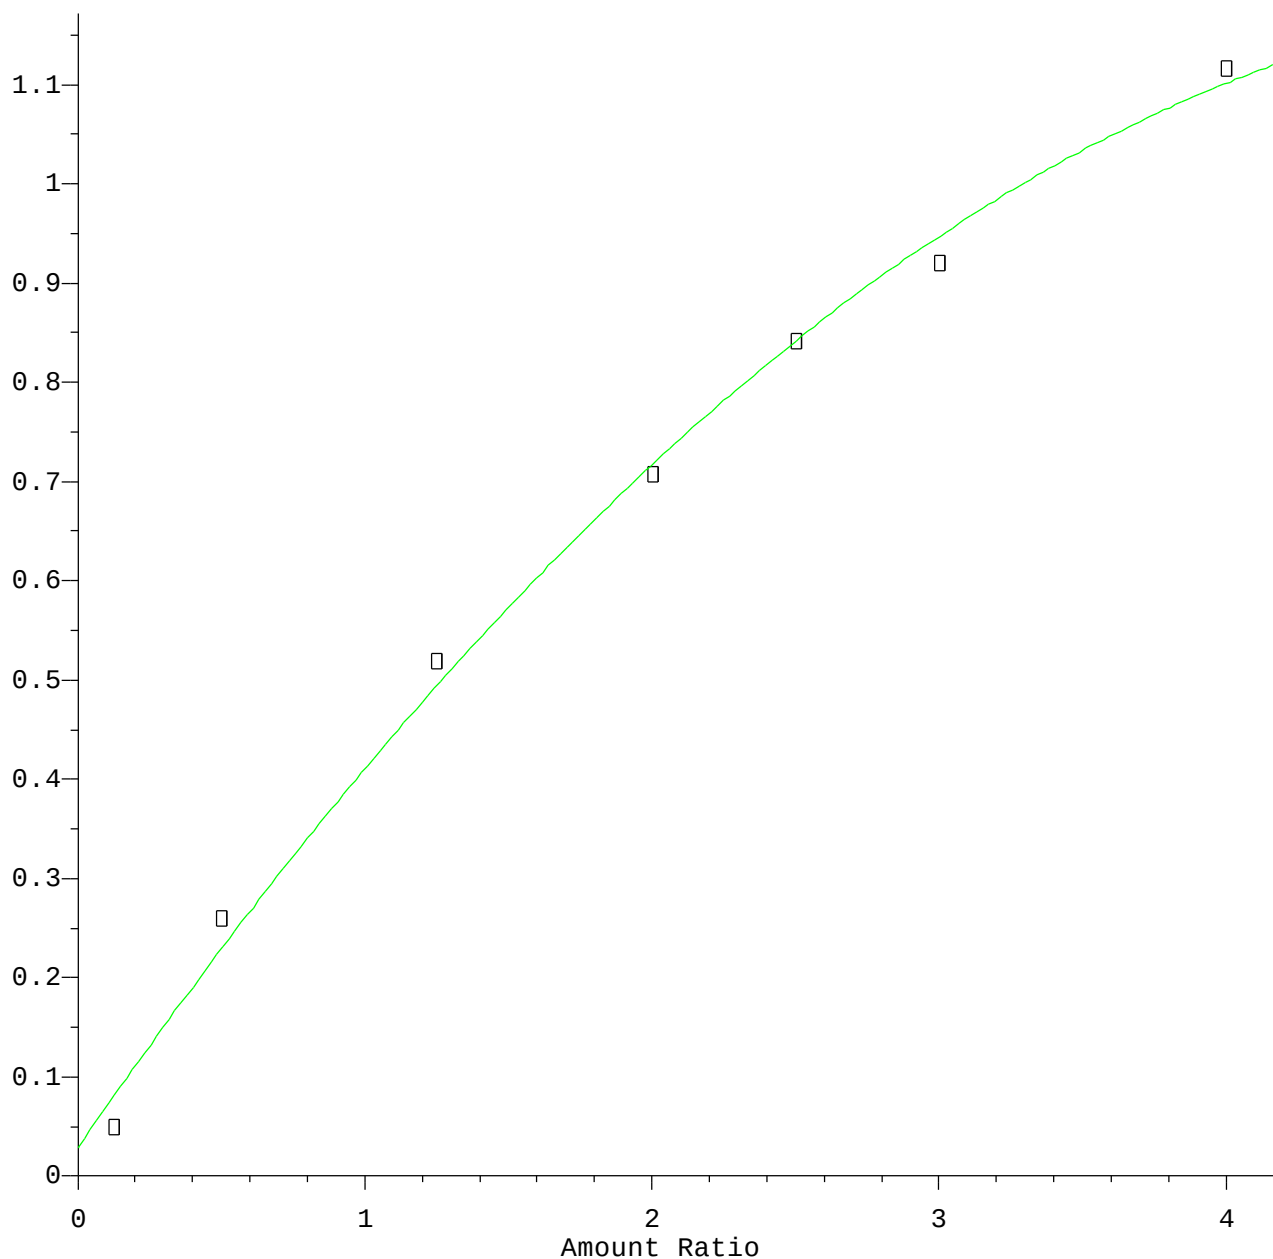

$R = -3.79e-002 A^2 + 4.20e-001 A + 2.89e-002$
Coef of Det (r^2) = 0.996 Curve Fit: Quadratic

Method Name: Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072018.M
Calibration Table Last Updated: Fri Jul 20 16:29:27 2018